

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030481.D
 Acq On : 06 Aug 2022 22:35
 Operator : JC/MD
 Sample : N4066-07DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	121599	140560	13.48%	1.559%
2	1.660	91	94	101	rBV	72658	91413	8.76%	1.014%
3	2.300	193	199	210	rVB	194514	313374	30.04%	3.475%
4	2.581	242	245	246	rBV2	622	569	0.05%	0.006%
5	2.788	275	279	286	rVB3	4326	7768	0.74%	0.086%
6	2.947	298	305	313	rBV2	15902	36172	3.47%	0.401%
7	3.203	345	347	350	rBV2	311	382	0.04%	0.004%
8	3.233	350	352	354	rBV2	409	519	0.05%	0.006%
9	3.428	382	384	387	rBV	496	417	0.04%	0.005%
10	3.538	401	402	406	rVB	671	625	0.06%	0.007%
11	3.581	406	409	411	rBV	374	496	0.05%	0.006%
12	3.605	411	413	415	rBV3	351	406	0.04%	0.005%
13	3.819	446	448	452	rVB	627	758	0.07%	0.008%
14	3.879	454	458	461	rBV2	452	862	0.08%	0.010%
15	3.953	465	470	473	rBV2	509	838	0.08%	0.009%
16	4.099	491	494	497	rBV2	259	374	0.04%	0.004%
17	4.233	513	516	519	rBV	350	498	0.05%	0.006%
18	4.282	523	524	529	rVB2	541	496	0.05%	0.006%
19	4.318	529	530	538	rVB2	543	775	0.07%	0.009%
20	4.483	546	557	572	rBV2	149665	470463	45.10%	5.217%
21	4.867	618	620	621	rBV	909	475	0.05%	0.005%
22	5.062	638	652	668	rBV	142610	428257	41.06%	4.749%
23	5.263	683	685	688	rBV2	404	558	0.05%	0.006%
24	5.379	703	704	705	rBV	556	370	0.04%	0.004%
25	5.538	727	730	732	rBV3	713	960	0.09%	0.011%
26	5.556	732	733	739	rVB2	1176	1212	0.12%	0.013%
27	5.763	766	767	770	rBV2	406	513	0.05%	0.006%
28	5.861	781	783	786	rVB3	437	401	0.04%	0.004%
29	5.897	786	789	790	rBV	422	400	0.04%	0.004%
30	5.971	790	801	822	rVV3	356699	1043052	100.00%	11.566%
31	6.153	829	831	834	rVB3	513	379	0.04%	0.004%
32	6.300	853	855	858	rBV2	319	420	0.04%	0.005%
33	6.367	860	866	873	rVB7	1842	5067	0.49%	0.056%
34	6.629	906	909	911	rBV2	360	389	0.04%	0.004%
35	6.763	922	931	945	rBV	298427	723130	69.33%	8.019%
36	7.129	981	991	1002	rBV	290456	614267	58.89%	6.812%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030481.D
 Acq On : 06 Aug 2022 22:35
 Operator : JC/MD
 Sample : N4066-07DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1035	rBV	223478	495364	47.49%	5.493%
38	7.452	1041	1044	1045	rBV	540	480	0.05%	0.005%
39	7.482	1045	1049	1050	rBV2	413	566	0.05%	0.006%
40	7.659	1076	1078	1081	rBV2	451	488	0.05%	0.005%
41	7.690	1081	1083	1086	rVB2	561	362	0.03%	0.004%
42	7.793	1097	1100	1102	rBV2	478	492	0.05%	0.005%
43	7.836	1102	1107	1108	rBV2	622	759	0.07%	0.008%
44	7.860	1108	1111	1113	rVV2	649	473	0.05%	0.005%
45	7.964	1124	1128	1135	rVB5	1537	3032	0.29%	0.034%
46	8.019	1135	1137	1140	rBV	385	548	0.05%	0.006%
47	8.220	1169	1170	1174	rBV2	520	560	0.05%	0.006%
48	8.263	1174	1177	1179	rVB	640	609	0.06%	0.007%
49	8.330	1181	1188	1200	rBV	133301	223410	21.42%	2.477%
50	8.653	1234	1241	1251	rBV	512867	788480	75.59%	8.743%
51	8.952	1285	1290	1301	rBV	95279	146317	14.03%	1.623%
52	9.275	1337	1343	1356	rVB	119002	176671	16.94%	1.959%
53	9.397	1356	1363	1376	rBV	355432	591115	56.67%	6.555%
54	9.714	1409	1415	1420	rBV3	3273	5986	0.57%	0.066%
55	9.817	1429	1432	1434	rBV2	596	756	0.07%	0.008%
56	10.055	1466	1471	1480	rVV	614468	840251	80.56%	9.318%
57	10.165	1486	1489	1491	rBV3	572	555	0.05%	0.006%
58	10.299	1510	1511	1517	rVB3	716	786	0.08%	0.009%
59	10.397	1523	1527	1529	rBV2	321	436	0.04%	0.005%
60	10.506	1543	1545	1547	rBV	529	536	0.05%	0.006%
61	10.653	1565	1569	1570	rBV3	393	408	0.04%	0.005%
62	10.768	1586	1588	1590	rBV2	425	379	0.04%	0.004%
63	10.860	1599	1603	1604	rBV2	564	591	0.06%	0.007%
64	10.970	1617	1621	1623	rBV2	717	732	0.07%	0.008%
65	11.018	1627	1629	1631	rVB2	465	426	0.04%	0.005%
66	11.067	1633	1637	1640	rBV	559	985	0.09%	0.011%
67	11.134	1647	1648	1652	rBV2	472	470	0.05%	0.005%
68	11.195	1652	1658	1668	rVV	373621	472405	45.29%	5.238%
69	11.342	1681	1682	1688	rVB3	525	725	0.07%	0.008%
70	11.403	1688	1692	1694	rBV2	838	736	0.07%	0.008%
71	11.451	1698	1700	1702	rBV2	757	603	0.06%	0.007%
72	11.512	1708	1710	1712	rBV	383	400	0.04%	0.004%
73	11.610	1724	1726	1729	rBV3	324	409	0.04%	0.005%
74	11.689	1735	1739	1741	rBV2	667	768	0.07%	0.009%
75	11.909	1771	1775	1776	rBV2	386	529	0.05%	0.006%
76	11.976	1783	1786	1789	rBV4	755	846	0.08%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030481.D
 Acq On : 06 Aug 2022 22:35
 Operator : JC/MD
 Sample : N4066-07DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1804	rVV	583028	711876	68.25%	7.894%
78	12.134	1811	1812	1815	rBV2	471	422	0.04%	0.005%
79	12.183	1818	1820	1823	rVB2	691	616	0.06%	0.007%
80	12.323	1837	1843	1854	rBV	522844	644652	61.80%	7.149%
81	12.512	1873	1874	1878	rVB2	684	632	0.06%	0.007%
82	12.622	1890	1892	1896	rVV3	903	1077	0.10%	0.012%
83	12.671	1898	1900	1903	rVB2	723	651	0.06%	0.007%
84	12.817	1922	1924	1926	rBV	375	386	0.04%	0.004%
85	12.896	1936	1937	1942	rBV2	579	562	0.05%	0.006%
86	12.975	1948	1950	1955	rBV2	491	594	0.06%	0.007%
87	13.347	2005	2011	2012	rBV3	408	688	0.07%	0.008%
88	13.646	2057	2060	2063	rBV2	356	461	0.04%	0.005%
89	13.780	2080	2082	2087	rVB2	462	502	0.05%	0.006%
90	13.853	2092	2094	2096	rBV2	430	455	0.04%	0.005%
91	13.951	2108	2110	2111	rBV	489	455	0.04%	0.005%
92	14.012	2118	2120	2125	rVB2	457	592	0.06%	0.007%
93	14.085	2129	2132	2135	rBV2	415	646	0.06%	0.007%
94	14.390	2181	2182	2187	rBV2	421	592	0.06%	0.007%
95	14.445	2189	2191	2194	rBV	778	718	0.07%	0.008%
96	14.664	2225	2227	2229	rVB2	626	494	0.05%	0.005%
97	14.707	2232	2234	2237	rBV2	638	636	0.06%	0.007%
98	15.371	2341	2343	2346	rBV3	745	818	0.08%	0.009%
99	15.792	2410	2412	2415	rBV3	641	819	0.08%	0.009%
100	16.767	2570	2572	2573	rBV2	654	547	0.05%	0.006%




Sum of corrected areas: 9017950

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030481.D
Acq On : 06 Aug 2022 22:35
Operator : JC/MD
Sample : N4066-07DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

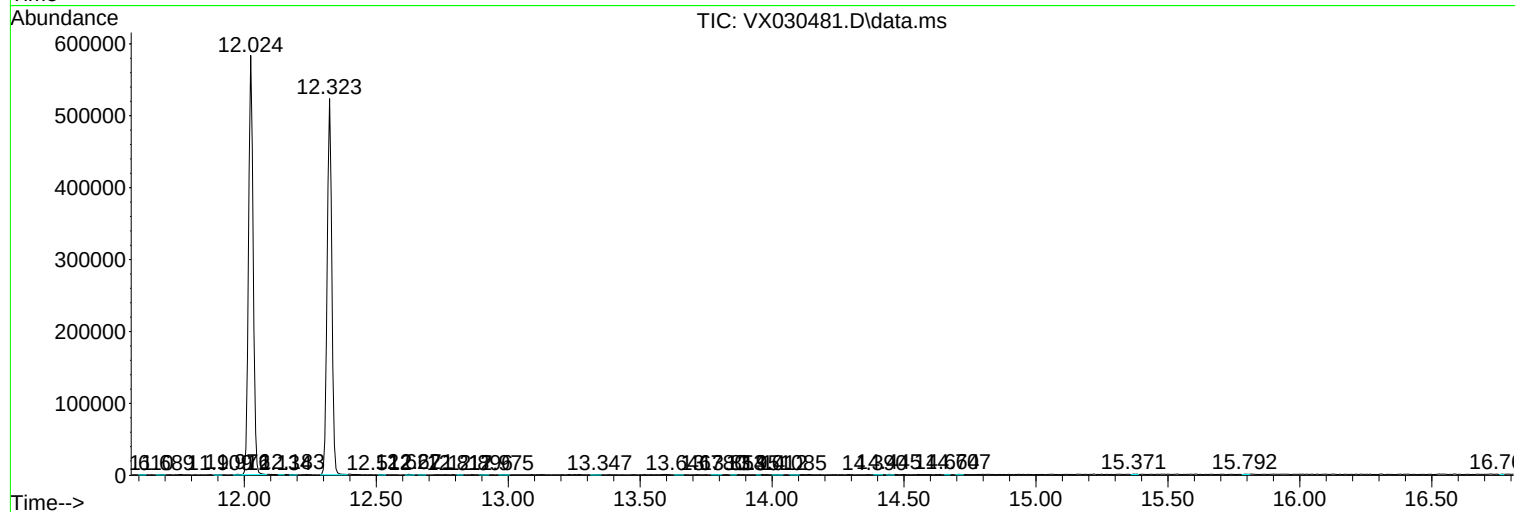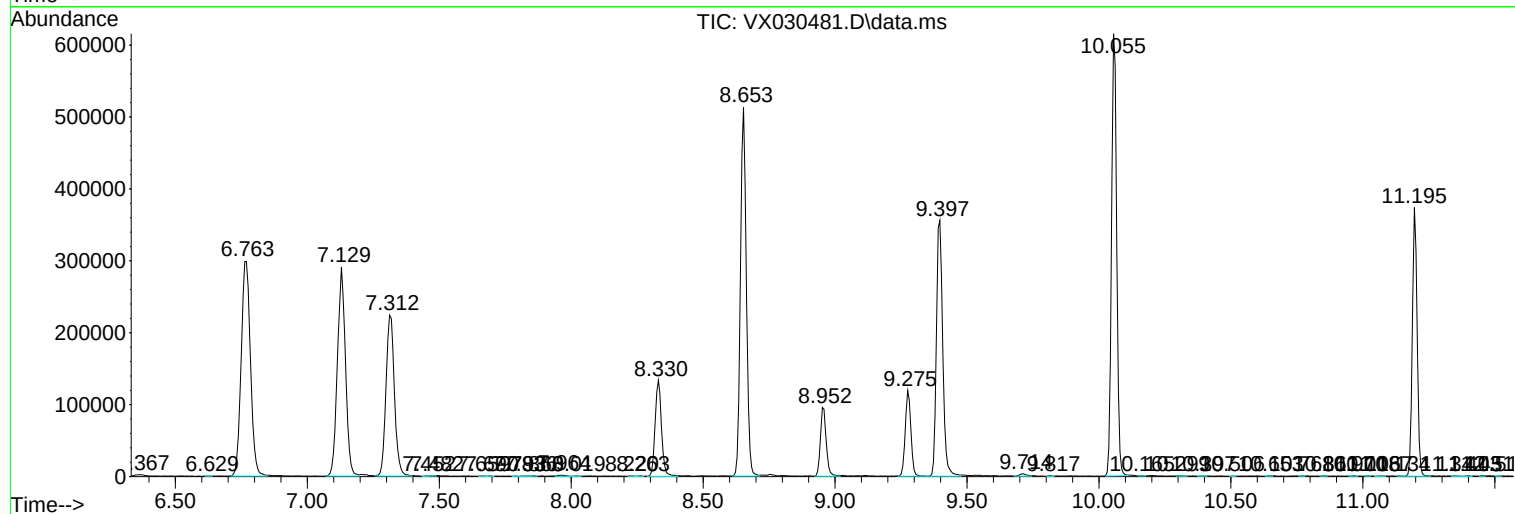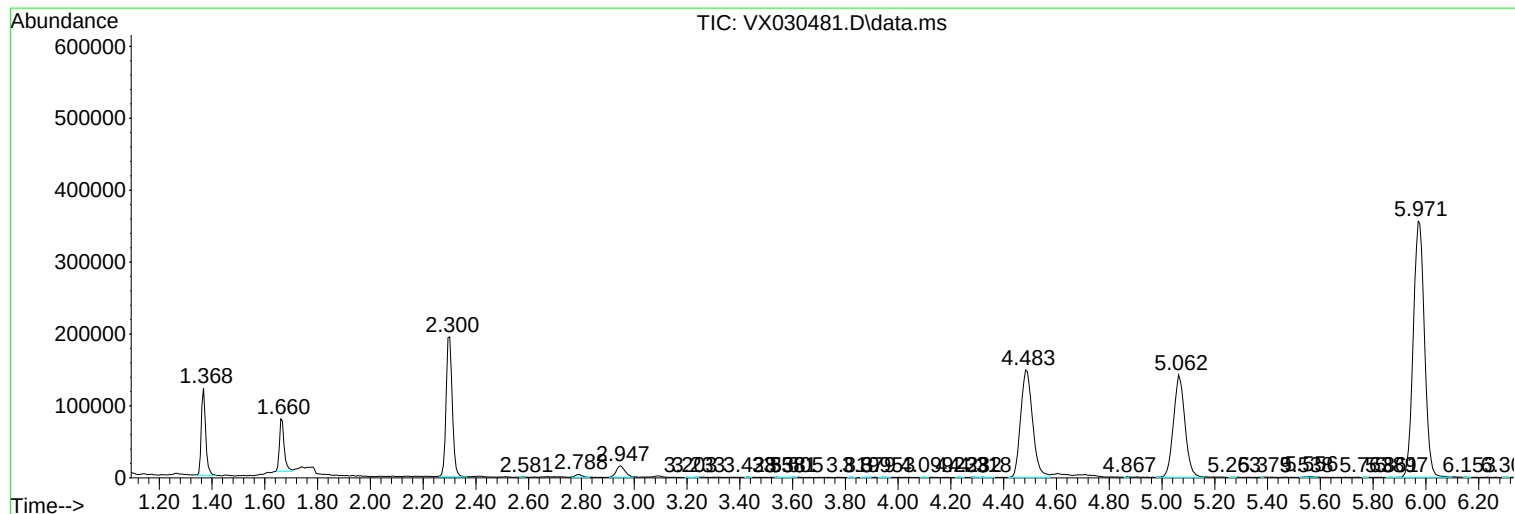

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030481.D
Acq On : 06 Aug 2022 22:35
Operator : JC/MD
Sample : N4066-07DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030481.D
Acq On : 06 Aug 2022 22:35
Operator : JC/MD
Sample : N4066-07DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc