

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030483.D
 Acq On : 06 Aug 2022 23:22
 Operator : JC/MD
 Sample : N4021-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB2	627223	693930	9.50%	4.320%
2	1.666	91	95	103	rVB	104608	124020	1.70%	0.772%
3	2.306	194	200	212	rVV2	233056	413688	5.67%	2.575%
4	2.398	212	215	219	rVB5	1253	2010	0.03%	0.013%
5	2.629	252	253	255	rBV	437	278	0.00%	0.002%
6	2.745	270	272	274	rVB	550	289	0.00%	0.002%
7	2.776	274	277	278	rBV2	732	598	0.01%	0.004%
8	2.892	295	296	299	rVB2	586	433	0.01%	0.003%
9	3.093	322	329	342	rVB	111771	217279	2.98%	1.353%
10	3.257	351	356	358	rBV2	456	697	0.01%	0.004%
11	3.343	369	370	373	rVB	554	345	0.00%	0.002%
12	3.434	384	385	388	rBV2	401	448	0.01%	0.003%
13	3.532	399	401	403	rVB2	430	293	0.00%	0.002%
14	3.562	403	406	407	rBV2	435	495	0.01%	0.003%
15	3.623	414	416	419	rVV	337	344	0.00%	0.002%
16	3.672	422	424	426	rBV2	486	448	0.01%	0.003%
17	3.696	426	428	430	rBV2	314	365	0.00%	0.002%
18	3.861	453	455	456	rVB	551	303	0.00%	0.002%
19	3.885	458	459	462	rVV	529	378	0.01%	0.002%
20	3.946	465	469	470	rVB2	296	270	0.00%	0.002%
21	4.062	485	488	489	rBV2	334	301	0.00%	0.002%
22	4.196	508	510	511	rBV2	396	349	0.00%	0.002%
23	4.251	514	519	520	rBV2	534	724	0.01%	0.005%
24	4.324	529	531	533	rBV	402	454	0.01%	0.003%
25	4.495	546	559	578	rBV	2691229	7300688	100.00%	45.448%
26	4.958	633	635	637	rBV3	414	381	0.01%	0.002%
27	5.062	640	652	669	rVV	133730	424593	5.82%	2.643%
28	5.537	728	730	731	rBV	435	281	0.00%	0.002%
29	5.684	753	754	757	rVB	499	380	0.01%	0.002%
30	5.720	759	760	763	rVB2	410	339	0.00%	0.002%
31	5.763	765	767	771	rBV2	355	368	0.01%	0.002%
32	5.830	775	778	781	rVB	352	333	0.00%	0.002%
33	5.976	791	802	819	rVV2	353176	1012866	13.87%	6.305%
34	6.360	863	865	866	rBV	498	323	0.00%	0.002%
35	6.403	870	872	874	rBV2	430	329	0.00%	0.002%
36	6.446	876	879	882	rBV2	404	496	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030483.D
 Acq On : 06 Aug 2022 23:22
 Operator : JC/MD
 Sample : N4021-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.501	886	888	889	rVB2	427	284	0.00%	0.002%
38	6.531	892	893	895	rBV2	425	331	0.00%	0.002%
39	6.562	895	898	901	rVB	419	526	0.01%	0.003%
40	6.769	922	932	943	rBV	298521	708507	9.70%	4.411%
41	7.129	981	991	1002	rVV2	101007	233842	3.20%	1.456%
42	7.318	1011	1022	1033	rBV	213641	471761	6.46%	2.937%
43	7.415	1037	1038	1041	rVB2	965	597	0.01%	0.004%
44	7.458	1041	1045	1047	rBV3	869	1158	0.02%	0.007%
45	7.561	1060	1062	1064	rVB2	457	349	0.00%	0.002%
46	7.714	1085	1087	1090	rVB2	424	339	0.00%	0.002%
47	7.824	1102	1105	1106	rBV2	264	281	0.00%	0.002%
48	8.043	1139	1141	1142	rBV2	393	346	0.00%	0.002%
49	8.128	1152	1155	1158	rBV2	368	593	0.01%	0.004%
50	8.250	1171	1175	1179	rBV2	407	546	0.01%	0.003%
51	8.330	1182	1188	1201	rBV	132578	216412	2.96%	1.347%
52	8.573	1227	1228	1231	rVB	410	265	0.00%	0.002%
53	8.653	1234	1241	1252	rBV	526228	794549	10.88%	4.946%
54	8.823	1267	1269	1271	rVB2	739	445	0.01%	0.003%
55	8.848	1271	1273	1276	rBV2	547	359	0.00%	0.002%
56	8.957	1285	1291	1303	rBV	91163	142480	1.95%	0.887%
57	9.171	1323	1326	1328	rBV2	735	741	0.01%	0.005%
58	9.275	1340	1343	1348	rBV4	3111	4118	0.06%	0.026%
59	9.390	1356	1362	1374	rBV	405822	577828	7.91%	3.597%
60	9.707	1412	1414	1416	rVB	460	341	0.00%	0.002%
61	9.994	1459	1461	1464	rVB	470	378	0.01%	0.002%
62	10.055	1466	1471	1485	rVB	601617	822077	11.26%	5.118%
63	10.280	1506	1508	1509	rBV	493	367	0.01%	0.002%
64	10.299	1509	1511	1513	rVB2	412	374	0.01%	0.002%
65	10.573	1554	1556	1559	rVB2	390	295	0.00%	0.002%
66	10.616	1559	1563	1565	rVB2	480	595	0.01%	0.004%
67	11.024	1627	1630	1633	rVB	560	750	0.01%	0.005%
68	11.195	1652	1658	1666	rBV	362777	463955	6.35%	2.888%
69	11.390	1688	1690	1693	rVV3	388	441	0.01%	0.003%
70	11.451	1698	1700	1701	rBV3	451	362	0.00%	0.002%
71	11.689	1736	1739	1740	rBV2	378	286	0.00%	0.002%
72	11.841	1762	1764	1765	rBV2	373	349	0.00%	0.002%
73	11.884	1768	1771	1772	rBV2	333	377	0.01%	0.002%
74	12.024	1789	1794	1803	rBV	612635	742443	10.17%	4.622%
75	12.164	1816	1817	1821	rBV2	433	465	0.01%	0.003%
76	12.213	1823	1825	1827	rBV3	400	354	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030483.D
 Acq On : 06 Aug 2022 23:22
 Operator : JC/MD
 Sample : N4021-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1851	rBV	529254	660545	9.05%	4.112%
78	12.518	1873	1875	1880	rBV2	608	722	0.01%	0.004%
79	12.719	1906	1908	1910	rBV2	457	375	0.01%	0.002%
80	12.853	1929	1930	1932	rBV2	527	509	0.01%	0.003%
81	13.109	1967	1972	1975	rBV2	513	879	0.01%	0.005%
82	13.286	1999	2001	2003	rVB2	564	340	0.00%	0.002%
83	13.432	2023	2025	2027	rBV	439	426	0.01%	0.003%
84	13.499	2034	2036	2039	rBV2	331	395	0.01%	0.002%
85	13.737	2073	2075	2077	rVB	481	370	0.01%	0.002%
86	13.792	2080	2084	2085	rVV4	723	812	0.01%	0.005%
87	13.835	2089	2091	2095	rBV	433	766	0.01%	0.005%
88	14.133	2138	2140	2143	rVB2	575	412	0.01%	0.003%
89	14.170	2143	2146	2149	rVB2	782	822	0.01%	0.005%
90	14.200	2149	2151	2152	rBV	473	436	0.01%	0.003%
91	14.328	2170	2172	2177	rBV2	536	735	0.01%	0.005%
92	14.463	2192	2194	2195	rBV	682	364	0.00%	0.002%
93	14.481	2195	2197	2201	rBV2	439	633	0.01%	0.004%
94	14.627	2219	2221	2225	rBV3	569	717	0.01%	0.004%
95	14.749	2239	2241	2242	rBV	581	288	0.00%	0.002%
96	15.097	2297	2298	2301	rVB2	686	382	0.01%	0.002%
97	15.828	2416	2418	2420	rBV2	614	704	0.01%	0.004%
98	16.072	2456	2458	2461	rVB2	774	547	0.01%	0.003%
99	16.096	2461	2462	2463	rBV	597	311	0.00%	0.002%
100	16.779	2573	2574	2575	rVB	1002	367	0.01%	0.002%




Sum of corrected areas: 16063839

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030483.D
Acq On : 06 Aug 2022 23:22
Operator : JC/MD
Sample : N4021-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

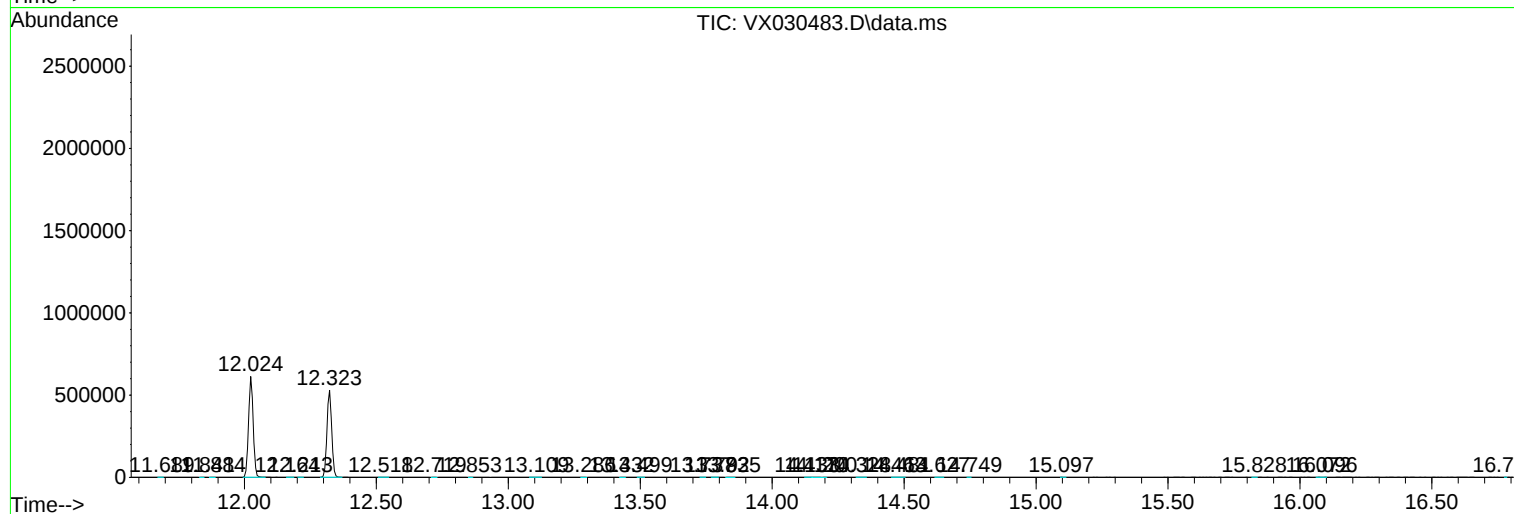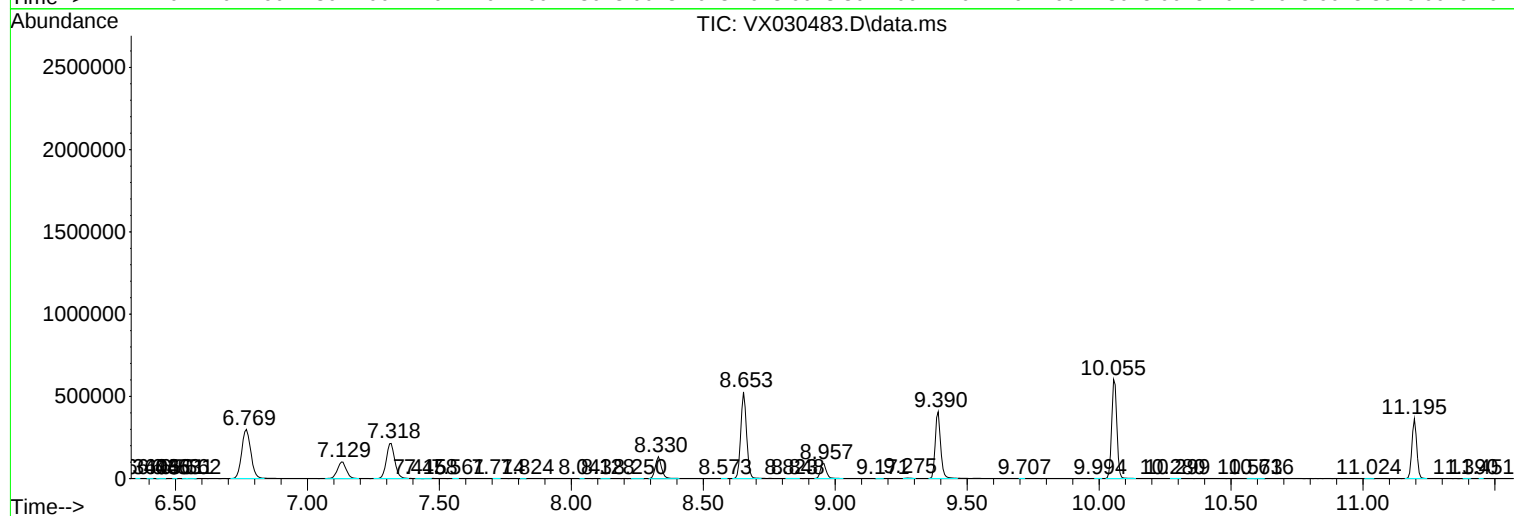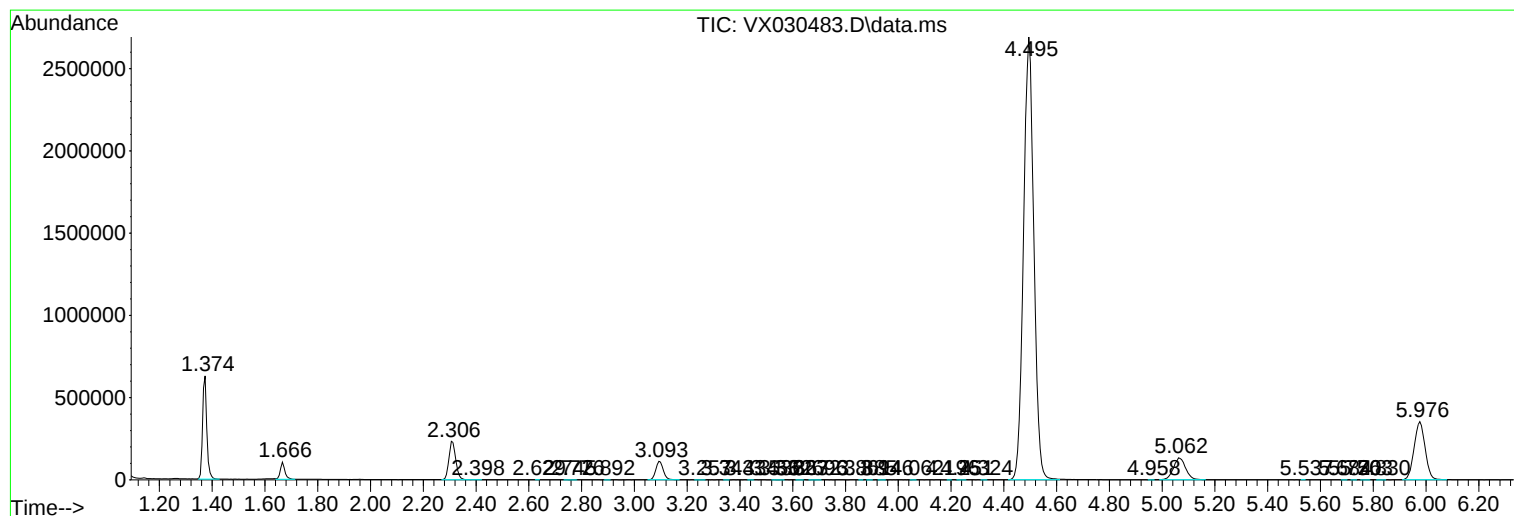

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030483.D
Acq On : 06 Aug 2022 23:22
Operator : JC/MD
Sample : N4021-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030483.D
Acq On : 06 Aug 2022 23:22
Operator : JC/MD
Sample : N4021-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc