

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030484.D
 Acq On : 06 Aug 2022 23:45
 Operator : JC/MD
 Sample : VIBLK654
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	122408	126429	12.26%	1.559%
2	1.666	91	95	102	rVB	107624	125286	12.15%	1.545%
3	2.093	163	165	167	rVB2	1088	906	0.09%	0.011%
4	2.307	194	200	211	rVB	207237	319752	31.00%	3.944%
5	2.624	250	252	258	rVB3	797	1099	0.11%	0.014%
6	2.697	262	264	267	rBV2	527	343	0.03%	0.004%
7	2.794	275	280	286	rVB5	3730	7523	0.73%	0.093%
8	2.843	286	288	290	rBV2	282	359	0.03%	0.004%
9	2.880	293	294	296	rBV	370	359	0.03%	0.004%
10	2.953	298	306	312	rBV2	7524	17901	1.74%	0.221%
11	3.099	325	330	333	rBV4	939	1432	0.14%	0.018%
12	3.270	353	358	362	rVB2	621	1212	0.12%	0.015%
13	3.319	362	366	367	rBV	470	519	0.05%	0.006%
14	3.428	381	384	386	rBV2	330	368	0.04%	0.005%
15	3.501	393	396	398	rBV	578	515	0.05%	0.006%
16	3.636	415	418	421	rVB3	560	649	0.06%	0.008%
17	3.709	429	430	433	rBV2	364	319	0.03%	0.004%
18	3.745	433	436	439	rVB	514	728	0.07%	0.009%
19	3.782	439	442	443	rVB2	519	469	0.05%	0.006%
20	3.800	443	445	447	rBV2	467	479	0.05%	0.006%
21	4.123	496	498	501	rBV2	489	417	0.04%	0.005%
22	4.221	512	514	515	rBV2	400	371	0.04%	0.005%
23	4.477	543	556	567	rBV2	93634	287383	27.86%	3.545%
24	4.873	620	621	623	rBV2	516	385	0.04%	0.005%
25	5.062	640	652	669	rVV	133652	417522	40.48%	5.150%
26	5.208	674	676	677	rBV2	547	345	0.03%	0.004%
27	5.391	701	706	711	rVV2	715	1359	0.13%	0.017%
28	5.489	721	722	726	rBV2	425	412	0.04%	0.005%
29	5.550	729	732	733	rBV2	651	605	0.06%	0.007%
30	5.757	763	766	768	rBV2	654	548	0.05%	0.007%
31	5.806	773	774	776	rBV2	478	308	0.03%	0.004%
32	5.867	782	784	787	rVB	366	357	0.03%	0.004%
33	5.977	790	802	816	rBV2	355936	1031363	100.00%	12.721%
34	6.470	880	883	886	rVV2	367	429	0.04%	0.005%
35	6.556	893	897	899	rBV2	554	779	0.08%	0.010%
36	6.769	922	932	948	rBV	304000	728538	70.64%	8.986%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030484.D
 Acq On : 06 Aug 2022 23:45
 Operator : JC/MD
 Sample : VIBLK654
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.031	973	975	978	rVB2	417	382	0.04%	0.005%
38	7.062	978	980	982	rBV	314	306	0.03%	0.004%
39	7.117	982	989	998	rVB4	13230	30723	2.98%	0.379%
40	7.226	1003	1007	1010	rBV2	584	1067	0.10%	0.013%
41	7.318	1012	1022	1033	rBV	213626	472917	45.85%	5.833%
42	7.470	1044	1047	1048	rBV2	463	494	0.05%	0.006%
43	7.598	1064	1068	1071	rBV2	462	625	0.06%	0.008%
44	7.671	1076	1080	1081	rVB2	330	327	0.03%	0.004%
45	7.952	1122	1126	1131	rVB3	688	1392	0.13%	0.017%
46	8.159	1158	1160	1161	rBV	423	342	0.03%	0.004%
47	8.196	1163	1166	1168	rBV	263	332	0.03%	0.004%
48	8.330	1181	1188	1198	rBV	131907	214793	20.83%	2.649%
49	8.653	1234	1241	1252	rBV	515524	796818	77.26%	9.828%
50	8.885	1275	1279	1280	rBV	430	529	0.05%	0.007%
51	8.952	1285	1290	1304	rVV	93659	144111	13.97%	1.777%
52	9.250	1336	1339	1340	rBV2	377	354	0.03%	0.004%
53	9.281	1340	1344	1346	rVB4	1096	1327	0.13%	0.016%
54	9.391	1356	1362	1375	rBV	415291	594718	57.66%	7.335%
55	9.708	1410	1414	1419	rVB4	1997	2878	0.28%	0.035%
56	9.811	1429	1431	1433	rBV2	473	426	0.04%	0.005%
57	9.921	1447	1449	1452	rBV	477	455	0.04%	0.006%
58	10.012	1461	1464	1465	rBV2	421	383	0.04%	0.005%
59	10.055	1466	1471	1482	rVV	624996	842892	81.73%	10.396%
60	10.208	1494	1496	1497	rBV	635	565	0.05%	0.007%
61	10.275	1506	1507	1509	rVV	662	431	0.04%	0.005%
62	10.317	1512	1514	1518	rVB3	794	800	0.08%	0.010%
63	10.354	1518	1520	1523	rBV3	427	510	0.05%	0.006%
64	10.445	1533	1535	1537	rBV2	393	360	0.03%	0.004%
65	10.494	1540	1543	1545	rVV	268	358	0.03%	0.004%
66	10.537	1549	1550	1553	rVB	619	423	0.04%	0.005%
67	10.579	1553	1557	1559	rBV2	516	701	0.07%	0.009%
68	10.628	1563	1565	1566	rVB	658	378	0.04%	0.005%
69	10.653	1566	1569	1571	rBV2	477	604	0.06%	0.007%
70	10.701	1574	1577	1579	rBV2	351	427	0.04%	0.005%
71	10.872	1601	1605	1609	rVB2	491	586	0.06%	0.007%
72	10.909	1609	1611	1612	rBV	419	409	0.04%	0.005%
73	10.963	1618	1620	1622	rBV	732	444	0.04%	0.005%
74	11.073	1635	1638	1641	rBV	408	616	0.06%	0.008%
75	11.195	1652	1658	1668	rVB	363687	462489	44.84%	5.704%
76	11.329	1678	1680	1682	rVB	502	368	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030484.D
 Acq On : 06 Aug 2022 23:45
 Operator : JC/MD
 Sample : VIBLK654
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK654

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.409	1692	1693	1696	rVB	520	349	0.03%	0.004%
78	11.713	1742	1743	1747	rBV2	453	581	0.06%	0.007%
79	11.854	1765	1766	1769	rBV2	596	522	0.05%	0.006%
80	11.902	1771	1774	1775	rBV	311	373	0.04%	0.005%
81	12.024	1789	1794	1805	rVV	623511	755340	73.24%	9.316%
82	12.323	1837	1843	1851	rBV	548862	684792	66.40%	8.446%
83	12.616	1887	1891	1893	rBV2	428	790	0.08%	0.010%
84	12.731	1909	1910	1912	rBV2	436	358	0.03%	0.004%
85	12.756	1912	1914	1918	rVV	373	427	0.04%	0.005%
86	13.097	1965	1970	1971	rBV2	515	685	0.07%	0.008%
87	13.134	1975	1976	1978	rBV	446	380	0.04%	0.005%
88	13.177	1981	1983	1986	rVB3	474	426	0.04%	0.005%
89	13.244	1992	1994	1997	rVB2	543	420	0.04%	0.005%
90	13.433	2023	2025	2028	rBV	376	400	0.04%	0.005%
91	13.481	2029	2033	2034	rVV2	430	385	0.04%	0.005%
92	13.871	2095	2097	2101	rVV2	380	364	0.04%	0.004%
93	14.012	2119	2120	2124	rBV	627	564	0.05%	0.007%
94	14.048	2124	2126	2127	rBV	555	334	0.03%	0.004%
95	14.396	2182	2183	2185	rBV	466	410	0.04%	0.005%
96	14.701	2229	2233	2234	rBV3	571	728	0.07%	0.009%
97	14.774	2243	2245	2248	rBV2	624	694	0.07%	0.009%
98	15.859	2421	2423	2424	rBV	582	440	0.04%	0.005%
99	15.920	2432	2433	2435	rBV	860	585	0.06%	0.007%
100	16.621	2546	2548	2549	rBV	631	399	0.04%	0.005%

Sum of corrected areas: 8107574




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030484.D
Acq On : 06 Aug 2022 23:45
Operator : JC/MD
Sample : VIBLK654
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

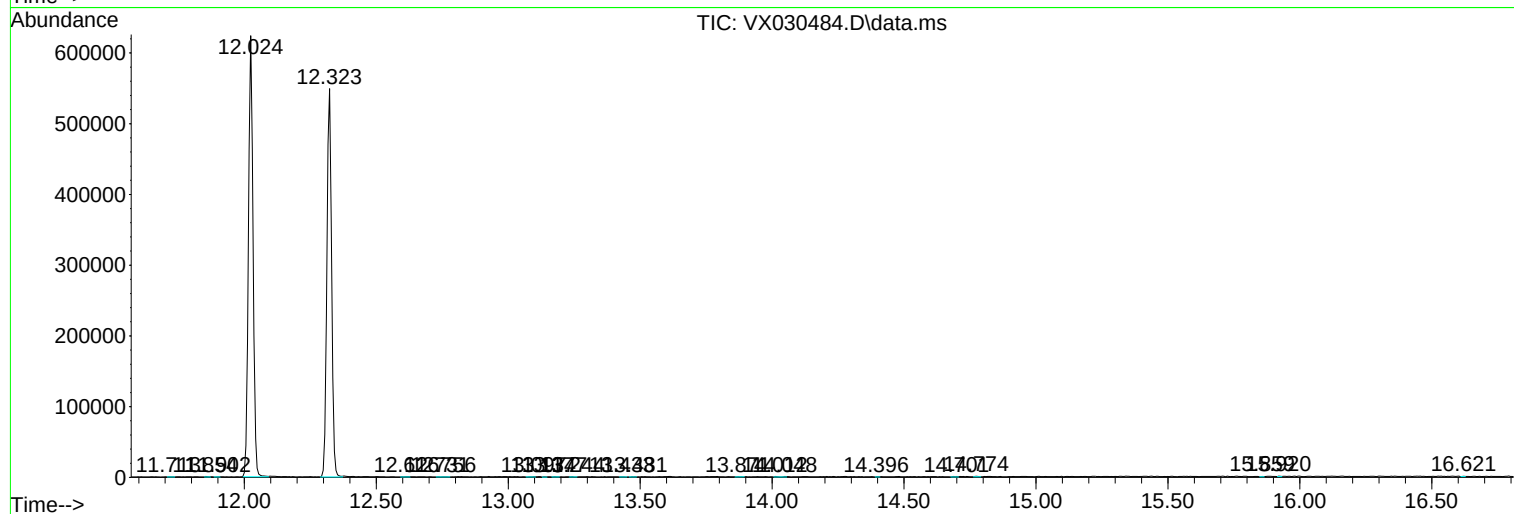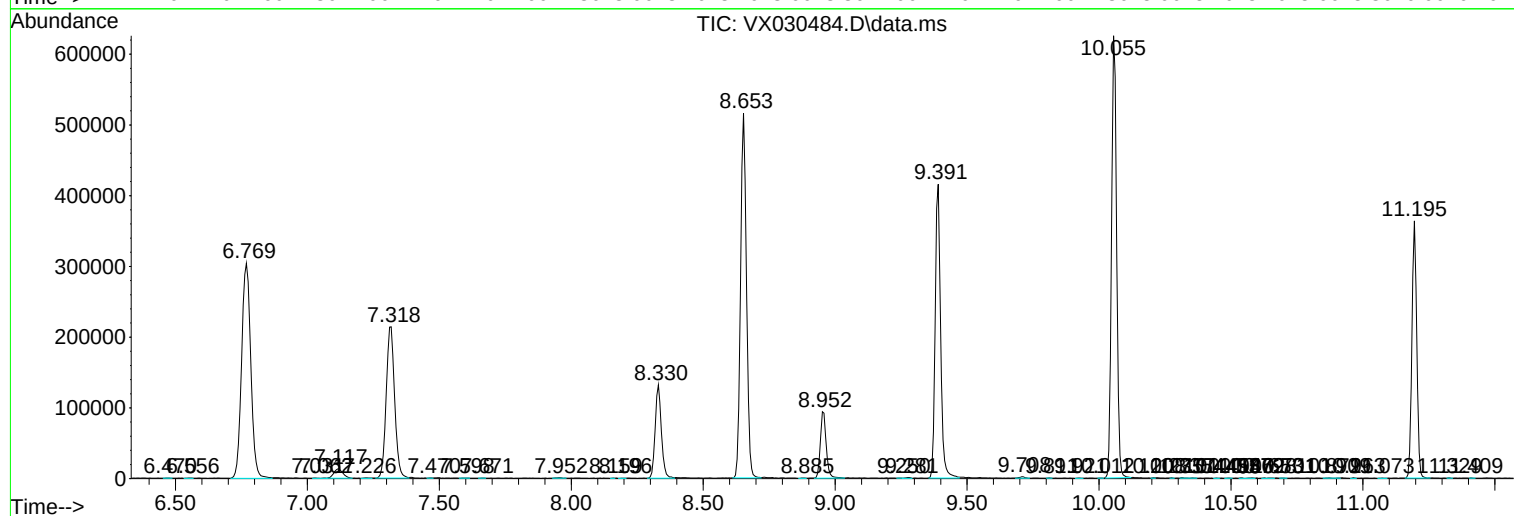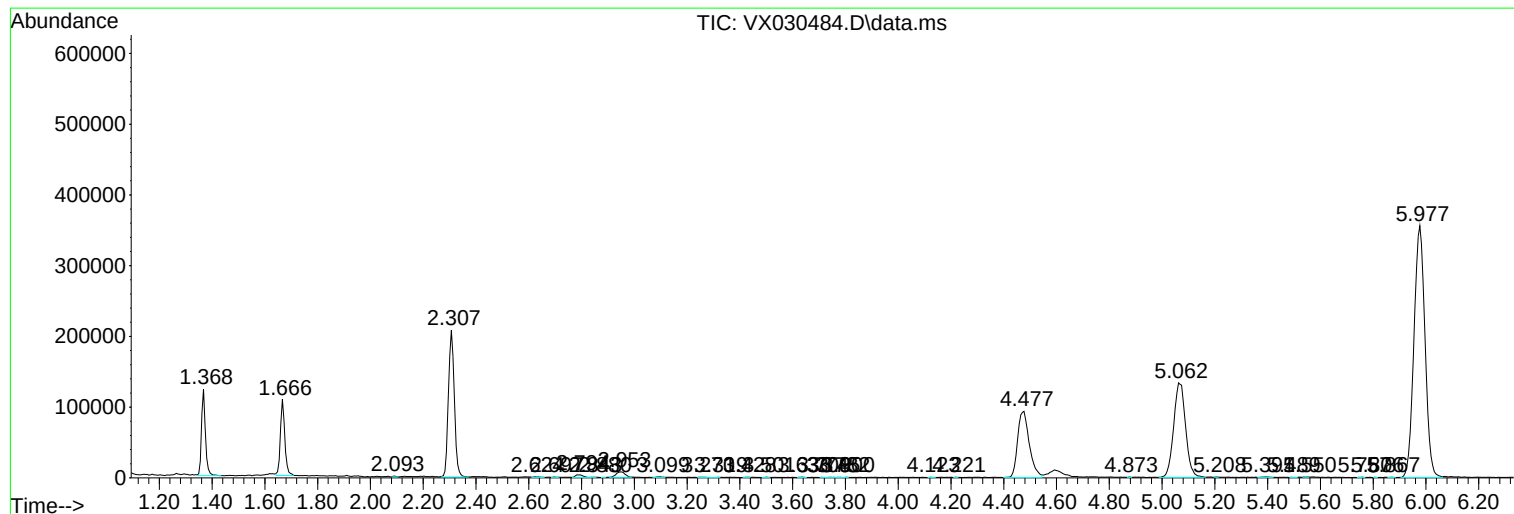

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030484.D
Acq On : 06 Aug 2022 23:45
Operator : JC/MD
Sample : VIBLK654
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030484.D
Acq On : 06 Aug 2022 23:45
Operator : JC/MD
Sample : VIBLK654
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK654

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc