

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030485.D
 Acq On : 07 Aug 2022 00:09
 Operator : JC/MD
 Sample : N4021-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB2	167483	181610	17.79%	2.148%
2	1.666	91	95	103	rVB	100545	121096	11.86%	1.432%
3	2.026	152	154	155	rBV2	1108	643	0.06%	0.008%
4	2.306	194	200	210	rVB	200709	313682	30.73%	3.710%
5	2.392	210	214	220	rVV4	2206	3877	0.38%	0.046%
6	2.440	220	222	225	rVB3	701	498	0.05%	0.006%
7	2.538	236	238	241	rVB2	432	412	0.04%	0.005%
8	2.568	241	243	246	rBV3	312	367	0.04%	0.004%
9	2.788	277	279	283	rVB2	700	901	0.09%	0.011%
10	2.946	302	305	306	rBV	458	517	0.05%	0.006%
11	3.093	322	329	343	rBV	47227	98762	9.67%	1.168%
12	3.318	361	366	367	rBV	489	574	0.06%	0.007%
13	3.532	396	401	402	rBV	762	648	0.06%	0.008%
14	3.611	411	414	416	rBV	493	537	0.05%	0.006%
15	3.648	418	420	423	rVV2	464	493	0.05%	0.006%
16	4.044	483	485	487	rBV2	595	567	0.06%	0.007%
17	4.166	501	505	506	rBV	283	333	0.03%	0.004%
18	4.306	526	528	531	rVB2	1116	1079	0.11%	0.013%
19	4.336	531	533	536	rVB	402	423	0.04%	0.005%
20	4.495	546	559	575	rBV2	190466	655995	64.26%	7.759%
21	4.660	584	586	588	rBV2	566	353	0.03%	0.004%
22	4.733	594	598	601	rBV4	1034	2079	0.20%	0.025%
23	4.910	625	627	630	rBV2	344	320	0.03%	0.004%
24	5.068	640	653	668	rBV2	135388	411361	40.30%	4.866%
25	5.324	691	695	697	rBV2	331	382	0.04%	0.005%
26	5.537	728	730	732	rBV	568	433	0.04%	0.005%
27	5.556	732	733	738	rVB2	977	935	0.09%	0.011%
28	5.690	753	755	758	rBV2	369	321	0.03%	0.004%
29	5.976	787	802	823	rBV3	344233	1020798	100.00%	12.074%
30	6.275	849	851	853	rVB	470	338	0.03%	0.004%
31	6.482	881	885	887	rBV	271	382	0.04%	0.005%
32	6.543	893	895	899	rVB2	469	685	0.07%	0.008%
33	6.769	921	932	946	rBV	292493	696354	68.22%	8.237%
34	6.952	960	962	964	rVB3	537	393	0.04%	0.005%
35	7.123	982	990	997	rBV7	9108	21866	2.14%	0.259%
36	7.318	1012	1022	1036	rBV	211332	466431	45.69%	5.517%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030485.D
 Acq On : 07 Aug 2022 00:09
 Operator : JC/MD
 Sample : N4021-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.482	1043	1049	1051	rBV4	1157	1385	0.14%	0.016%
38	7.811	1100	1103	1104	rBV	468	459	0.04%	0.005%
39	7.909	1116	1119	1122	rBV	484	551	0.05%	0.007%
40	8.116	1151	1153	1155	rBV	520	354	0.03%	0.004%
41	8.330	1182	1188	1199	rBV	129782	212583	20.83%	2.515%
42	8.525	1218	1220	1224	rVB2	675	485	0.05%	0.006%
43	8.653	1234	1241	1256	rBV	512483	787212	77.12%	9.311%
44	8.830	1268	1270	1271	rBV2	646	453	0.04%	0.005%
45	8.897	1279	1281	1284	rVB2	529	530	0.05%	0.006%
46	8.951	1285	1290	1301	rVV	90833	140043	13.72%	1.656%
47	9.390	1356	1362	1377	rBV	405361	578342	56.66%	6.841%
48	9.829	1432	1434	1437	rBV	637	559	0.05%	0.007%
49	9.982	1457	1459	1461	rVB	444	334	0.03%	0.004%
50	10.055	1466	1471	1485	rVV	596928	822457	80.57%	9.728%
51	10.274	1506	1507	1509	rBV2	371	328	0.03%	0.004%
52	10.305	1509	1512	1517	rVV3	798	1235	0.12%	0.015%
53	10.384	1522	1525	1527	rBV2	610	656	0.06%	0.008%
54	10.427	1530	1532	1533	rBV	437	320	0.03%	0.004%
55	10.646	1565	1568	1573	rVB4	813	1293	0.13%	0.015%
56	10.774	1588	1589	1592	rVB3	515	440	0.04%	0.005%
57	10.866	1603	1604	1607	rBV2	442	484	0.05%	0.006%
58	10.939	1615	1616	1619	rBV2	364	405	0.04%	0.005%
59	10.969	1619	1621	1623	rVB2	421	327	0.03%	0.004%
60	11.030	1628	1631	1632	rBV	465	480	0.05%	0.006%
61	11.195	1652	1658	1666	rBV	370363	473560	46.39%	5.601%
62	11.439	1695	1698	1699	rVV	886	679	0.07%	0.008%
63	11.482	1703	1705	1706	rVB2	578	340	0.03%	0.004%
64	11.884	1769	1771	1773	rBV2	617	633	0.06%	0.007%
65	11.908	1773	1775	1776	rVB2	478	328	0.03%	0.004%
66	11.939	1779	1780	1782	rBV	611	422	0.04%	0.005%
67	12.024	1788	1794	1804	rBV	613096	740398	72.53%	8.758%
68	12.323	1837	1843	1857	rBV	522819	663086	64.96%	7.843%
69	12.475	1865	1868	1869	rBV3	637	433	0.04%	0.005%
70	12.524	1874	1876	1879	rVB	578	562	0.06%	0.007%
71	12.548	1879	1880	1883	rBV	515	562	0.06%	0.007%
72	12.683	1899	1902	1904	rBV2	507	454	0.04%	0.005%
73	12.707	1904	1906	1909	rVB	518	437	0.04%	0.005%
74	12.737	1909	1911	1913	rBV	357	445	0.04%	0.005%
75	12.902	1937	1938	1943	rVB2	660	971	0.10%	0.011%
76	12.951	1943	1946	1948	rBV2	535	662	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030485.D
 Acq On : 07 Aug 2022 00:09
 Operator : JC/MD
 Sample : N4021-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.054	1962	1963	1966	rBV2	487	380	0.04%	0.004%
78	13.128	1973	1975	1976	rBV	433	421	0.04%	0.005%
79	13.268	1996	1998	2000	rVB	566	339	0.03%	0.004%
80	13.292	2000	2002	2007	rBB3	401	751	0.07%	0.009%
81	13.347	2009	2011	2015	rVB2	420	381	0.04%	0.005%
82	13.384	2015	2017	2019	rBV2	399	339	0.03%	0.004%
83	13.591	2048	2051	2052	rBV	631	702	0.07%	0.008%
84	13.987	2114	2116	2119	rBV2	817	505	0.05%	0.006%
85	14.115	2134	2137	2139	rBV3	427	565	0.06%	0.007%
86	14.140	2139	2141	2142	rBV2	560	402	0.04%	0.005%
87	14.329	2169	2172	2174	rBV3	637	573	0.06%	0.007%
88	14.420	2184	2187	2188	rBV2	470	386	0.04%	0.005%
89	14.530	2201	2205	2207	rBV2	517	668	0.07%	0.008%
90	14.804	2248	2250	2252	rBV	802	624	0.06%	0.007%
91	14.902	2264	2266	2268	rVB2	904	637	0.06%	0.008%
92	14.926	2268	2270	2274	rBV3	708	913	0.09%	0.011%
93	14.956	2274	2275	2276	rBV	574	404	0.04%	0.005%
94	15.267	2325	2326	2329	rVB2	730	416	0.04%	0.005%
95	15.298	2329	2331	2332	rVB	819	470	0.05%	0.006%
96	15.316	2332	2334	2335	rBV2	493	463	0.05%	0.005%
97	16.145	2469	2470	2471	rBV	581	322	0.03%	0.004%
98	16.194	2477	2478	2479	rBV	607	351	0.03%	0.004%
99	16.389	2508	2510	2512	rBV2	611	558	0.05%	0.007%
100	16.743	2566	2568	2570	rBV2	646	545	0.05%	0.006%




Sum of corrected areas: 8454247

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030485.D
Acq On : 07 Aug 2022 00:09
Operator : JC/MD
Sample : N4021-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

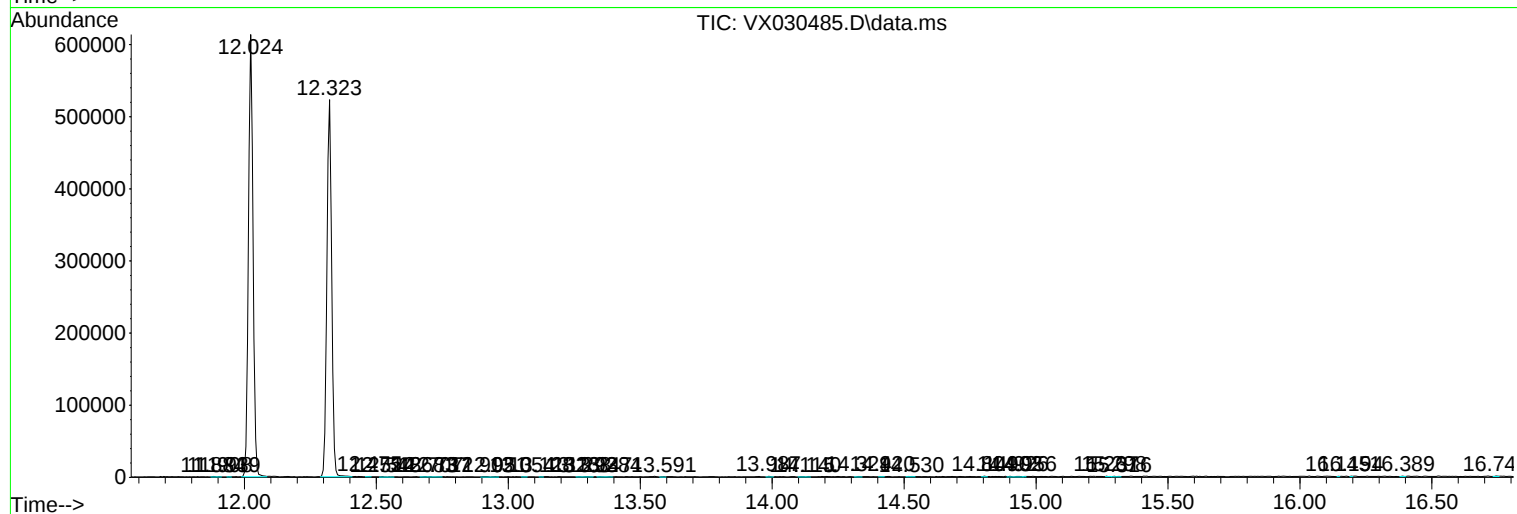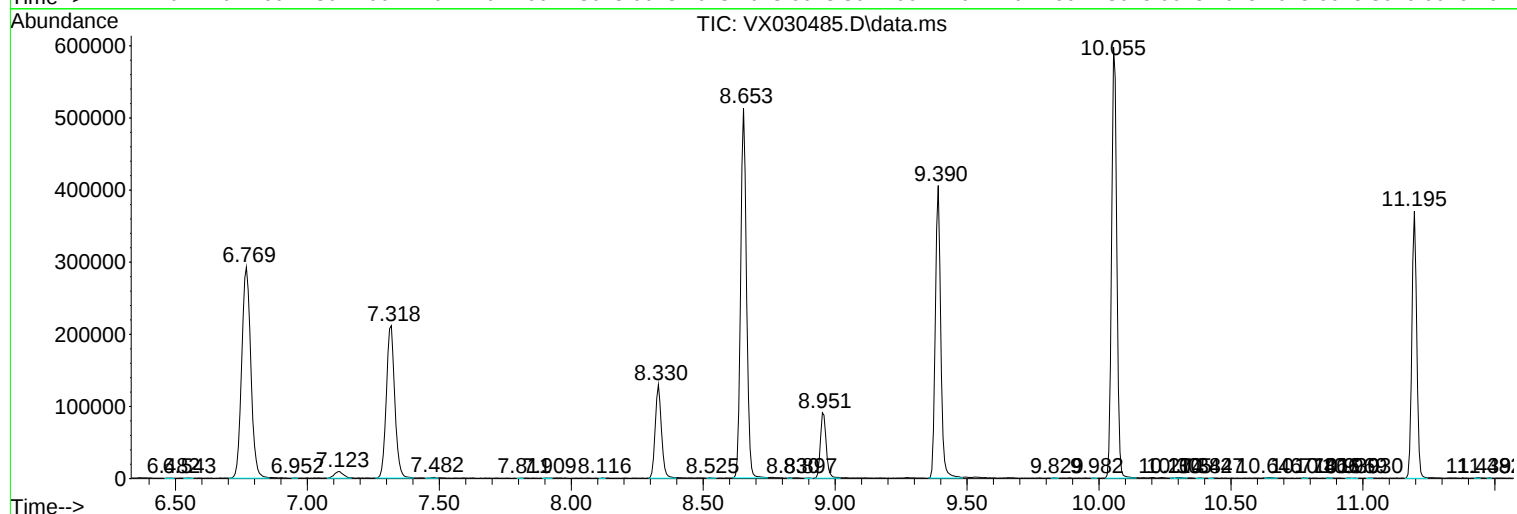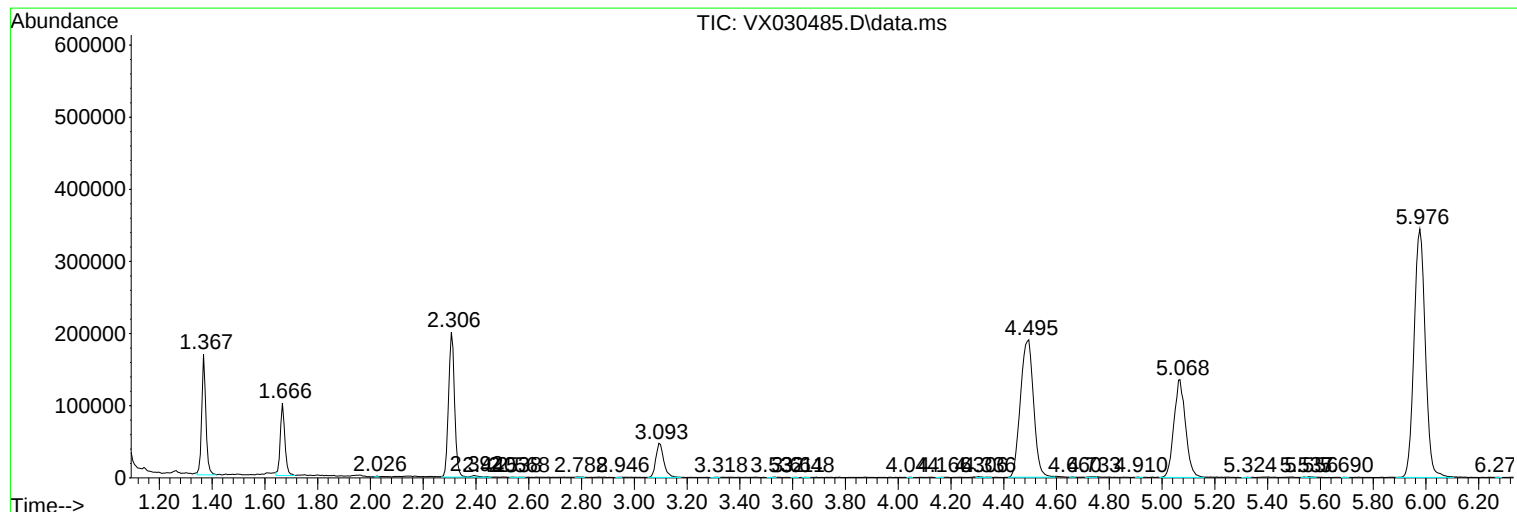

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030485.D
Acq On : 07 Aug 2022 00:09
Operator : JC/MD
Sample : N4021-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030485.D
Acq On : 07 Aug 2022 00:09
Operator : JC/MD
Sample : N4021-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc