

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030486.D
 Acq On : 07 Aug 2022 00:32
 Operator : JC/MD
 Sample : N4021-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	43	47	55	rVB2	482968	552623	32.36%	5.585%
2	1.666	91	95	104	rVB	98931	121401	7.11%	1.227%
3	2.129	169	171	174	rBV4	842	826	0.05%	0.008%
4	2.306	194	200	212	rVB	200192	305405	17.88%	3.087%
5	2.391	212	214	215	rBV	1600	1366	0.08%	0.014%
6	2.495	230	231	234	rBV3	607	769	0.05%	0.008%
7	2.556	239	241	246	rVB2	392	516	0.03%	0.005%
8	2.605	246	249	252	rBV3	545	927	0.05%	0.009%
9	2.788	277	279	281	rBV2	903	718	0.04%	0.007%
10	2.995	309	313	314	rBV2	622	829	0.05%	0.008%
11	3.093	320	329	342	rBV	90927	188592	11.04%	1.906%
12	3.202	345	347	355	rBV2	429	823	0.05%	0.008%
13	3.464	387	390	393	rVB2	313	463	0.03%	0.005%
14	3.513	396	398	401	rVB2	294	355	0.02%	0.004%
15	3.702	427	429	431	rBV	464	421	0.02%	0.004%
16	3.867	451	456	457	rBV2	397	426	0.02%	0.004%
17	4.257	516	520	521	rBV2	369	384	0.02%	0.004%
18	4.294	523	526	527	rBV	837	915	0.05%	0.009%
19	4.495	546	559	577	rBV2	566787	1707969	100.00%	17.263%
20	4.922	626	629	630	rBV	402	407	0.02%	0.004%
21	5.062	640	652	666	rBV	133447	404852	23.70%	4.092%
22	5.391	704	706	709	rVV2	595	367	0.02%	0.004%
23	5.464	713	718	722	rBV5	1546	2939	0.17%	0.030%
24	5.543	730	731	732	rVV	663	423	0.02%	0.004%
25	5.562	732	734	743	rVB4	1211	2143	0.13%	0.022%
26	5.720	757	760	763	rBV2	476	657	0.04%	0.007%
27	5.799	771	773	775	rVB	462	369	0.02%	0.004%
28	5.976	789	802	824	rBV2	340496	1009834	59.12%	10.207%
29	6.342	857	862	863	rBV2	516	714	0.04%	0.007%
30	6.403	870	872	874	rVB	733	397	0.02%	0.004%
31	6.458	879	881	882	rBV	481	423	0.02%	0.004%
32	6.531	889	893	894	rBV2	287	384	0.02%	0.004%
33	6.549	894	896	899	rVV	466	424	0.02%	0.004%
34	6.769	922	932	948	rBV	295278	700116	40.99%	7.076%
35	7.055	977	979	982	rVB3	506	439	0.03%	0.004%
36	7.122	982	990	999	rVB8	9765	23167	1.36%	0.234%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030486.D
 Acq On : 07 Aug 2022 00:32
 Operator : JC/MD
 Sample : N4021-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.195	999	1002	1003	rBV2	391	424	0.02%	0.004%
38	7.317	1013	1022	1034	rBV	210673	457728	26.80%	4.626%
39	7.433	1039	1041	1046	rVB2	584	727	0.04%	0.007%
40	7.488	1046	1050	1051	rBV2	570	782	0.05%	0.008%
41	7.653	1074	1077	1080	rBV2	435	577	0.03%	0.006%
42	7.677	1080	1081	1085	rVV	538	558	0.03%	0.006%
43	7.830	1103	1106	1108	rBV2	329	360	0.02%	0.004%
44	7.939	1123	1124	1128	rVV2	607	606	0.04%	0.006%
45	8.006	1134	1135	1139	rBV2	581	445	0.03%	0.004%
46	8.110	1150	1152	1154	rVV	525	467	0.03%	0.005%
47	8.140	1156	1157	1160	rBV	399	458	0.03%	0.005%
48	8.329	1182	1188	1201	rBV	126299	206066	12.06%	2.083%
49	8.488	1209	1214	1216	rVB3	681	1068	0.06%	0.011%
50	8.506	1216	1217	1219	rBV2	491	384	0.02%	0.004%
51	8.653	1234	1241	1249	rBV	497833	773991	45.32%	7.823%
52	8.799	1264	1265	1270	rVB2	622	456	0.03%	0.005%
53	8.909	1277	1283	1285	rBV2	479	895	0.05%	0.009%
54	8.957	1285	1291	1298	rBV	89433	136883	8.01%	1.384%
55	9.232	1334	1336	1339	rVV2	461	403	0.02%	0.004%
56	9.280	1341	1344	1346	rVV2	887	933	0.05%	0.009%
57	9.390	1356	1362	1377	rBV	410635	591028	34.60%	5.974%
58	9.561	1389	1390	1392	rVB	742	358	0.02%	0.004%
59	9.628	1399	1401	1403	rBV2	428	501	0.03%	0.005%
60	9.860	1436	1439	1441	rBV2	355	474	0.03%	0.005%
61	10.055	1464	1471	1487	rBV	594182	809586	47.40%	8.183%
62	10.201	1493	1495	1498	rBV3	512	561	0.03%	0.006%
63	10.305	1507	1512	1514	rVV3	790	822	0.05%	0.008%
64	10.396	1524	1527	1530	rVB3	606	515	0.03%	0.005%
65	10.585	1555	1558	1559	rBV	453	541	0.03%	0.005%
66	10.622	1562	1564	1567	rVV	522	475	0.03%	0.005%
67	10.652	1567	1569	1572	rVB	839	567	0.03%	0.006%
68	10.683	1572	1574	1575	rBV2	583	371	0.02%	0.004%
69	10.847	1599	1601	1605	rVB2	370	571	0.03%	0.006%
70	10.878	1605	1606	1608	rBV2	491	401	0.02%	0.004%
71	10.914	1610	1612	1613	rBV	626	431	0.03%	0.004%
72	10.951	1617	1618	1620	rBV2	359	381	0.02%	0.004%
73	11.195	1651	1658	1666	rBV	361861	464171	27.18%	4.691%
74	11.305	1674	1676	1680	rVB2	566	597	0.03%	0.006%
75	11.439	1694	1698	1699	rBV2	590	707	0.04%	0.007%
76	11.646	1730	1732	1735	rBV2	626	590	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030486.D
 Acq On : 07 Aug 2022 00:32
 Operator : JC/MD
 Sample : N4021-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D39

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.713	1740	1743	1745	rVB2	643	692	0.04%	0.007%
78	11.756	1745	1750	1752	rBV3	772	1274	0.07%	0.013%
79	11.823	1759	1761	1764	rBV	418	369	0.02%	0.004%
80	11.884	1770	1771	1776	rVB2	856	827	0.05%	0.008%
81	11.939	1776	1780	1781	rBV	568	415	0.02%	0.004%
82	12.024	1789	1794	1806	rBV	610777	732123	42.87%	7.400%
83	12.201	1819	1823	1826	rBV2	450	740	0.04%	0.007%
84	12.323	1837	1843	1852	rBV	540354	657361	38.49%	6.644%
85	12.682	1901	1902	1904	rVB	549	369	0.02%	0.004%
86	12.810	1919	1923	1924	rBV	516	393	0.02%	0.004%
87	13.243	1992	1994	1997	rBV2	453	406	0.02%	0.004%
88	13.505	2035	2037	2040	rBV2	328	481	0.03%	0.005%
89	13.554	2042	2045	2048	rBV	496	607	0.04%	0.006%
90	13.713	2068	2071	2074	rBV3	503	741	0.04%	0.007%
91	13.877	2096	2098	2102	rVB	701	664	0.04%	0.007%
92	13.914	2102	2104	2105	rBV	694	511	0.03%	0.005%
93	14.078	2130	2131	2135	rVB2	626	384	0.02%	0.004%
94	14.121	2135	2138	2139	rBV2	572	546	0.03%	0.006%
95	14.450	2190	2192	2193	rVB	600	355	0.02%	0.004%
96	14.584	2210	2214	2215	rBV	574	694	0.04%	0.007%
97	14.676	2227	2229	2232	rVB2	662	580	0.03%	0.006%
98	15.225	2317	2319	2323	rBV4	684	683	0.04%	0.007%
99	15.694	2394	2396	2398	rBV2	767	663	0.04%	0.007%
100	16.176	2474	2475	2476	rBV	1013	432	0.03%	0.004%




Sum of corrected areas: 9893952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030486.D
Acq On : 07 Aug 2022 00:32
Operator : JC/MD
Sample : N4021-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

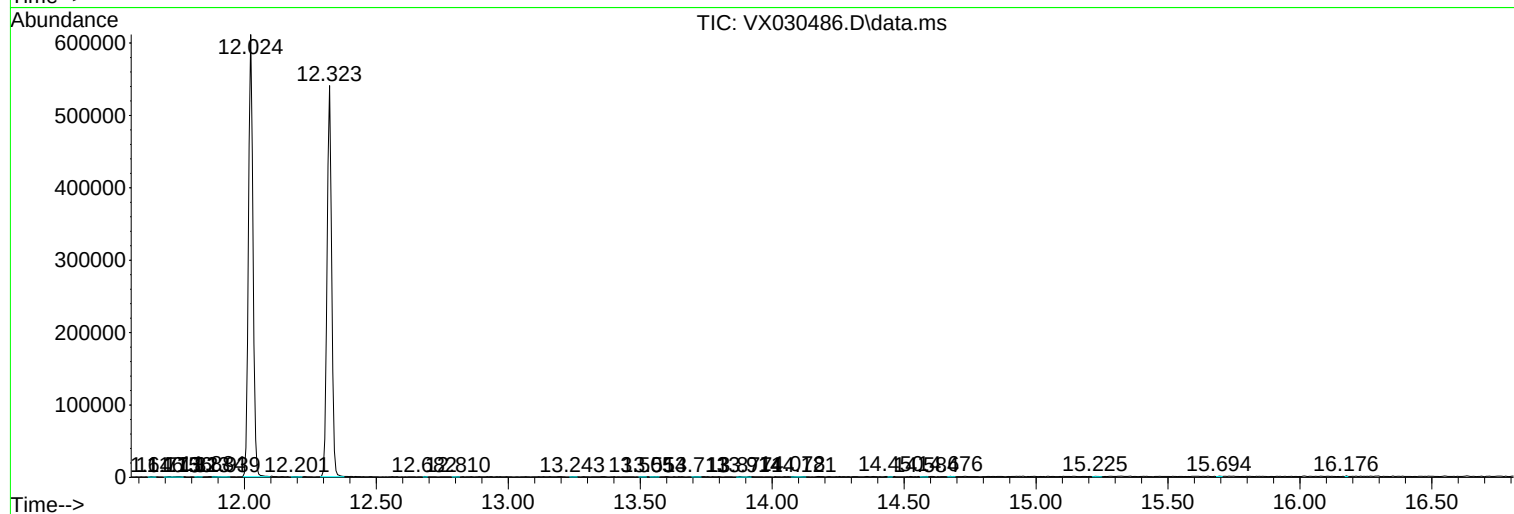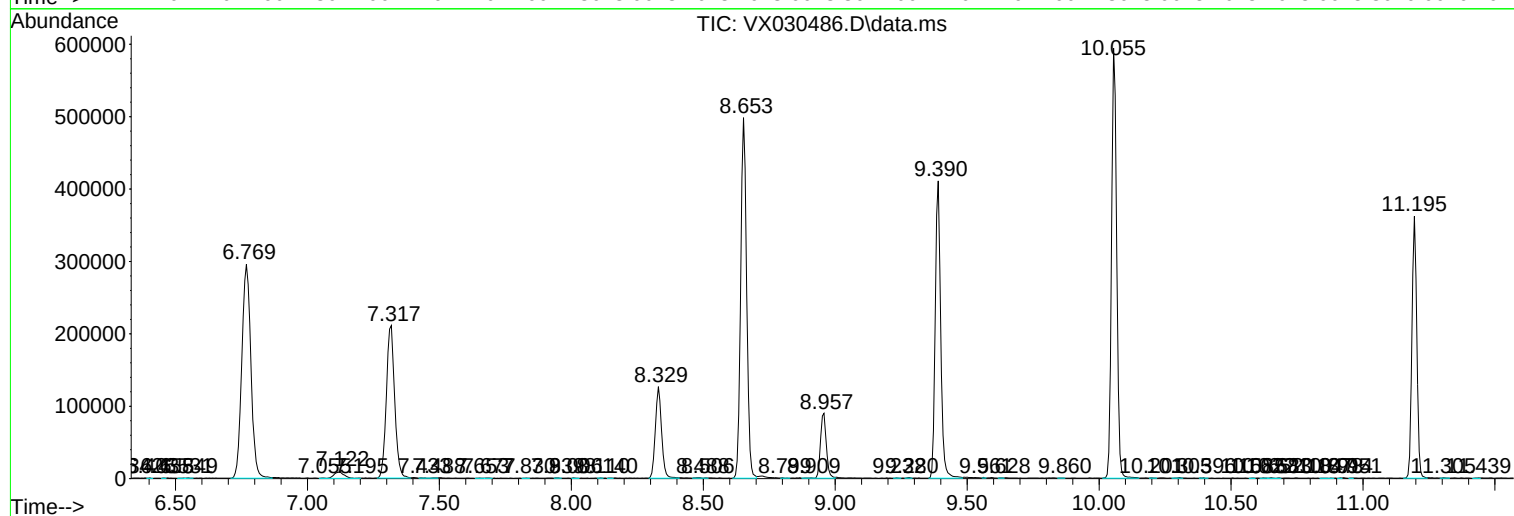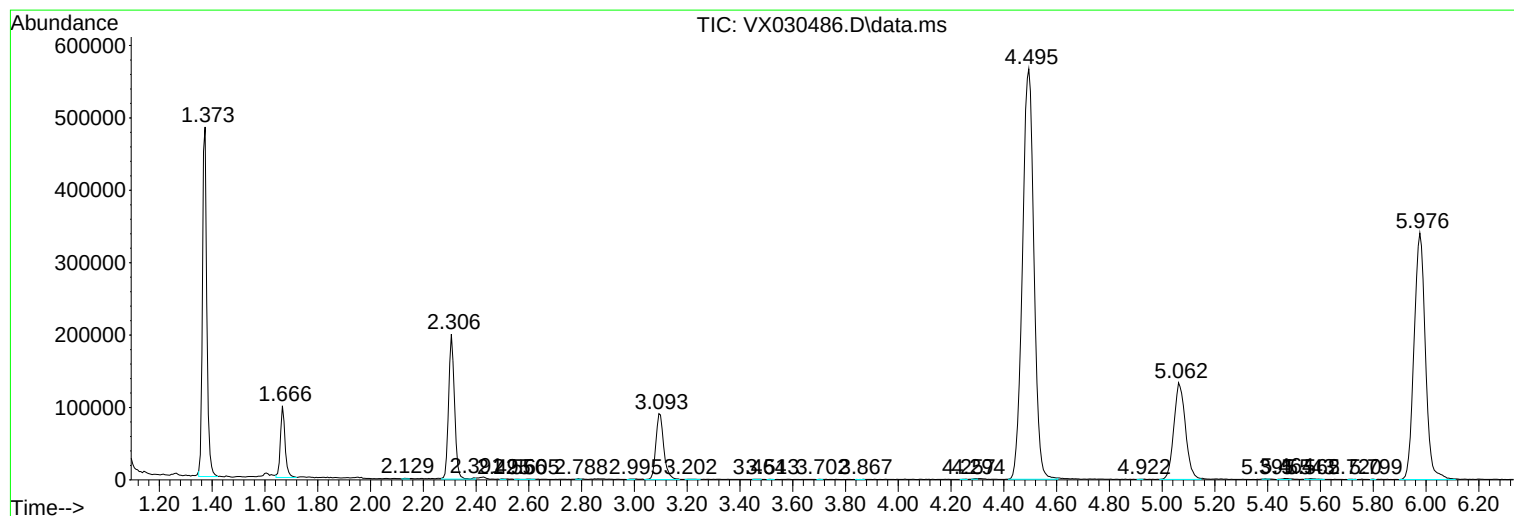

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030486.D
Acq On : 07 Aug 2022 00:32
Operator : JC/MD
Sample : N4021-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030486.D
Acq On : 07 Aug 2022 00:32
Operator : JC/MD
Sample : N4021-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc