

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030487.D
 Acq On : 07 Aug 2022 00:55
 Operator : JC/MD
 Sample : N4021-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	54	rVB	132247	134969	12.34%	1.484%
2	1.666	91	95	105	rVB	101801	121552	11.11%	1.337%
3	2.142	169	173	175	rBV3	1323	1501	0.14%	0.017%
4	2.306	193	200	210	rBV	212172	319455	29.21%	3.513%
5	2.398	210	215	223	rVB	9871	18292	1.67%	0.201%
6	2.794	275	280	284	rVB5	510	912	0.08%	0.010%
7	2.879	290	294	297	rBV3	300	349	0.03%	0.004%
8	2.983	309	311	314	rBV2	748	709	0.06%	0.008%
9	3.099	323	330	339	rVB	19250	37592	3.44%	0.413%
10	3.202	343	347	349	rBV	305	460	0.04%	0.005%
11	3.263	355	357	358	rVB2	591	369	0.03%	0.004%
12	3.501	394	396	398	rBV2	374	366	0.03%	0.004%
13	3.580	402	409	411	rBV3	1278	2312	0.21%	0.025%
14	3.672	422	424	426	rVB	508	361	0.03%	0.004%
15	3.751	436	437	440	rBV2	327	321	0.03%	0.004%
16	3.977	473	474	476	rBV2	573	351	0.03%	0.004%
17	4.111	494	496	501	rVB2	580	580	0.05%	0.006%
18	4.355	535	536	540	rVB2	482	399	0.04%	0.004%
19	4.410	543	545	546	rBV	450	369	0.03%	0.004%
20	4.495	546	559	577	rBV2	357542	1093778	100.00%	12.030%
21	4.824	611	613	614	rBV	446	361	0.03%	0.004%
22	4.934	627	631	635	rVB3	658	1022	0.09%	0.011%
23	5.068	640	653	670	rBV	134386	409143	37.41%	4.500%
24	5.550	730	732	733	rBV2	642	469	0.04%	0.005%
25	5.726	759	761	763	rBV	307	382	0.03%	0.004%
26	5.800	770	773	775	rBV	274	378	0.03%	0.004%
27	5.897	785	789	790	rBV2	341	472	0.04%	0.005%
28	5.976	790	802	819	rVV2	346628	1001001	91.52%	11.009%
29	6.293	850	854	855	rBV2	259	390	0.04%	0.004%
30	6.342	860	862	864	rBV	300	369	0.03%	0.004%
31	6.568	895	899	902	rVV2	426	637	0.06%	0.007%
32	6.769	921	932	944	rBV	303445	714048	65.28%	7.853%
33	7.129	982	991	1002	rBV2	136723	312940	28.61%	3.442%
34	7.311	1012	1021	1033	rBV	207278	461543	42.20%	5.076%
35	7.440	1039	1042	1045	rBV	445	599	0.05%	0.007%
36	7.610	1068	1070	1072	rVV2	445	382	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030487.D
 Acq On : 07 Aug 2022 00:55
 Operator : JC/MD
 Sample : N4021-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.659	1077	1078	1081	rVB2	361	326	0.03%	0.004%
38	7.738	1089	1091	1092	rBV	505	525	0.05%	0.006%
39	7.933	1121	1123	1125	rBV2	447	476	0.04%	0.005%
40	8.061	1141	1144	1147	rBV2	382	483	0.04%	0.005%
41	8.147	1156	1158	1160	rVB2	428	331	0.03%	0.004%
42	8.330	1180	1188	1200	rBV2	125161	211157	19.31%	2.322%
43	8.488	1212	1214	1217	rVV2	474	487	0.04%	0.005%
44	8.519	1217	1219	1221	rVB2	683	475	0.04%	0.005%
45	8.543	1221	1223	1224	rVB	486	324	0.03%	0.004%
46	8.653	1234	1241	1251	rBV	518708	782706	71.56%	8.608%
47	8.842	1270	1272	1273	rVB	662	382	0.03%	0.004%
48	8.860	1273	1275	1276	rBV	391	376	0.03%	0.004%
49	8.951	1285	1290	1299	rVV	90007	135178	12.36%	1.487%
50	9.140	1319	1321	1322	rVB	605	412	0.04%	0.005%
51	9.165	1322	1325	1326	rBV2	370	411	0.04%	0.005%
52	9.281	1339	1344	1350	rVB2	10809	15445	1.41%	0.170%
53	9.323	1350	1351	1355	rVB2	473	370	0.03%	0.004%
54	9.390	1356	1362	1378	rBV	398648	572874	52.38%	6.301%
55	9.695	1411	1412	1416	rVB3	795	670	0.06%	0.007%
56	9.756	1416	1422	1425	rBV4	541	977	0.09%	0.011%
57	9.841	1434	1436	1438	rBV2	531	377	0.03%	0.004%
58	9.909	1446	1447	1449	rBV	444	441	0.04%	0.005%
59	10.055	1465	1471	1482	rBV	597097	836860	76.51%	9.204%
60	10.238	1499	1501	1503	rBV	338	439	0.04%	0.005%
61	10.421	1528	1531	1532	rBV	649	554	0.05%	0.006%
62	10.518	1545	1547	1549	rVB2	570	444	0.04%	0.005%
63	10.543	1549	1551	1555	rBV	268	352	0.03%	0.004%
64	10.604	1560	1561	1564	rBV	558	429	0.04%	0.005%
65	10.683	1572	1574	1576	rBV	397	383	0.04%	0.004%
66	10.732	1579	1582	1584	rBV	511	493	0.05%	0.005%
67	10.768	1587	1588	1590	rVV2	541	326	0.03%	0.004%
68	10.786	1590	1591	1594	rVB2	452	403	0.04%	0.004%
69	11.049	1633	1634	1637	rVB3	467	342	0.03%	0.004%
70	11.195	1652	1658	1668	rBV	362149	459566	42.02%	5.054%
71	11.481	1702	1705	1709	rVV3	767	762	0.07%	0.008%
72	11.536	1711	1714	1716	rBV2	583	480	0.04%	0.005%
73	11.622	1725	1728	1729	rBV	473	351	0.03%	0.004%
74	11.829	1760	1762	1764	rVB2	439	345	0.03%	0.004%
75	11.847	1764	1765	1768	rBV2	342	330	0.03%	0.004%
76	11.902	1771	1774	1775	rBV2	542	531	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030487.D
 Acq On : 07 Aug 2022 00:55
 Operator : JC/MD
 Sample : N4021-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D47

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1806	rBV	632984	757433	69.25%	8.330%
78	12.225	1825	1827	1829	rBV2	403	360	0.03%	0.004%
79	12.323	1837	1843	1852	rBV	538184	655653	59.94%	7.211%
80	12.707	1904	1906	1909	rBV2	681	708	0.06%	0.008%
81	12.829	1923	1926	1929	rVB	483	650	0.06%	0.007%
82	12.865	1929	1932	1933	rBV	573	513	0.05%	0.006%
83	12.969	1945	1949	1950	rBV	458	458	0.04%	0.005%
84	13.121	1972	1974	1976	rVB2	667	473	0.04%	0.005%
85	13.146	1976	1978	1980	rBV	514	455	0.04%	0.005%
86	13.390	2016	2018	2020	rBV2	324	317	0.03%	0.003%
87	13.694	2066	2068	2070	rVB2	478	432	0.04%	0.005%
88	13.877	2096	2098	2099	rBV2	544	401	0.04%	0.004%
89	14.091	2132	2133	2134	rBV	471	315	0.03%	0.003%
90	14.249	2157	2159	2161	rBV2	563	459	0.04%	0.005%
91	14.505	2199	2201	2203	rVB2	496	360	0.03%	0.004%
92	14.743	2238	2240	2242	rBV2	499	357	0.03%	0.004%
93	14.877	2260	2262	2266	rVB2	682	729	0.07%	0.008%
94	14.975	2276	2278	2280	rVB2	782	591	0.05%	0.006%
95	15.170	2308	2310	2315	rBV4	766	1260	0.12%	0.014%
96	15.310	2331	2333	2334	rBV2	646	480	0.04%	0.005%
97	16.292	2492	2494	2496	rBV2	610	596	0.05%	0.007%
98	16.371	2505	2507	2509	rBV2	578	475	0.04%	0.005%
99	16.432	2515	2517	2519	rBV2	800	674	0.06%	0.007%
100	16.578	2539	2541	2543	rBV2	573	469	0.04%	0.005%




Sum of corrected areas: 9092344

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030487.D
Acq On : 07 Aug 2022 00:55
Operator : JC/MD
Sample : N4021-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

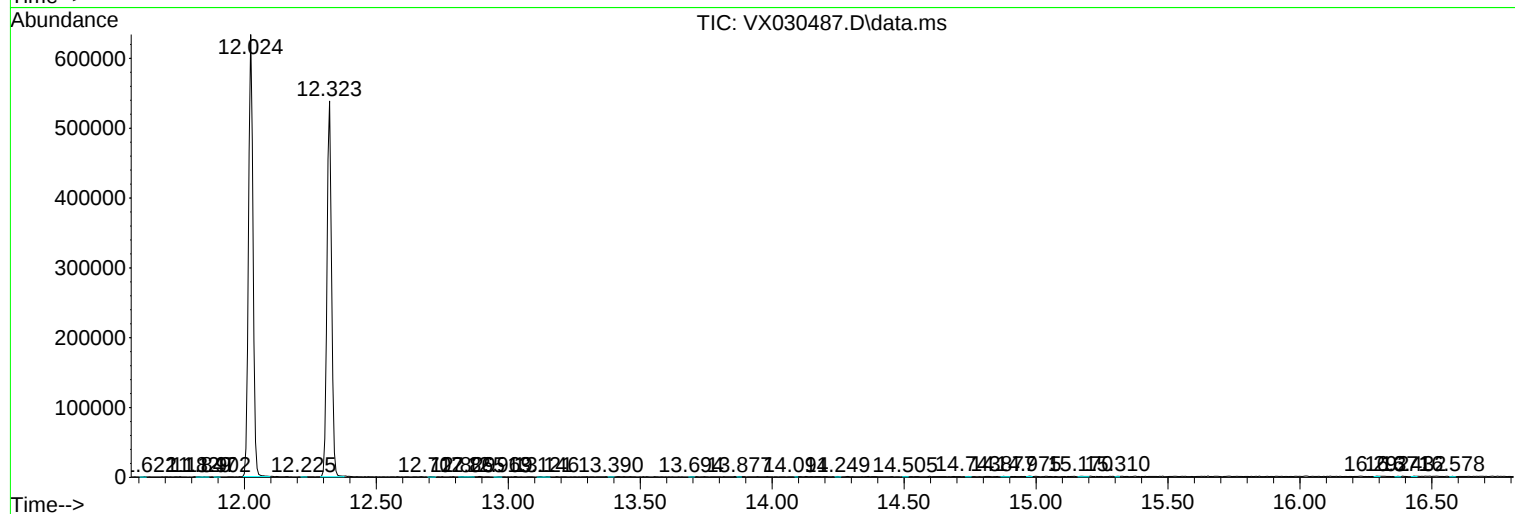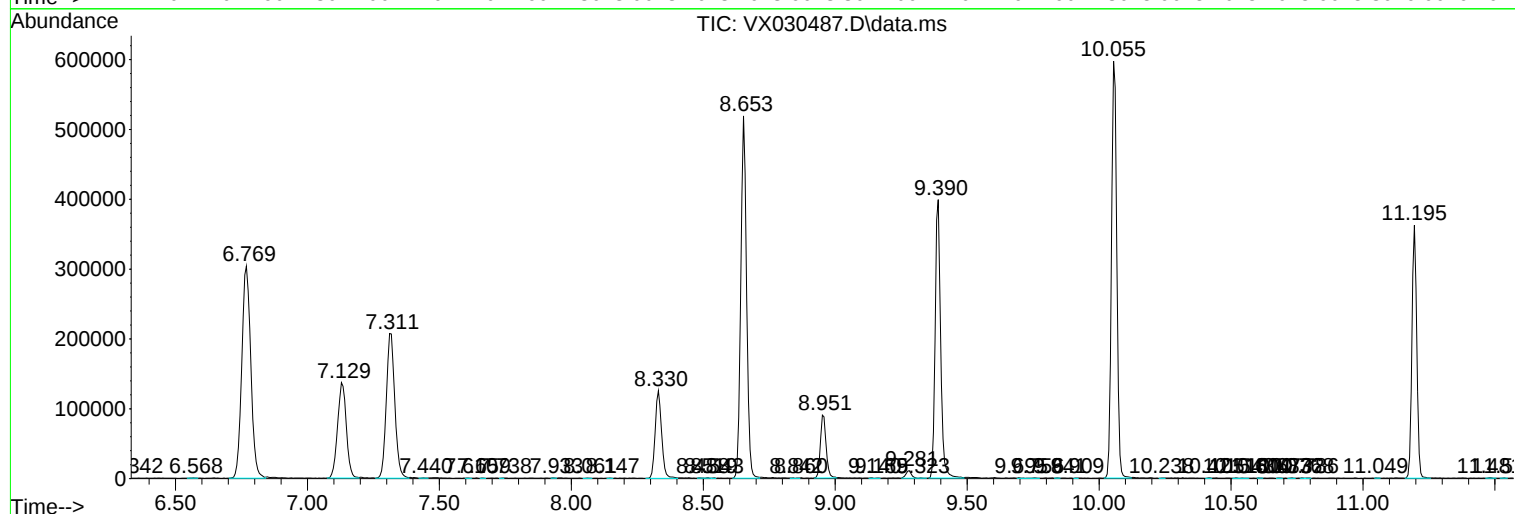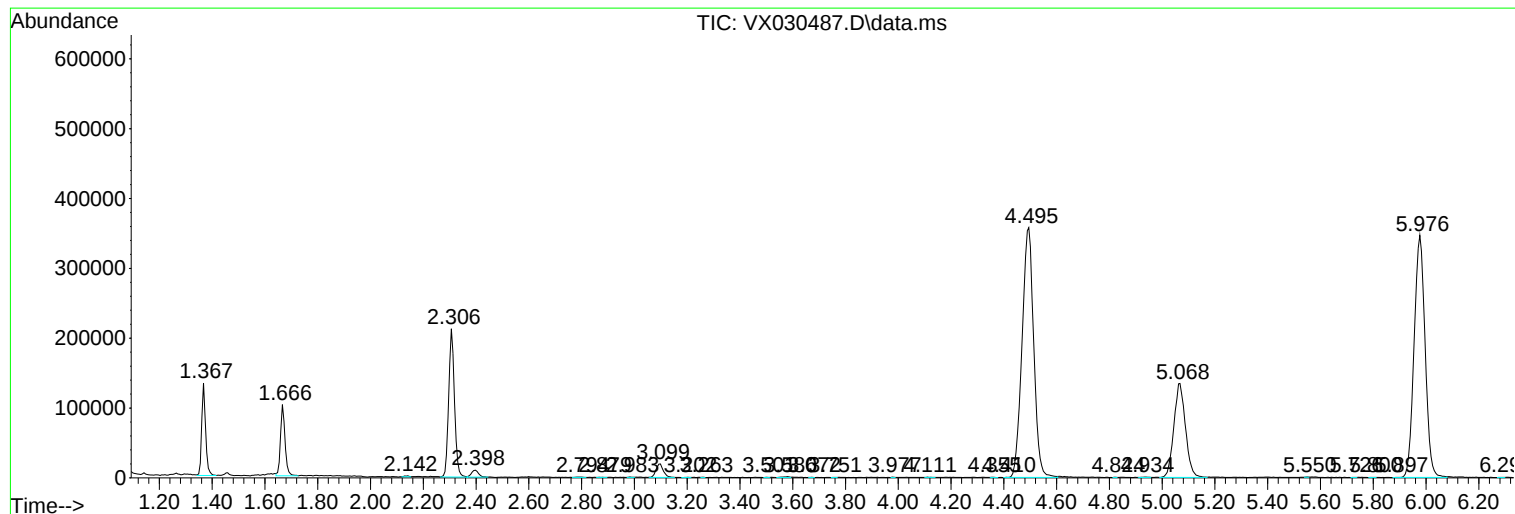

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030487.D
Acq On : 07 Aug 2022 00:55
Operator : JC/MD
Sample : N4021-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030487.D
Acq On : 07 Aug 2022 00:55
Operator : JC/MD
Sample : N4021-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc