

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030488.D
 Acq On : 07 Aug 2022 01:19
 Operator : JC/MD
 Sample : N4021-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	42	47	58	rVB2	438121	515912	25.28%	4.652%
2	1.666	91	95	105	rVB	98784	118441	5.80%	1.068%
3	2.307	194	200	212	rVB	210836	326139	15.98%	2.941%
4	2.392	212	214	215	rBV2	1423	1242	0.06%	0.011%
5	2.508	231	233	235	rVV2	724	480	0.02%	0.004%
6	2.727	267	269	272	rBV	522	424	0.02%	0.004%
7	2.983	310	311	312	rBV	583	368	0.02%	0.003%
8	3.026	315	318	320	rVB3	524	399	0.02%	0.004%
9	3.093	323	329	338	rVB	38339	74473	3.65%	0.672%
10	3.203	345	347	349	rBV2	343	376	0.02%	0.003%
11	3.544	401	403	406	rVB	638	515	0.03%	0.005%
12	3.581	406	409	411	rBV2	370	393	0.02%	0.004%
13	3.636	415	418	423	rVB3	460	545	0.03%	0.005%
14	3.678	423	425	427	rBV	383	404	0.02%	0.004%
15	3.794	441	444	445	rBV2	488	470	0.02%	0.004%
16	3.812	445	447	450	rVV2	342	328	0.02%	0.003%
17	3.892	457	460	463	rBV3	407	491	0.02%	0.004%
18	3.989	475	476	481	rBV2	396	658	0.03%	0.006%
19	4.276	520	523	525	rBV	455	473	0.02%	0.004%
20	4.300	525	527	529	rBV3	411	354	0.02%	0.003%
21	4.489	546	558	574	rBV2	470978	1404386	68.83%	12.663%
22	4.702	591	593	597	rBV3	493	538	0.03%	0.005%
23	4.843	614	616	619	rVB2	530	394	0.02%	0.004%
24	5.019	632	645	670	rBV2	535752	2040455	100.00%	18.399%
25	5.373	701	703	704	rBV2	542	407	0.02%	0.004%
26	5.391	704	706	709	rVV3	752	790	0.04%	0.007%
27	5.538	726	730	731	rBV2	638	793	0.04%	0.007%
28	5.611	740	742	747	rVB2	641	834	0.04%	0.008%
29	5.647	747	748	751	rBV	410	478	0.02%	0.004%
30	5.977	789	802	818	rBV2	337581	989433	48.49%	8.922%
31	6.105	821	823	829	rVV3	1122	1903	0.09%	0.017%
32	6.166	831	833	837	rVB3	514	588	0.03%	0.005%
33	6.294	853	854	857	rBV2	473	421	0.02%	0.004%
34	6.342	859	862	863	rBV2	572	585	0.03%	0.005%
35	6.367	864	866	869	rVV	520	387	0.02%	0.003%
36	6.537	892	894	897	rVV2	458	444	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030488.D
 Acq On : 07 Aug 2022 01:19
 Operator : JC/MD
 Sample : N4021-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	922	932	946	rBV	302709	704488	34.53%	6.352%
38	7.043	974	977	979	rBV2	405	441	0.02%	0.004%
39	7.117	983	989	997	rVV5	10223	23779	1.17%	0.214%
40	7.312	1013	1021	1035	rVV	204551	457697	22.43%	4.127%
41	7.476	1046	1048	1050	rBV2	708	820	0.04%	0.007%
42	7.586	1064	1066	1070	rVB2	425	325	0.02%	0.003%
43	7.757	1092	1094	1099	rBV2	383	602	0.03%	0.005%
44	7.909	1116	1119	1120	rBV	788	613	0.03%	0.006%
45	8.330	1181	1188	1198	rBV	123196	203989	10.00%	1.839%
46	8.525	1218	1220	1221	rBV	534	370	0.02%	0.003%
47	8.586	1226	1230	1231	rBV2	460	509	0.02%	0.005%
48	8.653	1234	1241	1249	rBV	490188	761187	37.30%	6.864%
49	8.952	1285	1290	1297	rBV	86262	132286	6.48%	1.193%
50	9.287	1341	1345	1346	rVB3	779	890	0.04%	0.008%
51	9.391	1356	1362	1375	rBV	407665	597522	29.28%	5.388%
52	9.531	1383	1385	1387	rVB3	1062	766	0.04%	0.007%
53	9.702	1411	1413	1418	rBV3	358	466	0.02%	0.004%
54	9.811	1427	1431	1433	rBV2	508	759	0.04%	0.007%
55	9.866	1437	1440	1441	rBV2	572	467	0.02%	0.004%
56	10.055	1466	1471	1484	rVB	625137	827707	40.56%	7.463%
57	10.195	1491	1494	1498	rBV3	808	1205	0.06%	0.011%
58	10.238	1498	1501	1504	rVV4	1007	1351	0.07%	0.012%
59	10.311	1511	1513	1517	rVB3	1382	1443	0.07%	0.013%
60	10.458	1534	1537	1540	rVB2	510	463	0.02%	0.004%
61	10.494	1540	1543	1545	rBV	422	551	0.03%	0.005%
62	10.842	1599	1600	1605	rVB2	363	413	0.02%	0.004%
63	10.884	1605	1607	1609	rBV	354	473	0.02%	0.004%
64	10.970	1619	1621	1622	rBV	473	474	0.02%	0.004%
65	11.104	1641	1643	1646	rVB3	430	491	0.02%	0.004%
66	11.195	1652	1658	1671	rVV	369655	463726	22.73%	4.181%
67	11.299	1673	1675	1679	rVB3	611	811	0.04%	0.007%
68	11.439	1694	1698	1699	rBV	973	954	0.05%	0.009%
69	11.683	1735	1738	1739	rBV	304	325	0.02%	0.003%
70	11.756	1748	1750	1753	rBV	513	709	0.03%	0.006%
71	11.890	1768	1772	1778	rVB6	3237	4116	0.20%	0.037%
72	11.969	1782	1785	1788	rBV2	558	599	0.03%	0.005%
73	12.024	1788	1794	1801	rBV	619297	743923	36.46%	6.708%
74	12.177	1818	1819	1823	rBV2	362	488	0.02%	0.004%
75	12.274	1833	1835	1837	rBV3	544	560	0.03%	0.005%
76	12.323	1837	1843	1849	rVV	502669	647967	31.76%	5.843%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030488.D
 Acq On : 07 Aug 2022 01:19
 Operator : JC/MD
 Sample : N4021-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.421	1857	1859	1862	rBV3	716	553	0.03%	0.005%
78	12.518	1870	1875	1879	rBV3	476	971	0.05%	0.009%
79	12.549	1879	1880	1886	rVB2	570	591	0.03%	0.005%
80	12.829	1923	1926	1928	rVB2	496	515	0.03%	0.005%
81	12.902	1937	1938	1943	rVB2	603	653	0.03%	0.006%
82	12.975	1946	1950	1951	rVB2	479	429	0.02%	0.004%
83	12.994	1951	1953	1956	rBV	489	442	0.02%	0.004%
84	13.128	1971	1975	1976	rBV	617	754	0.04%	0.007%
85	13.518	2038	2039	2041	rBV2	643	434	0.02%	0.004%
86	13.585	2047	2050	2055	rVB4	476	793	0.04%	0.007%
87	13.670	2063	2064	2068	rVB2	723	517	0.03%	0.005%
88	13.847	2092	2093	2095	rBV	641	431	0.02%	0.004%
89	13.932	2104	2107	2108	rBV2	404	462	0.02%	0.004%
90	14.128	2136	2139	2140	rBV2	527	383	0.02%	0.003%
91	14.317	2167	2170	2173	rBV2	410	716	0.04%	0.006%
92	14.378	2179	2180	2182	rBV	448	407	0.02%	0.004%
93	14.432	2187	2189	2192	rBV2	525	687	0.03%	0.006%
94	14.609	2216	2218	2220	rVB2	593	447	0.02%	0.004%
95	14.634	2220	2222	2224	rBV3	705	610	0.03%	0.006%
96	14.871	2258	2261	2262	rBV	838	755	0.04%	0.007%
97	15.316	2332	2334	2337	rBV	593	485	0.02%	0.004%
98	16.048	2452	2454	2455	rBV2	592	557	0.03%	0.005%
99	16.097	2458	2462	2467	rVV5	2826	4619	0.23%	0.042%
100	16.560	2536	2538	2540	rVV2	662	471	0.02%	0.004%


Sum of corrected areas: 11090128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030488.D
Acq On : 07 Aug 2022 01:19
Operator : JC/MD
Sample : N4021-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

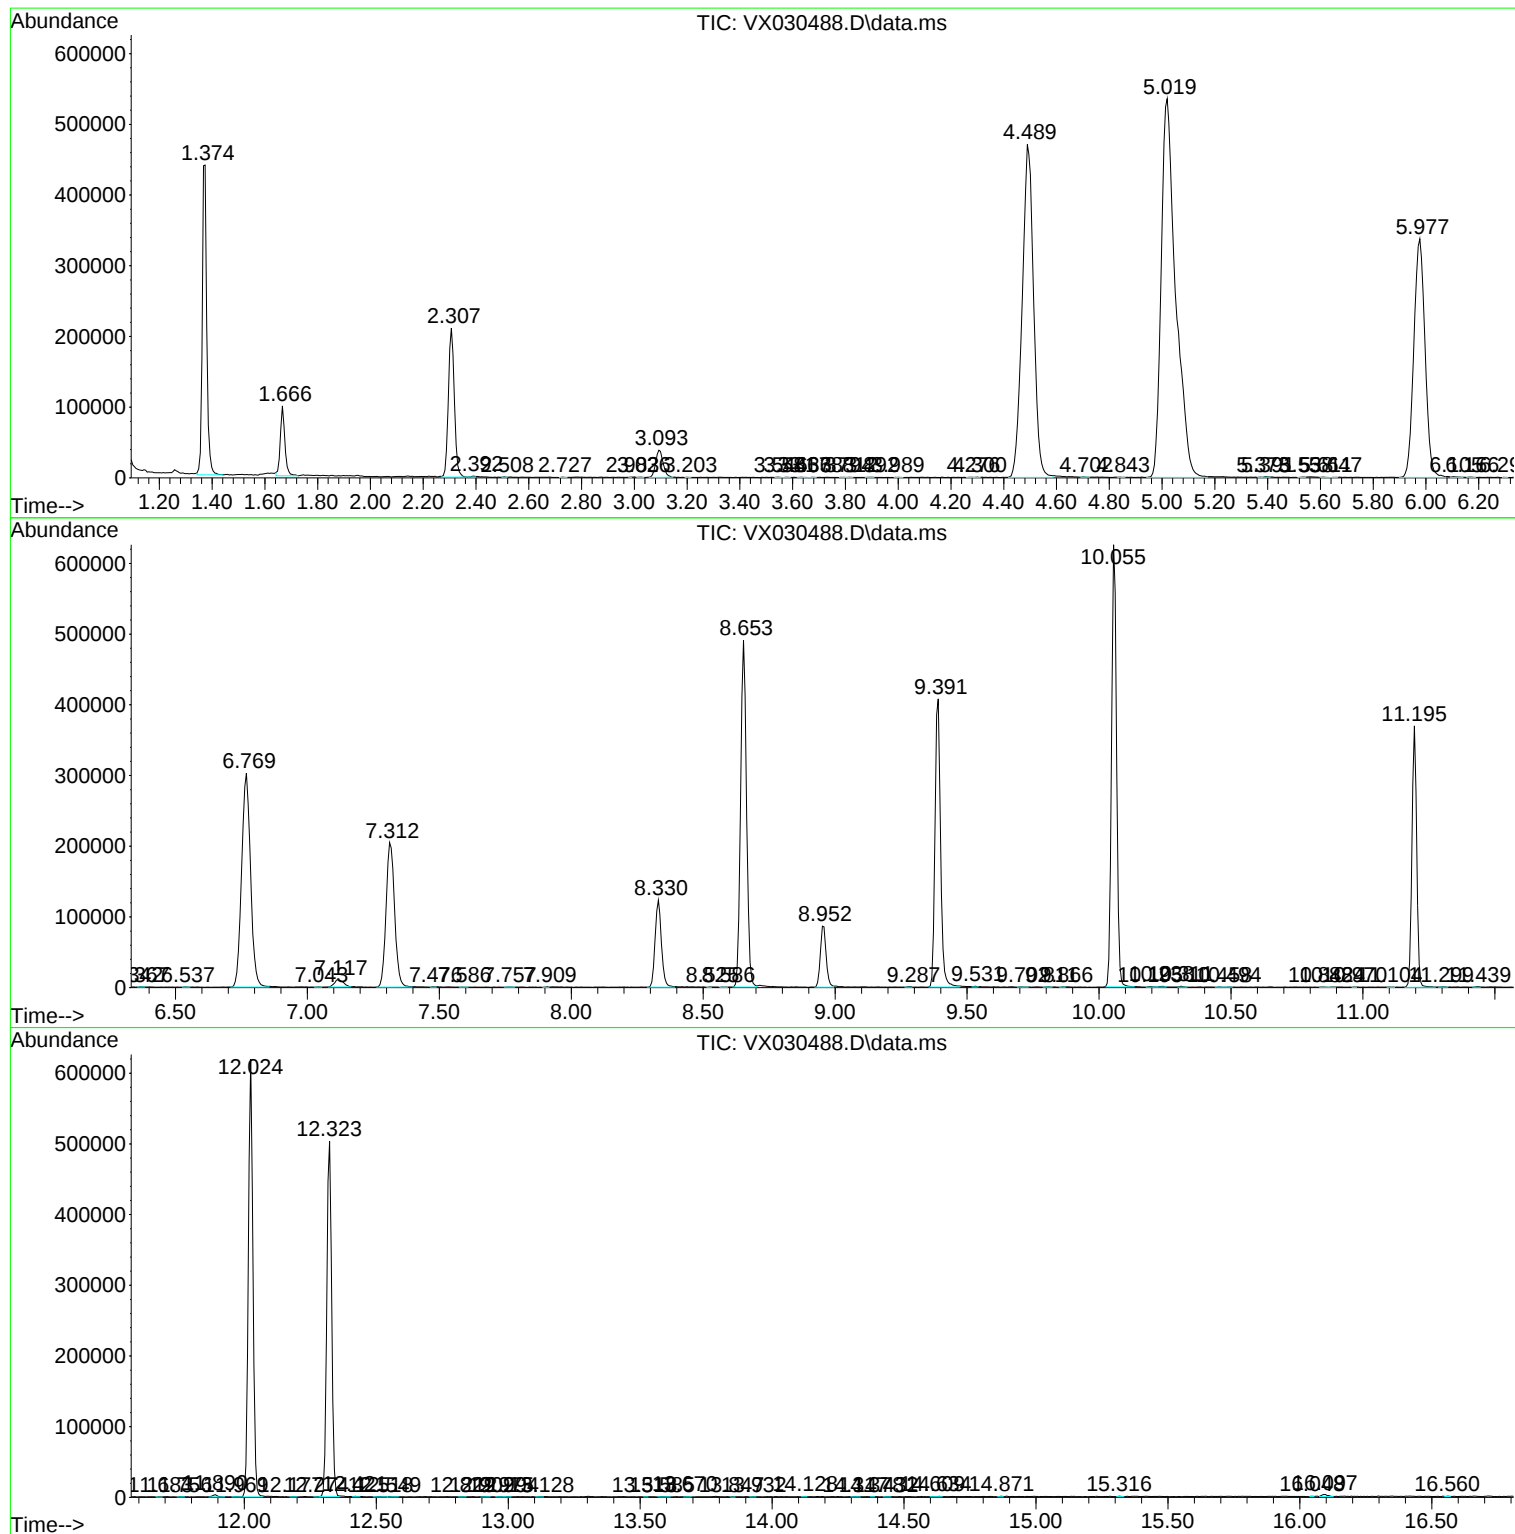

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030488.D
Acq On : 07 Aug 2022 01:19
Operator : JC/MD
Sample : N4021-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030488.D
Acq On : 07 Aug 2022 01:19
Operator : JC/MD
Sample : N4021-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc