

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030489.D
 Acq On : 07 Aug 2022 01:42
 Operator : JC/MD
 Sample : N4021-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	41	46	55	rVB2	193065	231163	12.28%	2.237%
2	1.666	91	95	105	rVB2	100991	137909	7.32%	1.334%
3	2.306	194	200	210	rVB	217107	338716	17.99%	3.277%
4	2.398	210	215	217	rBV3	2405	3621	0.19%	0.035%
5	2.514	232	234	237	rVB	1121	846	0.04%	0.008%
6	2.684	261	262	263	rBV	706	336	0.02%	0.003%
7	2.703	263	265	267	rVV2	566	579	0.03%	0.006%
8	2.825	283	285	289	rVB2	323	317	0.02%	0.003%
9	2.867	289	292	295	rBV2	500	647	0.03%	0.006%
10	3.001	309	314	316	rVB3	745	1123	0.06%	0.011%
11	3.026	316	318	320	rBV2	444	313	0.02%	0.003%
12	3.099	320	330	338	rVB3	18484	39419	2.09%	0.381%
13	3.440	385	386	388	rBV	533	321	0.02%	0.003%
14	3.477	388	392	393	rVV2	388	352	0.02%	0.003%
15	3.599	410	412	415	rBV2	396	478	0.03%	0.005%
16	3.885	456	459	462	rBV	723	573	0.03%	0.006%
17	3.971	472	473	479	rVB	469	749	0.04%	0.007%
18	4.111	494	496	498	rBV2	324	289	0.02%	0.003%
19	4.270	520	522	524	rVV	423	296	0.02%	0.003%
20	4.495	545	559	581	rBV2	644718	1883178	100.00%	18.221%
21	4.849	615	617	619	rVB	540	460	0.02%	0.004%
22	4.922	626	629	630	rBV3	306	333	0.02%	0.003%
23	4.971	635	637	639	rBV	399	323	0.02%	0.003%
24	5.062	639	652	667	rBV	131458	428869	22.77%	4.150%
25	5.288	688	689	694	rBV	355	391	0.02%	0.004%
26	5.367	699	702	704	rBV3	561	638	0.03%	0.006%
27	5.477	717	720	725	rVB3	682	1358	0.07%	0.013%
28	5.513	725	726	728	rBV	553	475	0.03%	0.005%
29	5.617	741	743	745	rVB2	487	429	0.02%	0.004%
30	5.830	776	778	779	rBV	400	289	0.02%	0.003%
31	5.977	790	802	821	rBV2	343591	1023981	54.38%	9.908%
32	6.269	848	850	852	rBV2	298	302	0.02%	0.003%
33	6.367	864	866	868	rVB2	521	445	0.02%	0.004%
34	6.629	907	909	911	rBV2	451	460	0.02%	0.004%
35	6.769	922	932	949	rBV	297231	705434	37.46%	6.826%
36	6.928	957	958	960	rBV2	570	428	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030489.D
 Acq On : 07 Aug 2022 01:42
 Operator : JC/MD
 Sample : N4021-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

37	7.129	982	991	1005	rBV2	174993	388146	20.61%	3.756%
38	7.312	1009	1021	1035	rBV	214579	470220	24.97%	4.550%
39	7.488	1048	1050	1052	rVB2	622	455	0.02%	0.004%
40	7.556	1059	1061	1063	rVB2	485	467	0.02%	0.005%
41	7.677	1077	1081	1082	rVB2	455	458	0.02%	0.004%
42	7.879	1112	1114	1115	rBV2	441	341	0.02%	0.003%
43	7.909	1115	1119	1123	rBV5	1351	2165	0.11%	0.021%
44	8.116	1152	1153	1155	rBV2	370	342	0.02%	0.003%
45	8.196	1164	1166	1167	rBV	426	370	0.02%	0.004%
46	8.257	1174	1176	1179	rBV	275	404	0.02%	0.004%
47	8.330	1181	1188	1197	rBV	127882	210505	11.18%	2.037%
48	8.458	1207	1209	1212	rBV3	830	1096	0.06%	0.011%
49	8.580	1228	1229	1233	rBV2	606	647	0.03%	0.006%
50	8.653	1234	1241	1250	rBV	512968	792145	42.06%	7.665%
51	8.952	1283	1290	1301	rBV	92955	140255	7.45%	1.357%
52	9.061	1307	1308	1309	rBV	564	352	0.02%	0.003%
53	9.275	1337	1343	1355	rVB	144730	211154	11.21%	2.043%
54	9.391	1355	1362	1376	rBV	390216	585652	31.10%	5.667%
55	9.732	1416	1418	1419	rBV	472	309	0.02%	0.003%
56	9.799	1425	1429	1433	rBV3	554	986	0.05%	0.010%
57	10.055	1465	1471	1487	rBV	617226	829158	44.03%	8.023%
58	10.201	1492	1495	1500	rVB5	1261	1363	0.07%	0.013%
59	10.275	1505	1507	1508	rBV	367	374	0.02%	0.004%
60	10.305	1508	1512	1517	rVB3	2384	3387	0.18%	0.033%
61	10.354	1517	1520	1525	rBV3	376	470	0.02%	0.005%
62	10.403	1525	1528	1530	rVB2	371	300	0.02%	0.003%
63	10.525	1547	1548	1550	rBV	371	335	0.02%	0.003%
64	10.646	1566	1568	1573	rVB2	913	1190	0.06%	0.012%
65	10.762	1585	1587	1590	rVB2	372	310	0.02%	0.003%
66	10.817	1594	1596	1598	rBV2	262	303	0.02%	0.003%
67	10.860	1602	1603	1605	rBV	425	295	0.02%	0.003%
68	11.098	1640	1642	1643	rBV	473	335	0.02%	0.003%
69	11.195	1652	1658	1666	rBV	375784	475791	25.27%	4.604%
70	11.476	1702	1704	1708	rVB	903	712	0.04%	0.007%
71	11.512	1708	1710	1711	rBV	594	423	0.02%	0.004%
72	11.537	1711	1714	1717	rVB3	591	700	0.04%	0.007%
73	11.683	1736	1738	1739	rBV	599	355	0.02%	0.003%
74	11.750	1747	1749	1753	rVB	548	673	0.04%	0.007%
75	11.786	1753	1755	1757	rBV	516	326	0.02%	0.003%
76	12.024	1788	1794	1803	rBV	621586	744588	39.54%	7.205%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030489.D
 Acq On : 07 Aug 2022 01:42
 Operator : JC/MD
 Sample : N4021-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.207	1823	1824	1827	rBV	498	380	0.02%	0.004%
78	12.232	1827	1828	1831	rVV3	711	589	0.03%	0.006%
79	12.323	1837	1843	1855	rVV	520204	649862	34.51%	6.288%
80	12.591	1885	1887	1889	rBV2	359	346	0.02%	0.003%
81	12.658	1895	1898	1899	rBV2	460	474	0.03%	0.005%
82	12.725	1907	1909	1911	rBV2	365	343	0.02%	0.003%
83	12.768	1913	1916	1917	rBV	535	484	0.03%	0.005%
84	13.042	1960	1961	1965	rBV2	372	544	0.03%	0.005%
85	13.073	1965	1966	1969	rVV	500	365	0.02%	0.004%
86	13.219	1988	1990	1993	rBV2	477	530	0.03%	0.005%
87	13.372	2012	2015	2017	rVB	485	504	0.03%	0.005%
88	13.408	2018	2021	2022	rBV	390	351	0.02%	0.003%
89	13.445	2025	2027	2030	rBV2	558	586	0.03%	0.006%
90	13.481	2031	2033	2037	rBV	463	449	0.02%	0.004%
91	13.682	2063	2066	2068	rBV2	435	402	0.02%	0.004%
92	14.170	2144	2146	2148	rBV	283	292	0.02%	0.003%
93	14.286	2163	2165	2166	rBV	520	372	0.02%	0.004%
94	14.749	2239	2241	2242	rBV	502	317	0.02%	0.003%
95	14.829	2253	2254	2256	rVB	736	362	0.02%	0.004%
96	14.969	2275	2277	2279	rBV2	556	445	0.02%	0.004%
97	15.103	2298	2299	2300	rVB	807	295	0.02%	0.003%
98	15.207	2314	2316	2323	rBV3	710	1186	0.06%	0.011%
99	16.121	2463	2466	2470	rBV3	704	1217	0.06%	0.012%
100	16.682	2557	2558	2560	rVB2	1054	573	0.03%	0.006%




Sum of corrected areas: 10334965

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030489.D
Acq On : 07 Aug 2022 01:42
Operator : JC/MD
Sample : N4021-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXL080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

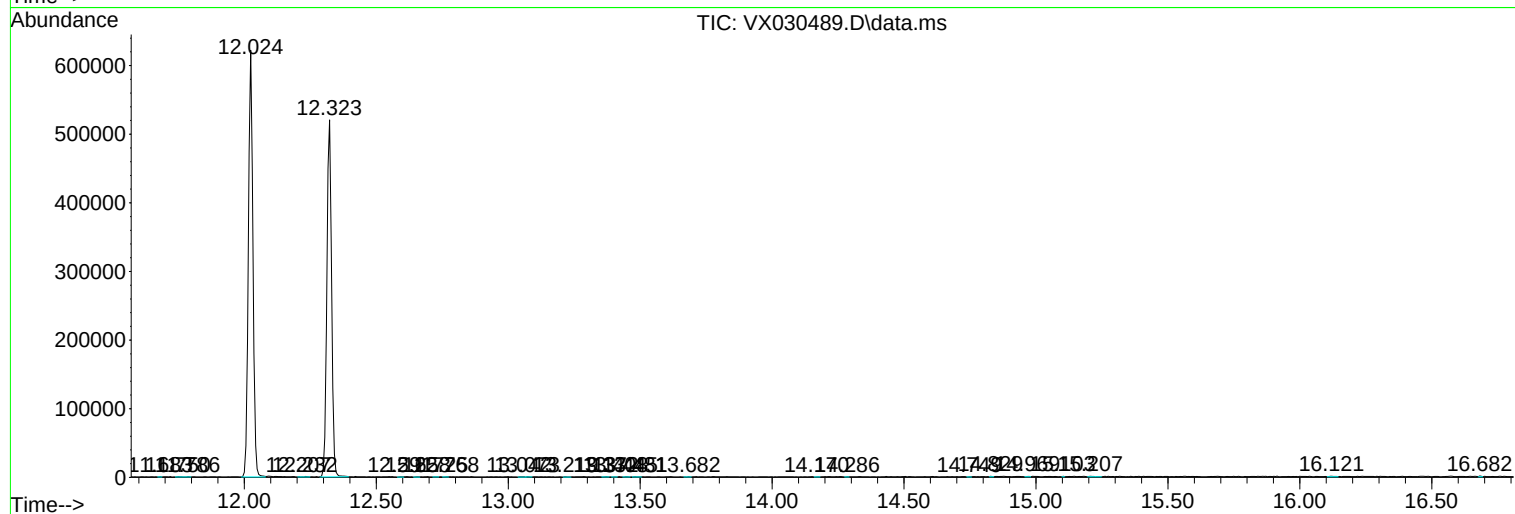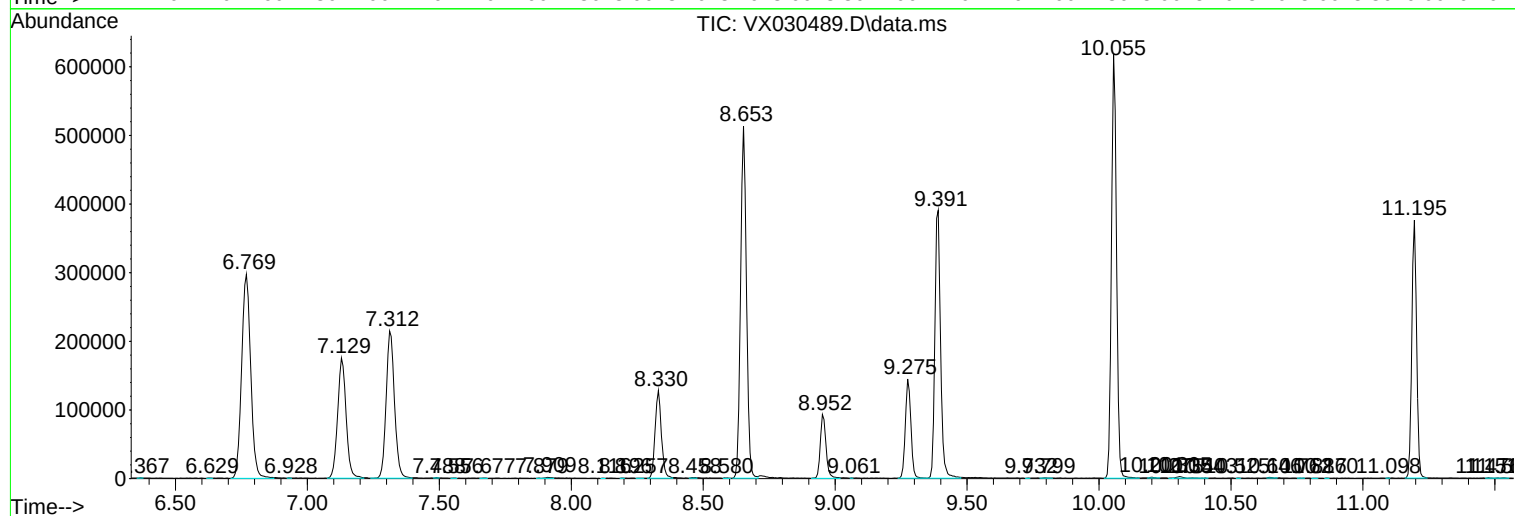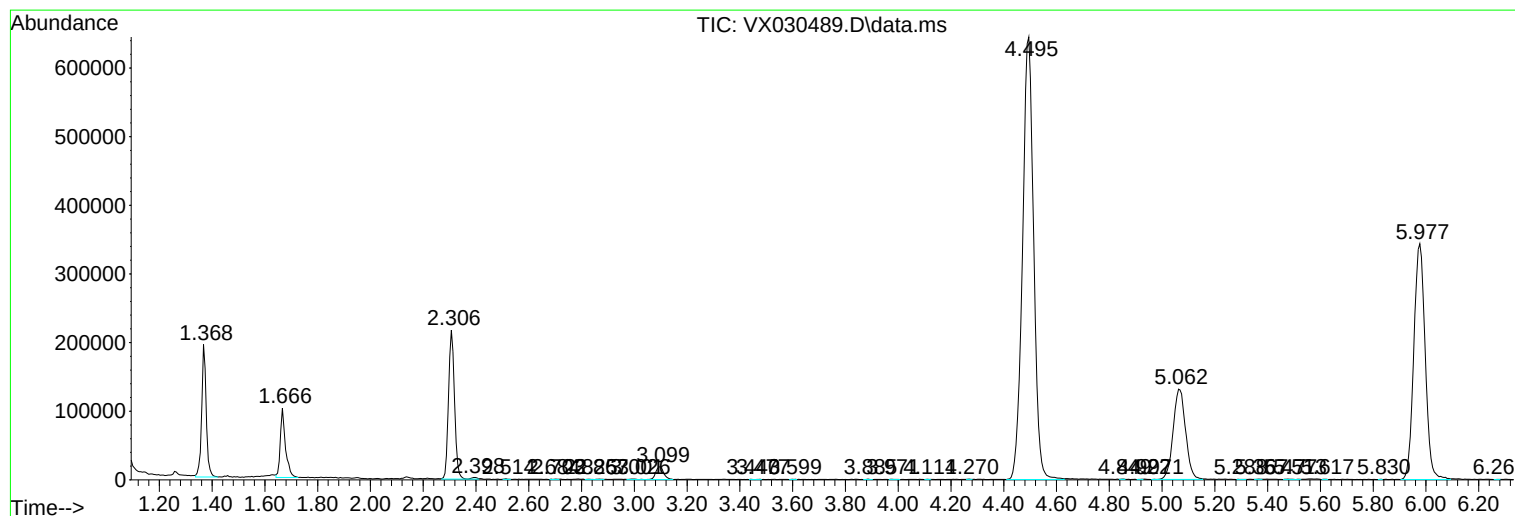

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030489.D
Acq On : 07 Aug 2022 01:42
Operator : JC/MD
Sample : N4021-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030489.D
Acq On : 07 Aug 2022 01:42
Operator : JC/MD
Sample : N4021-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------