

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030490.D
 Acq On : 07 Aug 2022 02:06
 Operator : JC/MD
 Sample : VIBLK655
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	126938	125432	12.67%	1.587%
2	1.666	91	95	103	rVB	98545	119947	12.12%	1.517%
3	2.307	194	200	210	rVB	204836	314855	31.81%	3.983%
4	2.459	223	225	229	rVB3	452	330	0.03%	0.004%
5	2.526	233	236	237	rVB2	658	590	0.06%	0.007%
6	2.563	239	242	243	rBV2	705	787	0.08%	0.010%
7	2.660	256	258	261	rBV3	452	409	0.04%	0.005%
8	2.794	272	280	285	rBV2	2980	5947	0.60%	0.075%
9	3.075	325	326	327	rBV	567	340	0.03%	0.004%
10	3.367	372	374	376	rVB2	483	395	0.04%	0.005%
11	3.404	376	380	382	rVB2	487	515	0.05%	0.007%
12	3.441	382	386	388	rBV2	387	447	0.05%	0.006%
13	3.459	388	389	393	rVB	367	406	0.04%	0.005%
14	3.569	405	407	411	rVB2	303	362	0.04%	0.005%
15	3.636	415	418	420	rBV2	392	613	0.06%	0.008%
16	3.940	467	468	471	rVV2	312	331	0.03%	0.004%
17	4.081	488	491	492	rBV	417	349	0.04%	0.004%
18	4.172	503	506	508	rBV2	463	467	0.05%	0.006%
19	4.196	508	510	511	rVB	612	328	0.03%	0.004%
20	4.215	511	513	517	rBV2	577	733	0.07%	0.009%
21	4.471	545	555	568	rBV	91662	265935	26.87%	3.364%
22	4.910	625	627	629	rBV2	513	492	0.05%	0.006%
23	4.946	631	633	635	rVB3	676	533	0.05%	0.007%
24	5.068	639	653	669	rBV	132718	410365	41.46%	5.191%
25	5.215	675	677	678	rBV2	366	329	0.03%	0.004%
26	5.397	706	707	710	rVV3	619	530	0.05%	0.007%
27	5.556	730	733	734	rBV	582	532	0.05%	0.007%
28	5.836	776	779	781	rBV3	594	544	0.05%	0.007%
29	5.891	785	788	789	rBV	414	458	0.05%	0.006%
30	5.977	791	802	815	rBV2	335240	989771	100.00%	12.521%
31	6.190	835	837	839	rVB2	521	383	0.04%	0.005%
32	6.391	869	870	872	rVB	691	357	0.04%	0.005%
33	6.416	872	874	878	rVB2	320	330	0.03%	0.004%
34	6.562	895	898	899	rBV	387	362	0.04%	0.005%
35	6.769	922	932	947	rVV	294326	713796	72.12%	9.030%
36	6.922	956	957	959	rBV2	586	348	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030490.D
 Acq On : 07 Aug 2022 02:06
 Operator : JC/MD
 Sample : VIBLK655
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.117	983	989	1000	rVV4	12158	30097	3.04%	0.381%
38	7.312	1012	1021	1035	rBV	212407	463618	46.84%	5.865%
39	7.867	1109	1112	1113	rBV2	348	365	0.04%	0.005%
40	7.952	1123	1126	1128	rBV2	606	823	0.08%	0.010%
41	7.995	1131	1133	1139	rVB2	552	777	0.08%	0.010%
42	8.086	1146	1148	1150	rVB2	627	479	0.05%	0.006%
43	8.330	1182	1188	1200	rBV	125596	208276	21.04%	2.635%
44	8.513	1217	1218	1220	rBV2	718	404	0.04%	0.005%
45	8.562	1225	1226	1228	rBV	618	376	0.04%	0.005%
46	8.653	1234	1241	1256	rBV	510540	780437	78.85%	9.873%
47	8.879	1276	1278	1279	rBV	489	385	0.04%	0.005%
48	8.958	1284	1291	1305	rVV	88491	139255	14.07%	1.762%
49	9.129	1317	1319	1320	rBV	425	325	0.03%	0.004%
50	9.257	1337	1340	1341	rBV	403	505	0.05%	0.006%
51	9.281	1342	1344	1348	rVB2	1258	1062	0.11%	0.013%
52	9.391	1356	1362	1373	rBV	401726	575342	58.13%	7.278%
53	9.598	1394	1396	1400	rVB	782	824	0.08%	0.010%
54	9.708	1409	1414	1419	rBV5	1985	2841	0.29%	0.036%
55	9.842	1433	1436	1438	rBV2	385	331	0.03%	0.004%
56	9.988	1458	1460	1464	rVB2	337	401	0.04%	0.005%
57	10.055	1464	1471	1483	rBV	624334	837412	84.61%	10.594%
58	10.226	1498	1499	1502	rVB2	672	441	0.04%	0.006%
59	10.939	1613	1616	1617	rVB	529	423	0.04%	0.005%
60	10.976	1617	1622	1623	rBV2	379	592	0.06%	0.007%
61	11.055	1632	1635	1637	rBV2	392	456	0.05%	0.006%
62	11.195	1653	1658	1669	rVB	366391	459477	46.42%	5.813%
63	11.695	1738	1740	1741	rBV2	473	357	0.04%	0.005%
64	11.823	1758	1761	1763	rBV2	479	471	0.05%	0.006%
65	11.902	1772	1774	1777	rVB2	398	364	0.04%	0.005%
66	11.988	1786	1788	1789	rBV	437	343	0.03%	0.004%
67	12.024	1789	1794	1802	rBV	639616	750201	75.80%	9.490%
68	12.152	1812	1815	1816	rBV	887	527	0.05%	0.007%
69	12.226	1826	1827	1831	rVB4	504	356	0.04%	0.005%
70	12.323	1837	1843	1852	rBV	529711	671894	67.88%	8.500%
71	12.390	1852	1854	1858	rVB3	910	909	0.09%	0.011%
72	12.549	1878	1880	1882	rVB	482	325	0.03%	0.004%
73	12.634	1891	1894	1896	rVB2	615	401	0.04%	0.005%
74	12.658	1896	1898	1901	rBV	354	451	0.05%	0.006%
75	12.701	1903	1905	1906	rBV2	454	434	0.04%	0.005%
76	12.774	1914	1917	1920	rBV2	521	800	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030490.D
 Acq On : 07 Aug 2022 02:06
 Operator : JC/MD
 Sample : VIBLK655
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK655

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.128	1972	1975	1976	rBV2	432	436	0.04%	0.006%
78	13.311	2001	2005	2006	rVB	461	485	0.05%	0.006%
79	13.341	2006	2010	2011	rBV2	406	554	0.06%	0.007%
80	13.390	2017	2018	2021	rBV	364	329	0.03%	0.004%
81	13.585	2047	2050	2052	rVB2	549	504	0.05%	0.006%
82	13.652	2060	2061	2063	rBV	452	430	0.04%	0.005%
83	13.731	2071	2074	2078	rVB2	637	789	0.08%	0.010%
84	14.018	2119	2121	2124	rBV2	519	471	0.05%	0.006%
85	14.115	2135	2137	2140	rBV2	553	470	0.05%	0.006%
86	14.219	2152	2154	2158	rBV3	331	338	0.03%	0.004%
87	14.640	2222	2223	2227	rVB2	553	480	0.05%	0.006%
88	14.688	2230	2231	2233	rBV	508	352	0.04%	0.004%
89	14.877	2261	2262	2267	rVB2	677	773	0.08%	0.010%
90	14.920	2267	2269	2273	rBV2	684	721	0.07%	0.009%
91	14.951	2273	2274	2279	rBV2	415	547	0.06%	0.007%
92	15.164	2306	2309	2311	rBV2	639	723	0.07%	0.009%
93	15.408	2347	2349	2352	rBV3	769	777	0.08%	0.010%
94	15.438	2352	2354	2355	rBV2	754	385	0.04%	0.005%
95	15.713	2397	2399	2401	rVB	901	622	0.06%	0.008%
96	15.731	2401	2402	2406	rBV2	731	828	0.08%	0.010%
97	15.792	2410	2412	2413	rBV2	503	324	0.03%	0.004%
98	15.810	2413	2415	2416	rBV	521	412	0.04%	0.005%
99	15.938	2434	2436	2438	rBV2	768	561	0.06%	0.007%
100	16.566	2537	2539	2541	rBV2	595	340	0.03%	0.004%




Sum of corrected areas: 7904856

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030490.D
Acq On : 07 Aug 2022 02:06
Operator : JC/MD
Sample : VIBLK655
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

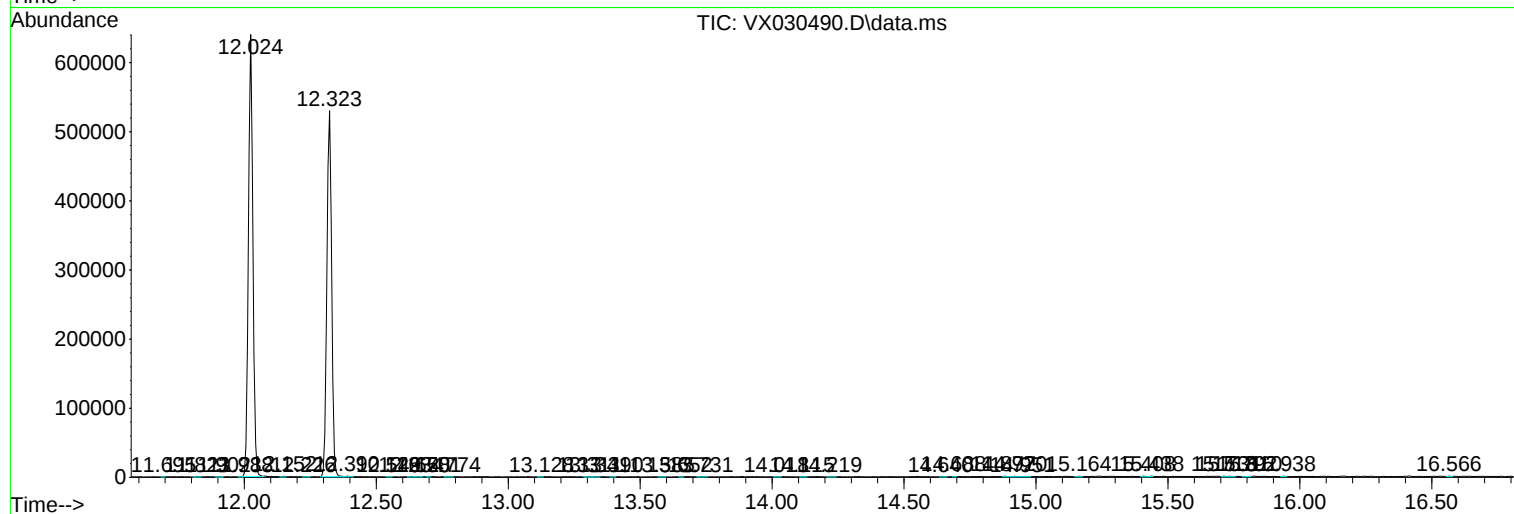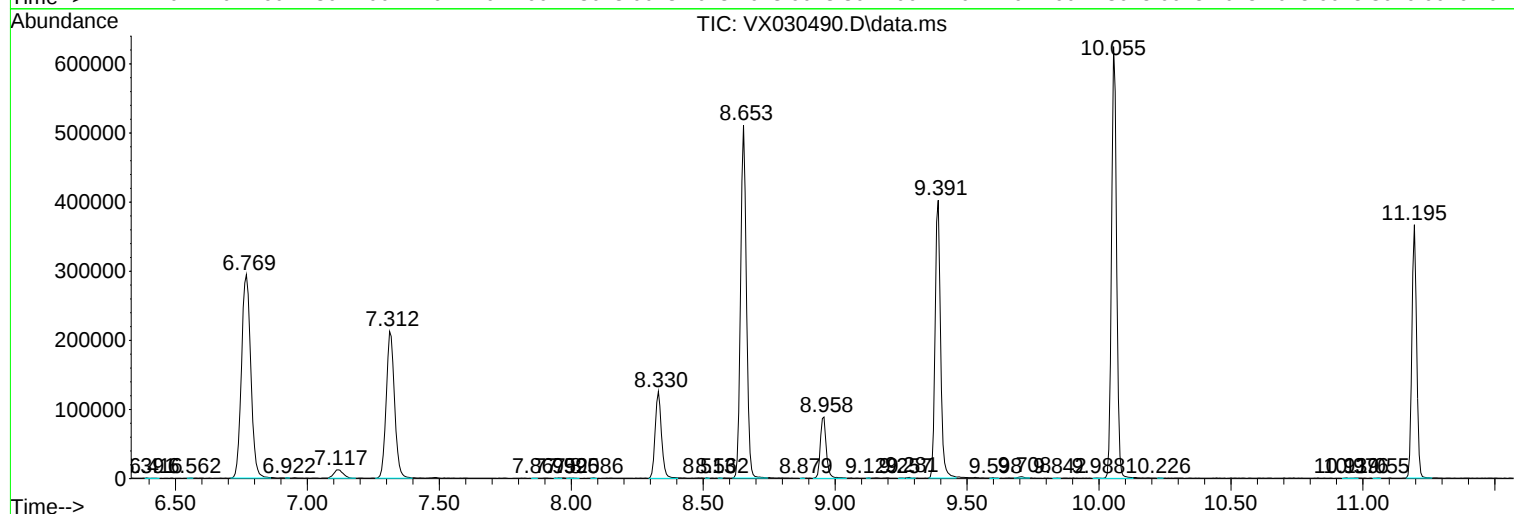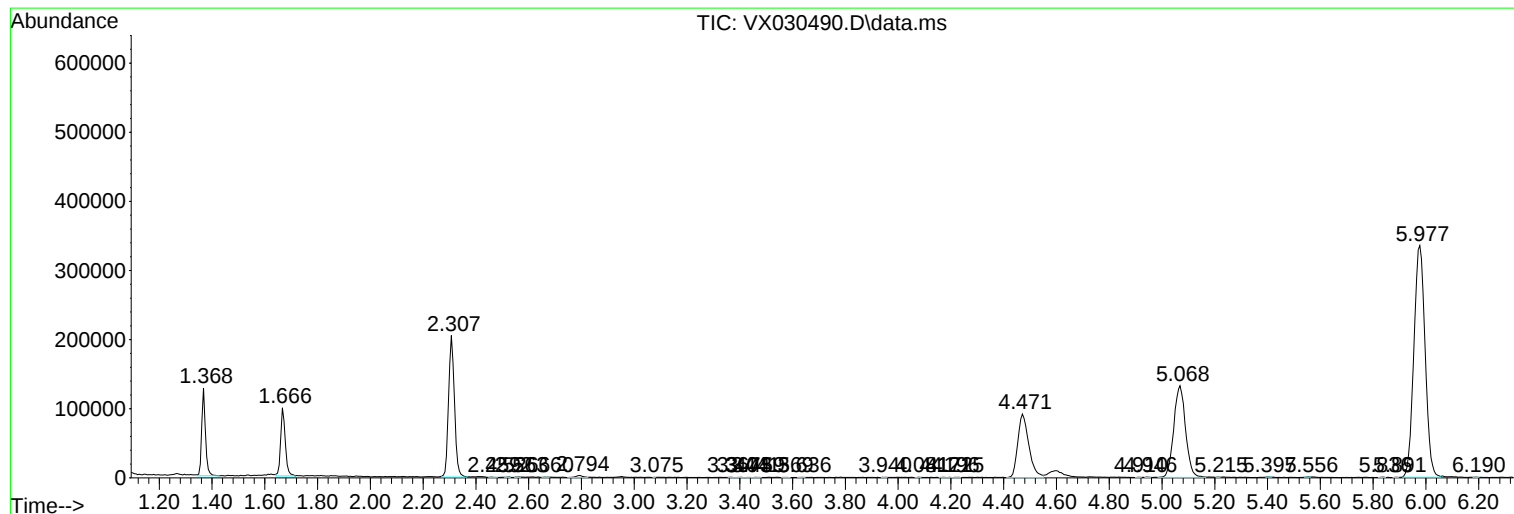

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030490.D
Acq On : 07 Aug 2022 02:06
Operator : JC/MD
Sample : VIBLK655
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030490.D
Acq On : 07 Aug 2022 02:06
Operator : JC/MD
Sample : VIBLK655
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK655

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc