

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030491.D
 Acq On : 07 Aug 2022 02:29
 Operator : JC/MD
 Sample : N4021-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	133086	146742	3.28%	1.116%
2	1.666	91	95	105	rVB	94316	115238	2.58%	0.876%
3	2.130	169	171	178	rVB5	2880	5121	0.11%	0.039%
4	2.306	194	200	211	rVB	209471	323320	7.23%	2.459%
5	2.660	256	258	259	rVB	730	417	0.01%	0.003%
6	2.678	259	261	262	rBV	414	400	0.01%	0.003%
7	2.751	272	273	275	rBV	554	401	0.01%	0.003%
8	2.995	311	313	318	rVB2	708	1283	0.03%	0.010%
9	3.093	322	329	338	rVV	68553	126322	2.83%	0.961%
10	3.203	345	347	348	rVB	661	361	0.01%	0.003%
11	3.343	369	370	373	rVB2	409	361	0.01%	0.003%
12	3.373	373	375	377	rVB	576	433	0.01%	0.003%
13	3.392	377	378	382	rBV	401	479	0.01%	0.004%
14	3.593	408	411	414	rVB2	345	421	0.01%	0.003%
15	3.788	439	443	444	rBV2	383	447	0.01%	0.003%
16	3.806	444	446	449	rVV2	297	331	0.01%	0.003%
17	3.959	467	471	472	rBV	279	400	0.01%	0.003%
18	4.032	480	483	486	rBV2	528	669	0.01%	0.005%
19	4.166	504	505	508	rVB2	440	347	0.01%	0.003%
20	4.495	546	559	579	rBV2	1586795	4469912	100.00%	33.990%
21	4.800	607	609	610	rVB2	631	357	0.01%	0.003%
22	5.068	640	653	666	rBV	129727	417049	9.33%	3.171%
23	5.202	673	675	678	rBV3	628	686	0.02%	0.005%
24	5.391	701	706	708	rBV2	748	1215	0.03%	0.009%
25	5.489	720	722	723	rVB2	535	351	0.01%	0.003%
26	5.525	727	728	730	rBV	418	389	0.01%	0.003%
27	5.842	778	780	783	rVB	499	470	0.01%	0.004%
28	5.885	783	787	789	rBV2	421	525	0.01%	0.004%
29	5.976	789	802	817	rBV2	338666	1001211	22.40%	7.613%
30	6.348	861	863	864	rVV2	452	338	0.01%	0.003%
31	6.367	864	866	869	rVB2	671	671	0.02%	0.005%
32	6.586	900	902	905	rVB	496	398	0.01%	0.003%
33	6.623	905	908	910	rVB	467	482	0.01%	0.004%
34	6.647	910	912	913	rBV	597	391	0.01%	0.003%
35	6.769	922	932	950	rBV	301900	721599	16.14%	5.487%
36	6.988	964	968	969	rBV	450	566	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030491.D
 Acq On : 07 Aug 2022 02:29
 Operator : JC/MD
 Sample : N4021-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.043	975	977	981	rVB	662	513	0.01%	0.004%
38	7.129	981	991	1005	rBV	407074	872989	19.53%	6.638%
39	7.312	1011	1021	1034	rBV	206720	460335	10.30%	3.500%
40	7.562	1060	1062	1065	rBV2	487	419	0.01%	0.003%
41	7.683	1078	1082	1083	rBV2	408	500	0.01%	0.004%
42	7.720	1086	1088	1093	rBV2	431	676	0.02%	0.005%
43	7.818	1102	1104	1106	rVV	452	378	0.01%	0.003%
44	7.909	1114	1119	1127	rVV5	2591	6087	0.14%	0.046%
45	7.994	1130	1133	1134	rVV2	597	447	0.01%	0.003%
46	8.031	1137	1139	1143	rVB	483	720	0.02%	0.005%
47	8.068	1143	1145	1149	rBV2	439	642	0.01%	0.005%
48	8.104	1149	1151	1154	rBV2	302	362	0.01%	0.003%
49	8.183	1161	1164	1165	rBV2	380	361	0.01%	0.003%
50	8.275	1177	1179	1182	rBV2	399	436	0.01%	0.003%
51	8.330	1182	1188	1197	rBV	125867	203646	4.56%	1.549%
52	8.458	1206	1209	1214	rVB4	1639	2654	0.06%	0.020%
53	8.494	1214	1215	1218	rBV2	719	669	0.01%	0.005%
54	8.574	1225	1228	1231	rVB	541	638	0.01%	0.005%
55	8.653	1233	1241	1253	rBV	504341	781864	17.49%	5.945%
56	8.866	1274	1276	1279	rVB2	493	564	0.01%	0.004%
57	8.915	1281	1284	1285	rBV2	498	464	0.01%	0.004%
58	8.952	1285	1290	1303	rBV	91676	139376	3.12%	1.060%
59	9.275	1337	1343	1350	rBV3	10144	15210	0.34%	0.116%
60	9.390	1356	1362	1375	rBV	409765	589598	13.19%	4.483%
61	9.555	1387	1389	1390	rBV	641	404	0.01%	0.003%
62	9.683	1407	1410	1412	rBV2	568	747	0.02%	0.006%
63	10.055	1465	1471	1484	rBV	623284	842655	18.85%	6.408%
64	10.415	1528	1530	1533	rVV2	480	594	0.01%	0.005%
65	10.512	1543	1546	1548	rVB2	492	518	0.01%	0.004%
66	10.543	1548	1551	1553	rBV2	592	734	0.02%	0.006%
67	10.646	1566	1568	1571	rBV2	415	557	0.01%	0.004%
68	10.805	1591	1594	1596	rBV	444	444	0.01%	0.003%
69	11.073	1633	1638	1639	rBV4	338	501	0.01%	0.004%
70	11.195	1652	1658	1666	rBV	386346	477422	10.68%	3.630%
71	11.347	1679	1683	1684	rBV2	442	534	0.01%	0.004%
72	11.561	1716	1718	1723	rBV	829	859	0.02%	0.007%
73	11.597	1723	1724	1728	rVV2	460	405	0.01%	0.003%
74	11.634	1728	1730	1732	rVB	774	578	0.01%	0.004%
75	11.701	1739	1741	1744	rVB2	424	455	0.01%	0.003%
76	11.786	1752	1755	1759	rBV2	576	815	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030491.D
 Acq On : 07 Aug 2022 02:29
 Operator : JC/MD
 Sample : N4021-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	11.872	1767	1769	1771	rBV	555	391	0.01%	0.003%
78	11.957	1782	1783	1787	rVB2	521	368	0.01%	0.003%
79	12.024	1789	1794	1802	rVV	624397	751839	16.82%	5.717%
80	12.219	1825	1826	1829	rBV2	766	633	0.01%	0.005%
81	12.323	1837	1843	1852	rBV	512155	640209	14.32%	4.868%
82	12.500	1870	1872	1874	rBV2	591	514	0.01%	0.004%
83	12.774	1915	1917	1919	rVB	702	458	0.01%	0.003%
84	12.798	1919	1921	1922	rBV2	444	367	0.01%	0.003%
85	12.884	1932	1935	1936	rBV2	670	682	0.02%	0.005%
86	12.908	1936	1939	1940	rVV2	445	515	0.01%	0.004%
87	12.945	1943	1945	1948	rVV2	477	378	0.01%	0.003%
88	13.115	1971	1973	1976	rBV2	522	536	0.01%	0.004%
89	13.323	2006	2007	2010	rBV2	379	343	0.01%	0.003%
90	13.579	2047	2049	2052	rVB2	575	582	0.01%	0.004%
91	13.609	2052	2054	2057	rBV	502	766	0.02%	0.006%
92	13.835	2089	2091	2094	rVB	403	330	0.01%	0.003%
93	13.951	2106	2110	2111	rBV	355	385	0.01%	0.003%
94	14.158	2140	2144	2145	rBV2	588	510	0.01%	0.004%
95	14.353	2174	2176	2180	rVB2	593	751	0.02%	0.006%
96	14.383	2180	2181	2182	rBV	694	372	0.01%	0.003%
97	14.987	2278	2280	2282	rBV2	562	335	0.01%	0.003%
98	15.280	2326	2328	2329	rBV2	561	405	0.01%	0.003%
99	15.816	2414	2416	2418	rVB2	664	405	0.01%	0.003%
100	15.841	2418	2420	2422	rBV2	962	807	0.02%	0.006%




Sum of corrected areas: 13150754

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030491.D
Acq On : 07 Aug 2022 02:29
Operator : JC/MD
Sample : N4021-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

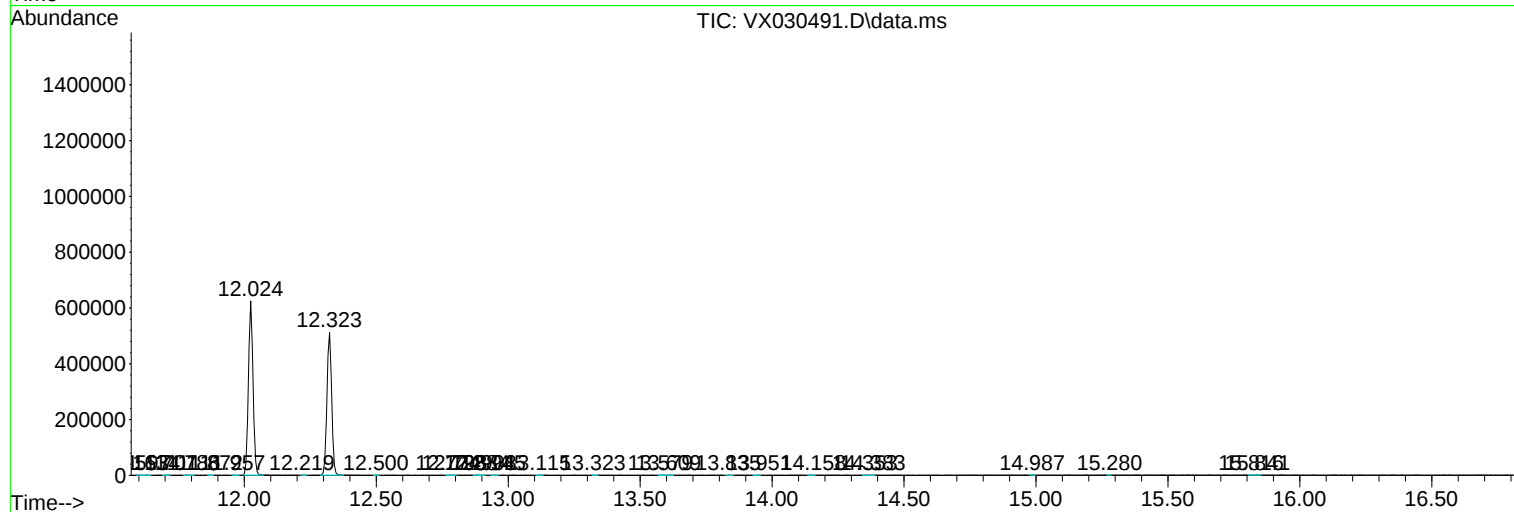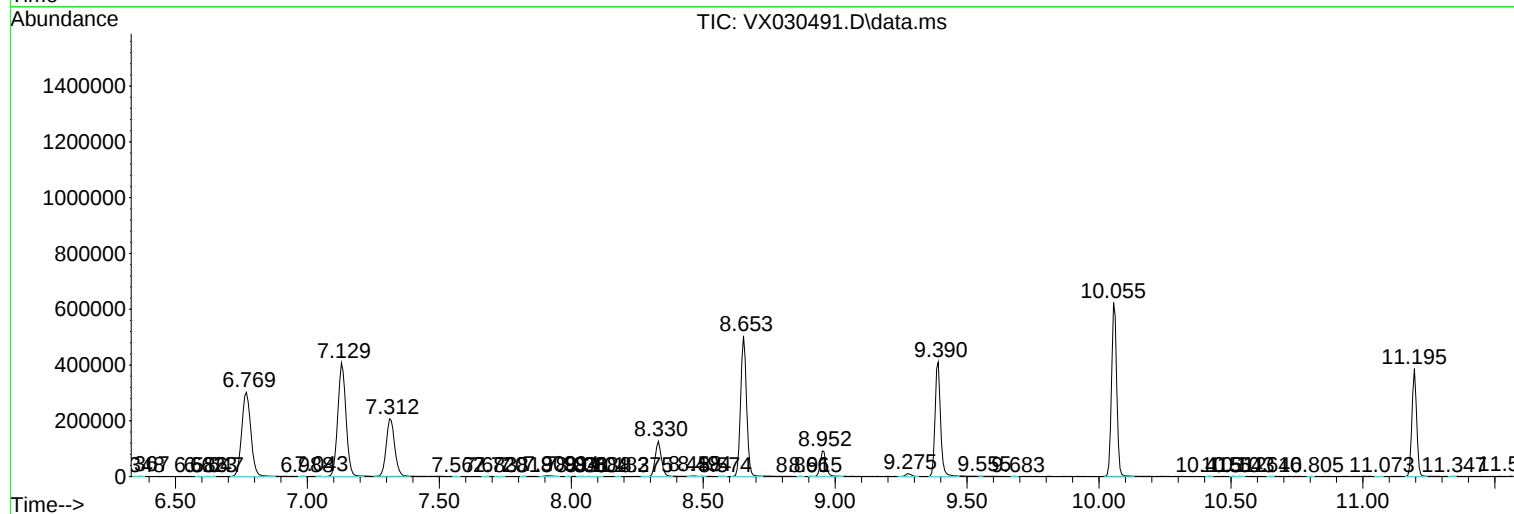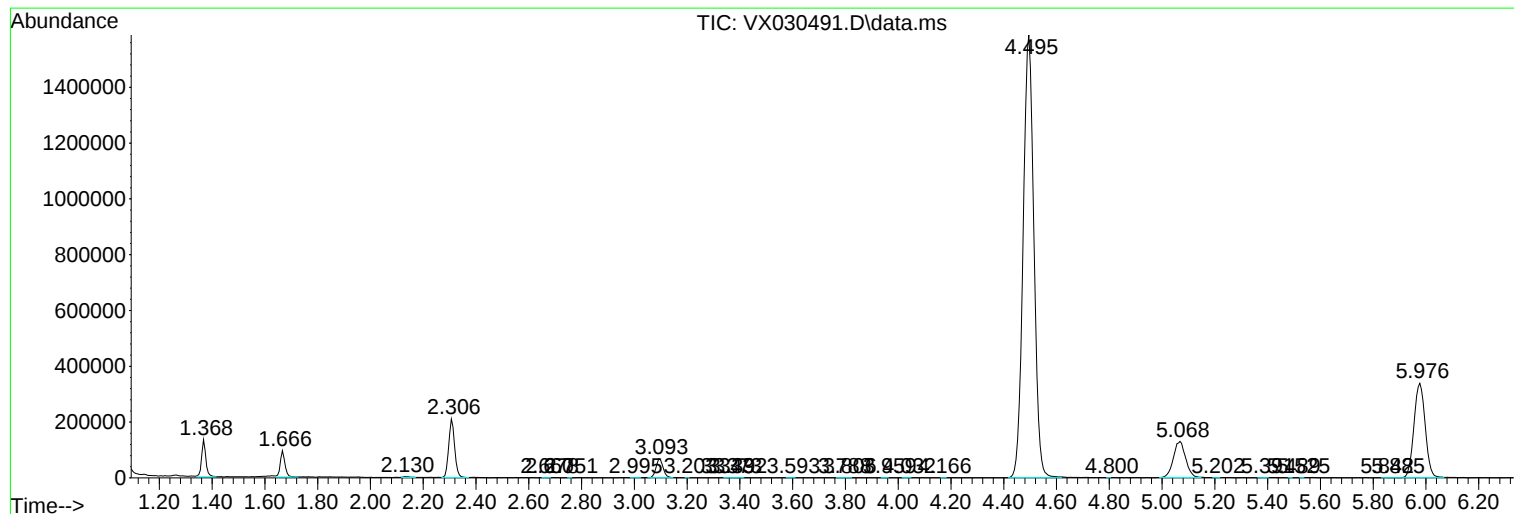

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030491.D
Acq On : 07 Aug 2022 02:29
Operator : JC/MD
Sample : N4021-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030491.D
Acq On : 07 Aug 2022 02:29
Operator : JC/MD
Sample : N4021-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D66

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc