

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030492.D
 Acq On : 07 Aug 2022 02:53
 Operator : JC/MD
 Sample : VIBLK656
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	120222	126584	12.56%	1.582%
2	1.666	91	95	103	rVB	104289	120851	11.99%	1.510%
3	2.307	194	200	210	rVB	223036	333036	33.04%	4.161%
4	2.495	230	231	234	rBV3	690	490	0.05%	0.006%
5	2.563	240	242	244	rBV2	753	655	0.06%	0.008%
6	2.758	270	274	276	rBV3	765	1010	0.10%	0.013%
7	2.794	276	280	285	rVV3	3293	5160	0.51%	0.064%
8	2.855	288	290	291	rBV2	469	334	0.03%	0.004%
9	2.953	299	306	314	rVV	7119	15922	1.58%	0.199%
10	3.166	340	341	345	rVV3	459	514	0.05%	0.006%
11	3.215	347	349	353	rBV2	703	715	0.07%	0.009%
12	3.331	366	368	372	rVB	283	344	0.03%	0.004%
13	3.373	372	375	376	rBV	310	299	0.03%	0.004%
14	3.605	411	413	415	rVV	501	342	0.03%	0.004%
15	3.879	455	458	459	rVV	326	334	0.03%	0.004%
16	3.898	459	461	464	rVV2	316	369	0.04%	0.005%
17	4.093	491	493	495	rBV2	420	384	0.04%	0.005%
18	4.123	495	498	499	rBV	299	311	0.03%	0.004%
19	4.245	517	518	521	rVB2	424	366	0.04%	0.005%
20	4.288	521	525	526	rBV	228	334	0.03%	0.004%
21	4.477	545	556	568	rBV2	89429	274077	27.19%	3.425%
22	4.922	626	629	631	rBV2	502	446	0.04%	0.006%
23	5.062	641	652	666	rVV2	132677	409843	40.66%	5.121%
24	5.245	680	682	684	rVB2	608	436	0.04%	0.005%
25	5.550	727	732	733	rBV2	899	1054	0.10%	0.013%
26	5.788	770	771	774	rBV	446	452	0.04%	0.006%
27	5.830	776	778	781	rVB2	528	398	0.04%	0.005%
28	5.977	787	802	820	rBV2	346093	1008052	100.00%	12.596%
29	6.153	829	831	833	rVB2	630	492	0.05%	0.006%
30	6.464	881	882	885	rBV	279	322	0.03%	0.004%
31	6.489	885	886	889	rVB2	419	337	0.03%	0.004%
32	6.568	898	899	903	rVB	592	336	0.03%	0.004%
33	6.769	922	932	947	rBV	304395	727205	72.14%	9.087%
34	6.885	950	951	954	rBV3	933	692	0.07%	0.009%
35	7.056	976	979	981	rBV2	383	474	0.05%	0.006%
36	7.117	981	989	997	rVV4	13955	30095	2.99%	0.376%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030492.D
 Acq On : 07 Aug 2022 02:53
 Operator : JC/MD
 Sample : VIBLK656
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1013	1021	1036	rBV	208293	465183	46.15%	5.813%
38	7.488	1048	1050	1053	rVB3	474	382	0.04%	0.005%
39	7.647	1074	1076	1078	rBV2	277	317	0.03%	0.004%
40	7.696	1082	1084	1088	rVB2	420	417	0.04%	0.005%
41	7.745	1088	1092	1094	rBV	268	475	0.05%	0.006%
42	7.927	1121	1122	1124	rBV2	573	398	0.04%	0.005%
43	8.074	1144	1146	1149	rBV2	613	602	0.06%	0.008%
44	8.098	1149	1150	1152	rBV	364	322	0.03%	0.004%
45	8.244	1172	1174	1176	rVB2	491	323	0.03%	0.004%
46	8.275	1176	1179	1181	rBV2	417	460	0.05%	0.006%
47	8.330	1181	1188	1199	rBV	129081	207361	20.57%	2.591%
48	8.580	1226	1229	1230	rBV2	579	578	0.06%	0.007%
49	8.653	1234	1241	1255	rBV	497282	781667	77.54%	9.767%
50	8.958	1285	1291	1299	rVV	87670	135732	13.46%	1.696%
51	9.116	1315	1317	1318	rBV	477	361	0.04%	0.005%
52	9.189	1327	1329	1331	rVB2	436	332	0.03%	0.004%
53	9.263	1338	1341	1342	rBV2	438	393	0.04%	0.005%
54	9.391	1356	1362	1374	rBV	395740	576107	57.15%	7.199%
55	9.708	1409	1414	1418	rBV4	2140	2956	0.29%	0.037%
56	9.775	1423	1425	1428	rVB	496	334	0.03%	0.004%
57	9.994	1458	1461	1462	rBV	321	408	0.04%	0.005%
58	10.006	1462	1463	1465	rVV	484	324	0.03%	0.004%
59	10.055	1465	1471	1486	rVV	611807	844208	83.75%	10.549%
60	10.244	1500	1502	1503	rVV	492	301	0.03%	0.004%
61	10.293	1507	1510	1513	rBV2	589	653	0.06%	0.008%
62	10.372	1520	1523	1528	rVB2	742	1000	0.10%	0.012%
63	10.415	1528	1530	1532	rBV	315	372	0.04%	0.005%
64	10.653	1565	1569	1571	rBV	394	449	0.04%	0.006%
65	10.677	1571	1573	1575	rVV2	459	468	0.05%	0.006%
66	10.823	1594	1597	1599	rBV	333	477	0.05%	0.006%
67	10.994	1623	1625	1627	rVB	423	408	0.04%	0.005%
68	11.195	1652	1658	1667	rBV	358717	454243	45.06%	5.676%
69	11.543	1714	1715	1718	rBV2	451	476	0.05%	0.006%
70	11.573	1718	1720	1724	rVB2	357	306	0.03%	0.004%
71	11.701	1739	1741	1745	rBV2	317	591	0.06%	0.007%
72	11.933	1775	1779	1781	rBV	368	637	0.06%	0.008%
73	12.024	1788	1794	1804	rBV	632082	764823	75.87%	9.557%
74	12.213	1823	1825	1827	rVB	775	407	0.04%	0.005%
75	12.232	1827	1828	1830	rBV	457	361	0.04%	0.005%
76	12.323	1837	1843	1849	rBV	528681	681969	67.65%	8.522%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030492.D
 Acq On : 07 Aug 2022 02:53
 Operator : JC/MD
 Sample : VIBLK656
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.482	1867	1869	1871	rBV2	380	408	0.04%	0.005%
78	12.664	1897	1899	1901	rBV	359	346	0.03%	0.004%
79	12.841	1926	1928	1931	rVB3	331	326	0.03%	0.004%
80	12.988	1949	1952	1954	rVB	427	468	0.05%	0.006%
81	13.036	1958	1960	1962	rBV	502	478	0.05%	0.006%
82	13.268	1994	1998	1999	rBV	333	350	0.03%	0.004%
83	13.298	2001	2003	2006	rBV2	367	388	0.04%	0.005%
84	13.506	2034	2037	2039	rBV2	387	533	0.05%	0.007%
85	13.823	2087	2089	2091	rVB	368	377	0.04%	0.005%
86	13.987	2114	2116	2122	rBV2	330	612	0.06%	0.008%
87	14.079	2129	2131	2134	rVB	623	437	0.04%	0.005%
88	14.109	2134	2136	2137	rBV2	402	318	0.03%	0.004%
89	14.249	2157	2159	2161	rBV2	394	310	0.03%	0.004%
90	14.310	2166	2169	2170	rBV2	336	402	0.04%	0.005%
91	14.371	2176	2179	2180	rVB2	571	487	0.05%	0.006%
92	14.408	2183	2185	2190	rVB2	813	920	0.09%	0.011%
93	14.451	2190	2192	2194	rBV2	679	714	0.07%	0.009%
94	14.627	2218	2221	2224	rBV2	584	982	0.10%	0.012%
95	14.676	2227	2229	2230	rBV2	663	451	0.04%	0.006%
96	15.194	2311	2314	2315	rBV2	802	721	0.07%	0.009%
97	15.792	2410	2412	2413	rBV2	681	451	0.04%	0.006%
98	16.054	2453	2455	2457	rVV3	630	348	0.03%	0.004%
99	16.097	2460	2462	2465	rBV2	604	540	0.05%	0.007%
100	16.353	2502	2504	2507	rBV	775	845	0.08%	0.011%



Sum of corrected areas: 8002858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030492.D
Acq On : 07 Aug 2022 02:53
Operator : JC/MD
Sample : VIBLK656
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK656

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

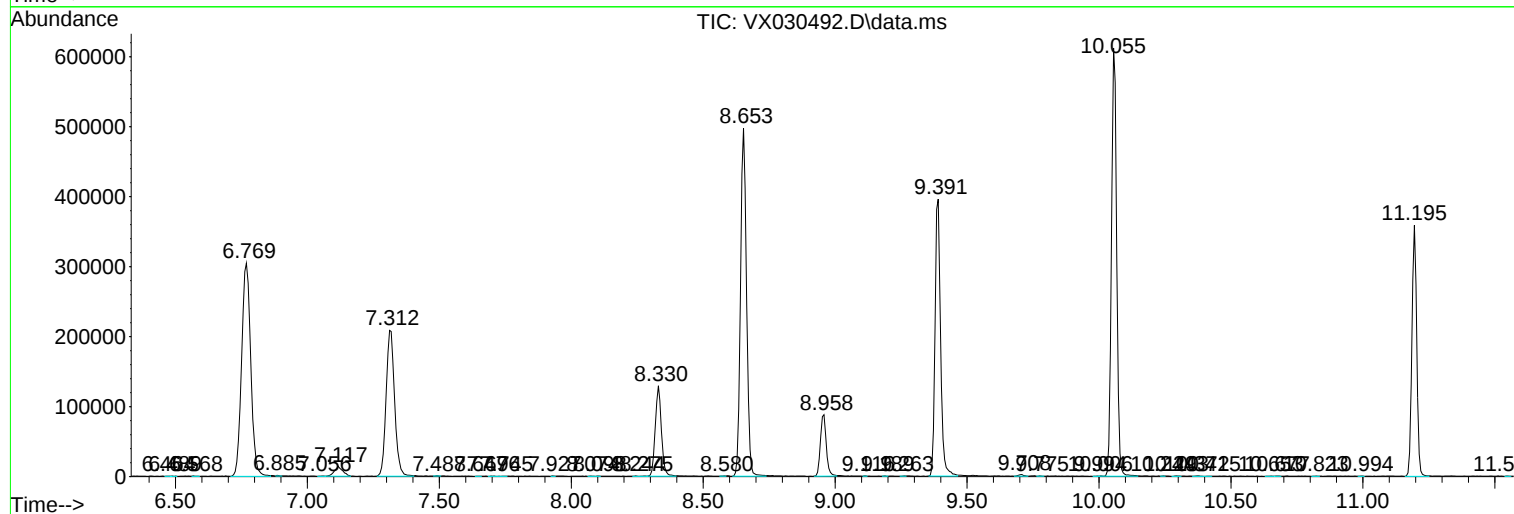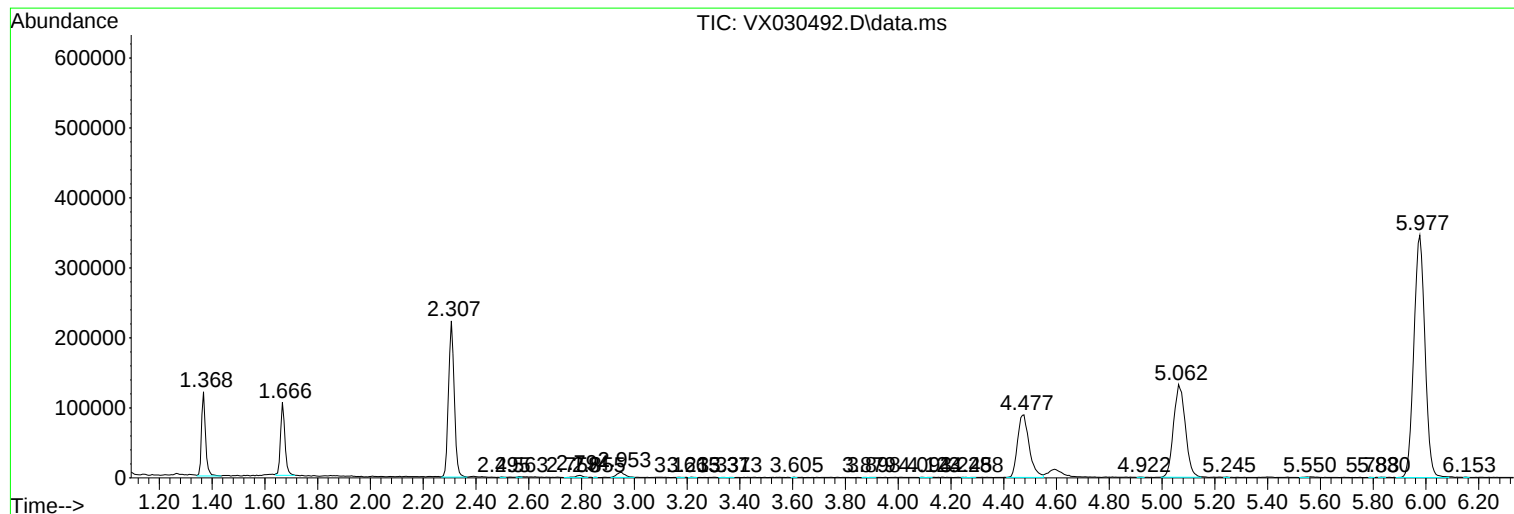

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030492.D
Acq On : 07 Aug 2022 02:53
Operator : JC/MD
Sample : VIBLK656
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK656

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030492.D
Acq On : 07 Aug 2022 02:53
Operator : JC/MD
Sample : VIBLK656
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK656

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------