

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030494.D
 Acq On : 07 Aug 2022 03:39
 Operator : JC/MD
 Sample : VIBLK657
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	52	rVB	117035	119697	12.31%	1.618%
2	1.666	91	95	104	rVB	96670	117269	12.06%	1.585%
3	2.306	194	200	210	rVB	181975	284654	29.28%	3.848%
4	2.428	219	220	222	rBV	668	529	0.05%	0.007%
5	2.508	230	233	237	rVB2	770	850	0.09%	0.011%
6	2.569	240	243	244	rBV2	836	918	0.09%	0.012%
7	2.788	273	279	287	rBV5	2672	5513	0.57%	0.075%
8	2.898	295	297	299	rBV2	534	543	0.06%	0.007%
9	2.947	299	305	314	rVB2	8561	20219	2.08%	0.273%
10	3.093	326	329	334	rVV3	825	1180	0.12%	0.016%
11	3.130	334	335	339	rVB2	377	385	0.04%	0.005%
12	3.318	361	366	367	rBV	357	429	0.04%	0.006%
13	3.471	386	391	395	rBV2	412	669	0.07%	0.009%
14	3.538	400	402	405	rBV2	305	380	0.04%	0.005%
15	3.983	469	475	476	rVB2	462	612	0.06%	0.008%
16	4.001	476	478	479	rBV2	410	362	0.04%	0.005%
17	4.178	504	507	508	rVV	435	335	0.03%	0.005%
18	4.282	520	524	526	rBV2	464	667	0.07%	0.009%
19	4.330	530	532	535	rBV2	304	348	0.04%	0.005%
20	4.471	546	555	568	rBV	94255	274436	28.23%	3.710%
21	4.715	594	595	599	rBV4	591	477	0.05%	0.006%
22	4.794	607	608	612	rBB2	405	344	0.04%	0.005%
23	5.062	640	652	669	rBV	133693	401447	41.30%	5.427%
24	5.367	700	702	705	rVV3	574	725	0.07%	0.010%
25	5.391	705	706	712	rVB3	703	1003	0.10%	0.014%
26	5.550	726	732	733	rBV4	618	1148	0.12%	0.016%
27	5.708	755	758	761	rBV	402	508	0.05%	0.007%
28	5.830	777	778	782	rBV2	347	412	0.04%	0.006%
29	5.873	782	785	790	rBV2	523	661	0.07%	0.009%
30	5.977	790	802	821	rBV3	326300	972109	100.00%	13.141%
31	6.245	842	846	847	rVB	465	511	0.05%	0.007%
32	6.342	859	862	863	rBV2	669	533	0.05%	0.007%
33	6.361	863	865	868	rVB4	723	710	0.07%	0.010%
34	6.452	877	880	883	rVB2	552	497	0.05%	0.007%
35	6.635	907	910	913	rBV2	401	566	0.06%	0.008%
36	6.769	921	932	943	rBV	266923	645475	66.40%	8.725%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030494.D
 Acq On : 07 Aug 2022 03:39
 Operator : JC/MD
 Sample : VIBLK657
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.117	981	989	998	rBV3	11226	27203	2.80%	0.368%
38	7.312	1011	1021	1033	rBV	201985	452011	46.50%	6.110%
39	7.464	1044	1046	1047	rBV2	371	363	0.04%	0.005%
40	7.696	1082	1084	1086	rVV	496	370	0.04%	0.005%
41	7.940	1123	1124	1127	rBV2	571	509	0.05%	0.007%
42	8.043	1140	1141	1144	rBV	418	377	0.04%	0.005%
43	8.080	1146	1147	1150	rVB2	441	359	0.04%	0.005%
44	8.135	1153	1156	1157	rVB2	551	407	0.04%	0.006%
45	8.330	1179	1188	1198	rBV	122722	202751	20.86%	2.741%
46	8.500	1212	1216	1217	rVB2	455	475	0.05%	0.006%
47	8.592	1226	1231	1233	rBV2	995	1222	0.13%	0.017%
48	8.653	1234	1241	1255	rBV	451814	710290	73.07%	9.601%
49	8.842	1269	1272	1273	rBV2	472	429	0.04%	0.006%
50	8.860	1273	1275	1277	rBV2	304	330	0.03%	0.004%
51	8.952	1285	1290	1300	rBV	84222	131290	13.51%	1.775%
52	9.256	1336	1340	1341	rBV2	531	552	0.06%	0.007%
53	9.391	1355	1362	1377	rBV	400072	581915	59.86%	7.866%
54	9.525	1382	1384	1387	rBV2	797	972	0.10%	0.013%
55	9.665	1406	1407	1409	rVB2	505	360	0.04%	0.005%
56	9.708	1409	1414	1418	rBV3	3369	5535	0.57%	0.075%
57	9.878	1439	1442	1443	rVB	455	410	0.04%	0.006%
58	9.903	1443	1446	1448	rBV2	287	405	0.04%	0.005%
59	9.976	1455	1458	1459	rVB	484	441	0.05%	0.006%
60	10.055	1465	1471	1482	rBV	536449	734199	75.53%	9.925%
61	10.616	1561	1563	1565	rVB2	384	390	0.04%	0.005%
62	10.646	1565	1568	1570	rBV2	369	424	0.04%	0.006%
63	10.902	1607	1610	1612	rVB2	349	427	0.04%	0.006%
64	10.927	1612	1614	1620	rVB	597	919	0.09%	0.012%
65	11.195	1652	1658	1665	rBV	359246	453242	46.62%	6.127%
66	11.274	1670	1671	1676	rVV2	494	658	0.07%	0.009%
67	11.341	1679	1682	1685	rBV2	315	414	0.04%	0.006%
68	11.427	1694	1696	1698	rBV	452	400	0.04%	0.005%
69	11.604	1721	1725	1727	rBV2	447	591	0.06%	0.008%
70	11.713	1738	1743	1745	rBV2	316	536	0.06%	0.007%
71	11.774	1751	1753	1755	rBV2	463	385	0.04%	0.005%
72	11.829	1760	1762	1766	rVB2	496	512	0.05%	0.007%
73	11.866	1766	1768	1771	rVB2	489	493	0.05%	0.007%
74	11.951	1780	1782	1785	rBV2	433	512	0.05%	0.007%
75	12.024	1789	1794	1802	rBV	514331	614514	63.21%	8.307%
76	12.244	1828	1830	1831	rBV2	545	357	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030494.D
 Acq On : 07 Aug 2022 03:39
 Operator : JC/MD
 Sample : VIBLK657
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK657

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1850	rBV	488226	601099	61.83%	8.125%
78	12.628	1892	1893	1897	rVB2	588	660	0.07%	0.009%
79	12.664	1897	1899	1902	rBV2	334	488	0.05%	0.007%
80	12.719	1907	1908	1910	rVV	599	378	0.04%	0.005%
81	13.030	1958	1959	1961	rVB	653	426	0.04%	0.006%
82	13.682	2064	2066	2071	rVB2	736	956	0.10%	0.013%
83	13.792	2082	2084	2086	rBV2	521	456	0.05%	0.006%
84	13.835	2088	2091	2094	rBV2	367	328	0.03%	0.004%
85	14.030	2122	2123	2126	rBV	327	353	0.04%	0.005%
86	14.128	2137	2139	2140	rBV	426	432	0.04%	0.006%
87	14.170	2144	2146	2149	rVV2	396	405	0.04%	0.005%
88	14.353	2175	2176	2178	rBV2	513	356	0.04%	0.005%
89	14.603	2215	2217	2221	rBV2	578	545	0.06%	0.007%
90	14.816	2248	2252	2254	rVB2	453	543	0.06%	0.007%
91	14.841	2254	2256	2257	rBV	617	339	0.03%	0.005%
92	15.310	2331	2333	2336	rVB2	863	681	0.07%	0.009%
93	15.359	2340	2341	2343	rVB2	502	357	0.04%	0.005%
94	15.566	2372	2375	2377	rBV3	791	902	0.09%	0.012%
95	15.804	2413	2414	2417	rVB2	730	576	0.06%	0.008%
96	15.950	2436	2438	2441	rBV2	681	857	0.09%	0.012%
97	15.993	2444	2445	2446	rBV	774	411	0.04%	0.006%
98	16.103	2462	2463	2466	rVB2	534	382	0.04%	0.005%
99	16.133	2466	2468	2469	rBV2	471	354	0.04%	0.005%
100	16.402	2510	2512	2513	rBV2	700	411	0.04%	0.006%




Sum of corrected areas: 7397765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030494.D
Acq On : 07 Aug 2022 03:39
Operator : JC/MD
Sample : VIBLK657
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK657

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

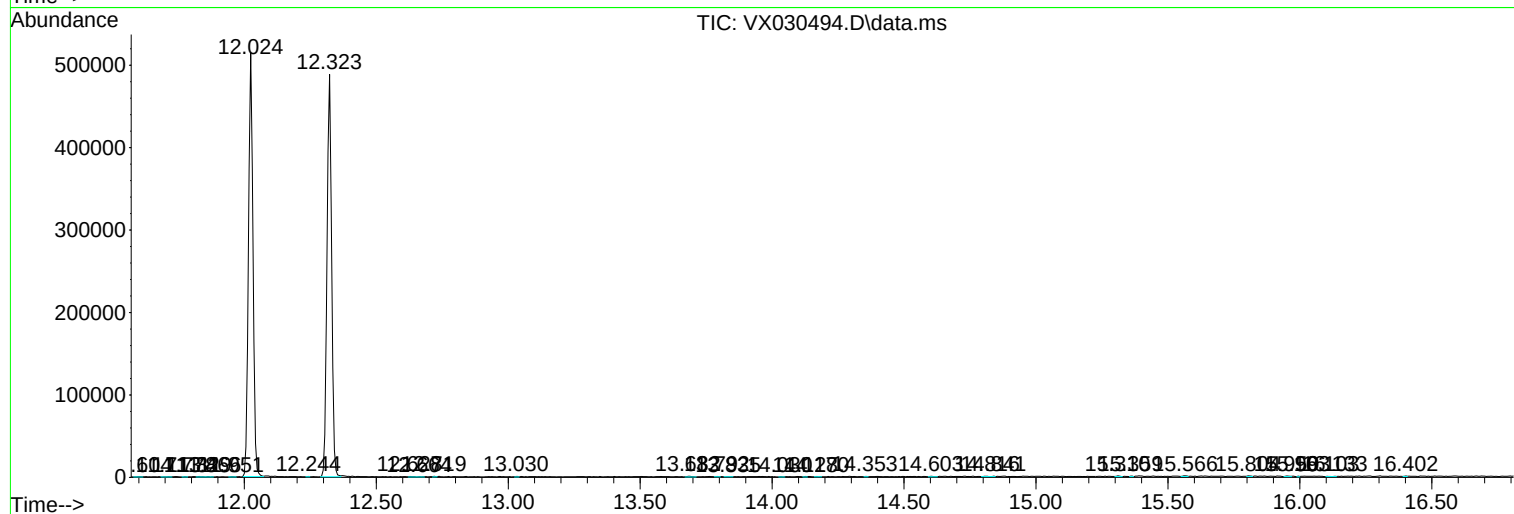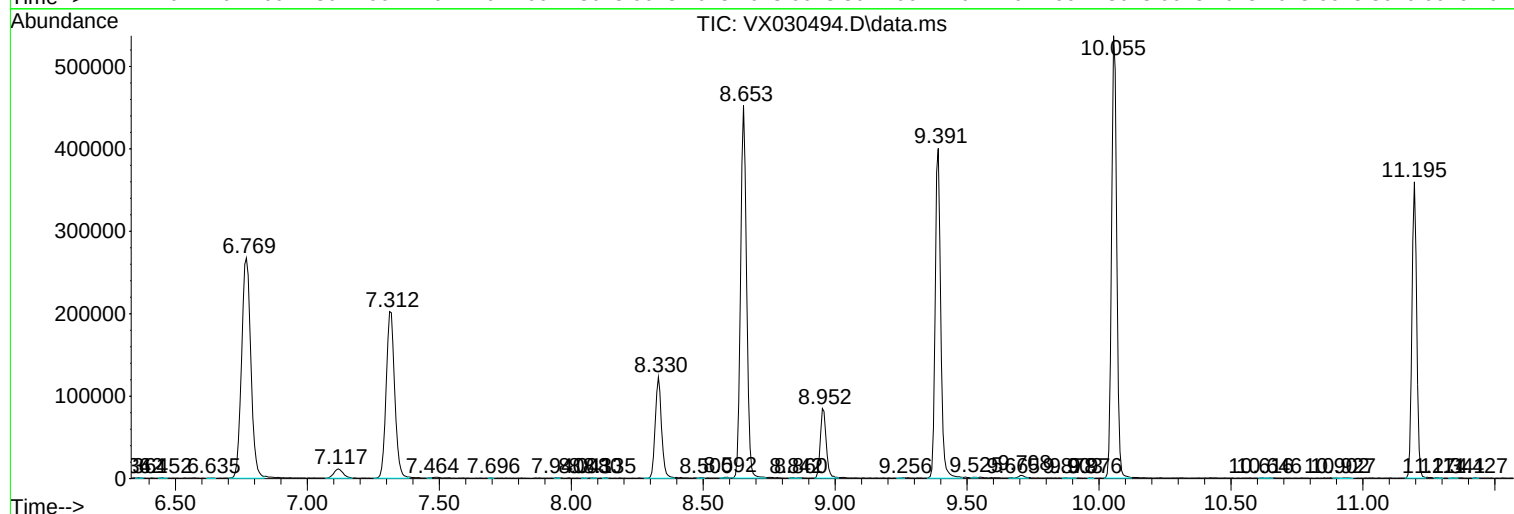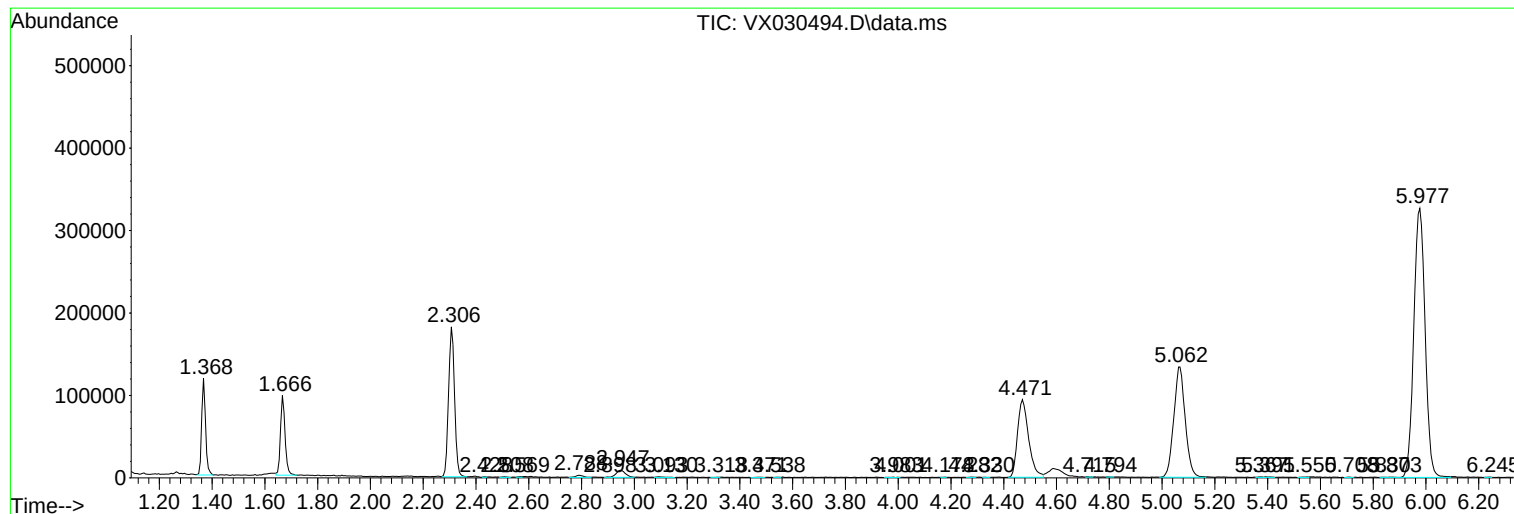

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030494.D
Acq On : 07 Aug 2022 03:39
Operator : JC/MD
Sample : VIBLK657
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK657

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030494.D
Acq On : 07 Aug 2022 03:39
Operator : JC/MD
Sample : VIBLK657
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK657

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc