

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030495.D
 Acq On : 07 Aug 2022 04:03
 Operator : JC/MD
 Sample : N4021-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	42	47	59	rVB2	361182	413511	5.23%	2.602%
2	1.666	91	95	103	rVB	95334	112762	1.43%	0.710%
3	1.746	106	108	116	rVB	8344	10372	0.13%	0.065%
4	2.306	194	200	210	rBV	210491	325525	4.11%	2.049%
5	2.392	210	214	218	rBV	5025	7173	0.09%	0.045%
6	2.526	231	236	239	rBV3	774	1582	0.02%	0.010%
7	2.867	286	292	298	rVB5	2410	4984	0.06%	0.031%
8	3.093	321	329	343	rBV	45141	95962	1.21%	0.604%
9	3.276	357	359	364	rVB2	333	522	0.01%	0.003%
10	3.422	380	383	385	rVB	428	439	0.01%	0.003%
11	3.465	385	390	392	rBV2	655	870	0.01%	0.005%
12	3.587	406	410	414	rVV2	578	648	0.01%	0.004%
13	3.727	431	433	435	rVV	431	355	0.00%	0.002%
14	3.788	439	443	447	rBV2	299	513	0.01%	0.003%
15	3.849	451	453	455	rVB2	440	390	0.00%	0.002%
16	4.306	520	528	536	rBV5	2487	6651	0.08%	0.042%
17	4.495	545	559	582	rBV	2816251	7912308	100.00%	49.794%
18	5.068	641	653	671	rVB	122155	405417	5.12%	2.551%
19	5.221	677	678	681	rVB3	729	524	0.01%	0.003%
20	5.294	689	690	694	rVB	684	686	0.01%	0.004%
21	5.385	704	705	707	rBV2	454	372	0.00%	0.002%
22	5.477	715	720	726	rVB7	2308	5416	0.07%	0.034%
23	5.714	756	759	763	rBV3	586	806	0.01%	0.005%
24	5.763	763	767	768	rBV2	467	694	0.01%	0.004%
25	5.977	789	802	820	rBV2	341513	1005997	12.71%	6.331%
26	6.190	834	837	839	rBV3	535	396	0.01%	0.002%
27	6.342	860	862	864	rVB2	539	443	0.01%	0.003%
28	6.367	864	866	869	rBV2	575	805	0.01%	0.005%
29	6.483	883	885	888	rVB2	535	521	0.01%	0.003%
30	6.531	888	893	894	rBV2	477	637	0.01%	0.004%
31	6.550	894	896	898	rVV3	449	366	0.00%	0.002%
32	6.629	906	909	910	rBV	529	508	0.01%	0.003%
33	6.769	922	932	947	rBV	280839	670480	8.47%	4.219%
34	6.921	955	957	958	rBV	559	364	0.00%	0.002%
35	6.940	958	960	963	rVB2	795	705	0.01%	0.004%
36	6.964	963	964	967	rVB3	701	534	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030495.D
 Acq On : 07 Aug 2022 04:03
 Operator : JC/MD
 Sample : N4021-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.129	979	991	1006	rBV2	74929	187589	2.37%	1.181%
38	7.312	1011	1021	1036	rBV	204357	460827	5.82%	2.900%
39	7.616	1069	1071	1073	rVB2	441	436	0.01%	0.003%
40	7.653	1073	1077	1080	rBV2	511	692	0.01%	0.004%
41	7.738	1089	1091	1094	rVB	635	460	0.01%	0.003%
42	7.946	1122	1125	1130	rVB3	533	925	0.01%	0.006%
43	7.988	1130	1132	1135	rVB2	324	328	0.00%	0.002%
44	8.025	1135	1138	1142	rVB2	641	860	0.01%	0.005%
45	8.153	1157	1159	1163	rVV2	409	442	0.01%	0.003%
46	8.330	1181	1188	1198	rBV	128431	205181	2.59%	1.291%
47	8.580	1225	1229	1234	rBV4	3241	5494	0.07%	0.035%
48	8.653	1234	1241	1251	rBV	504103	775022	9.80%	4.877%
49	8.952	1285	1290	1301	rBV	88337	134802	1.70%	0.848%
50	9.086	1308	1312	1314	rBV2	453	485	0.01%	0.003%
51	9.244	1335	1338	1339	rBV	619	453	0.01%	0.003%
52	9.275	1339	1343	1350	rVB3	6504	10172	0.13%	0.064%
53	9.391	1356	1362	1380	rBV	374217	550452	6.96%	3.464%
54	9.531	1383	1385	1390	rVV4	1428	1793	0.02%	0.011%
55	9.701	1411	1413	1414	rBV	486	436	0.01%	0.003%
56	9.756	1418	1422	1424	rBV2	606	912	0.01%	0.006%
57	9.799	1427	1429	1430	rBV	495	311	0.00%	0.002%
58	9.933	1449	1451	1453	rVB3	597	635	0.01%	0.004%
59	10.055	1465	1471	1486	rBV	580436	793807	10.03%	4.996%
60	10.177	1489	1491	1492	rBV2	406	391	0.00%	0.002%
61	10.244	1500	1502	1503	rBV2	451	367	0.00%	0.002%
62	10.299	1510	1511	1514	rBV2	399	536	0.01%	0.003%
63	10.348	1517	1519	1522	rVB3	494	479	0.01%	0.003%
64	10.439	1531	1534	1535	rBV2	471	486	0.01%	0.003%
65	10.646	1564	1568	1569	rBV	487	413	0.01%	0.003%
66	10.793	1587	1592	1593	rBV2	473	672	0.01%	0.004%
67	11.134	1647	1648	1650	rVB2	732	376	0.00%	0.002%
68	11.195	1653	1658	1668	rVB	312362	401930	5.08%	2.529%
69	11.408	1691	1693	1695	rBV2	365	421	0.01%	0.003%
70	11.750	1747	1749	1750	rBV	390	313	0.00%	0.002%
71	12.024	1788	1794	1808	rBV	589489	709473	8.97%	4.465%
72	12.225	1824	1827	1832	rVB3	1433	1739	0.02%	0.011%
73	12.323	1838	1843	1849	rBV	523254	635173	8.03%	3.997%
74	12.750	1911	1913	1917	rVV2	682	701	0.01%	0.004%
75	12.939	1941	1944	1945	rBV	352	401	0.01%	0.003%
76	13.024	1956	1958	1960	rBV2	486	516	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030495.D
 Acq On : 07 Aug 2022 04:03
 Operator : JC/MD
 Sample : N4021-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5D68

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.103	1968	1971	1973	rBV2	558	693	0.01%	0.004%
78	13.152	1978	1979	1983	rBV2	582	518	0.01%	0.003%
79	13.213	1986	1989	1990	rBV	405	428	0.01%	0.003%
80	13.396	2017	2019	2020	rBV	439	381	0.00%	0.002%
81	13.414	2020	2022	2025	rVB2	520	541	0.01%	0.003%
82	13.439	2025	2026	2032	rBV3	415	766	0.01%	0.005%
83	13.579	2046	2049	2050	rBV3	604	598	0.01%	0.004%
84	13.646	2059	2060	2063	rBV2	402	312	0.00%	0.002%
85	13.762	2075	2079	2080	rBV2	406	418	0.01%	0.003%
86	13.999	2116	2118	2121	rBV2	472	569	0.01%	0.004%
87	14.085	2131	2132	2136	rBV2	335	369	0.00%	0.002%
88	14.292	2164	2166	2171	rBV3	582	765	0.01%	0.005%
89	14.335	2171	2173	2175	rBV2	395	338	0.00%	0.002%
90	14.384	2179	2181	2182	rBV2	541	478	0.01%	0.003%
91	14.438	2188	2190	2191	rBV	347	325	0.00%	0.002%
92	14.682	2228	2230	2231	rBV2	495	389	0.00%	0.002%
93	14.981	2277	2279	2282	rBV2	688	767	0.01%	0.005%
94	15.072	2292	2294	2298	rBV4	613	790	0.01%	0.005%
95	15.286	2327	2329	2330	rBV	789	456	0.01%	0.003%
96	15.627	2383	2385	2388	rBV3	700	824	0.01%	0.005%
97	15.652	2388	2389	2391	rVV	651	313	0.00%	0.002%
98	15.816	2413	2416	2419	rBV3	705	1028	0.01%	0.006%
99	16.066	2455	2457	2458	rBV2	483	397	0.01%	0.002%
100	16.554	2535	2537	2540	rBV2	526	484	0.01%	0.003%




Sum of corrected areas: 15890086

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030495.D
Acq On : 07 Aug 2022 04:03
Operator : JC/MD
Sample : N4021-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

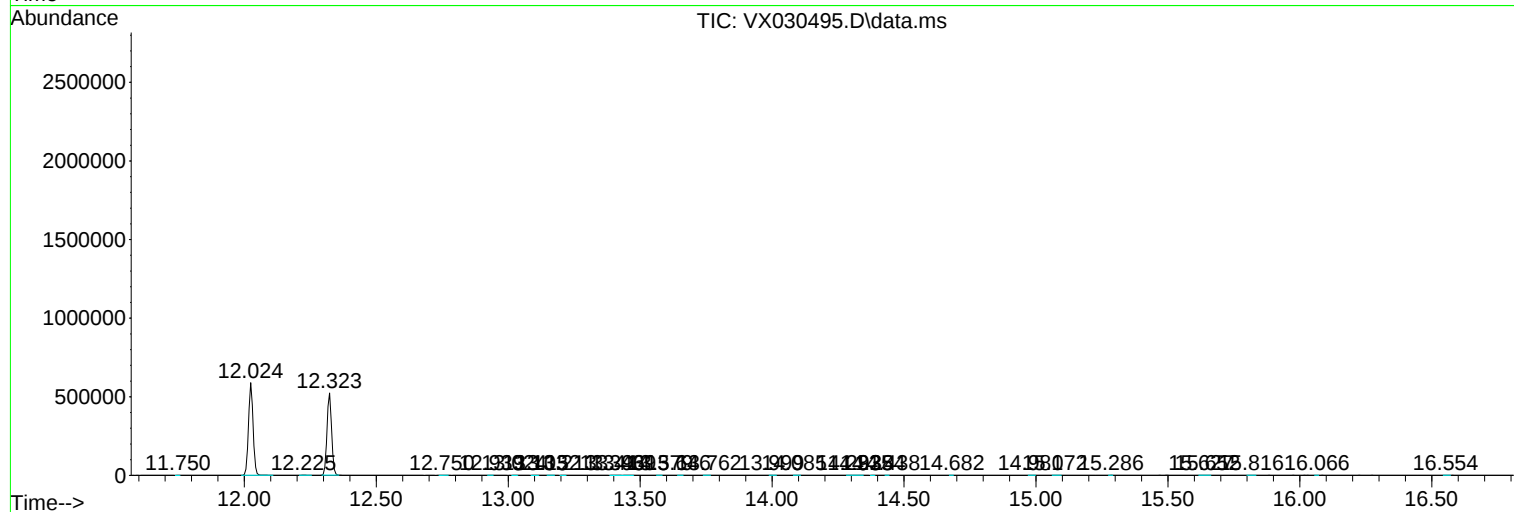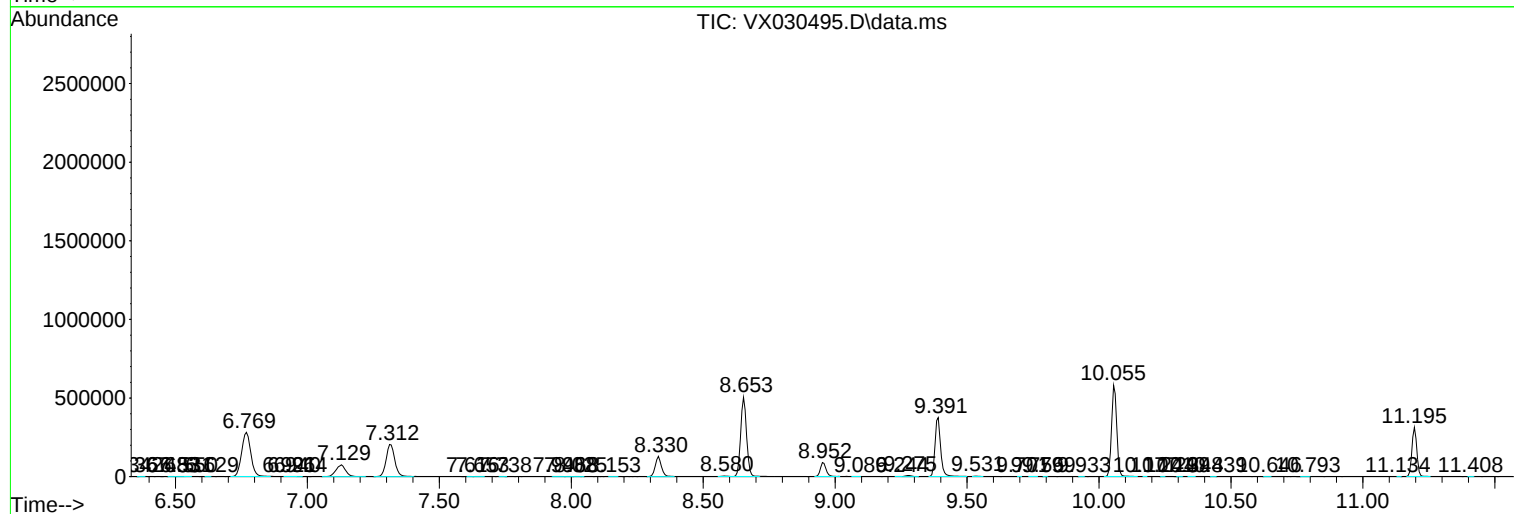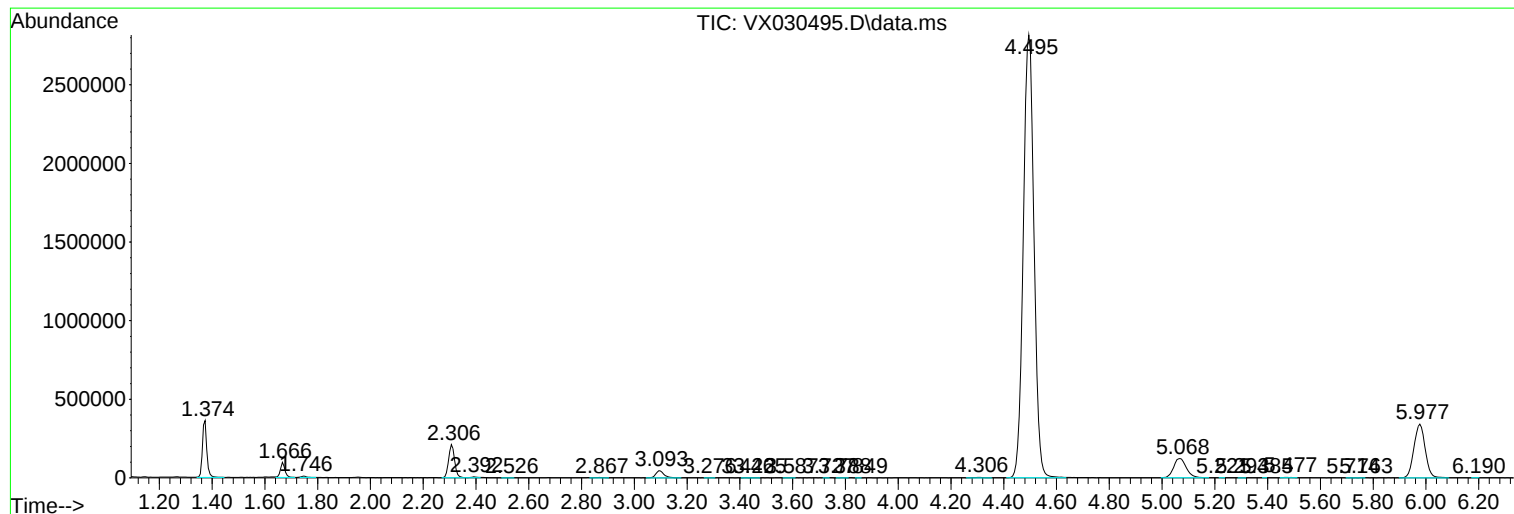

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030495.D
Acq On : 07 Aug 2022 04:03
Operator : JC/MD
Sample : N4021-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030495.D
Acq On : 07 Aug 2022 04:03
Operator : JC/MD
Sample : N4021-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5D68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc