

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030496.D
 Acq On : 07 Aug 2022 04:26
 Operator : JC/MD
 Sample : VIBLK658
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK658

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030496.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB	113443	115461	12.25%	1.585%
2	1.666	91	95	105	rVB	94962	114539	12.15%	1.572%
3	2.118	167	169	171	rBV2	997	947	0.10%	0.013%
4	2.307	194	200	212	rVB	187587	281367	29.85%	3.863%
5	2.398	212	215	219	rBV3	1267	2035	0.22%	0.028%
6	2.508	232	233	236	rBV2	654	402	0.04%	0.006%
7	2.593	246	247	250	rBV	952	507	0.05%	0.007%
8	2.715	265	267	270	rVB3	574	393	0.04%	0.005%
9	2.788	274	279	286	rBV3	3859	7657	0.81%	0.105%
10	2.892	294	296	299	rVB2	479	463	0.05%	0.006%
11	2.947	299	305	312	rBV	6037	12592	1.34%	0.173%
12	3.099	329	330	333	rBV2	690	594	0.06%	0.008%
13	3.136	333	336	339	rVB2	337	424	0.04%	0.006%
14	3.197	342	346	347	rBV	455	476	0.05%	0.007%
15	3.416	377	382	384	rBV	364	544	0.06%	0.007%
16	3.690	425	427	430	rVB2	338	422	0.04%	0.006%
17	3.873	456	457	460	rVB2	501	402	0.04%	0.006%
18	3.940	465	468	470	rBV2	419	433	0.05%	0.006%
19	3.977	472	474	475	rBV	716	401	0.04%	0.006%
20	4.062	486	488	493	rBV	456	531	0.06%	0.007%
21	4.154	500	503	506	rVB2	504	606	0.06%	0.008%
22	4.196	506	510	511	rBV	509	574	0.06%	0.008%
23	4.239	515	517	519	rBV	482	392	0.04%	0.005%
24	4.471	545	555	568	rBV	90799	275615	29.24%	3.784%
25	4.818	610	612	614	rBV2	427	493	0.05%	0.007%
26	4.965	634	636	637	rBV2	653	619	0.07%	0.008%
27	5.068	640	653	669	rVV	120540	387532	41.12%	5.320%
28	5.263	683	685	688	rVB2	490	414	0.04%	0.006%
29	5.318	692	694	697	rVB2	424	417	0.04%	0.006%
30	5.367	700	702	703	rBV2	438	397	0.04%	0.005%
31	5.556	731	733	735	rVV2	807	718	0.08%	0.010%
32	5.653	747	749	751	rVB2	537	383	0.04%	0.005%
33	5.678	751	753	755	rVB2	454	415	0.04%	0.006%
34	5.977	789	802	819	rBV2	322561	942513	100.00%	12.939%
35	6.141	827	829	833	rVB2	726	656	0.07%	0.009%
36	6.684	916	918	921	rBV2	413	516	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030496.D
 Acq On : 07 Aug 2022 04:26
 Operator : JC/MD
 Sample : VIBLK658
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK658

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.769	922	932	946	rBV	271388	646649	68.61%	8.877%
38	6.989	966	968	970	rBV3	370	395	0.04%	0.005%
39	7.031	973	975	976	rBV	474	448	0.05%	0.006%
40	7.117	982	989	999	rVB6	11395	27617	2.93%	0.379%
41	7.226	1005	1007	1008	rBV	563	397	0.04%	0.005%
42	7.312	1012	1021	1034	rBV	197988	437594	46.43%	6.007%
43	7.946	1123	1125	1130	rVB2	735	750	0.08%	0.010%
44	8.251	1172	1175	1176	rVB2	449	385	0.04%	0.005%
45	8.330	1182	1188	1199	rBV	114998	191092	20.27%	2.623%
46	8.586	1225	1230	1234	rBV4	744	1271	0.13%	0.017%
47	8.653	1234	1241	1254	rBV	451164	696692	73.92%	9.564%
48	8.952	1285	1290	1301	rBV	82666	125227	13.29%	1.719%
49	9.177	1322	1327	1330	rVB3	606	935	0.10%	0.013%
50	9.208	1330	1332	1335	rVB2	521	418	0.04%	0.006%
51	9.244	1335	1338	1340	rBV	332	469	0.05%	0.006%
52	9.275	1340	1343	1347	rBV3	580	878	0.09%	0.012%
53	9.391	1356	1362	1374	rBV	384584	561473	59.57%	7.708%
54	9.702	1410	1413	1417	rVV3	3043	4231	0.45%	0.058%
55	9.787	1425	1427	1432	rBV2	409	489	0.05%	0.007%
56	10.055	1465	1471	1479	rBV	569126	754997	80.10%	10.364%
57	10.220	1496	1498	1500	rBV2	573	417	0.04%	0.006%
58	10.287	1507	1509	1514	rVV2	332	399	0.04%	0.005%
59	10.403	1523	1528	1531	rBV2	403	489	0.05%	0.007%
60	10.482	1539	1541	1543	rBV2	334	381	0.04%	0.005%
61	10.628	1563	1565	1568	rBV2	416	417	0.04%	0.006%
62	10.781	1588	1590	1595	rVB2	469	670	0.07%	0.009%
63	10.829	1595	1598	1599	rBV2	463	427	0.05%	0.006%
64	10.951	1615	1618	1622	rVB	508	531	0.06%	0.007%
65	11.195	1652	1658	1666	rVV	342564	435251	46.18%	5.975%
66	11.372	1686	1687	1691	rVB2	369	387	0.04%	0.005%
67	11.476	1701	1704	1705	rVV	875	703	0.07%	0.010%
68	11.732	1744	1746	1750	rVB2	387	416	0.04%	0.006%
69	11.762	1750	1751	1754	rBV2	429	393	0.04%	0.005%
70	11.927	1776	1778	1782	rBV2	333	398	0.04%	0.005%
71	12.024	1789	1794	1803	rBV	539022	647258	68.67%	8.885%
72	12.110	1806	1808	1810	rBV	461	553	0.06%	0.008%
73	12.177	1815	1819	1820	rBV	507	550	0.06%	0.008%
74	12.268	1831	1834	1836	rBV2	406	412	0.04%	0.006%
75	12.323	1837	1843	1850	rVV	453741	576046	61.12%	7.908%
76	12.439	1861	1862	1864	rBV	595	382	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030496.D
 Acq On : 07 Aug 2022 04:26
 Operator : JC/MD
 Sample : VIBLK658
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK658

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.536	1874	1878	1879	rBV3	342	440	0.05%	0.006%
78	12.597	1885	1888	1890	rBV	592	444	0.05%	0.006%
79	12.731	1906	1910	1911	rBV	418	466	0.05%	0.006%
80	12.762	1913	1915	1918	rVB	594	551	0.06%	0.008%
81	12.841	1925	1928	1929	rBV	437	493	0.05%	0.007%
82	12.902	1936	1938	1942	rBV2	538	548	0.06%	0.008%
83	12.939	1942	1944	1947	rVB2	557	642	0.07%	0.009%
84	13.268	1995	1998	2000	rBV2	409	507	0.05%	0.007%
85	13.366	2012	2014	2017	rBV2	496	473	0.05%	0.006%
86	13.554	2043	2045	2049	rBV2	470	534	0.06%	0.007%
87	13.591	2049	2051	2055	rBV	564	679	0.07%	0.009%
88	13.683	2065	2066	2068	rBV	507	423	0.04%	0.006%
89	13.841	2090	2092	2095	rBV2	541	499	0.05%	0.007%
90	13.939	2106	2108	2111	rBV	300	424	0.04%	0.006%
91	13.993	2114	2117	2118	rBV	408	460	0.05%	0.006%
92	14.128	2137	2139	2142	rVB	722	614	0.07%	0.008%
93	14.170	2144	2146	2147	rBV	480	392	0.04%	0.005%
94	14.359	2175	2177	2178	rBV	527	391	0.04%	0.005%
95	14.481	2193	2197	2199	rBV	463	675	0.07%	0.009%
96	14.585	2211	2214	2217	rBV2	444	742	0.08%	0.010%
97	14.786	2245	2247	2248	rBV2	537	566	0.06%	0.008%
98	16.005	2445	2447	2449	rVB3	609	559	0.06%	0.008%
99	16.030	2449	2451	2454	rBV3	588	790	0.08%	0.011%
100	16.322	2497	2499	2501	rBV2	524	405	0.04%	0.006%

Sum of corrected areas: 7284454




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030496.D
Acq On : 07 Aug 2022 04:26
Operator : JC/MD
Sample : VIBLK658
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK658

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

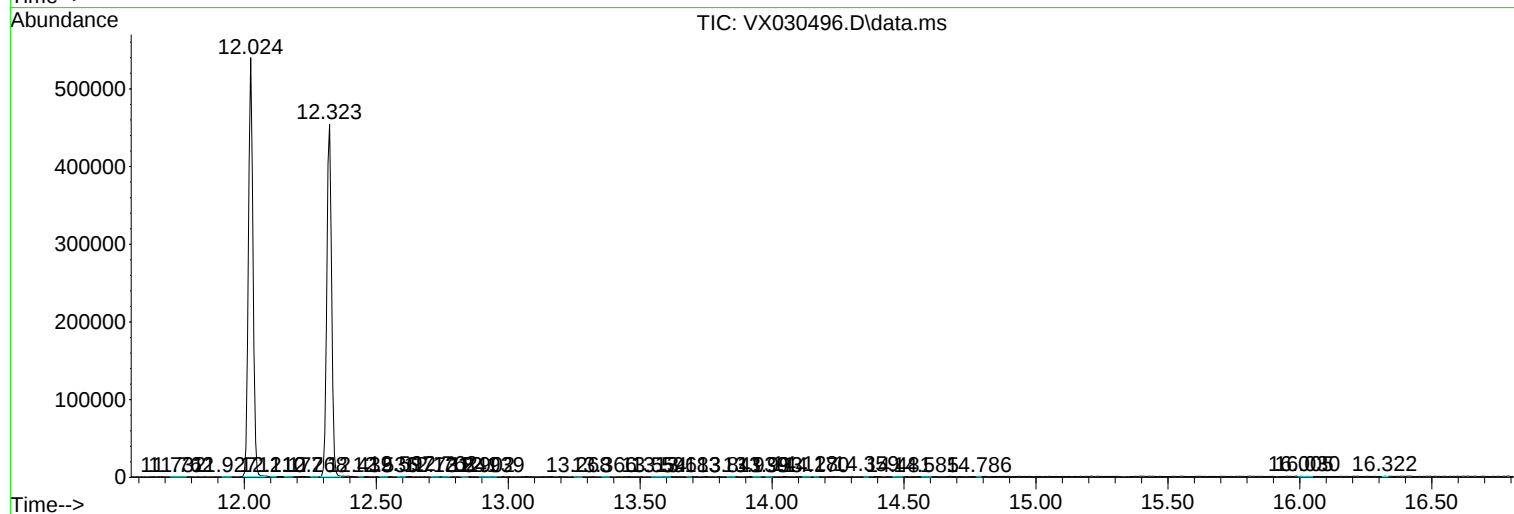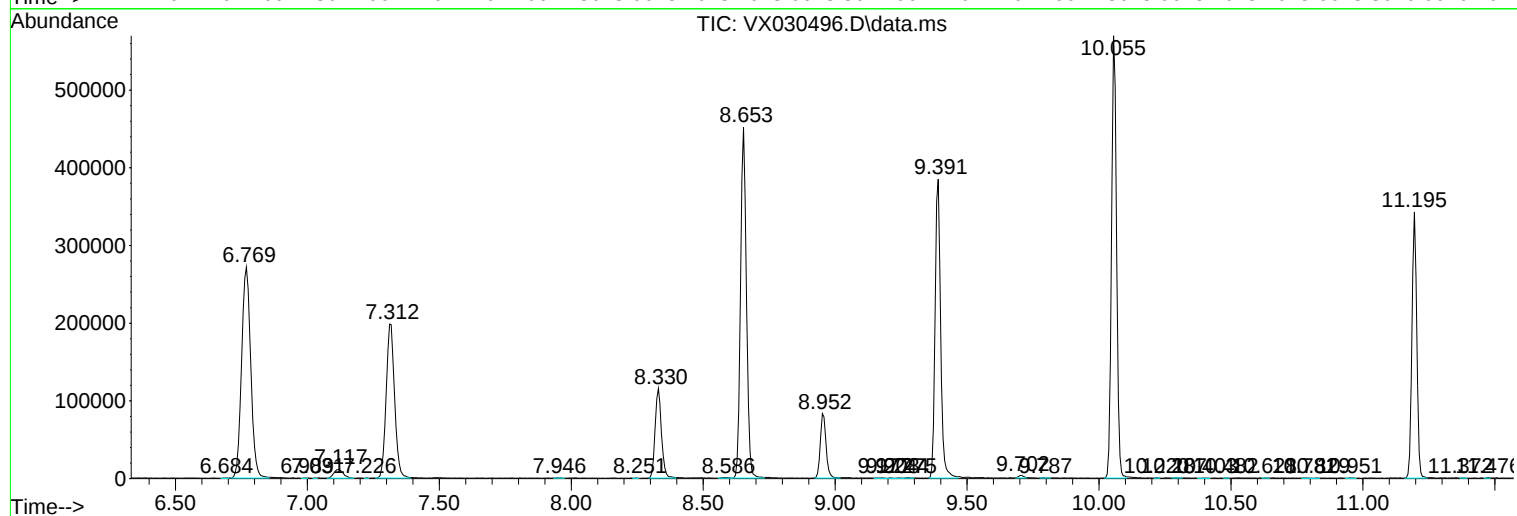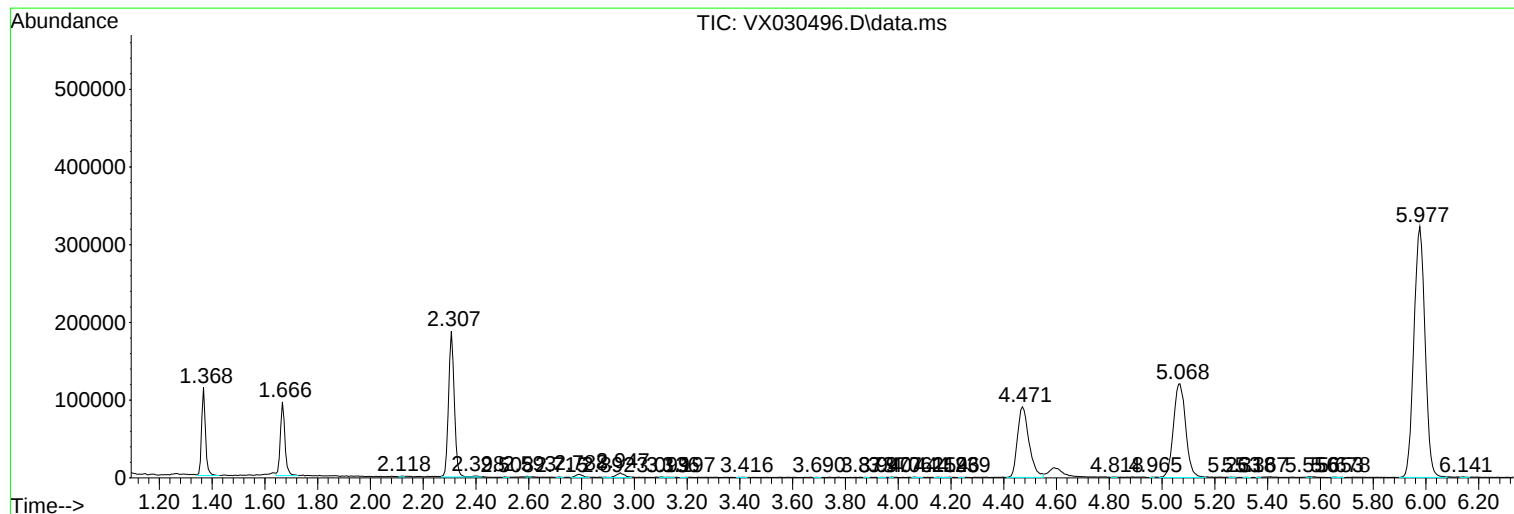

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030496.D
Acq On : 07 Aug 2022 04:26
Operator : JC/MD
Sample : VIBLK658
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK658

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030496.D
Acq On : 07 Aug 2022 04:26
Operator : JC/MD
Sample : VIBLK658
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK658

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc