

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030497.D
 Acq On : 07 Aug 2022 04:50
 Operator : JC/MD
 Sample : N4021-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030497.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	59	rVB2	698820	779749	4.48%	2.278%
2	1.666	91	95	104	rVB	96928	118569	0.68%	0.346%
3	2.306	194	200	211	rVB	218606	329425	1.89%	0.962%
4	2.502	229	232	233	rBV	417	431	0.00%	0.001%
5	2.538	236	238	240	rBV3	514	396	0.00%	0.001%
6	2.575	242	244	245	rBV	517	398	0.00%	0.001%
7	2.739	267	271	273	rBV	471	504	0.00%	0.001%
8	2.788	278	279	282	rVV	475	600	0.00%	0.002%
9	2.904	296	298	303	rVB2	510	595	0.00%	0.002%
10	2.947	303	305	311	rVB2	443	562	0.00%	0.002%
11	3.008	313	315	320	rVB2	370	406	0.00%	0.001%
12	3.093	320	329	341	rBV	87744	170817	0.98%	0.499%
13	3.258	353	356	359	rBV	388	539	0.00%	0.002%
14	3.806	444	446	449	rVV2	344	385	0.00%	0.001%
15	3.873	455	457	460	rVV	434	473	0.00%	0.001%
16	3.995	471	477	479	rVV2	394	844	0.00%	0.002%
17	4.306	524	528	530	rBV2	324	486	0.00%	0.001%
18	4.495	543	559	580	rBV	2425660	6809934	39.13%	19.893%
19	4.861	618	619	622	rBV2	529	501	0.00%	0.001%
20	5.068	637	653	668	rBV	129799	416141	2.39%	1.216%
21	5.227	676	679	680	rBV2	762	527	0.00%	0.002%
22	5.385	702	705	706	rBV	595	548	0.00%	0.002%
23	5.489	719	722	724	rBV2	546	738	0.00%	0.002%
24	5.647	745	748	751	rVB2	460	569	0.00%	0.002%
25	5.812	773	775	777	rBV2	393	422	0.00%	0.001%
26	5.977	787	802	819	rBV2	339908	1009398	5.80%	2.949%
27	6.208	838	840	846	rBV	423	745	0.00%	0.002%
28	6.263	846	849	851	rBB	624	392	0.00%	0.001%
29	6.330	858	860	864	rBV2	504	733	0.00%	0.002%
30	6.470	880	883	886	rBV3	387	431	0.00%	0.001%
31	6.556	894	897	899	rBV	413	416	0.00%	0.001%
32	6.635	907	910	913	rBV2	598	748	0.00%	0.002%
33	6.769	923	932	946	rBV	287761	693368	3.98%	2.025%
34	6.897	951	953	955	rVV2	839	765	0.00%	0.002%
35	6.946	959	961	962	rVB2	747	462	0.00%	0.001%
36	7.135	981	992	1013	rBV	8181113	17404722	100.00%	50.841%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030497.D
 Acq On : 07 Aug 2022 04:50
 Operator : JC/MD
 Sample : N4021-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.318	1014	1022	1034	rVB	209968	462604	2.66%	1.351%
38	7.653	1075	1077	1083	rVB3	508	774	0.00%	0.002%
39	7.757	1092	1094	1096	rBV3	577	736	0.00%	0.002%
40	7.836	1105	1107	1110	rBV3	534	533	0.00%	0.002%
41	8.007	1132	1135	1138	rBV2	464	697	0.00%	0.002%
42	8.037	1138	1140	1143	rVV2	551	686	0.00%	0.002%
43	8.080	1145	1147	1151	rVB2	826	900	0.01%	0.003%
44	8.116	1151	1153	1155	rBV2	452	455	0.00%	0.001%
45	8.244	1172	1174	1177	rBV2	637	618	0.00%	0.002%
46	8.330	1181	1188	1200	rBV	125106	207445	1.19%	0.606%
47	8.507	1214	1217	1219	rBV2	440	437	0.00%	0.001%
48	8.592	1227	1231	1233	rBV2	360	468	0.00%	0.001%
49	8.653	1234	1241	1250	rBV	505516	781017	4.49%	2.281%
50	8.799	1264	1265	1268	rVB	591	470	0.00%	0.001%
51	8.836	1270	1271	1274	rBV2	596	584	0.00%	0.002%
52	8.952	1284	1290	1299	rBV	89248	135118	0.78%	0.395%
53	9.220	1330	1334	1336	rVB3	596	767	0.00%	0.002%
54	9.275	1337	1343	1356	rVV	1141127	1622920	9.32%	4.741%
55	9.391	1356	1362	1374	rBV	386184	567622	3.26%	1.658%
56	9.708	1412	1414	1417	rVB2	494	431	0.00%	0.001%
57	10.055	1465	1471	1488	rVV	613589	826005	4.75%	2.413%
58	10.305	1510	1512	1515	rBV2	321	400	0.00%	0.001%
59	10.372	1520	1523	1526	rVB3	534	742	0.00%	0.002%
60	10.506	1543	1545	1549	rVB2	447	432	0.00%	0.001%
61	10.537	1549	1550	1553	rBV2	326	388	0.00%	0.001%
62	10.604	1560	1561	1565	rVB	491	414	0.00%	0.001%
63	10.646	1565	1568	1569	rBV	499	563	0.00%	0.002%
64	10.866	1602	1604	1608	rVB2	612	650	0.00%	0.002%
65	10.903	1608	1610	1611	rBV	591	409	0.00%	0.001%
66	11.128	1646	1647	1650	rBV	542	420	0.00%	0.001%
67	11.195	1652	1658	1666	rVV	364343	462833	2.66%	1.352%
68	11.482	1703	1705	1708	rBV3	648	657	0.00%	0.002%
69	11.579	1719	1721	1724	rVB	503	400	0.00%	0.001%
70	11.695	1737	1740	1741	rBV2	582	423	0.00%	0.001%
71	11.854	1765	1766	1769	rVB2	612	425	0.00%	0.001%
72	11.896	1769	1773	1774	rBV2	411	396	0.00%	0.001%
73	12.024	1789	1794	1806	rVB	615366	739061	4.25%	2.159%
74	12.232	1827	1828	1831	rVB2	545	426	0.00%	0.001%
75	12.323	1837	1843	1856	rVV	522182	653846	3.76%	1.910%
76	12.427	1858	1860	1864	rVB3	695	590	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030497.D
 Acq On : 07 Aug 2022 04:50
 Operator : JC/MD
 Sample : N4021-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E21

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.579	1883	1885	1888	rVB2	459	414	0.00%	0.001%
78	12.634	1891	1894	1895	rBV	643	485	0.00%	0.001%
79	13.445	2026	2027	2030	rBV2	409	517	0.00%	0.002%
80	13.518	2036	2039	2041	rBV	599	442	0.00%	0.001%
81	13.542	2041	2043	2047	rVB2	431	501	0.00%	0.001%
82	13.579	2047	2049	2052	rBV	554	444	0.00%	0.001%
83	13.670	2062	2064	2066	rBV	335	413	0.00%	0.001%
84	13.896	2100	2101	2103	rVV	648	434	0.00%	0.001%
85	13.920	2104	2105	2107	rVV	568	397	0.00%	0.001%
86	13.951	2109	2110	2114	rVB	462	573	0.00%	0.002%
87	14.085	2130	2132	2134	rBV	504	569	0.00%	0.002%
88	14.134	2138	2140	2144	rBV2	495	675	0.00%	0.002%
89	14.286	2162	2165	2166	rVB2	424	420	0.00%	0.001%
90	14.390	2180	2182	2185	rVB2	473	472	0.00%	0.001%
91	14.560	2208	2210	2214	rBV2	532	544	0.00%	0.002%
92	14.884	2262	2263	2266	rVB2	794	605	0.00%	0.002%
93	14.975	2277	2278	2281	rVB2	644	636	0.00%	0.002%
94	15.201	2313	2315	2317	rVB	664	431	0.00%	0.001%
95	15.298	2329	2331	2335	rBV3	591	488	0.00%	0.001%
96	15.383	2343	2345	2346	rBV2	629	486	0.00%	0.001%
97	16.432	2515	2517	2519	rBV	606	466	0.00%	0.001%
98	16.517	2529	2531	2532	rBV	623	498	0.00%	0.001%
99	16.591	2542	2543	2546	rBV2	691	565	0.00%	0.002%
100	16.767	2571	2572	2575	rBV2	646	651	0.00%	0.002%




Sum of corrected areas: 34233627

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030497.D
Acq On : 07 Aug 2022 04:50
Operator : JC/MD
Sample : N4021-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

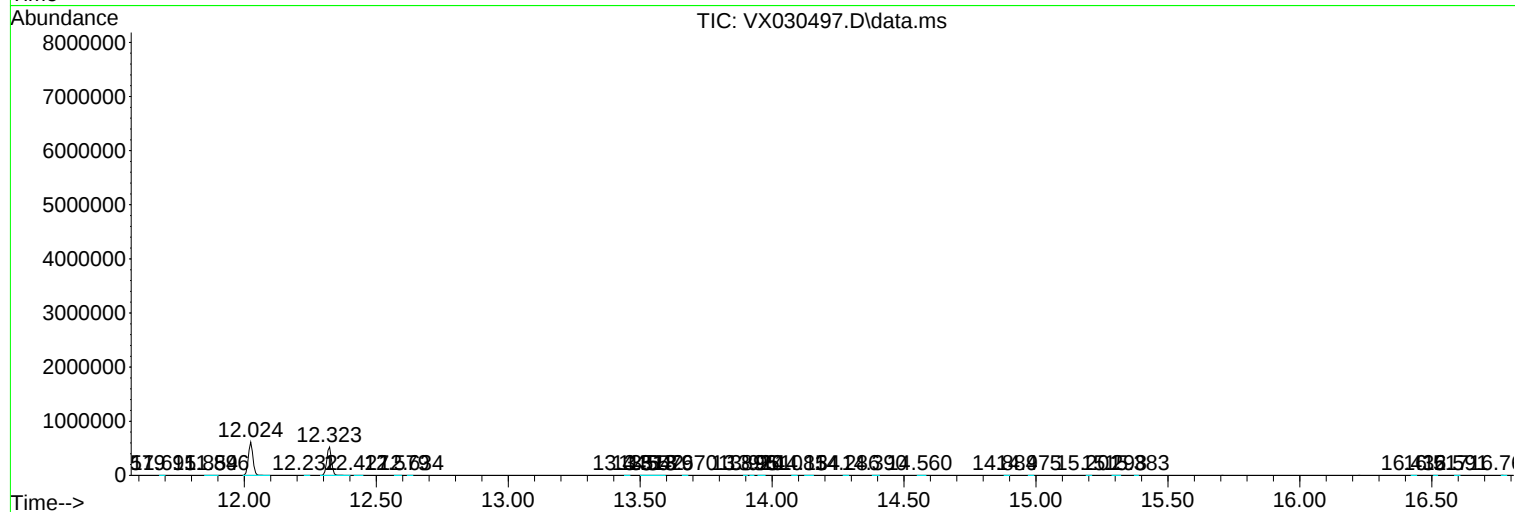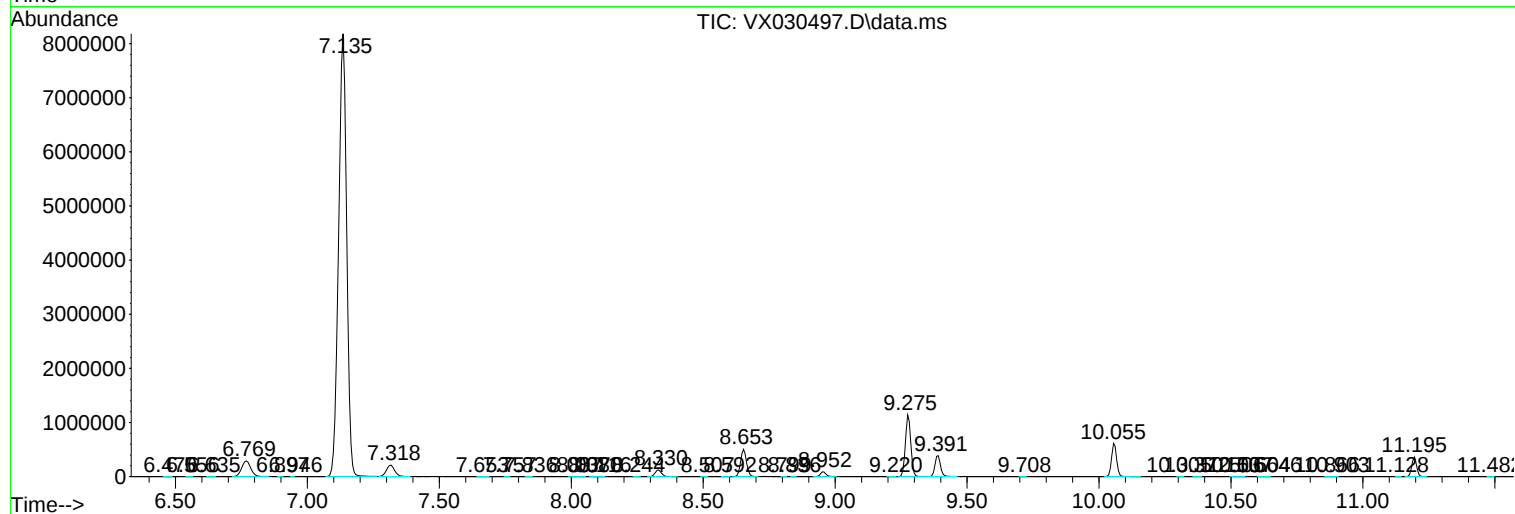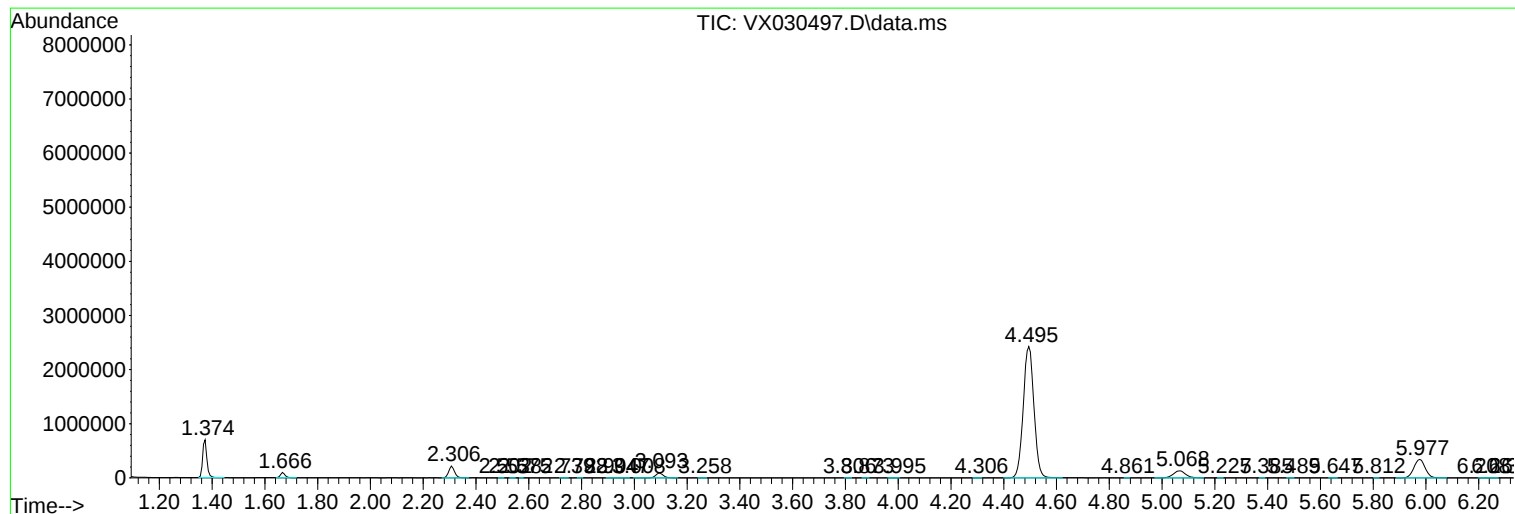

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030497.D
Acq On : 07 Aug 2022 04:50
Operator : JC/MD
Sample : N4021-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030497.D
Acq On : 07 Aug 2022 04:50
Operator : JC/MD
Sample : N4021-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E21

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc