

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030498.D
 Acq On : 07 Aug 2022 05:13
 Operator : JC/MD
 Sample : VIBLK659
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	52	rVB	108666	109383	11.75%	1.529%
2	1.666	91	95	103	rVB	91380	113231	12.17%	1.583%
3	2.306	194	200	210	rVB	183615	275533	29.61%	3.853%
4	2.495	230	231	232	rBV	427	291	0.03%	0.004%
5	2.568	242	243	245	rBV2	614	424	0.05%	0.006%
6	2.660	257	258	259	rBV	666	393	0.04%	0.005%
7	2.788	274	279	285	rBV5	3339	6403	0.69%	0.090%
8	2.953	298	306	313	rVV	6388	14523	1.56%	0.203%
9	3.087	325	328	332	rBV2	640	937	0.10%	0.013%
10	3.148	335	338	339	rVB2	584	468	0.05%	0.007%
11	3.300	360	363	364	rBV	492	366	0.04%	0.005%
12	3.361	370	373	374	rBV2	478	365	0.04%	0.005%
13	3.434	383	385	390	rVB2	597	690	0.07%	0.010%
14	3.568	403	407	408	rBV	527	443	0.05%	0.006%
15	3.995	476	477	479	rVV	450	292	0.03%	0.004%
16	4.062	485	488	492	rVV2	451	598	0.06%	0.008%
17	4.117	495	497	499	rVV2	391	462	0.05%	0.006%
18	4.172	504	506	508	rVV2	440	451	0.05%	0.006%
19	4.245	516	518	521	rVV2	337	319	0.03%	0.004%
20	4.336	532	533	535	rBV	585	329	0.04%	0.005%
21	4.471	546	555	567	rBV	91944	275433	29.59%	3.851%
22	4.800	607	609	610	rBV2	398	327	0.04%	0.005%
23	4.922	625	629	632	rBV2	487	809	0.09%	0.011%
24	4.958	634	635	638	rVV2	460	390	0.04%	0.005%
25	5.068	640	653	671	rBV	125469	391995	42.12%	5.481%
26	5.281	686	688	691	rBV3	404	405	0.04%	0.006%
27	5.336	694	697	698	rBV2	336	329	0.04%	0.005%
28	5.476	717	720	723	rBV2	465	539	0.06%	0.008%
29	5.544	728	731	734	rBV4	1045	1584	0.17%	0.022%
30	5.574	734	736	738	rVB2	1099	898	0.10%	0.013%
31	5.635	744	746	751	rVB2	459	667	0.07%	0.009%
32	5.800	770	773	774	rBV2	478	357	0.04%	0.005%
33	5.848	779	781	783	rBV	322	307	0.03%	0.004%
34	5.976	790	802	817	rBV2	312852	930677	100.00%	13.013%
35	6.239	844	845	848	rBV	468	440	0.05%	0.006%
36	6.299	853	855	856	rVB	501	336	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030498.D
 Acq On : 07 Aug 2022 05:13
 Operator : JC/MD
 Sample : VIBLK659
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.604	903	905	906	rBV2	450	439	0.05%	0.006%
38	6.769	921	932	944	rBV	265274	635477	68.28%	8.886%
39	7.025	972	974	977	rBV2	448	458	0.05%	0.006%
40	7.123	981	990	999	rVV3	28992	76032	8.17%	1.063%
41	7.312	1013	1021	1035	rVV	195089	435801	46.83%	6.094%
42	7.446	1042	1043	1044	rBV	485	298	0.03%	0.004%
43	7.488	1048	1050	1053	rVV3	995	1212	0.13%	0.017%
44	7.854	1109	1110	1114	rVB	421	396	0.04%	0.006%
45	7.891	1114	1116	1119	rBV	387	560	0.06%	0.008%
46	7.946	1120	1125	1132	rVB5	636	1483	0.16%	0.021%
47	8.153	1157	1159	1160	rBV	457	317	0.03%	0.004%
48	8.220	1168	1170	1172	rVB2	361	331	0.04%	0.005%
49	8.330	1181	1188	1199	rBV	115087	191316	20.56%	2.675%
50	8.653	1234	1241	1251	rBV	430329	663992	71.35%	9.284%
51	8.897	1280	1281	1285	rBV2	430	398	0.04%	0.006%
52	8.951	1285	1290	1299	rBV	82429	124958	13.43%	1.747%
53	9.073	1308	1310	1312	rBV2	596	567	0.06%	0.008%
54	9.201	1329	1331	1333	rBV2	259	334	0.04%	0.005%
55	9.275	1339	1343	1349	rVB5	4659	6714	0.72%	0.094%
56	9.390	1356	1362	1373	rBV	379413	567333	60.96%	7.933%
57	9.531	1383	1385	1391	rVB6	708	1207	0.13%	0.017%
58	9.701	1410	1413	1425	rVB2	4909	7398	0.79%	0.103%
59	9.829	1432	1434	1437	rBV	334	457	0.05%	0.006%
60	9.921	1447	1449	1450	rVB	536	331	0.04%	0.005%
61	10.055	1465	1471	1483	rBV	554179	722995	77.68%	10.110%
62	10.226	1495	1499	1500	rBV	433	531	0.06%	0.007%
63	10.256	1500	1504	1505	rBV	426	583	0.06%	0.008%
64	10.402	1526	1528	1531	rVV2	364	458	0.05%	0.006%
65	10.482	1538	1541	1542	rBV2	371	426	0.05%	0.006%
66	11.195	1652	1658	1668	rBV	350642	440533	47.33%	6.160%
67	11.475	1703	1704	1706	rBV	569	424	0.05%	0.006%
68	11.683	1736	1738	1740	rBV2	434	352	0.04%	0.005%
69	11.799	1756	1757	1759	rBV2	350	330	0.04%	0.005%
70	11.884	1766	1771	1773	rBV2	562	1012	0.11%	0.014%
71	12.024	1789	1794	1803	rVB	480834	587202	63.09%	8.211%
72	12.140	1811	1813	1816	rBV3	623	481	0.05%	0.007%
73	12.164	1816	1817	1819	rVB	578	394	0.04%	0.006%
74	12.189	1819	1821	1824	rBV2	350	512	0.06%	0.007%
75	12.323	1837	1843	1849	rBV	431870	533062	57.28%	7.454%
76	12.542	1877	1879	1882	rBV2	564	544	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030498.D
 Acq On : 07 Aug 2022 05:13
 Operator : JC/MD
 Sample : VIBLK659
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK659

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.762	1912	1915	1916	rBV3	338	343	0.04%	0.005%
78	12.829	1924	1926	1929	rBV2	279	288	0.03%	0.004%
79	13.054	1959	1963	1964	rVB2	402	432	0.05%	0.006%
80	13.231	1989	1992	1993	rBV2	431	400	0.04%	0.006%
81	13.335	2007	2009	2010	rBV	486	346	0.04%	0.005%
82	13.402	2018	2020	2022	rBV2	477	478	0.05%	0.007%
83	13.475	2030	2032	2035	rBV2	487	363	0.04%	0.005%
84	13.573	2046	2048	2050	rVB2	485	349	0.04%	0.005%
85	14.201	2150	2151	2154	rVV2	331	356	0.04%	0.005%
86	14.304	2164	2168	2170	rVB2	651	834	0.09%	0.012%
87	14.322	2170	2171	2173	rBV	492	474	0.05%	0.007%
88	14.396	2180	2183	2184	rBV2	638	560	0.06%	0.008%
89	14.524	2200	2204	2206	rBV2	586	893	0.10%	0.012%
90	14.578	2208	2213	2217	rBB2	688	930	0.10%	0.013%
91	14.646	2220	2224	2226	rBV	591	556	0.06%	0.008%
92	14.694	2230	2232	2234	rBV	493	398	0.04%	0.006%
93	14.920	2268	2269	2271	rVB2	594	305	0.03%	0.004%
94	14.944	2271	2273	2274	rBV	647	506	0.05%	0.007%
95	15.054	2287	2291	2292	rBV3	573	733	0.08%	0.010%
96	15.682	2392	2394	2395	rBV	723	569	0.06%	0.008%
97	16.194	2476	2478	2479	rBV2	598	515	0.06%	0.007%
98	16.322	2497	2499	2501	rBV	734	605	0.07%	0.008%
99	16.468	2521	2523	2524	rBV	624	288	0.03%	0.004%
100	16.517	2529	2531	2534	rBV4	708	1065	0.11%	0.015%




Sum of corrected areas: 7151628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030498.D
Acq On : 07 Aug 2022 05:13
Operator : JC/MD
Sample : VIBLK659
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

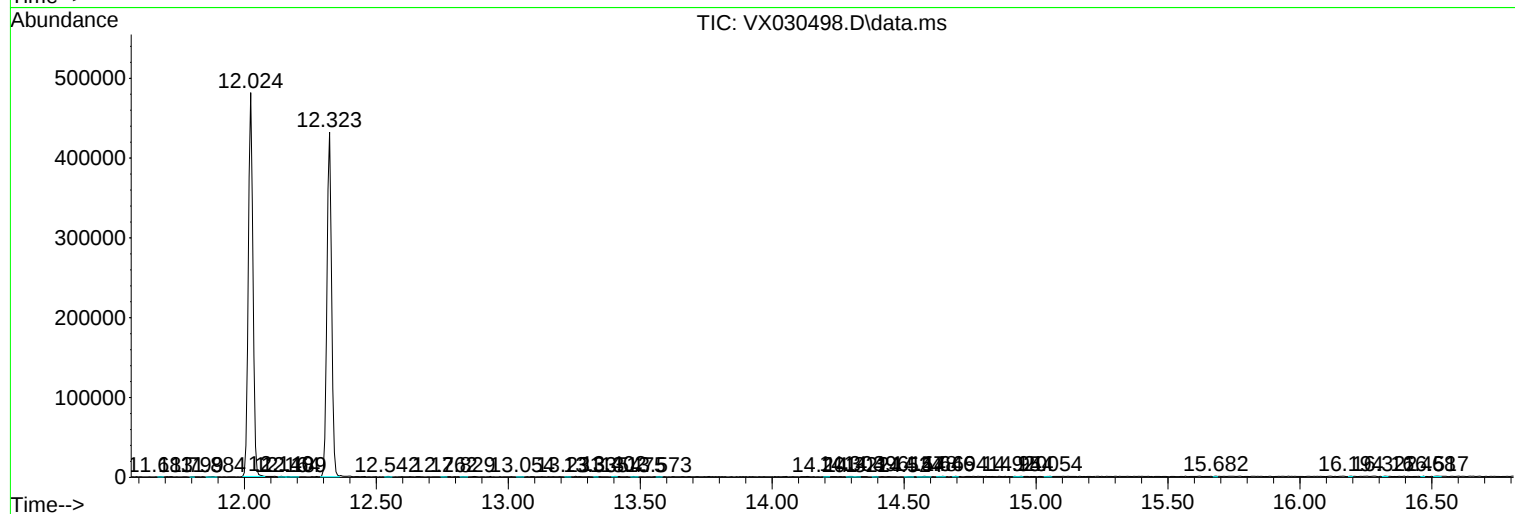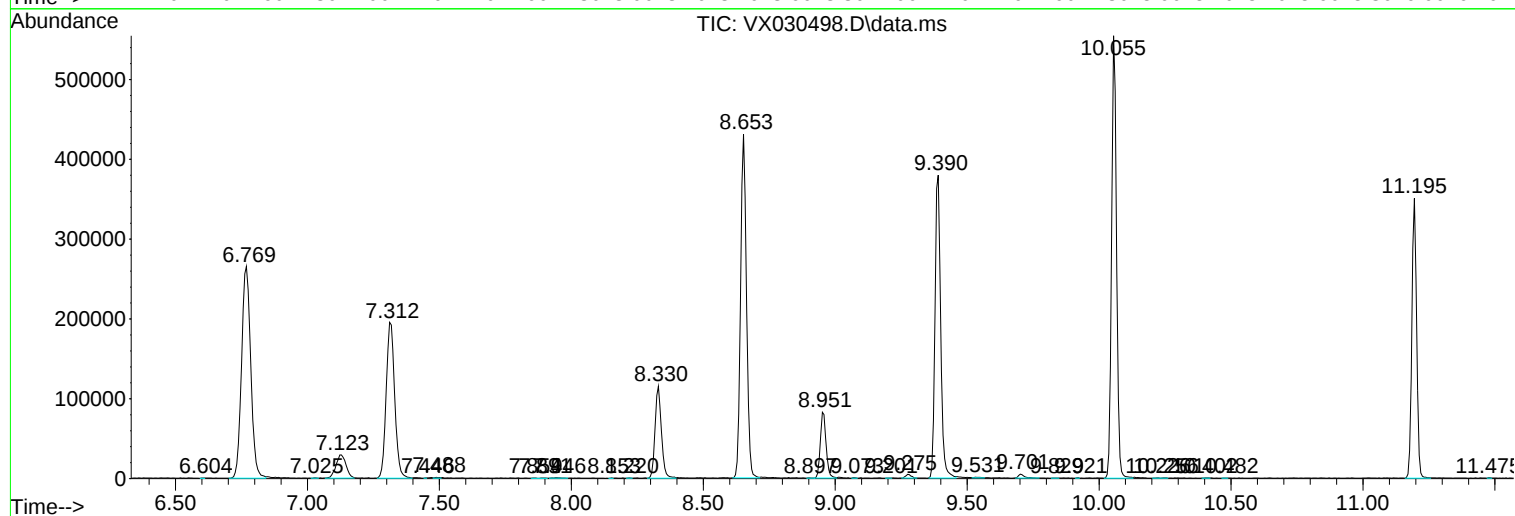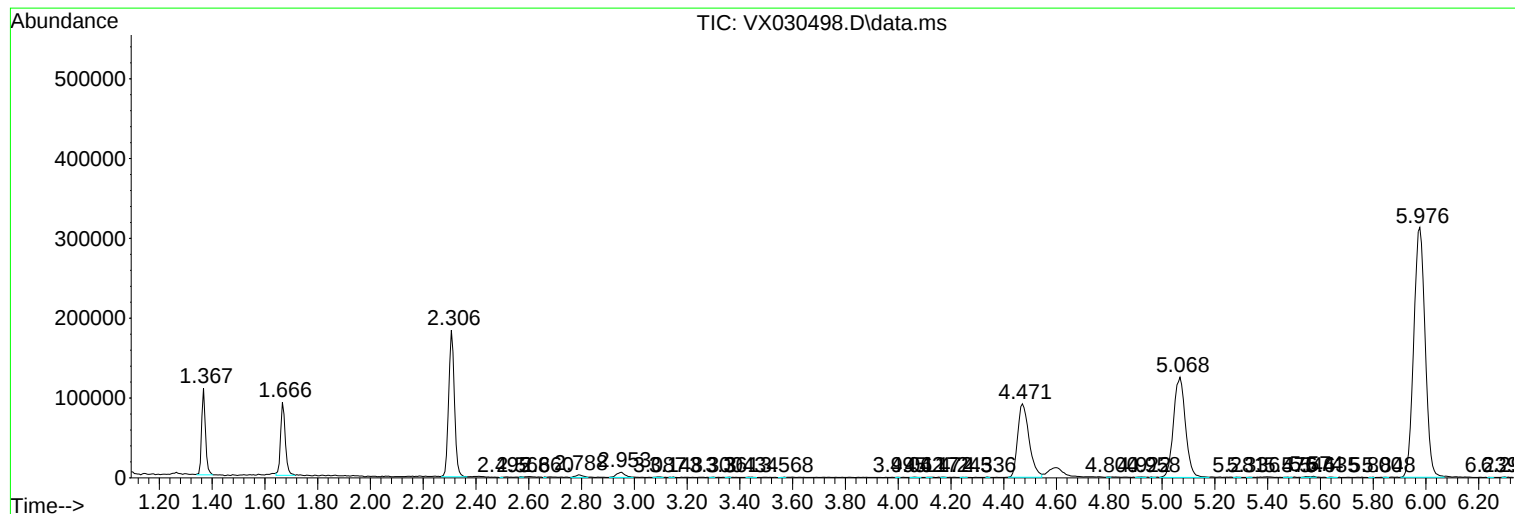

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030498.D
Acq On : 07 Aug 2022 05:13
Operator : JC/MD
Sample : VIBLK659
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030498.D
Acq On : 07 Aug 2022 05:13
Operator : JC/MD
Sample : VIBLK659
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK659

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
