

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030499.D
 Acq On : 07 Aug 2022 05:36
 Operator : JC/MD
 Sample : N4021-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030499.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB2	233382	291182	8.73%	1.844%
2	1.666	91	95	105	rVB2	95423	136051	4.08%	0.862%
3	2.306	194	200	210	rVB	212493	336711	10.10%	2.133%
4	2.373	210	211	212	rBV	1108	660	0.02%	0.004%
5	2.507	231	233	237	rVB4	487	606	0.02%	0.004%
6	2.678	259	261	263	rVB	435	283	0.01%	0.002%
7	2.696	263	264	267	rBV2	549	617	0.02%	0.004%
8	2.855	288	290	293	rBV3	509	554	0.02%	0.004%
9	2.897	296	297	300	rVB2	532	360	0.01%	0.002%
10	3.038	318	320	321	rBV2	556	432	0.01%	0.003%
11	3.093	323	329	342	rVV	25951	52697	1.58%	0.334%
12	3.403	377	380	382	rBV	373	384	0.01%	0.002%
13	3.678	422	425	428	rBV2	296	404	0.01%	0.003%
14	3.751	434	437	439	rBV	317	316	0.01%	0.002%
15	3.855	453	454	456	rBV2	445	324	0.01%	0.002%
16	3.885	456	459	462	rVB2	404	555	0.02%	0.004%
17	4.105	494	495	499	rBV2	417	548	0.02%	0.003%
18	4.227	512	515	516	rBV	370	285	0.01%	0.002%
19	4.269	520	522	524	rBV	544	564	0.02%	0.004%
20	4.355	532	536	538	rVB	471	529	0.02%	0.003%
21	4.397	538	543	544	rBV2	410	602	0.02%	0.004%
22	4.495	546	559	577	rBV2	983344	2753036	82.55%	17.437%
23	5.068	637	653	671	rBV2	136559	430991	12.92%	2.730%
24	5.208	674	676	679	rVB3	556	592	0.02%	0.004%
25	5.245	679	682	685	rBV3	486	580	0.02%	0.004%
26	5.281	685	688	690	rVB3	436	448	0.01%	0.003%
27	5.385	701	705	710	rBV2	624	1365	0.04%	0.009%
28	5.866	783	784	787	rVB2	561	521	0.02%	0.003%
29	5.976	790	802	822	rVV2	340255	1002886	30.07%	6.352%
30	6.177	833	835	839	rVB2	476	466	0.01%	0.003%
31	6.470	881	883	885	rBV2	329	317	0.01%	0.002%
32	6.610	903	906	908	rBV2	649	620	0.02%	0.004%
33	6.769	922	932	944	rBV	292055	686640	20.59%	4.349%
34	7.019	971	973	977	rBV3	406	475	0.01%	0.003%
35	7.128	981	991	1003	rBV	904908	1954803	58.61%	12.381%
36	7.311	1013	1021	1037	rVB	207298	457606	13.72%	2.898%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030499.D
 Acq On : 07 Aug 2022 05:36
 Operator : JC/MD
 Sample : N4021-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.610	1067	1070	1072	rBV2	444	503	0.02%	0.003%
38	7.647	1074	1076	1077	rBV	421	302	0.01%	0.002%
39	7.909	1114	1119	1120	rBV2	476	635	0.02%	0.004%
40	7.927	1120	1122	1124	rBV2	463	433	0.01%	0.003%
41	7.994	1131	1133	1135	rBV2	376	310	0.01%	0.002%
42	8.012	1135	1136	1138	rVB	445	273	0.01%	0.002%
43	8.079	1144	1147	1149	rVB2	425	372	0.01%	0.002%
44	8.098	1149	1150	1153	rBV2	313	307	0.01%	0.002%
45	8.177	1161	1163	1164	rBV	473	311	0.01%	0.002%
46	8.262	1176	1177	1180	rBV	294	362	0.01%	0.002%
47	8.329	1182	1188	1199	rVV	120101	198937	5.97%	1.260%
48	8.512	1217	1218	1220	rVB2	966	521	0.02%	0.003%
49	8.585	1228	1230	1231	rVB	562	264	0.01%	0.002%
50	8.653	1234	1241	1250	rBV	502346	775449	23.25%	4.912%
51	8.951	1284	1290	1301	rBV	84013	130180	3.90%	0.825%
52	9.195	1327	1330	1331	rVB2	423	408	0.01%	0.003%
53	9.274	1336	1343	1354	rVV	2225531	3335065	100.00%	21.124%
54	9.390	1356	1362	1375	rVB	393248	571869	17.15%	3.622%
55	9.622	1398	1400	1403	rVB2	741	477	0.01%	0.003%
56	9.652	1403	1405	1408	rBV3	854	716	0.02%	0.005%
57	9.811	1429	1431	1433	rBV2	309	273	0.01%	0.002%
58	9.927	1447	1450	1452	rBV2	328	399	0.01%	0.003%
59	9.951	1452	1454	1457	rBV2	470	422	0.01%	0.003%
60	9.982	1457	1459	1461	rVB	627	506	0.02%	0.003%
61	10.055	1465	1471	1481	rBV	598640	816725	24.49%	5.173%
62	10.201	1492	1495	1497	rBV2	429	520	0.02%	0.003%
63	10.244	1500	1502	1506	rVB3	583	575	0.02%	0.004%
64	10.299	1509	1511	1512	rBV	491	321	0.01%	0.002%
65	10.366	1520	1522	1524	rBV3	459	492	0.01%	0.003%
66	10.469	1538	1539	1542	rBV2	390	327	0.01%	0.002%
67	10.597	1558	1560	1564	rVB2	414	529	0.02%	0.003%
68	10.646	1566	1568	1570	rVB	393	294	0.01%	0.002%
69	10.780	1587	1590	1592	rBV2	490	524	0.02%	0.003%
70	10.847	1600	1601	1603	rBV2	397	411	0.01%	0.003%
71	11.195	1653	1658	1668	rVB	369625	458370	13.74%	2.903%
72	11.396	1689	1691	1693	rBV2	395	295	0.01%	0.002%
73	11.530	1711	1713	1715	rBV	602	396	0.01%	0.003%
74	11.628	1726	1729	1732	rVV2	473	720	0.02%	0.005%
75	11.951	1781	1782	1785	rBV2	296	264	0.01%	0.002%
76	12.024	1789	1794	1804	rBV	600148	721725	21.64%	4.571%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030499.D
 Acq On : 07 Aug 2022 05:36
 Operator : JC/MD
 Sample : N4021-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1854	rBV	520644	639982	19.19%	4.054%
78	12.768	1913	1916	1918	rBV	332	449	0.01%	0.003%
79	12.841	1926	1928	1931	rBV2	412	446	0.01%	0.003%
80	12.871	1931	1933	1936	rBV2	496	423	0.01%	0.003%
81	13.103	1970	1971	1972	rBV	453	266	0.01%	0.002%
82	13.158	1978	1980	1982	rBV2	335	302	0.01%	0.002%
83	13.182	1982	1984	1987	rVB2	522	506	0.02%	0.003%
84	13.292	2000	2002	2004	rBV	526	374	0.01%	0.002%
85	13.658	2060	2062	2064	rBV	587	590	0.02%	0.004%
86	13.743	2075	2076	2078	rVB	718	269	0.01%	0.002%
87	13.767	2078	2080	2081	rBV	445	399	0.01%	0.003%
88	13.786	2081	2083	2084	rVB2	546	288	0.01%	0.002%
89	14.231	2155	2156	2159	rVB2	593	437	0.01%	0.003%
90	14.341	2172	2174	2177	rBV	526	536	0.02%	0.003%
91	14.450	2190	2192	2194	rBV	569	527	0.02%	0.003%
92	14.572	2210	2212	2214	rBV	361	265	0.01%	0.002%
93	15.042	2288	2289	2291	rVB2	784	317	0.01%	0.002%
94	15.218	2316	2318	2321	rBV2	524	467	0.01%	0.003%
95	15.474	2359	2360	2362	rBV2	904	548	0.02%	0.003%
96	15.517	2365	2367	2371	rBV	591	1014	0.03%	0.006%
97	15.596	2378	2380	2381	rBV2	632	404	0.01%	0.003%
98	16.041	2451	2453	2456	rBV2	770	639	0.02%	0.004%
99	16.511	2528	2530	2532	rBV2	742	492	0.01%	0.003%
100	16.615	2545	2547	2549	rBV2	702	569	0.02%	0.004%




Sum of corrected areas: 15788301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030499.D
Acq On : 07 Aug 2022 05:36
Operator : JC/MD
Sample : N4021-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

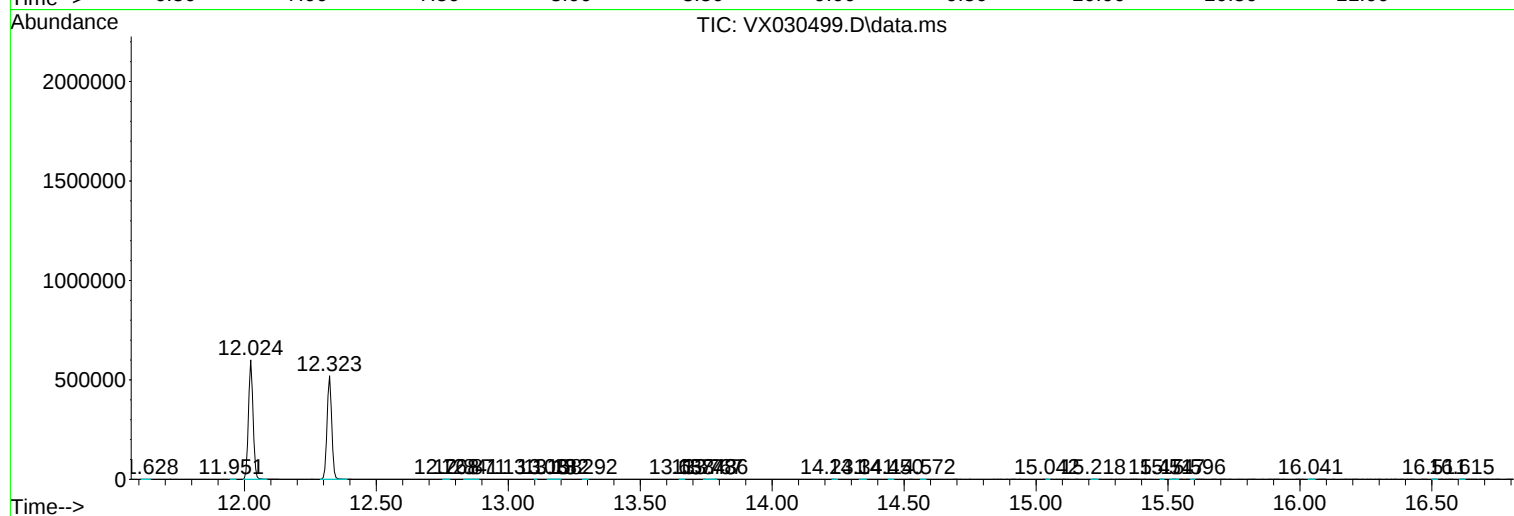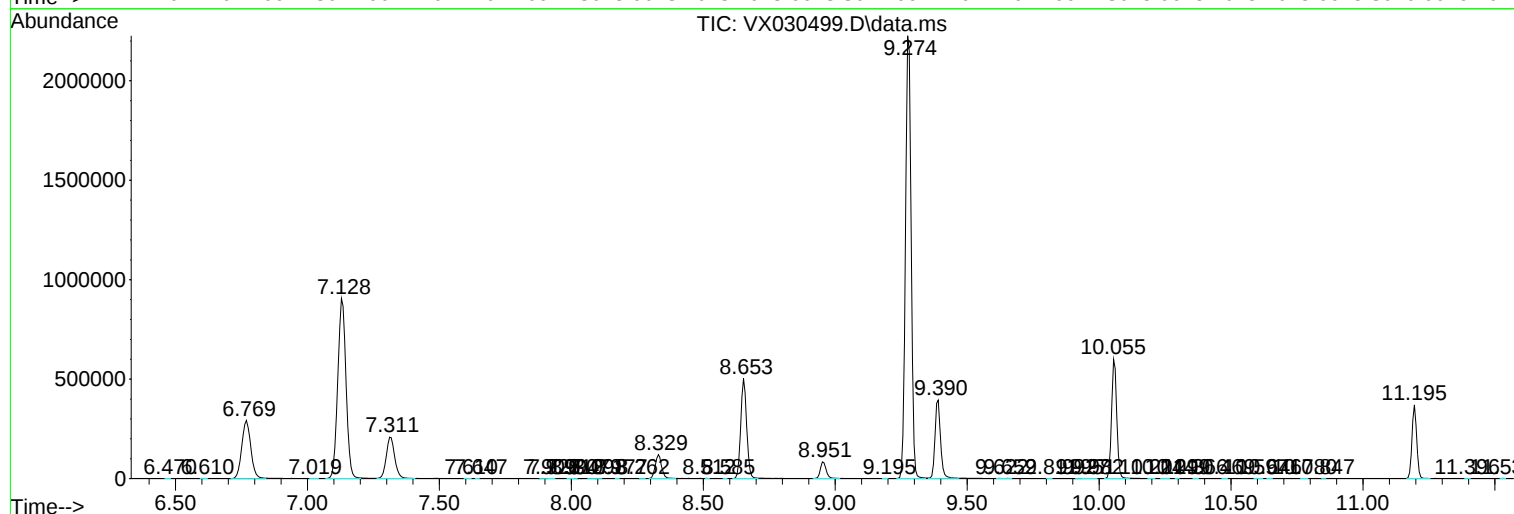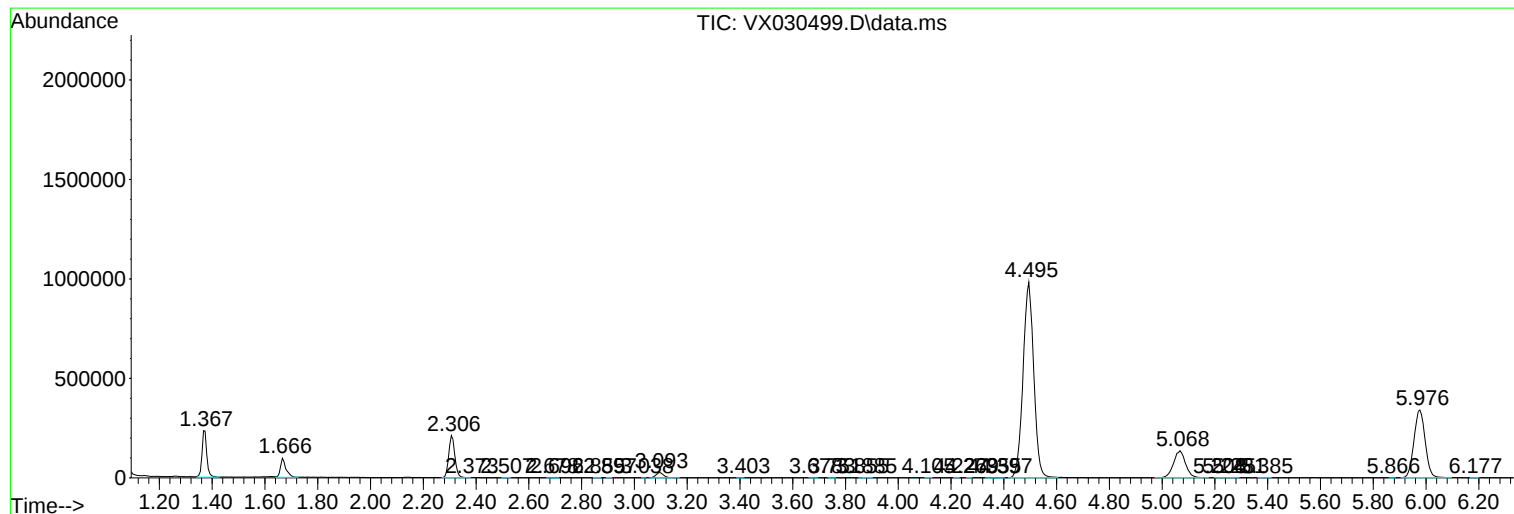

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030499.D
Acq On : 07 Aug 2022 05:36
Operator : JC/MD
Sample : N4021-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030499.D
Acq On : 07 Aug 2022 05:36
Operator : JC/MD
Sample : N4021-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc