

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030502.D
 Acq On : 07 Aug 2022 06:47
 Operator : JC/MD
 Sample : VIBLK661
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030502.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB	117131	119160	12.28%	1.588%
2	1.666	91	95	106	rVB	98232	119069	12.27%	1.587%
3	2.306	194	200	210	rVB	210051	313905	32.34%	4.185%
4	2.556	239	241	243	rBV2	481	357	0.04%	0.005%
5	2.672	259	260	266	rVB3	493	627	0.06%	0.008%
6	2.794	274	280	285	rVB4	3468	6262	0.65%	0.083%
7	2.953	298	306	313	rBV3	8566	20079	2.07%	0.268%
8	3.001	313	314	317	rVB	458	381	0.04%	0.005%
9	3.129	333	335	338	rVB2	394	366	0.04%	0.005%
10	3.160	338	340	342	rBV2	396	415	0.04%	0.006%
11	3.337	367	369	371	rVV2	389	394	0.04%	0.005%
12	3.440	382	386	387	rBV	439	541	0.06%	0.007%
13	3.452	387	388	392	rBV2	450	490	0.05%	0.007%
14	3.513	395	398	399	rVV2	457	418	0.04%	0.006%
15	3.538	399	402	403	rVB2	435	345	0.04%	0.005%
16	3.568	403	407	409	rVB2	319	338	0.03%	0.005%
17	3.599	409	412	415	rBV	415	496	0.05%	0.007%
18	3.965	471	472	475	rBV2	286	330	0.03%	0.004%
19	3.995	475	477	480	rVB2	392	469	0.05%	0.006%
20	4.123	496	498	500	rBV	435	338	0.03%	0.005%
21	4.245	517	518	521	rBV	430	324	0.03%	0.004%
22	4.269	521	522	525	rBV2	393	401	0.04%	0.005%
23	4.385	539	541	544	rBV2	327	339	0.03%	0.005%
24	4.471	546	555	568	rBV	89001	262536	27.05%	3.500%
25	4.891	622	624	625	rBV	355	348	0.04%	0.005%
26	4.940	629	632	633	rBV	384	322	0.03%	0.004%
27	5.068	639	653	668	rBV	132316	401352	41.35%	5.350%
28	5.464	715	718	721	rBV	619	544	0.06%	0.007%
29	5.544	729	731	732	rBV	758	491	0.05%	0.007%
30	5.568	732	735	739	rVV2	990	1681	0.17%	0.022%
31	5.635	743	746	750	rVV3	518	703	0.07%	0.009%
32	5.690	753	755	757	rBV	676	640	0.07%	0.009%
33	5.720	757	760	762	rVV	435	419	0.04%	0.006%
34	5.781	768	770	777	rVB2	359	530	0.05%	0.007%
35	5.976	789	802	817	rBV2	330837	970526	100.00%	12.938%
36	6.568	897	899	902	rVB	479	455	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030502.D
 Acq On : 07 Aug 2022 06:47
 Operator : JC/MD
 Sample : VIBLK661
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.665	912	915	916	rBV	417	343	0.04%	0.005%
38	6.769	922	932	946	rBV	280369	670156	69.05%	8.934%
39	6.958	961	963	965	rVB2	512	402	0.04%	0.005%
40	7.123	982	990	999	rBV6	13457	34646	3.57%	0.462%
41	7.312	1012	1021	1035	rBV	204128	453608	46.74%	6.047%
42	7.458	1041	1045	1047	rBV3	496	841	0.09%	0.011%
43	7.482	1047	1049	1051	rVV2	1049	1169	0.12%	0.016%
44	7.537	1055	1058	1061	rVB2	386	510	0.05%	0.007%
45	7.561	1061	1062	1065	rBV	440	442	0.05%	0.006%
46	7.750	1091	1093	1098	rBV2	253	380	0.04%	0.005%
47	7.879	1112	1114	1117	rVB2	444	392	0.04%	0.005%
48	7.939	1122	1124	1127	rVV2	508	529	0.05%	0.007%
49	7.964	1127	1128	1132	rVV2	486	543	0.06%	0.007%
50	8.110	1150	1152	1155	rBV2	318	398	0.04%	0.005%
51	8.171	1161	1162	1166	rVB2	417	422	0.04%	0.006%
52	8.202	1166	1167	1171	rBV	350	387	0.04%	0.005%
53	8.330	1181	1188	1198	rBV	120392	192981	19.88%	2.573%
54	8.531	1219	1221	1224	rVB	500	533	0.05%	0.007%
55	8.653	1234	1241	1257	rBV	483190	725936	74.80%	9.677%
56	8.897	1279	1281	1284	rBV2	519	514	0.05%	0.007%
57	8.951	1284	1290	1297	rBV	83535	128765	13.27%	1.717%
58	9.183	1326	1328	1330	rBV2	376	361	0.04%	0.005%
59	9.275	1335	1343	1350	rBV4	2605	5234	0.54%	0.070%
60	9.390	1356	1362	1377	rBV	376322	566213	58.34%	7.548%
61	9.701	1410	1413	1419	rVB4	2564	3611	0.37%	0.048%
62	9.781	1423	1426	1429	rBV2	433	533	0.05%	0.007%
63	10.055	1465	1471	1480	rBV	568174	769499	79.29%	10.258%
64	10.305	1510	1512	1515	rBV2	442	349	0.04%	0.005%
65	10.378	1522	1524	1527	rVB	477	394	0.04%	0.005%
66	10.415	1527	1530	1533	rBV2	431	612	0.06%	0.008%
67	10.500	1541	1544	1546	rVB2	339	423	0.04%	0.006%
68	10.518	1546	1547	1550	rBV	407	544	0.06%	0.007%
69	10.817	1594	1596	1599	rBV2	554	763	0.08%	0.010%
70	11.018	1627	1629	1634	rVB3	497	686	0.07%	0.009%
71	11.067	1634	1637	1639	rBV	316	356	0.04%	0.005%
72	11.122	1644	1646	1652	rVV4	395	518	0.05%	0.007%
73	11.195	1652	1658	1669	rVV	346095	438779	45.21%	5.849%
74	11.299	1674	1675	1681	rVB4	448	754	0.08%	0.010%
75	11.378	1686	1688	1690	rVB	495	340	0.04%	0.005%
76	11.475	1702	1704	1706	rBV	618	417	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
 Data File : VX030502.D
 Acq On : 07 Aug 2022 06:47
 Operator : JC/MD
 Sample : VIBLK661
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK661

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

77	11.920	1774	1777	1781	rVB2	371	509	0.05%	0.007%
78	12.024	1788	1794	1802	rVV	545170	665711	68.59%	8.874%
79	12.323	1837	1843	1851	rBV	463982	593266	61.13%	7.909%
80	12.683	1898	1902	1903	rVB	565	467	0.05%	0.006%
81	13.103	1969	1971	1975	rVB	567	704	0.07%	0.009%
82	13.182	1983	1984	1988	rBV	407	420	0.04%	0.006%
83	13.341	2007	2010	2013	rBV3	384	652	0.07%	0.009%
84	13.487	2027	2034	2038	rBV3	451	1030	0.11%	0.014%
85	13.548	2042	2044	2048	rVB	486	474	0.05%	0.006%
86	13.621	2054	2056	2058	rBV3	569	464	0.05%	0.006%
87	13.713	2069	2071	2073	rBV2	499	431	0.04%	0.006%
88	14.005	2118	2119	2121	rBV	455	343	0.04%	0.005%
89	14.091	2132	2133	2136	rBV	368	409	0.04%	0.005%
90	14.359	2174	2177	2178	rBV2	460	520	0.05%	0.007%
91	14.572	2210	2212	2214	rVB	655	465	0.05%	0.006%
92	14.591	2214	2215	2217	rBV	654	509	0.05%	0.007%
93	14.688	2230	2231	2234	rBV2	518	402	0.04%	0.005%
94	14.737	2237	2239	2240	rVV	798	420	0.04%	0.006%
95	14.786	2244	2247	2248	rBV	535	437	0.05%	0.006%
96	14.957	2273	2275	2277	rBV2	502	504	0.05%	0.007%
97	15.091	2296	2297	2299	rBV	729	577	0.06%	0.008%
98	15.292	2328	2330	2331	rBV	594	408	0.04%	0.005%
99	15.712	2397	2399	2401	rVB2	989	536	0.06%	0.007%
100	16.194	2474	2478	2481	rBV3	783	1222	0.13%	0.016%




Sum of corrected areas: 7501554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030502.D
Acq On : 07 Aug 2022 06:47
Operator : JC/MD
Sample : VIBLK661
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

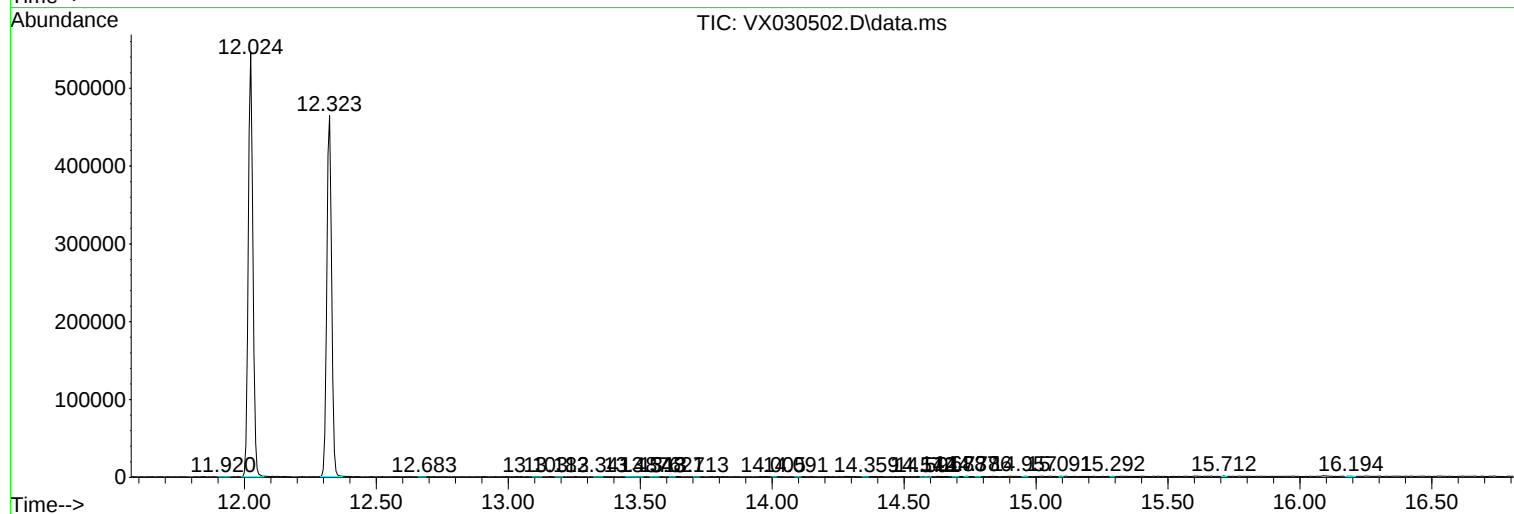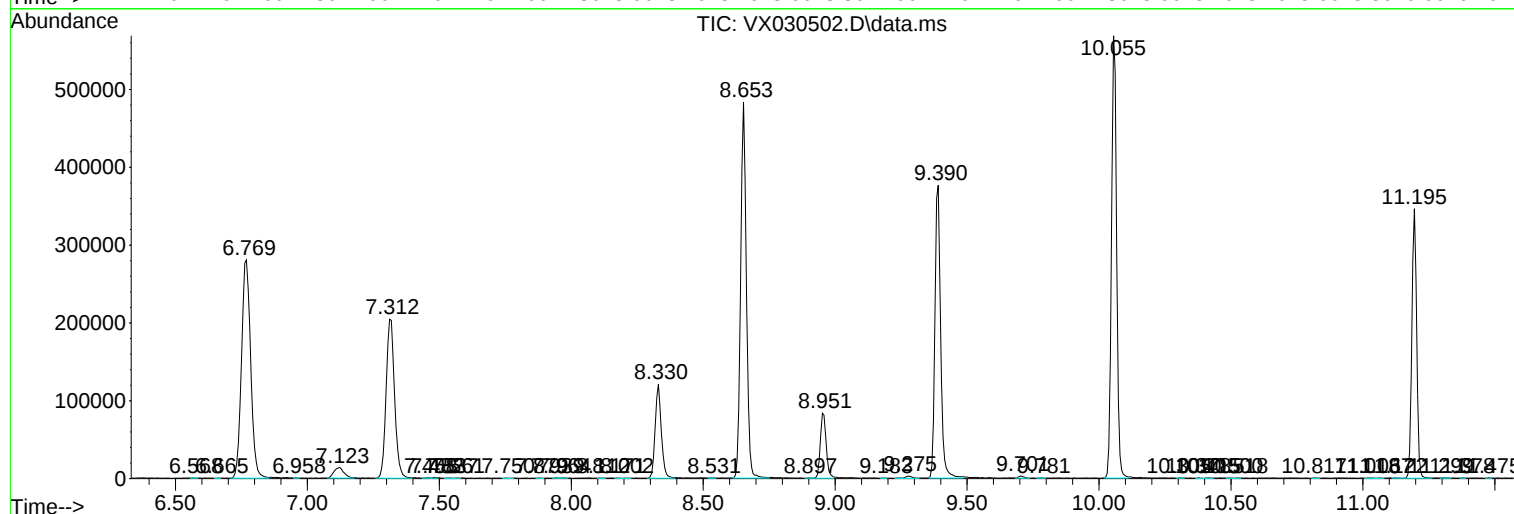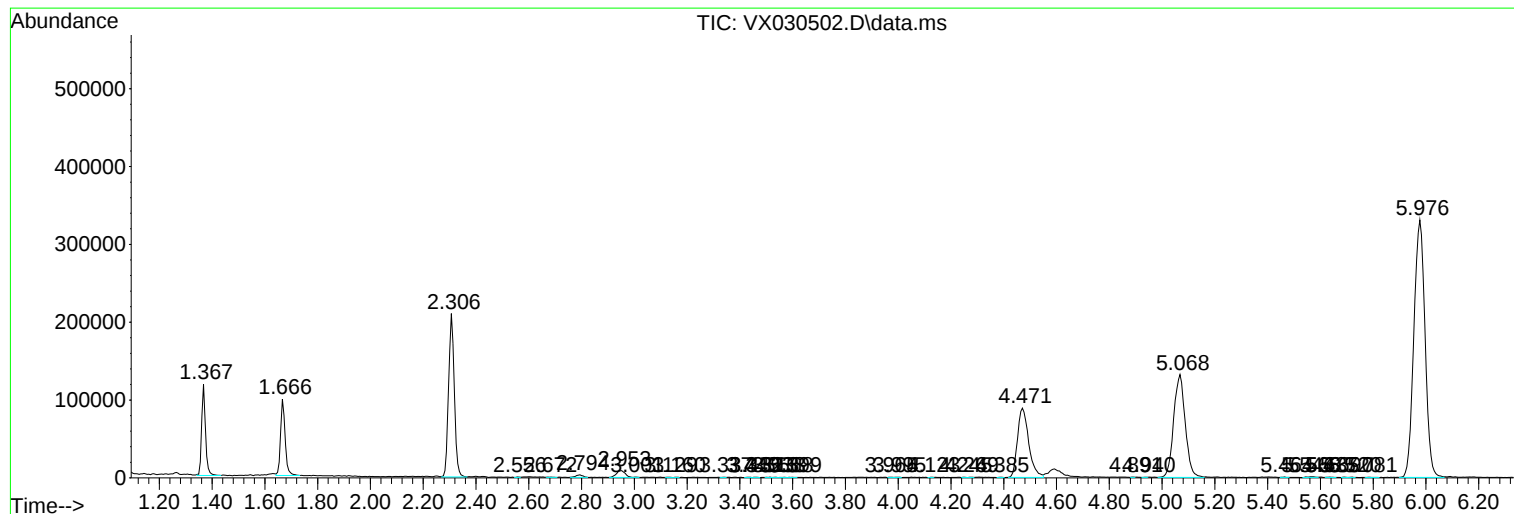

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030502.D
Acq On : 07 Aug 2022 06:47
Operator : JC/MD
Sample : VIBLK661
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080622\
Data File : VX030502.D
Acq On : 07 Aug 2022 06:47
Operator : JC/MD
Sample : VIBLK661
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK661

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc