
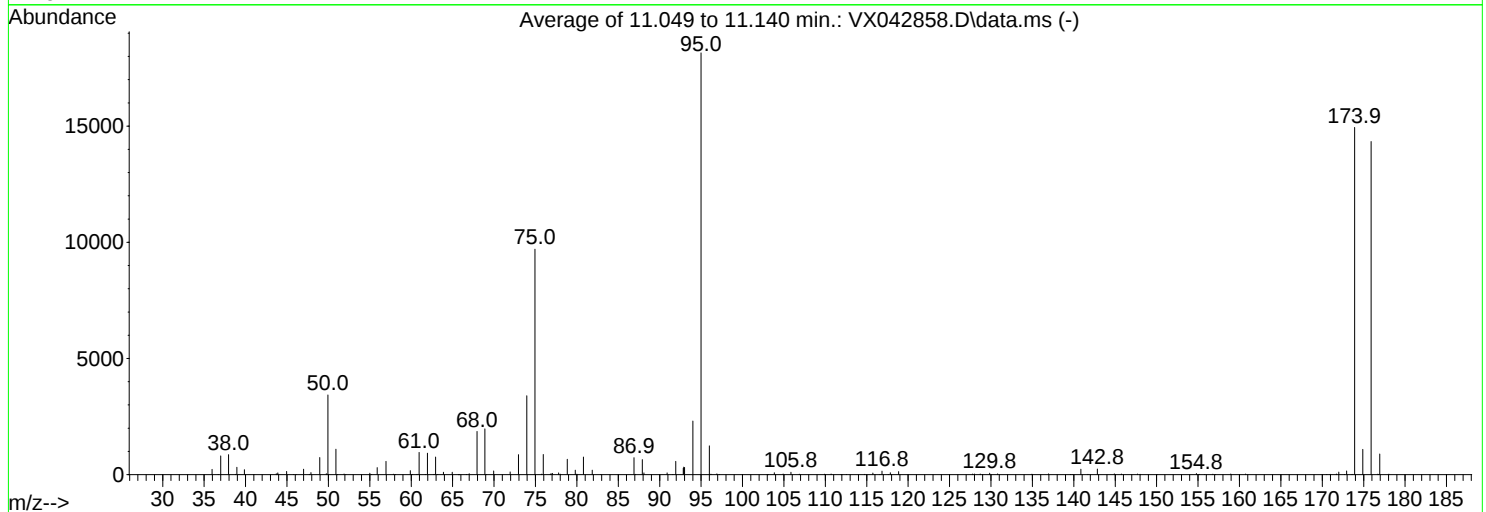


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080624\
Data File : VX042858.D
Acq On : 06 Aug 2024 09:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 07 04:53:59 2024

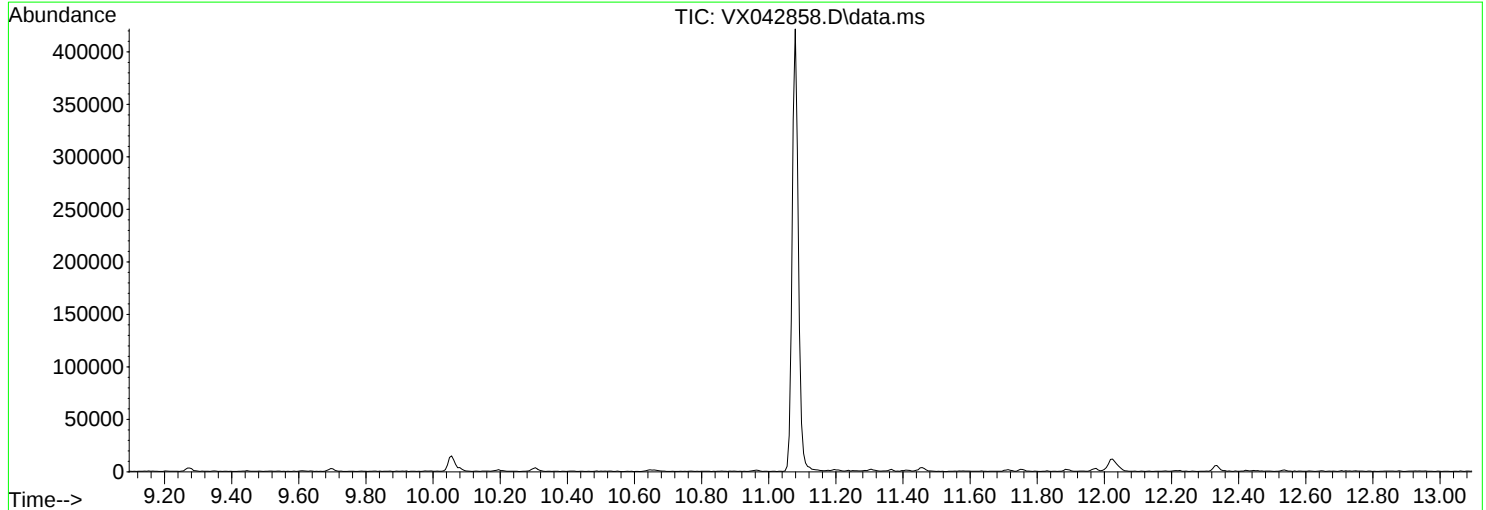

AutoFind: Averaged scan 1634 to 1649; Bkg corrected with scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	3428	PASS
75	95	30	60	53.4	9700	PASS
95	95	100	100	100.0	18153	PASS
96	95	5	9	6.8	1243	PASS
173	174	0.00	2	1.1	162	PASS
174	95	50	100	82.3	14943	PASS
175	174	5	9	7.3	1090	PASS
176	174	95	101	95.9	14336	PASS
177	176	5	9	6.2	890	PASS