

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080718\
Data File : VX003901.D
Acq On : 08 Aug 2018 01:25
Operator : JC/MD
Sample : J4341-01 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN001-SEWER-OUTLET-001

Integration Parameters: RTEINT3.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X072718W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.453	299	306	323	rBV	825482	1438547	1.93%	1.826%
2	2.690	327	345	350	rBV2	20859515	74685072	100.00%	94.813%
3	6.860	1019	1029	1044	rBV	326925	755103	1.01%	0.959%
4	8.714	1326	1333	1342	rBV	637265	1010384	1.35%	1.283%
5	10.116	1556	1563	1576	rBV	655202	881574	1.18%	1.119%




Sum of corrected areas: 78770680

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080718\
Data File : VX003901.D
Acq On : 08 Aug 2018 01:25
Operator : JC/MD
Sample : J4341-01 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN001-SEWER-OUTLET-001

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X072718W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

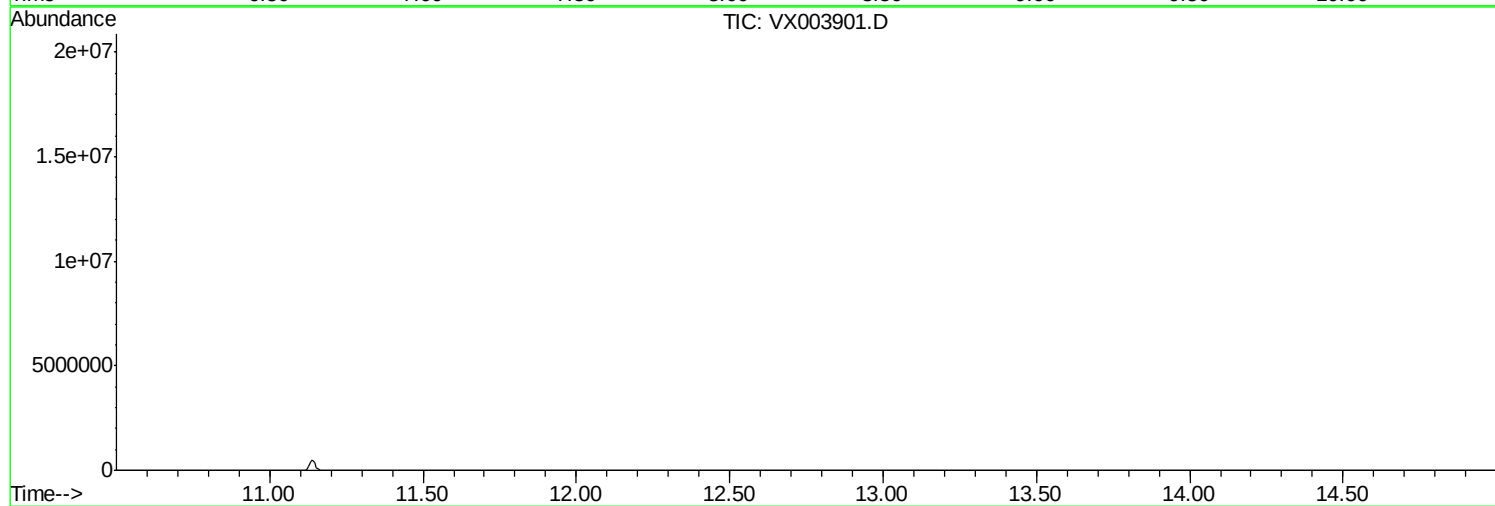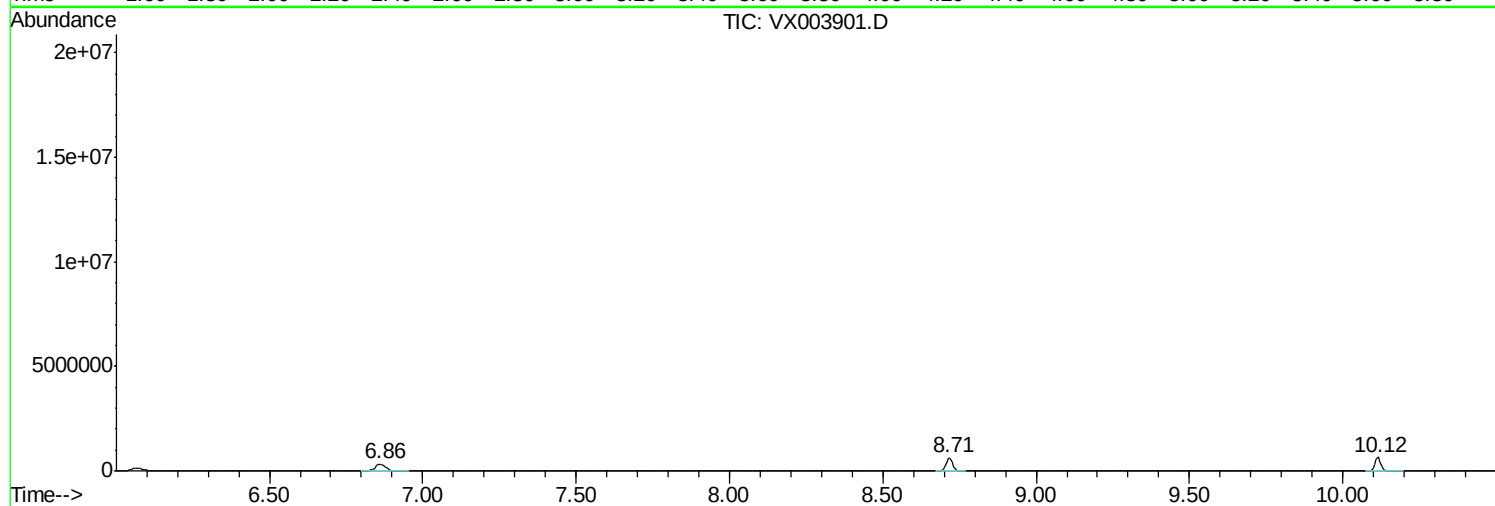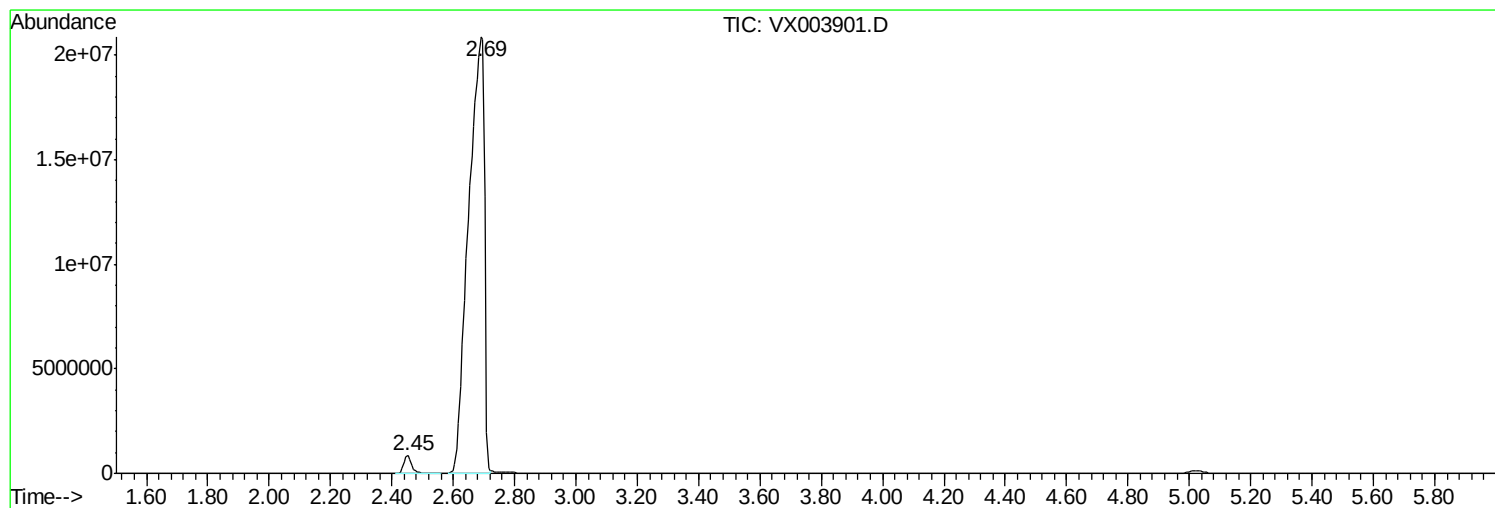

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080718\
Data File : VX003901.D
Acq On : 08 Aug 2018 01:25
Operator : JC/MD
Sample : J4341-01 10X
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN001-SEWER-OUTLET-001










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X072718W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown2.69 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.69	2967.21 ug/l	74685100	Bromochloromethane	5.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	10
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	10
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	8
4		Ethylamine	45	C2H7N	000075-04-7	5
5		Methane, nitroso-	45	CH3NO	000865-40-7	4

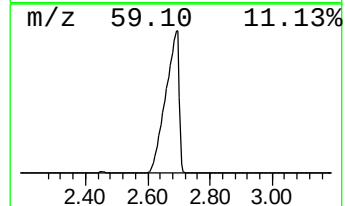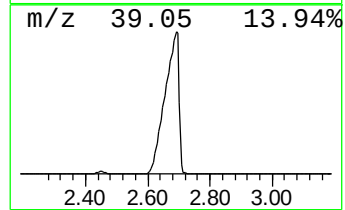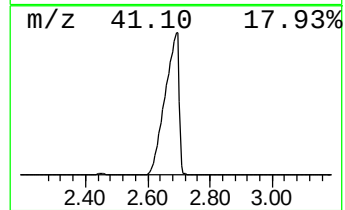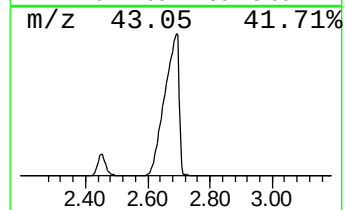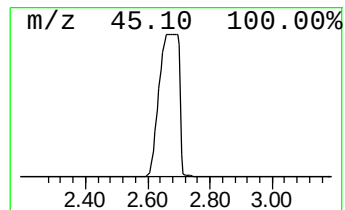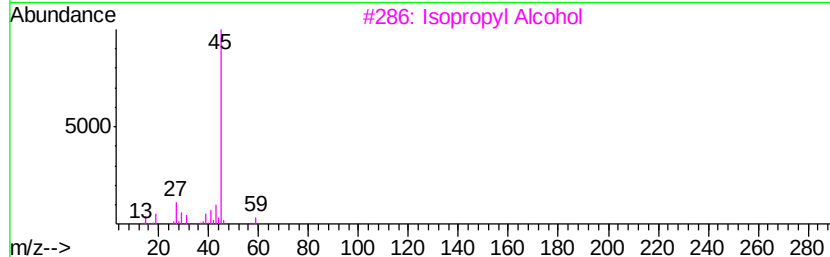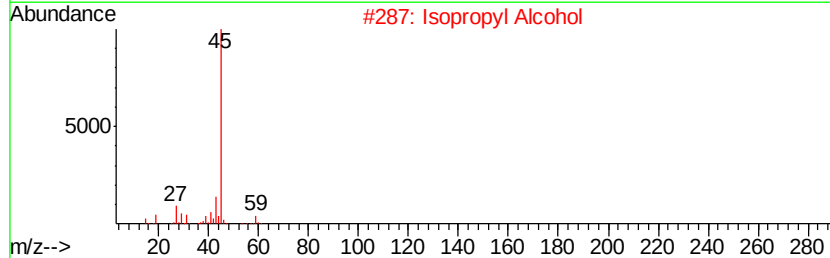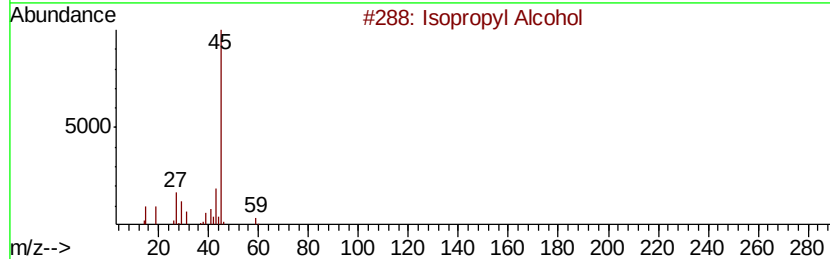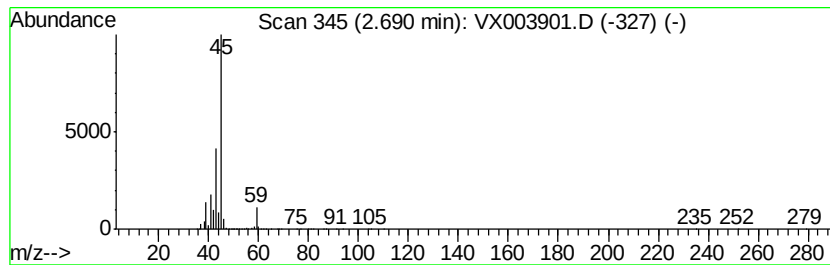

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080718\
Data File : VX003901.D
Acq On : 08 Aug 2018 01:25
Operator : JC/MD
Sample : J4341-01 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN001-SEWER-OUTLET-001

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X072718W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown2.69	2.69	2967.2	ug/l	74685100	1	5.02	755103	30.0