

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080718\
 Data File : VX003912.D
 Acq On : 08 Aug 2018 06:44
 Operator : JC/MD
 Sample : J4344-14
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0537

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	68	80	94	rBV	1128433	1539633	79.13%	13.433%
2	1.605	160	167	172	rBV4	9729	19696	1.01%	0.172%
3	2.617	327	333	344	rVB	57559	106597	5.48%	0.930%
4	4.775	674	687	699	rBV	15462	50890	2.62%	0.444%
5	5.507	792	807	821	rBV	228068	648519	33.33%	5.658%
6	5.666	821	833	847	rVB	334403	926472	47.62%	8.083%
7	6.068	886	899	916	rBV	251097	638964	32.84%	5.575%
8	6.860	1019	1029	1043	rBV	512435	1195134	61.43%	10.428%
9	8.720	1326	1334	1345	rBV	1235169	1945674	100.00%	16.976%
10	10.116	1556	1563	1581	rBV	1086110	1450378	74.54%	12.655%
11	11.140	1725	1731	1742	rBV	1074191	1326557	68.18%	11.574%
12	12.079	1880	1885	1894	rBV	1333614	1612779	82.89%	14.072%


Sum of corrected areas: 11461293

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080718\
Data File : VX003912.D
Acq On : 08 Aug 2018 06:44
Operator : JC/MD
Sample : J4344-14
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0537

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

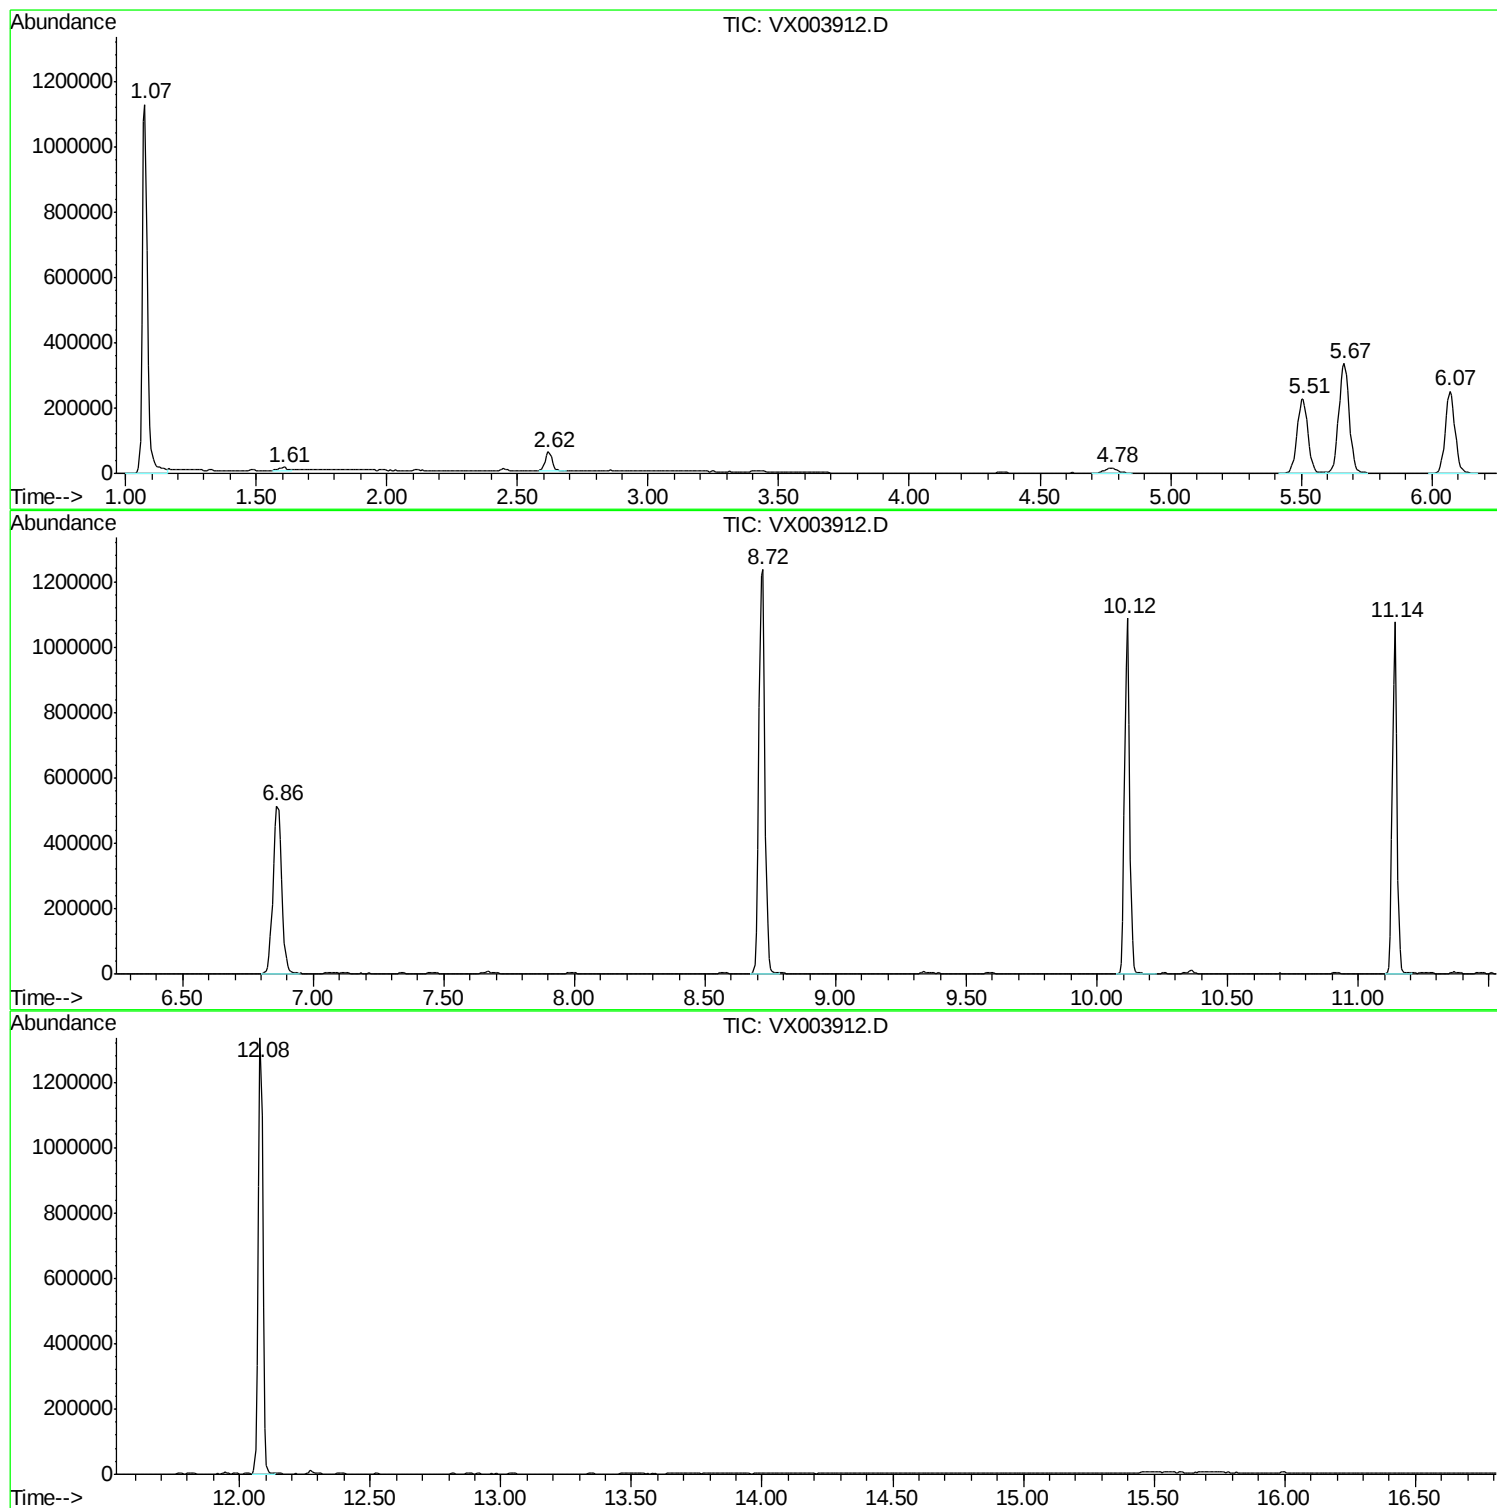

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080718\
Data File : VX003912.D
Acq On : 08 Aug 2018 06:44
Operator : JC/MD
Sample : J4344-14
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0537










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.62	5.75 ug/l	106597	Pentafluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56
3		(R)-(-)-2-Pentanol	88	C5H12O	031087-44-2	9
4		4-Penten-2-ol	86	C5H10O	000625-31-0	9
5		Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9

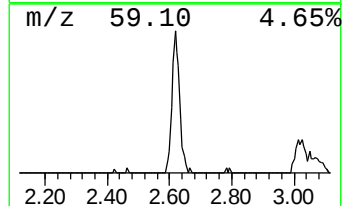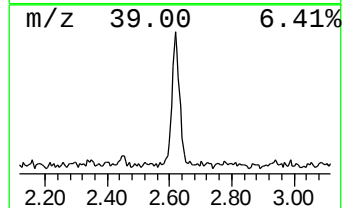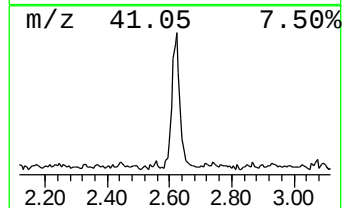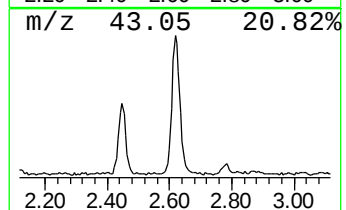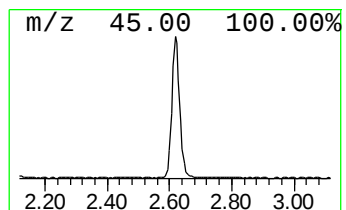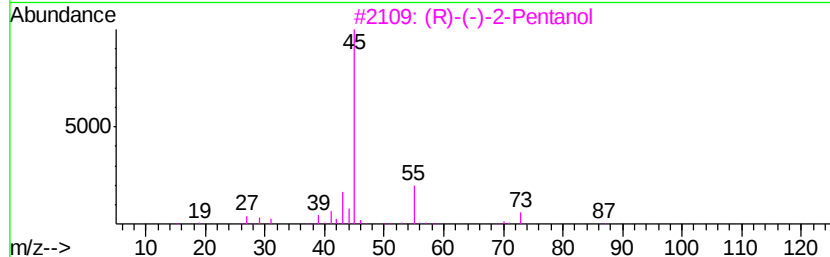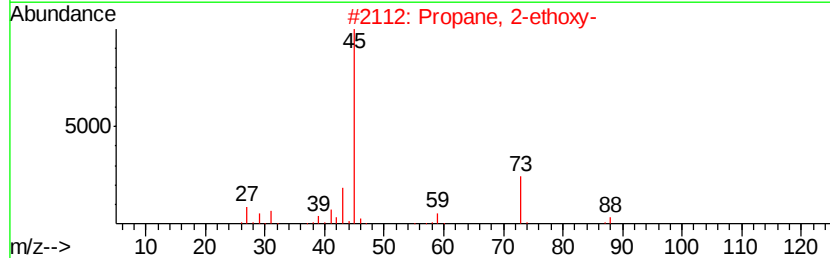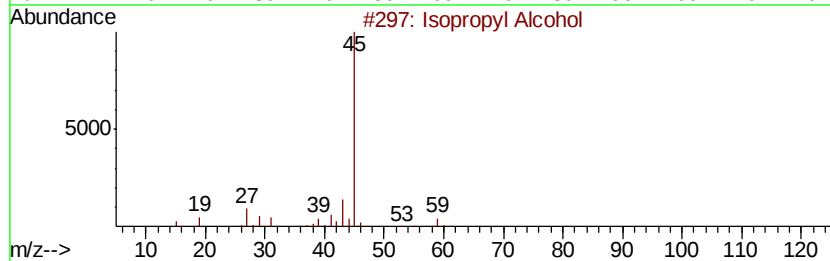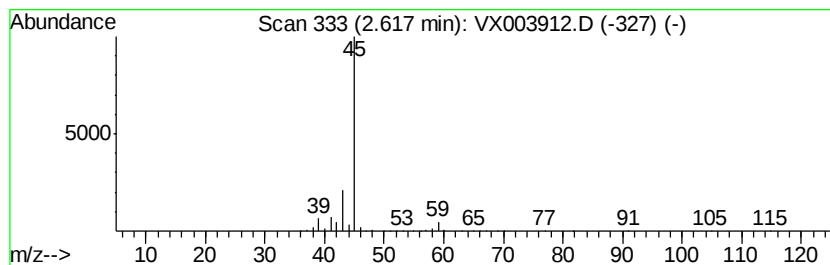

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX080718\
Data File : VX003912.D
Acq On : 08 Aug 2018 06:44
Operator : JC/MD
Sample : J4344-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0537

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.62	5.8	ug/l	106597	1	5.67	926472	50.0