


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX080718\
 Data File : VX003894.D
 Acq On : 07 Aug 2018 21:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
 Title : SW846 8260
 Last Update : Tue Aug 07 07:45:48 2018

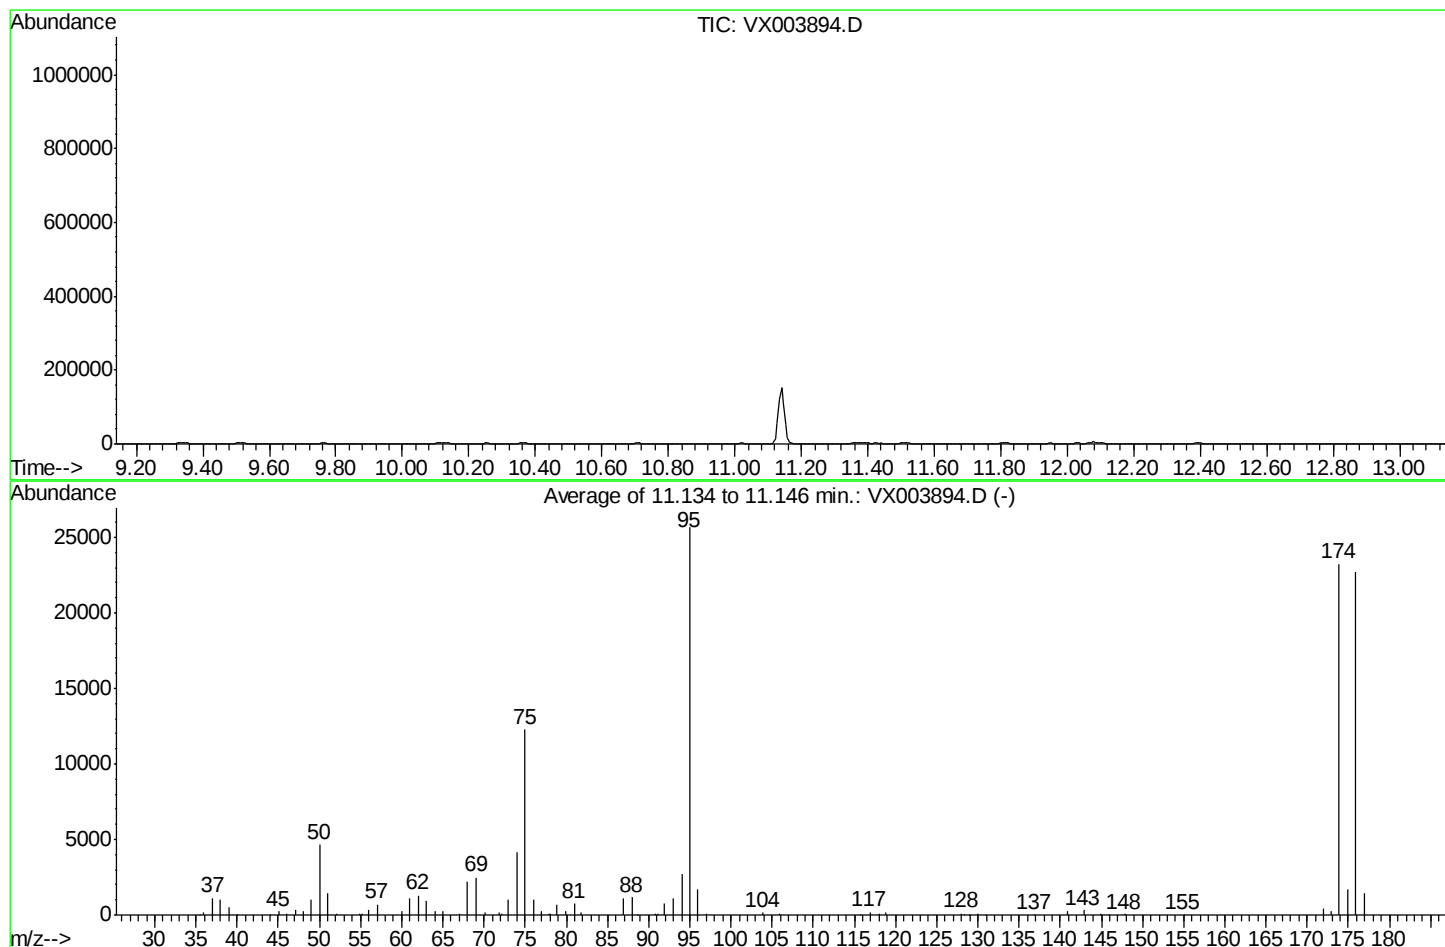

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	4641	PASS
75	95	30	60	47.8	12278	PASS
95	95	100	100	100.0	25672	PASS
96	95	5	9	6.7	1727	PASS
173	174	0.00	2	1.2	278	PASS
174	95	50	100	90.6	23264	PASS
175	174	5	9	7.3	1697	PASS
176	174	95	101	97.7	22733	PASS
177	176	5	9	6.3	1436	PASS