

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080719\
Data File : VX011374.D
Acq On : 07 Aug 2019 19:38
Operator : JC/SP
Sample : K4220-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24S_080719

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	9.360	1334	1346	1351	rBV	50406307	104882336	100.00%	100.000%


Sum of corrected areas: 104882336

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080719\
Data File : VX011374.D
Acq On : 07 Aug 2019 19:38
Operator : JC/SP
Sample : K4220-07
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24S_080719

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

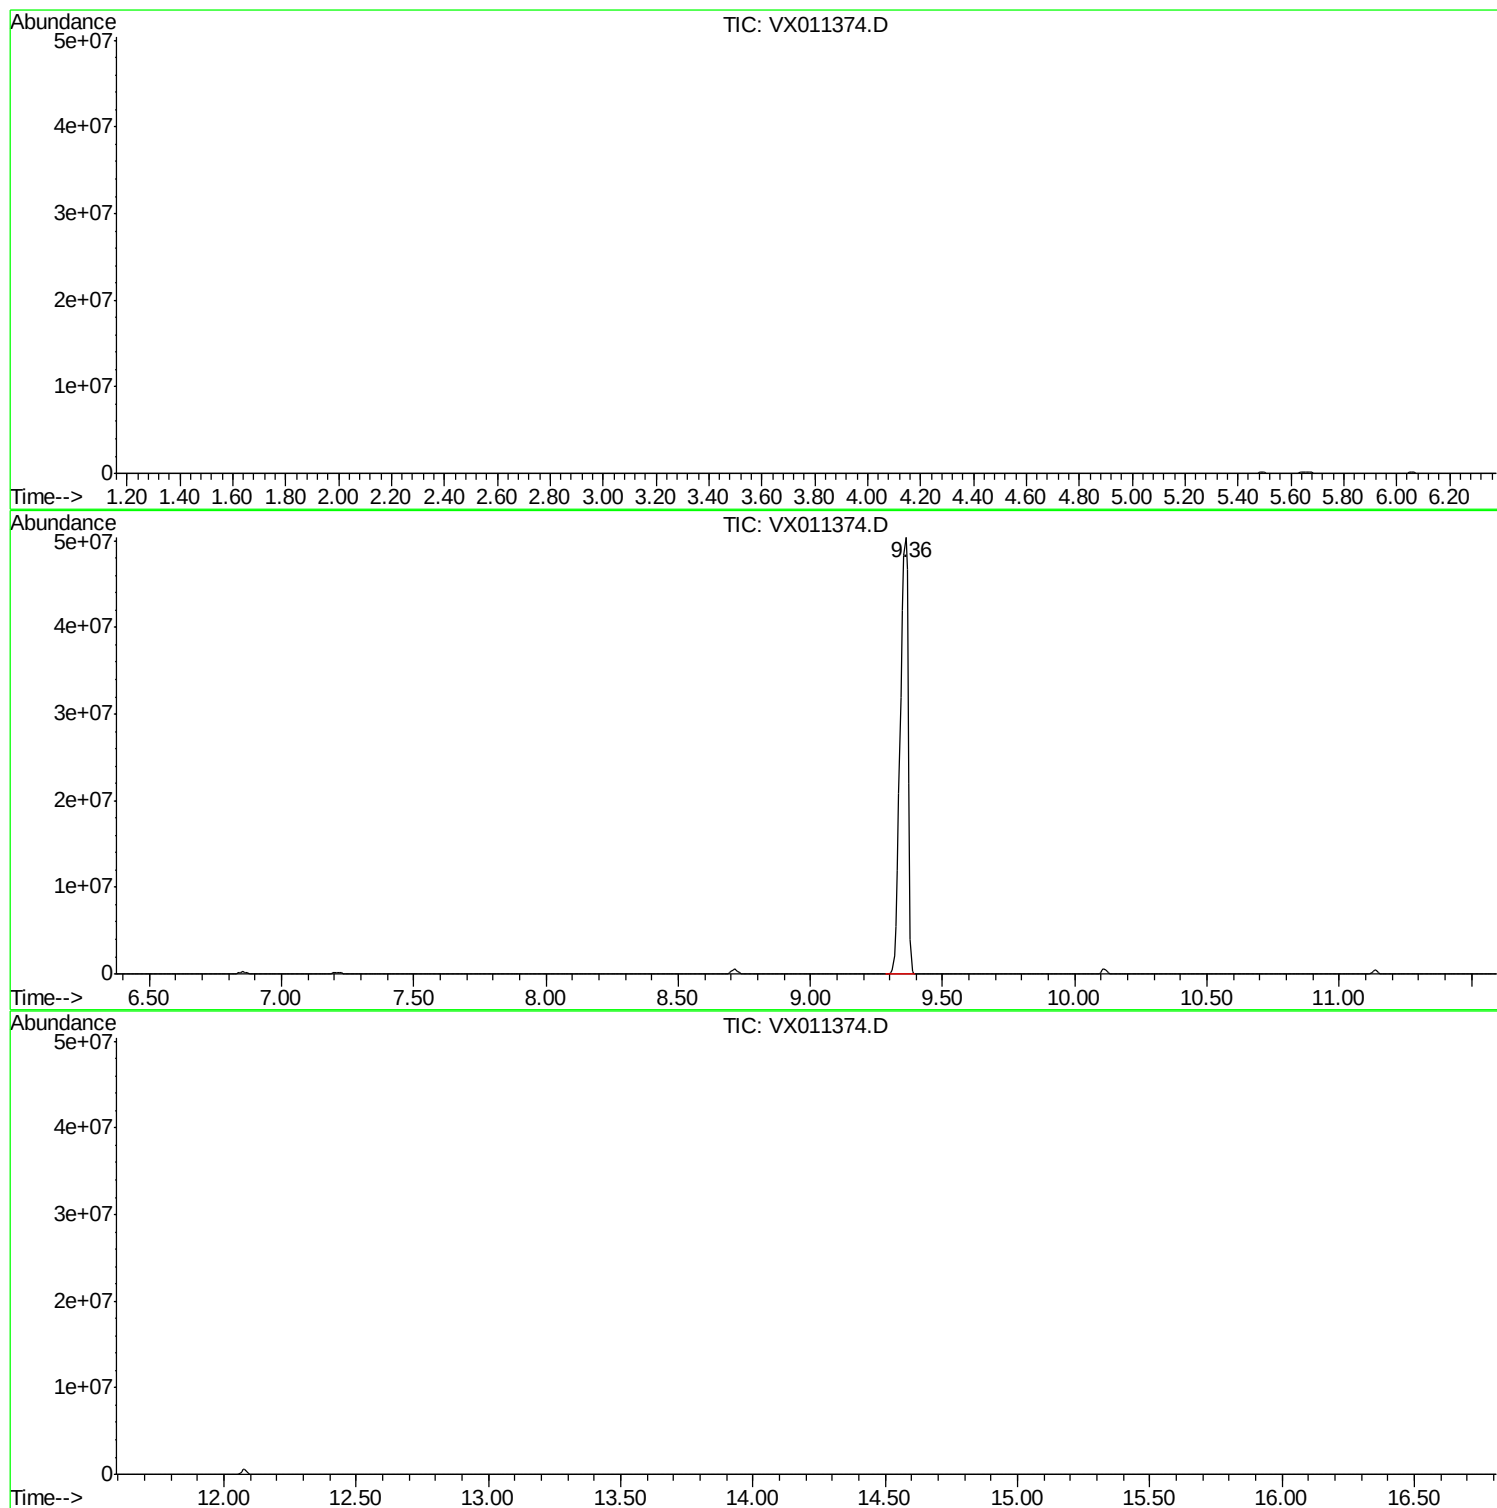

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080719\
Data File : VX011374.D
Acq On : 07 Aug 2019 19:38
Operator : JC/SP
Sample : K4220-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24S_080719

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080719\
Data File : VX011374.D
Acq On : 07 Aug 2019 19:38
Operator : JC/SP
Sample : K4220-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-24S_080719

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc