

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VO080720\
 Data File : VX017828.D
 Acq On : 07 Aug 2020 16:24
 Operator : JC/SP
 Sample : L3675-12
 Misc : 25.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 GAYA6

Quant Time: Aug 08 01:27:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 08 00:10:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.83	114	259524	5.00	ug/L	0.00
28) Chlorobenzene-d5	10.10	117	241050	5.00	ug/L	0.00
61) 1,4-Dichlorobenzene-d4	12.06	152	133392	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	97022	5.41	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	108.20%
7) Chloroethane-d5	1.69	69	79379	5.58	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	111.60%
11) 1,1-Dichloroethene-d2	2.34	63	146449	3.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.40%
20) 2-Butanone-d5	4.53	46	247636	52.00	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.00%
24) Chloroform-d	5.14	84	184206	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
26) 1,2-Dichloroethane-d4	6.03	65	100214	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
32) Benzene-d6	6.05	84	327326	4.95	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.00%
36) 1,2-Dichloropropane-d6	7.37	67	100691	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.40%
41) Toluene-d8	8.70	98	338534	5.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.40%
45) trans-1,3-Dichloropropene-	8.99	79	41920	4.73	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.60%
48) 2-Hexanone-d5	9.43	63	190860	51.84	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.68%
59) 1,1,2,2-Tetrachloroethane-	11.23	84	84550	5.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	108.80%
65) 1,2-Dichlorobenzene-d4	12.36	152	131345	5.11	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.20%


Target Compounds					Qvalue
53) Chlorobenzene	10.12	112	11477	0.190 ug/L	95
55) m,p-xylene	10.34	106	4282	0.111 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080720\
Data File : VX017828.D
Acq On : 07 Aug 2020 16:24
Operator : JC/SP
Sample : L3675-12
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
GAYA6

Quant Time: Aug 08 01:27:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SOMXTR080720WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 08 00:10:20 2020
Response via : Initial Calibration

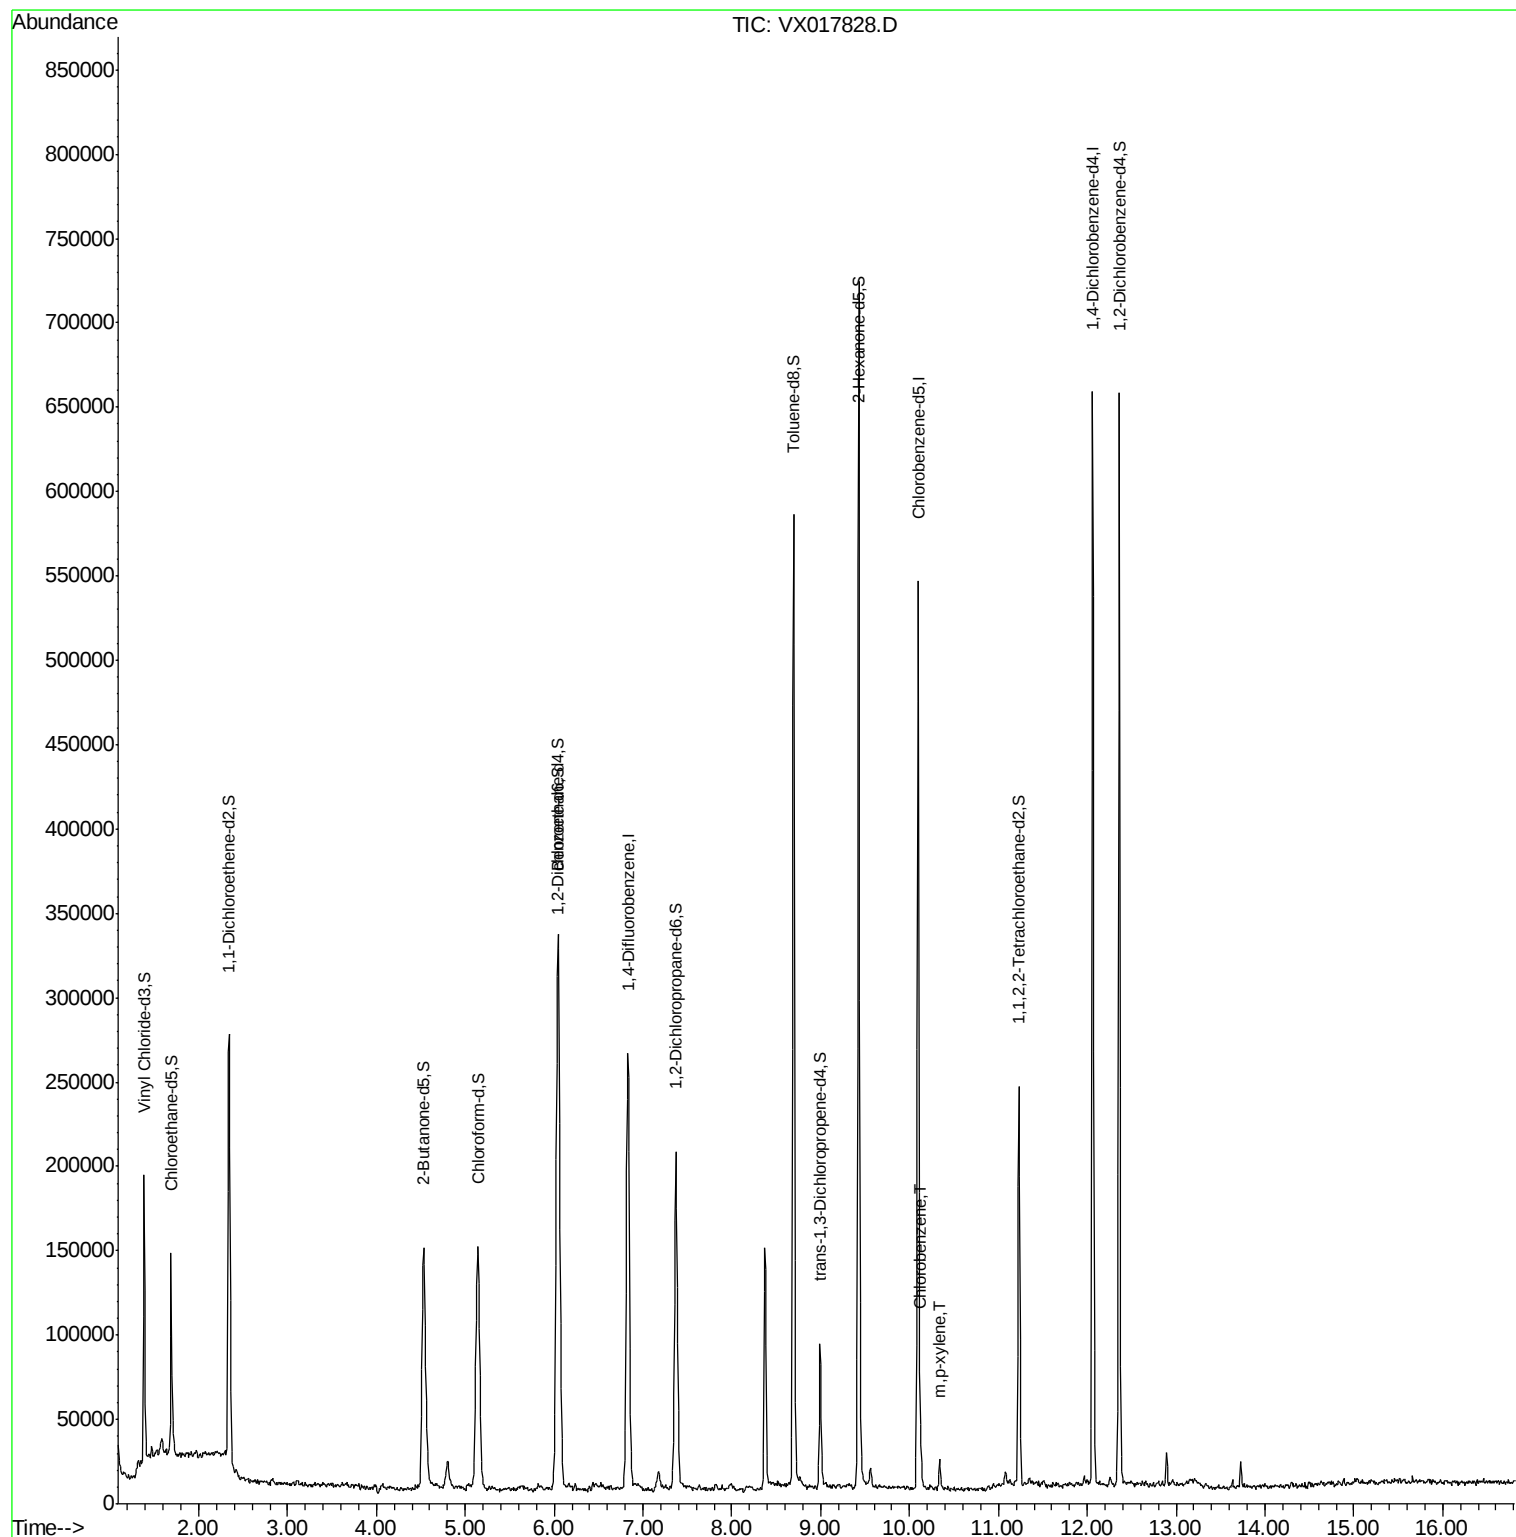

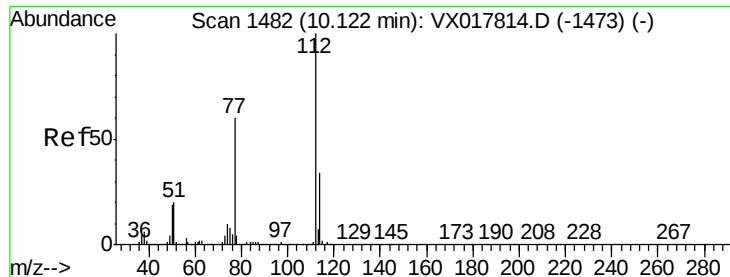

#53

Chlorobenzene

Concen: 0.190 ug/L

RT: 10.12 min Scan# 1482

Delta R.T. 0.00 min

Lab File: VX017828.D

Acq: 07 Aug 2020 16:24

Instrument :

MSVOA_X

ClientSampled :

GAYA6


Tgt Ion:112 Resp: 11477

Ion Ratio Lower Upper

112 100

114 30.5 23.5 43.7




77 55.4 46.7 70.1

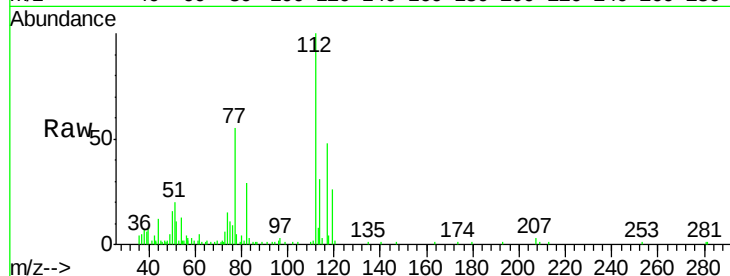

Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VX0

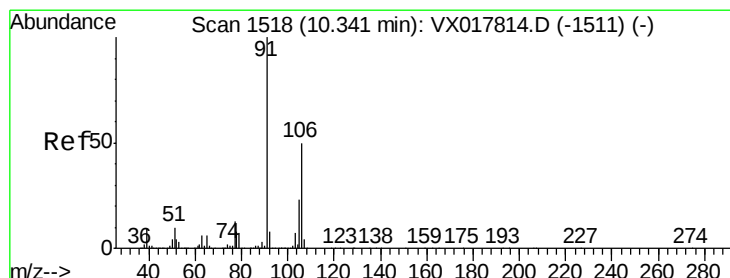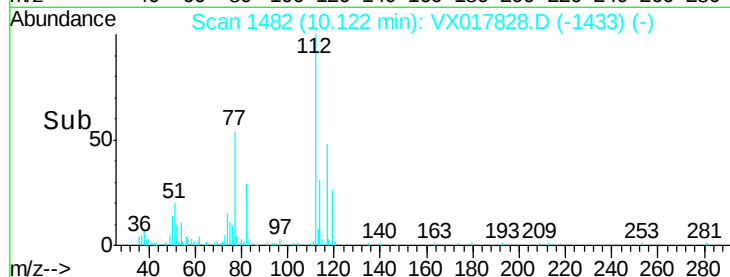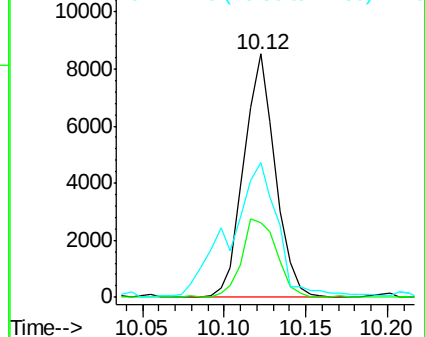

#55

m,p-xylene

Concen: 0.111 ug/L

RT: 10.34 min Scan# 1518

Delta R.T. 0.00 min

Lab File: VX017828.D


Acq: 07 Aug 2020 16:24

Tgt Ion:106 Resp: 4282

Ion Ratio Lower Upper

106 100

91 187.7 143.3 266.1

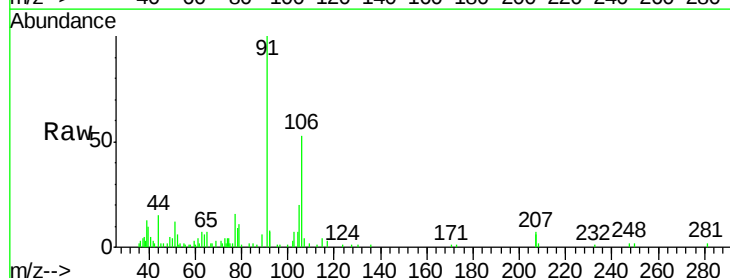

Abundance Ion 106.15 (105.85 to 106.85): V

Ion 91.15 (90.85 to 91.85): VX0

