

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080724\
 Data File : VX042892.D
 Acq On : 07 Aug 2024 01:43
 Operator : JC/MD
 Sample : P3448-06RE
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP3

Quant Time: Aug 07 06:31:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 07 02:55:22 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	136976	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	261160	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	256093	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	105032	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	108874	57.899	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 115.800%	
35) Dibromofluoromethane	5.385	113	91939	53.841	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 107.680%	
50) Toluene-d8	8.647	98	320574	52.882	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 105.760%	
62) 4-Bromofluorobenzene	11.079	95	116286	53.382	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 106.760%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.288	50	350	0.218	ug/l #	43
5) Bromomethane	1.611	94	924	1.000	ug/l #	73
6) Chloroethane	1.648	64	626	0.720	ug/l #	43
11) Tert butyl alcohol	2.995	59	998	2.668	ug/l #	78
13) Acrolein	2.239	56	202	0.548	ug/l #	1
14) Allyl chloride	2.654	41	1220	0.535	ug/l #	47
16) Acetone	2.392	43	84052	103.054	ug/l	99
17) Carbon Disulfide	2.501	76	1521	0.414	ug/l	97
18) Methyl Acetate	2.715	43	5126	1.982	ug/l	98
20) Methylene Chloride	2.788	84	12913	6.796	ug/l #	86
25) 2-Butanone	4.586	43	11660	9.103	ug/l #	86
29) Tetrahydrofuran	5.037	42	582	0.672	ug/l #	34
31) Cyclohexane	5.550	56	3046	1.295	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	10323	4.459	ug/l #	51
37) Ethyl Acetate	4.751	43	2918	1.007	ug/l #	93
38) Carbon Tetrachloride	5.550	117	13982	5.350	ug/l #	15
43) Isopropyl Acetate	6.348	43	157306	36.720	ug/l	97
48) Methyl methacrylate	7.616	41	4993	2.431	ug/l #	16
49) 1,4-Dioxane	7.805	88	193	4.233	ug/l #	1
51) 4-Methyl-2-Pentanone	8.549	43	114249	39.815	ug/l #	47
53) t-1,3-Dichloropropene	8.964	75	971	0.422	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	52159	20.545	ug/l #	56
57) 1,3-Dichloropropane	9.482	76	6274	2.162	ug/l #	42
59) 2-Hexanone	9.482	43	80901	36.384	ug/l #	53
74) N-amyl acetate	10.640	43	14533	4.253	ug/l #	54
76) 1,2,3-Trichloropropane	11.079	75	59093	25.017	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.079	75	59093	81.342	ug/l #	5
84) 1,2,4-Trimethylbenzene	11.756	105	1948	0.308	ug/l	100
93) 1,2,4-Trichlorobenzene	13.597	180	540	0.253	ug/l #	86
95) Naphthalene	13.780	128	1599	0.216	ug/l #	81
96) 1,2,3-Trichlorobenzene	13.963	180	539	0.251	ug/l #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080724\
Data File : VX042892.D
Acq On : 07 Aug 2024 01:43
Operator : JC/MD
Sample : P3448-06RE
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP3

Quant Time: Aug 07 06:31:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 07 02:55:22 2024
Response via : Initial Calibration




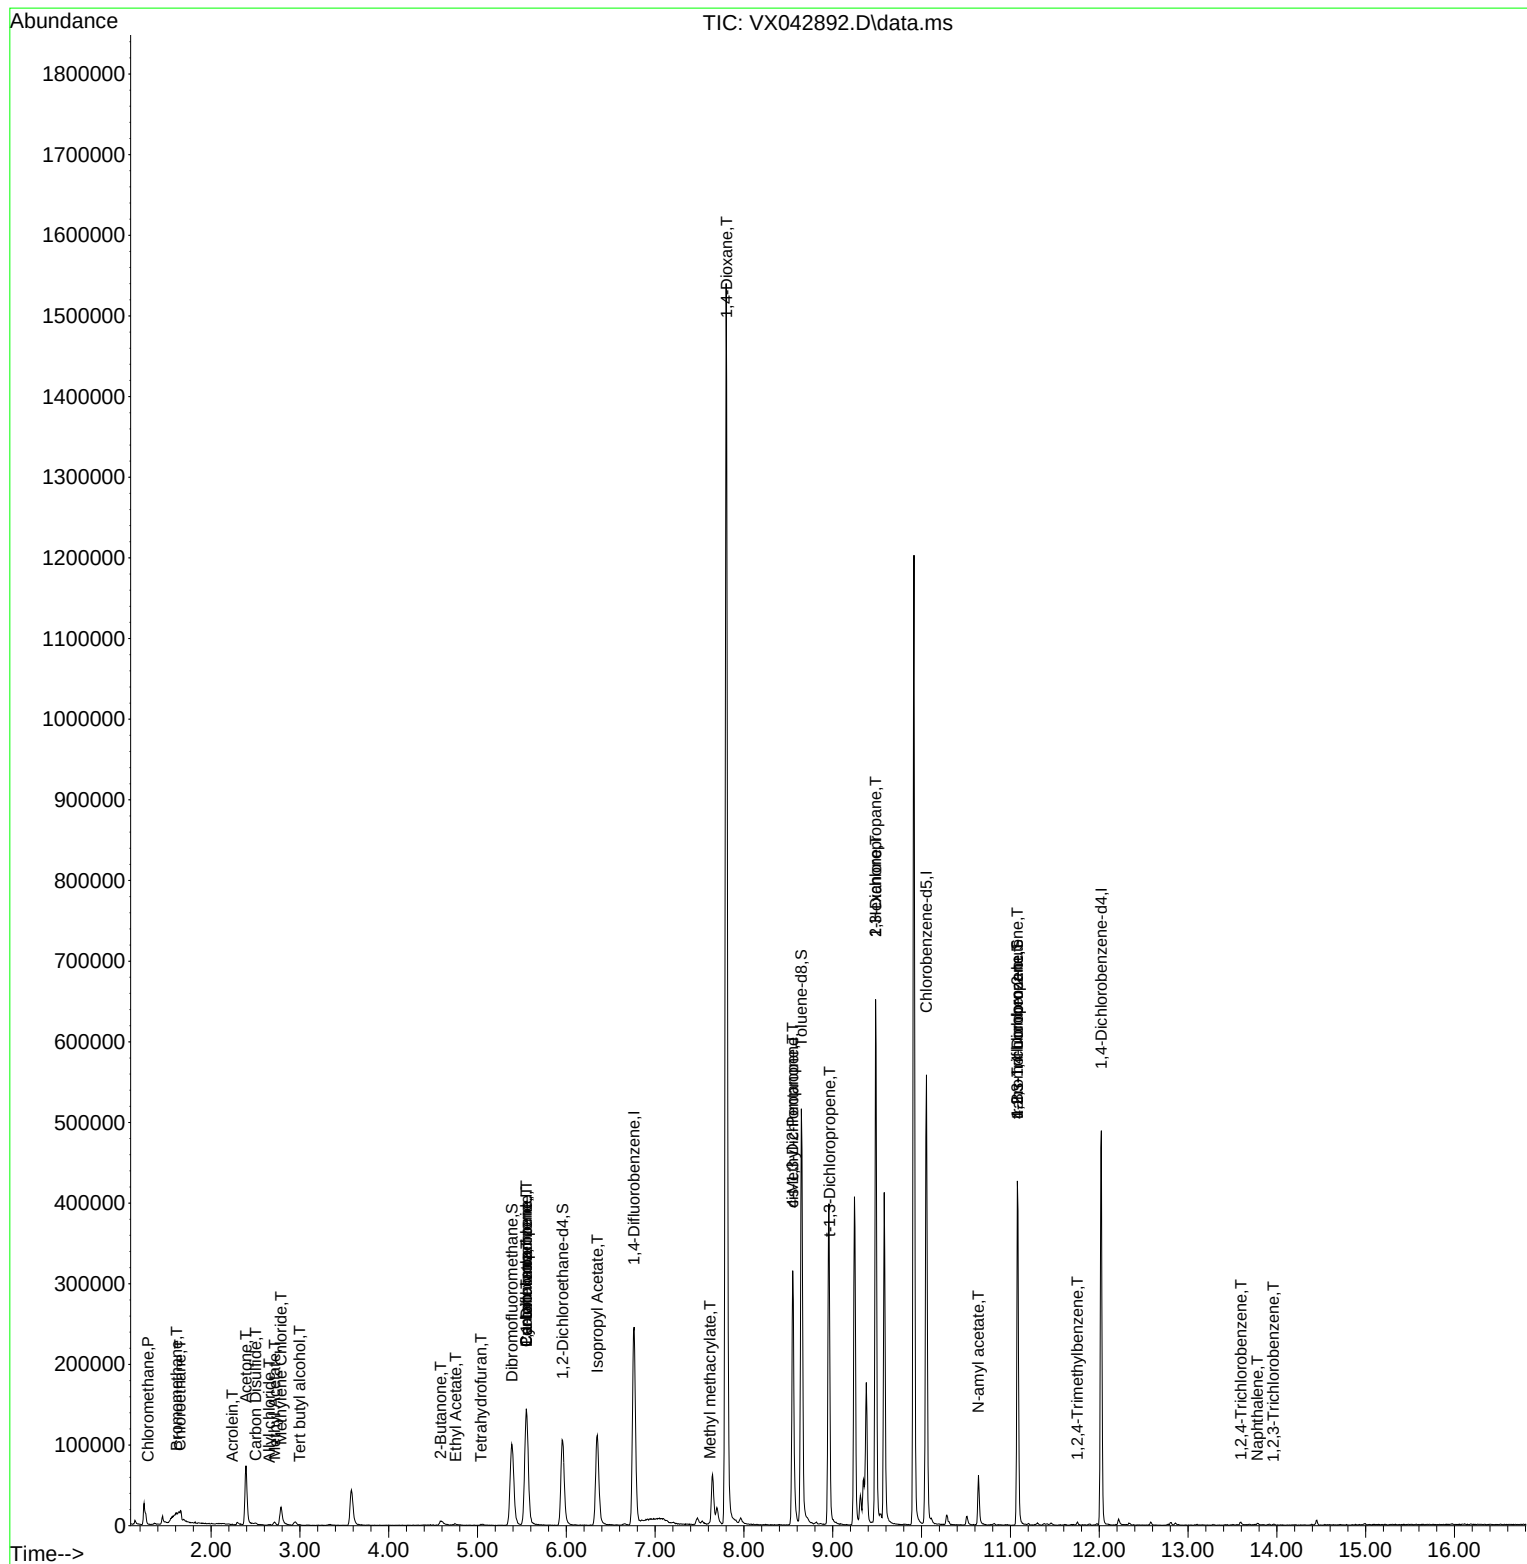




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion:168 Resp: 136976
Ion Ratio Lower Upper
168 100
99 60.7 56.6 85.0

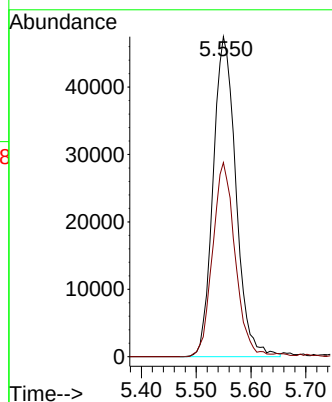

#3
Chloromethane
Concen: 0.218 ug/l
RT: 1.288 min Scan# 33
Delta R.T. -0.013 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 50 Resp: 350
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#




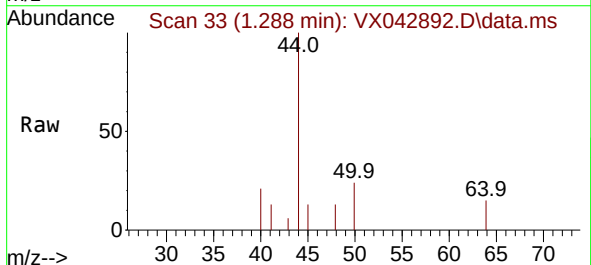


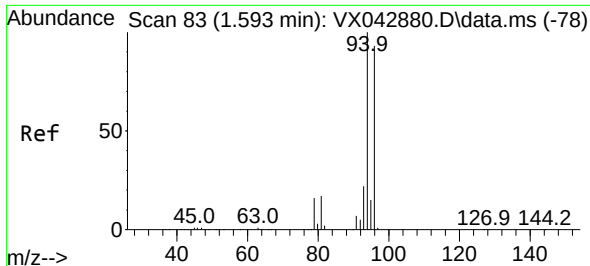

#5
Bromomethane
Concen: 1.000 ug/l
RT: 1.611 min Scan# 80
Delta R.T. 0.018 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion: 94 Resp: 924
Ion Ratio Lower Upper
94 100
96 67.0 74.6 111.8#

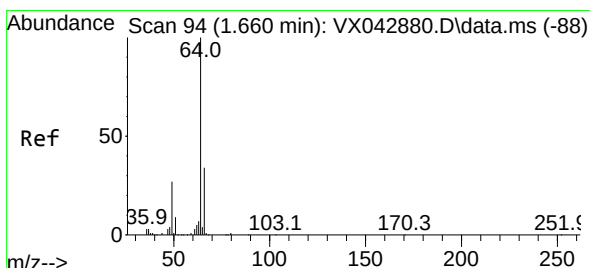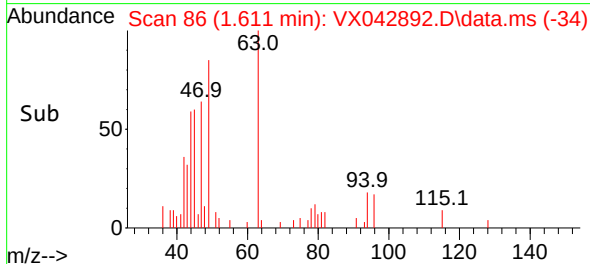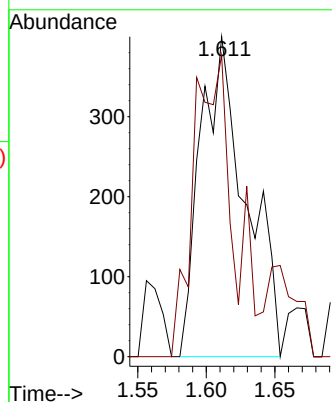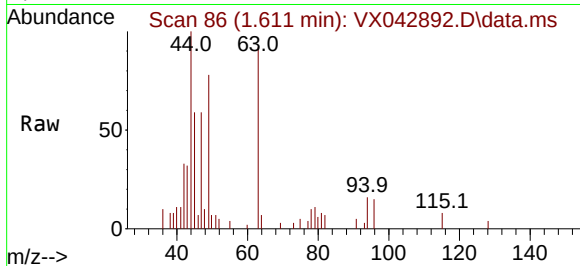

#6
Chloroethane
Concen: 0.720 ug/l
RT: 1.648 min Scan# 92
Delta R.T. -0.013 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 64 Resp: 626
Ion Ratio Lower Upper
64 100
66 0.0 25.1 37.7#

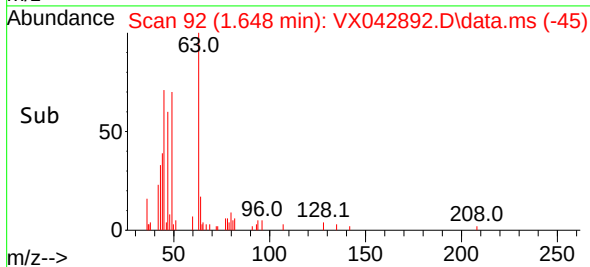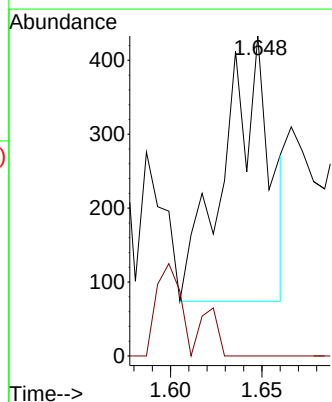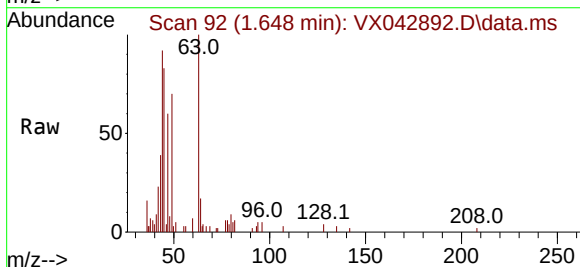

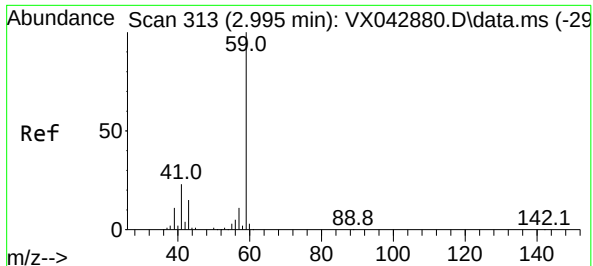

#11

Tert butyl alcohol

Concen: 2.668 ug/l

RT: 2.995 min Scan# 313

Delta R.T. -0.000 min

Lab File: VX042892.D

Acq: 07 Aug 2024 01:43

Instrument :

MSVOA_X

ClientSampleId :





TP3

Tgt Ion: 59 Resp: 998

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#

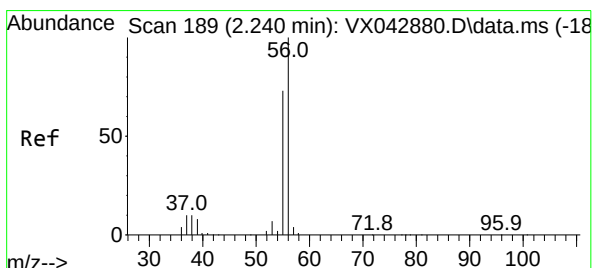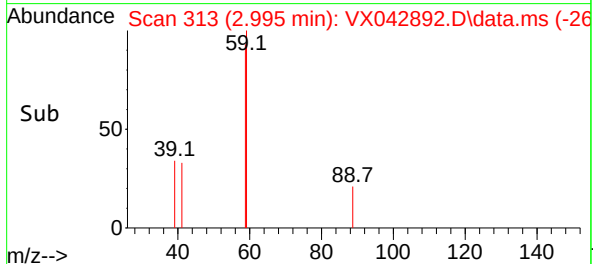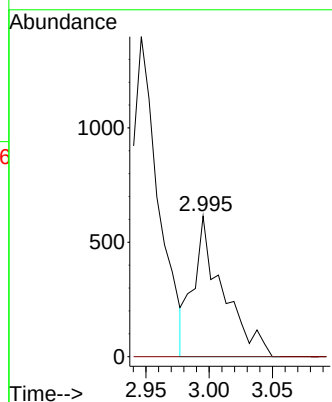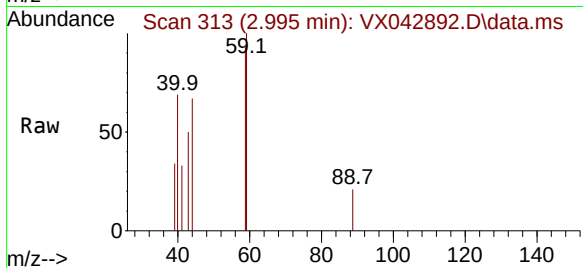

#13

Acrolein

Concen: 0.548 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.000 min

Lab File: VX042892.D




Acq: 07 Aug 2024 01:43


Tgt Ion: 56 Resp: 202

Ion Ratio Lower Upper

56 100

55 185.6 57.1 85.7#


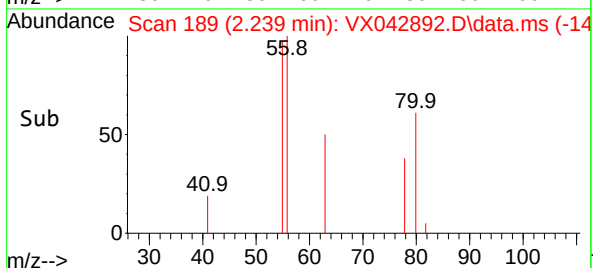

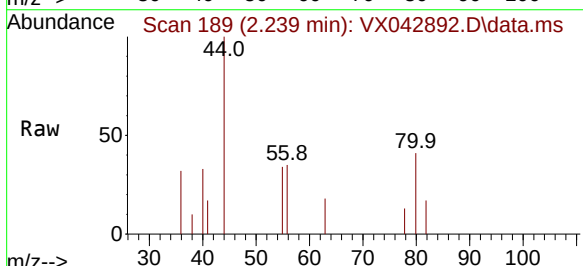




#14
 Allyl chloride
 Concen: 0.535 ug/l
 RT: 2.654 min Scan# 214
 Delta R.T. -0.006 min
 Lab File: VX042892.D
 Acq: 07 Aug 2024 01:43




Instrument :
 MSVOA_X
 ClientSampleId :
 TP3


Tgt Ion: 41 Resp: 1220
 Ion Ratio Lower Upper
 41 100
 39 27.4 55.8 83.6#
 76 0.0 24.3 36.5#

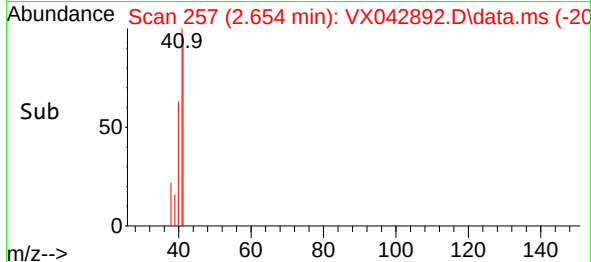

#16
 Acetone
 Concen: 103.054 ug/l
 RT: 2.392 min Scan# 214
 Delta R.T. -0.000 min
 Lab File: VX042892.D
 Acq: 07 Aug 2024 01:43

Tgt Ion: 43 Resp: 84052
 Ion Ratio Lower Upper
 43 100
 58 28.2 21.9 32.9




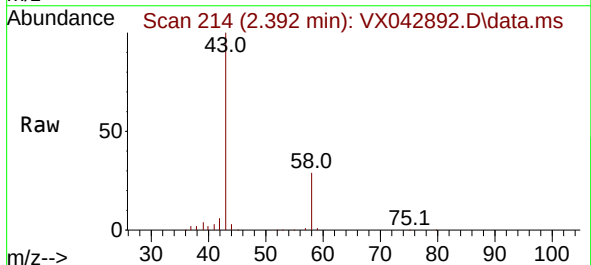




#17
Carbon Disulfide
Concen: 0.414 ug/l
RT: 2.501 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion: 76 Resp: 1521
Ion Ratio Lower Upper
76 100
78 9.8 7.0 10.6



#18
Methyl Acetate
Concen: 1.982 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 43 Resp: 5126
Ion Ratio Lower Upper
43 100
74 21.3 17.8 26.8


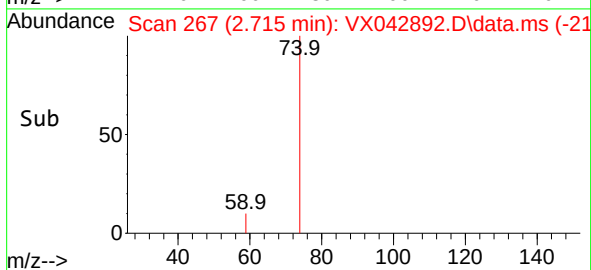






#20
Methylene Chloride
Concen: 6.796 ug/l
RT: 2.788 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion:	84	Resp:	12913
Ion	Ratio	Lower	Upper
84	100		
49	107.6	103.6	155.4
51	33.4	33.8	50.6#
86	63.3	49.4	74.0

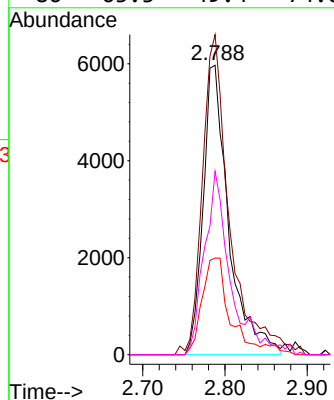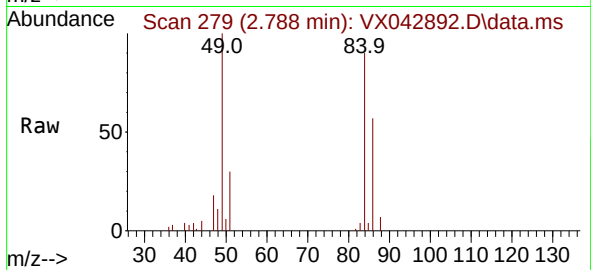

#25
2-Butanone
Concen: 9.103 ug/l
RT: 4.586 min Scan# 574
Delta R.T. 0.018 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion:	43	Resp:	11660
Ion	Ratio	Lower	Upper
43	100		
72	17.6	19.4	29.2#

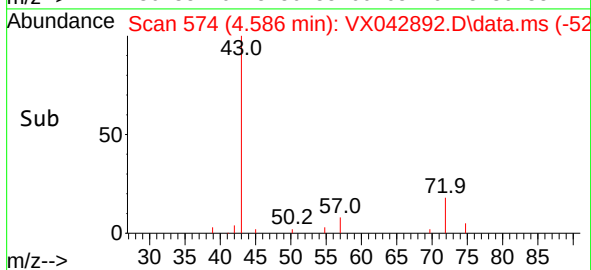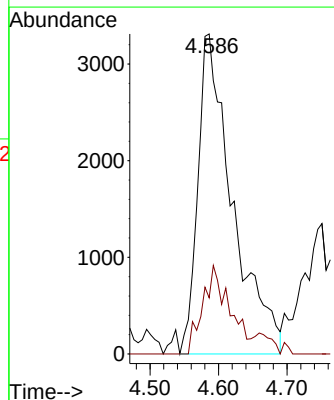

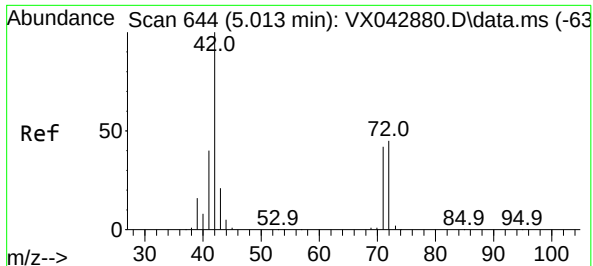

#29

Tetrahydrofuran

Concen: 0.672 ug/l

RT: 5.037 min Scan# 644

Delta R.T. 0.024 min

Lab File: VX042892.D

Acq: 07 Aug 2024 01:43

Instrument :

MSVOA_X

ClientSampleId :

TP3





Tgt Ion: 42 Resp: 582

Ion Ratio Lower Upper

42 100

72 0.0 34.2 51.4#

71 0.0 32.2 48.2#

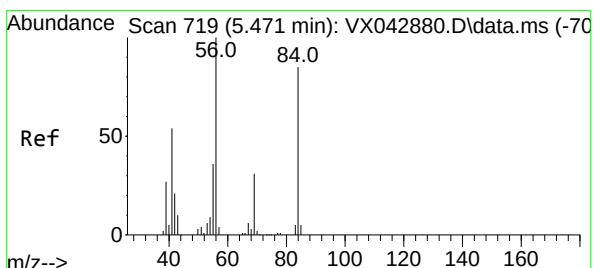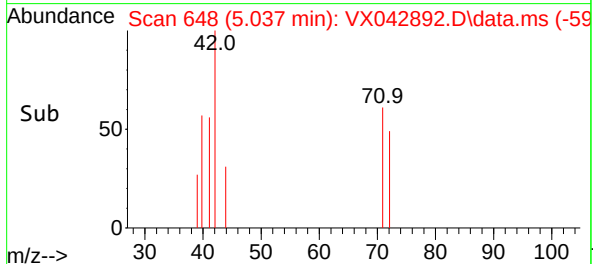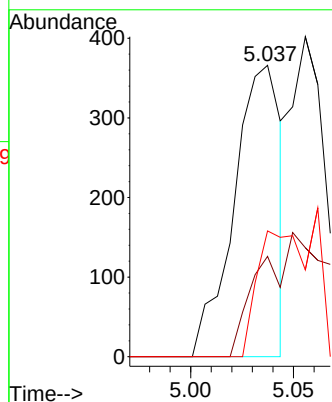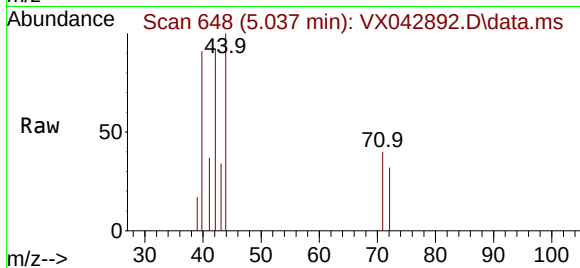

#31

Cyclohexane

Concen: 1.295 ug/l

RT: 5.550 min Scan# 732

Delta R.T. 0.079 min

Lab File: VX042892.D

Acq: 07 Aug 2024 01:43




Tgt Ion: 56 Resp: 3046


Ion Ratio Lower Upper

56 100

69 162.4 23.4 35.2#

84 132.1 65.9 98.9#

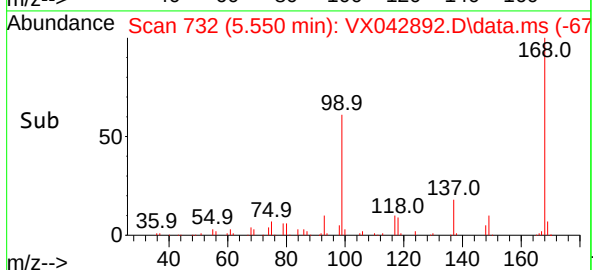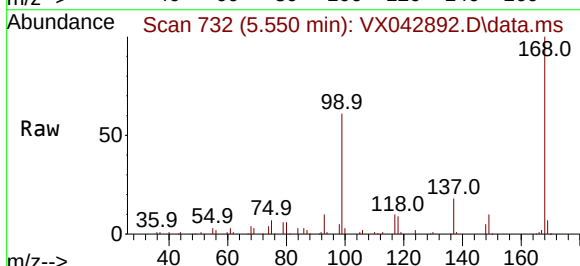



#33

1,2-Dichloroethane-d4

Concen: 57.899 ug/l

RT: 5.958 min Scan# 798

Delta R.T. 0.006 min

Lab File: VX042892.D

Acq: 07 Aug 2024 01:43

Instrument :

MSVOA_X

ClientSampleId :





TP3

Tgt Ion: 65 Resp: 108874

Ion Ratio Lower Upper

65 100

67 52.3 0.0 100.2

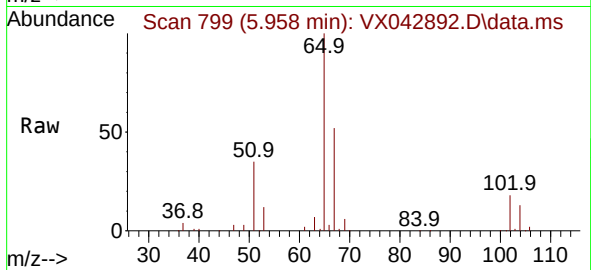

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX042892.D

Acq: 07 Aug 2024 01:43




Tgt Ion: 114 Resp: 261160


Ion Ratio Lower Upper

114 100

63 20.8 0.0 45.0

88 16.9 0.0 36.6


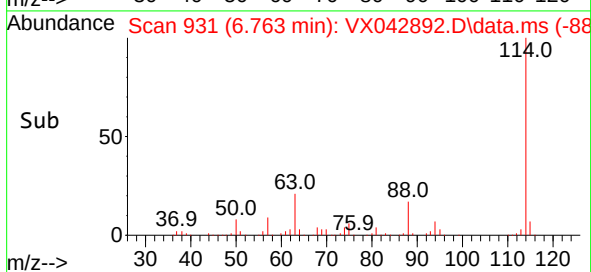






#35
Dibromofluoromethane
Concen: 53.841 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion:113 Resp: 91939
Ion Ratio Lower Upper
113 100
111 103.4 82.9 124.3
192 19.1 13.3 19.9

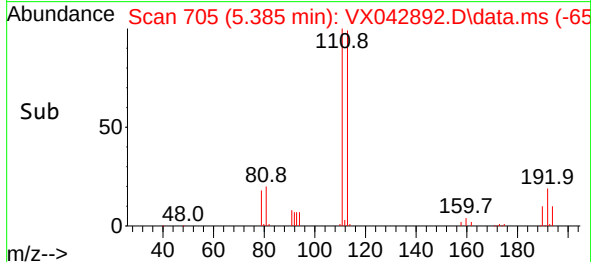

#36
1,1-Dichloropropene
Concen: 4.459 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.134 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 75 Resp: 10323
Ion Ratio Lower Upper
75 100
110 10.0 17.0 50.9#
77 0.0 24.7 37.1#




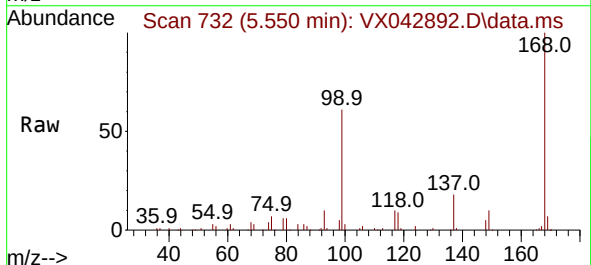




#37
Ethyl Acetate
Concen: 1.007 ug/l
RT: 4.751 min Scan# 601
Delta R.T. 0.030 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion: 43 Resp: 2918
Ion Ratio Lower Upper
43 100
61 11.3 10.6 16.0
70 6.9 8.3 12.5#

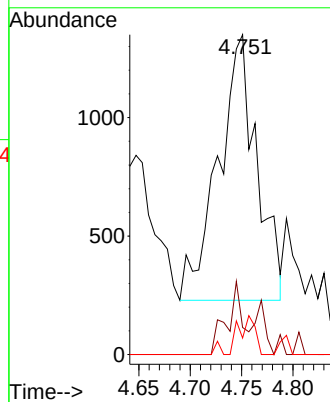

#38
Carbon Tetrachloride
Concen: 5.350 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.128 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 117 Resp: 13982
Ion Ratio Lower Upper
117 100
119 5.3 78.2 117.2#
121 0.0 24.4 36.6#


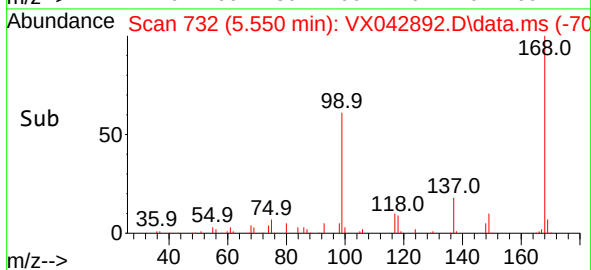
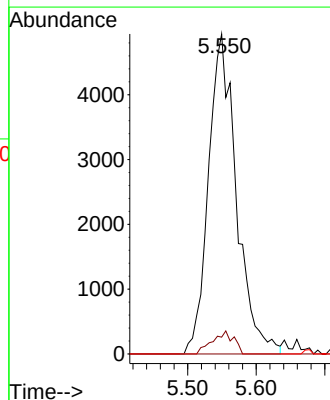





#43
Isopropyl Acetate
Concen: 36.720 ug/l
RT: 6.348 min Scan# 863
Delta R.T. -0.000 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion: 43 Resp: 157306
Ion Ratio Lower Upper
43 100
61 20.6 15.2 22.8
87 13.4 9.8 14.6

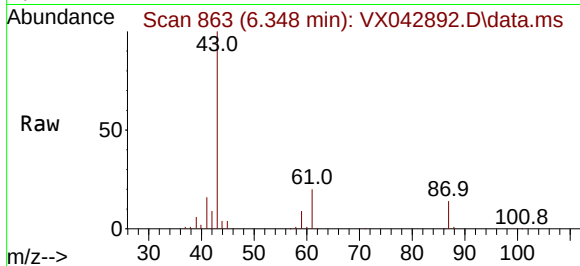

#48
Methyl methacrylate
Concen: 2.431 ug/l
RT: 7.616 min Scan# 1071
Delta R.T. -0.080 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 41 Resp: 4993
Ion Ratio Lower Upper
41 100
69 0.0 59.2 88.8#
39 0.0 47.7 71.5#

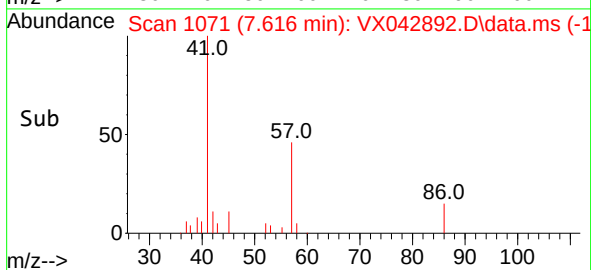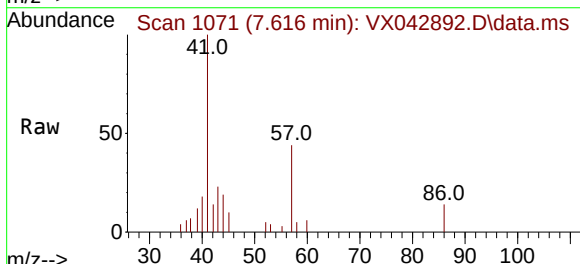



#49

1,4-Dioxane

Concen: 4.233 ug/l

RT: 7.805 min Scan# 1102

Delta R.T. 0.140 min

Lab File: VX042892.D

Acq: 07 Aug 2024 01:43

Instrument :

MSVOA_X

ClientSampleId :

TP3





Tgt Ion: 88 Resp: 193

Ion Ratio Lower Upper

88 100

43 740208.3 0.0 0.0#

58 3569.9 60.1 90.1#



#50

Toluene-d8

Concen: 52.882 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. -0.000 min

Lab File: VX042892.D




Acq: 07 Aug 2024 01:43


Tgt Ion: 98 Resp: 320574

Ion Ratio Lower Upper

98 100

100 63.5 53.1 79.7


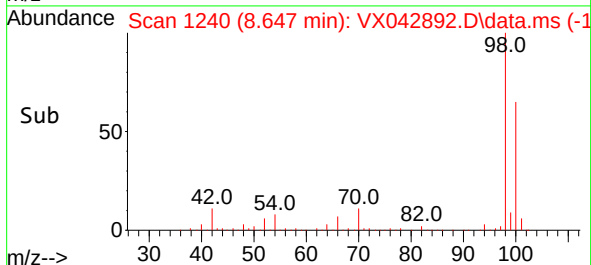






#51
4-Methyl-2-Pentanone
Concen: 39.815 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.031 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion: 43 Resp: 114249
Ion Ratio Lower Upper
43 100
58 6.2 30.4 45.6#

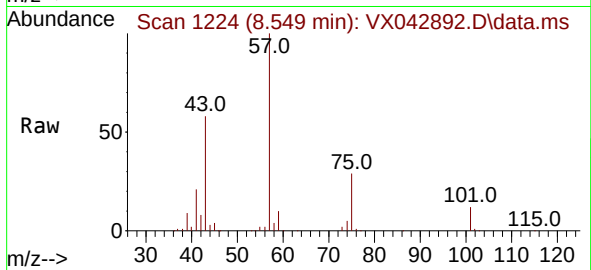

#53
t-1,3-Dichloropropene
Concen: 0.422 ug/l
RT: 8.964 min Scan# 1292
Delta R.T. -0.019 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 75 Resp: 971
Ion Ratio Lower Upper
75 100
77 0.0 25.7 38.5#



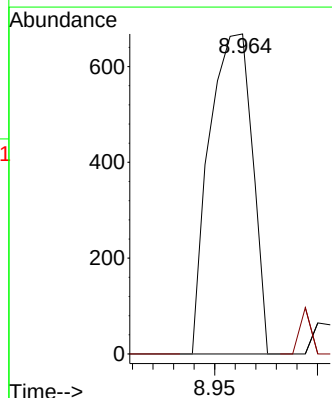





#54
 cis-1,3-Dichloropropene
 Concen: 20.545 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX042892.D
 Acq: 07 Aug 2024 01:43




Instrument :
 MSVOA_X
 ClientSampleId :
 TP3


Tgt Ion: 75 Resp: 52159
 Ion Ratio Lower Upper
 75 100
 77 0.9 25.3 37.9#
 39 29.7 46.7 70.1#

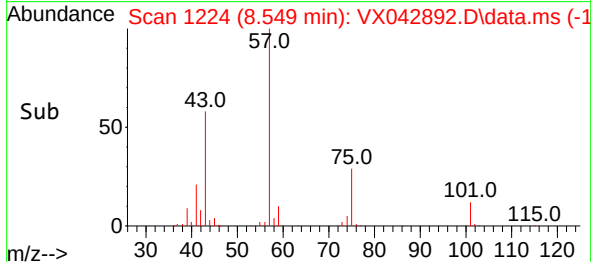

#57
 1,3-Dichloropropane
 Concen: 2.162 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.170 min
 Lab File: VX042892.D
 Acq: 07 Aug 2024 01:43

Tgt Ion: 76 Resp: 6274
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.1 39.1#




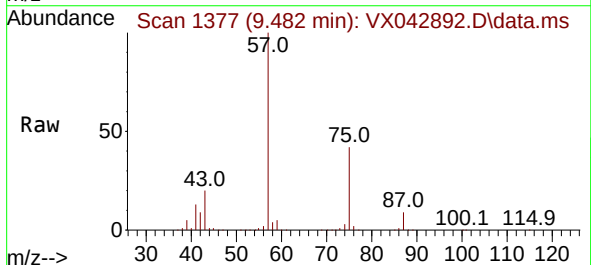




#59
2-Hexanone
Concen: 36.384 ug/l
RT: 9.482 min Scan# 1377
Delta R.T. 0.048 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion: 43 Resp: 80901
Ion Ratio Lower Upper
43 100
58 19.1 26.2 78.5#



#62
4-Bromofluorobenzene
Concen: 53.382 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 95 Resp: 116286
Ion Ratio Lower Upper
95 100
174 79.2 0.0 135.6
176 77.5 0.0 131.0


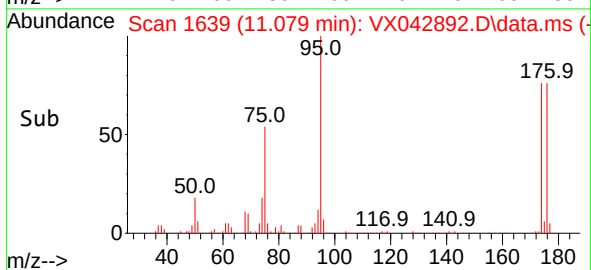






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion:117 Resp: 256093
Ion Ratio Lower Upper
117 100
82 56.5 46.2 69.4
119 31.2 25.5 38.3

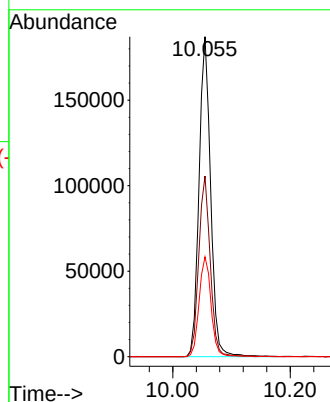

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion:152 Resp: 105032
Ion Ratio Lower Upper
152 100
115 60.6 43.3 129.9
150 158.3 0.0 345.0

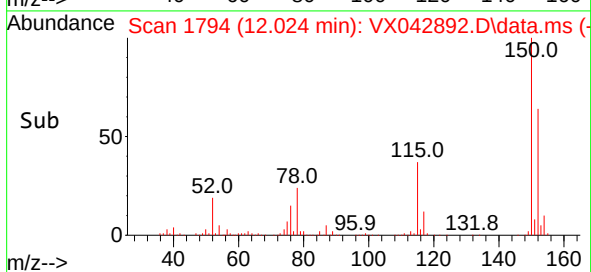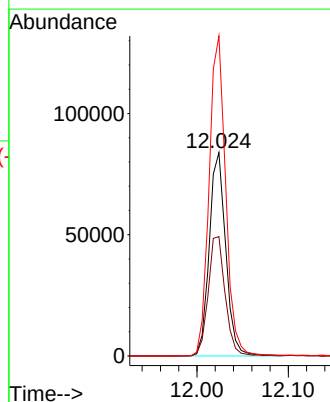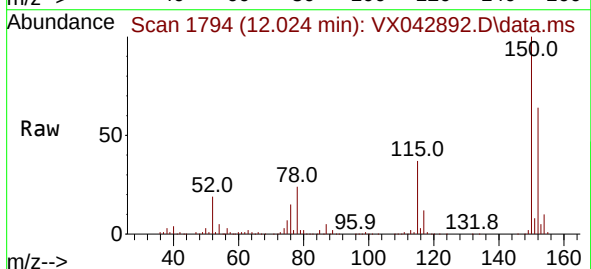



#74

N-amy1 acetate

Concen: 4.253 ug/l

RT: 10.640 min Scan# 1

Delta R.T. -0.202 min

Lab File: VX042892.D

Acq: 07 Aug 2024 01:43

Instrument :

MSVOA_X

ClientSampleId :

TP3

Tgt Ion: 43 Resp: 14533





Ion Ratio Lower Upper

43 100

70 2.7 32.9 49.3#

55 4.6 19.3 28.9#

61 10.8 18.8 28.2#

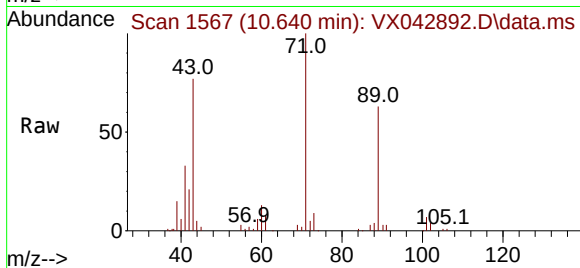

#76

1,2,3-Trichloropropane

Concen: 25.017 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX042892.D




Acq: 07 Aug 2024 01:43


Tgt Ion: 75 Resp: 59093

Ion Ratio Lower Upper

75 100

77 1.3 19.1 57.5#




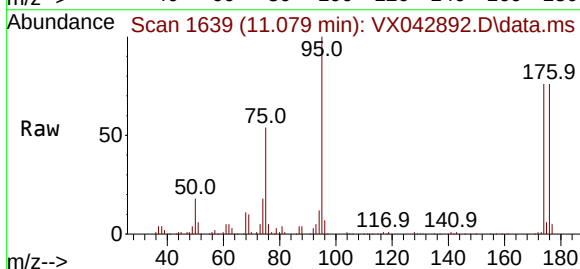




#81
trans-1,4-Dichloro-2-butene
Concen: 81.342 ug/l
RT: 11.079 min Scan# 1629
Delta R.T. 0.061 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion: 75 Resp: 59093
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 36.9 55.3#

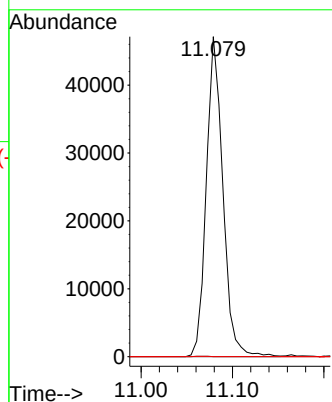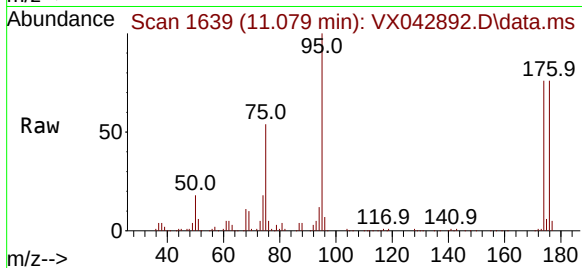

#84
1,2,4-Trimethylbenzene
Concen: 0.308 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion: 105 Resp: 1948
Ion Ratio Lower Upper
105 100
120 42.1 21.2 63.6



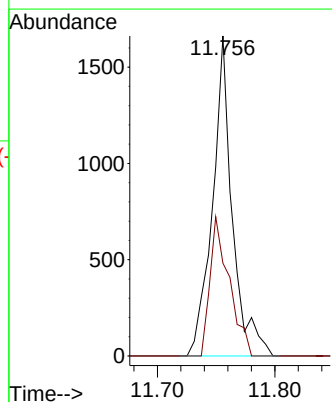
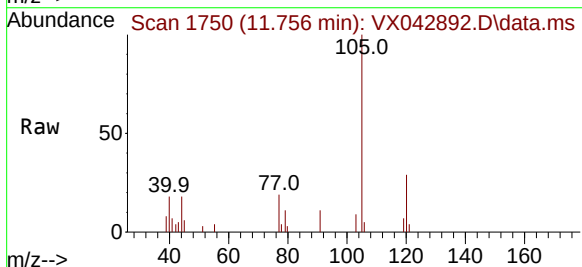




#93
1,2,4-Trichlorobenzene
Concen: 0.253 ug/l
RT: 13.597 min Scan# 2050
Delta R.T. 0.012 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43




Instrument :
MSVOA_X
ClientSampleId :
TP3


Tgt Ion:180 Resp: 540
Ion Ratio Lower Upper
180 100
182 90.4 48.3 144.8
145 14.6 18.0 54.0#

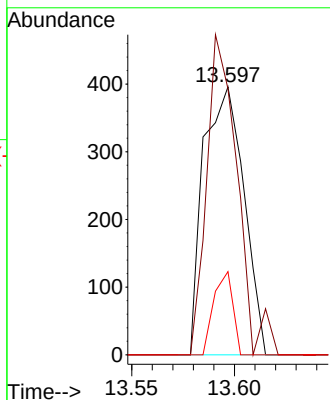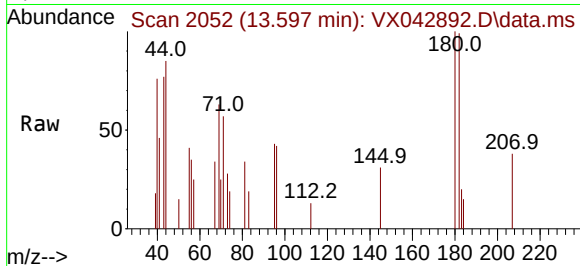

#95
Naphthalene
Concen: 0.216 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX042892.D
Acq: 07 Aug 2024 01:43

Tgt Ion:128 Resp: 1599
Ion Ratio Lower Upper
128 100
127 1.5 10.3 15.5#
129 13.8 8.8 13.2#

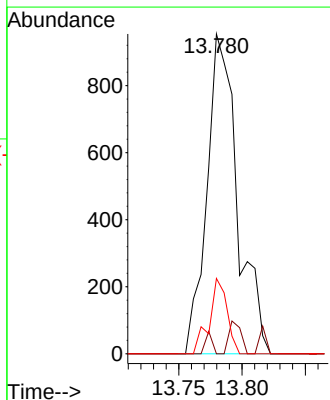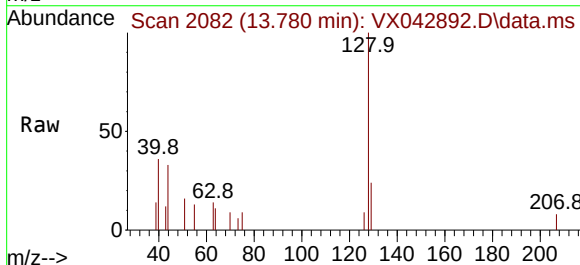



#96

1,2,3-Trichlorobenzene

Concen: 0.251 ug/l

RT: 13.963 min Scan# 21

Delta R.T. 0.006 min

Lab File: VX042892.D


Acq: 07 Aug 2024 01:43

Instrument :

MSVOA_X

ClientSampleId :

TP3

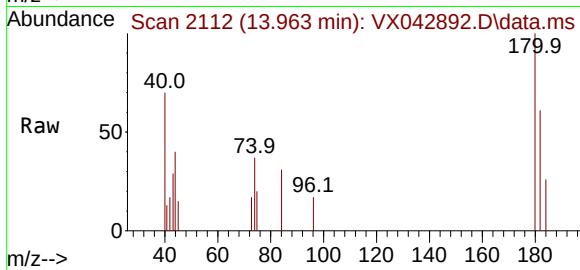

Tgt Ion:180 Resp: 539

Ion Ratio Lower Upper

180 100

182 69.9 46.9 140.6

145 10.9 17.8 53.5#

