

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080724\
 Data File : VX042930.D
 Acq On : 07 Aug 2024 23:09
 Operator : JC/MD
 Sample : VX0807WBL03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0807WBL03

Quant Time: Aug 08 04:02:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 07 02:55:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	158861	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	297458	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	284079	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	117506	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	120671	55.332	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 110.660%	
35) Dibromofluoromethane	5.385	113	102149	52.521	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.040%	
50) Toluene-d8	8.647	98	357654	51.800	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 103.600%	
62) 4-Bromofluorobenzene	11.079	95	130397	52.556	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 105.120%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080724\
Data File : VX042930.D
Acq On : 07 Aug 2024 23:09
Operator : JC/MD
Sample : VX0807WBL03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0807WBL03

Quant Time: Aug 08 04:02:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 07 02:55:22 2024
Response via : Initial Calibration




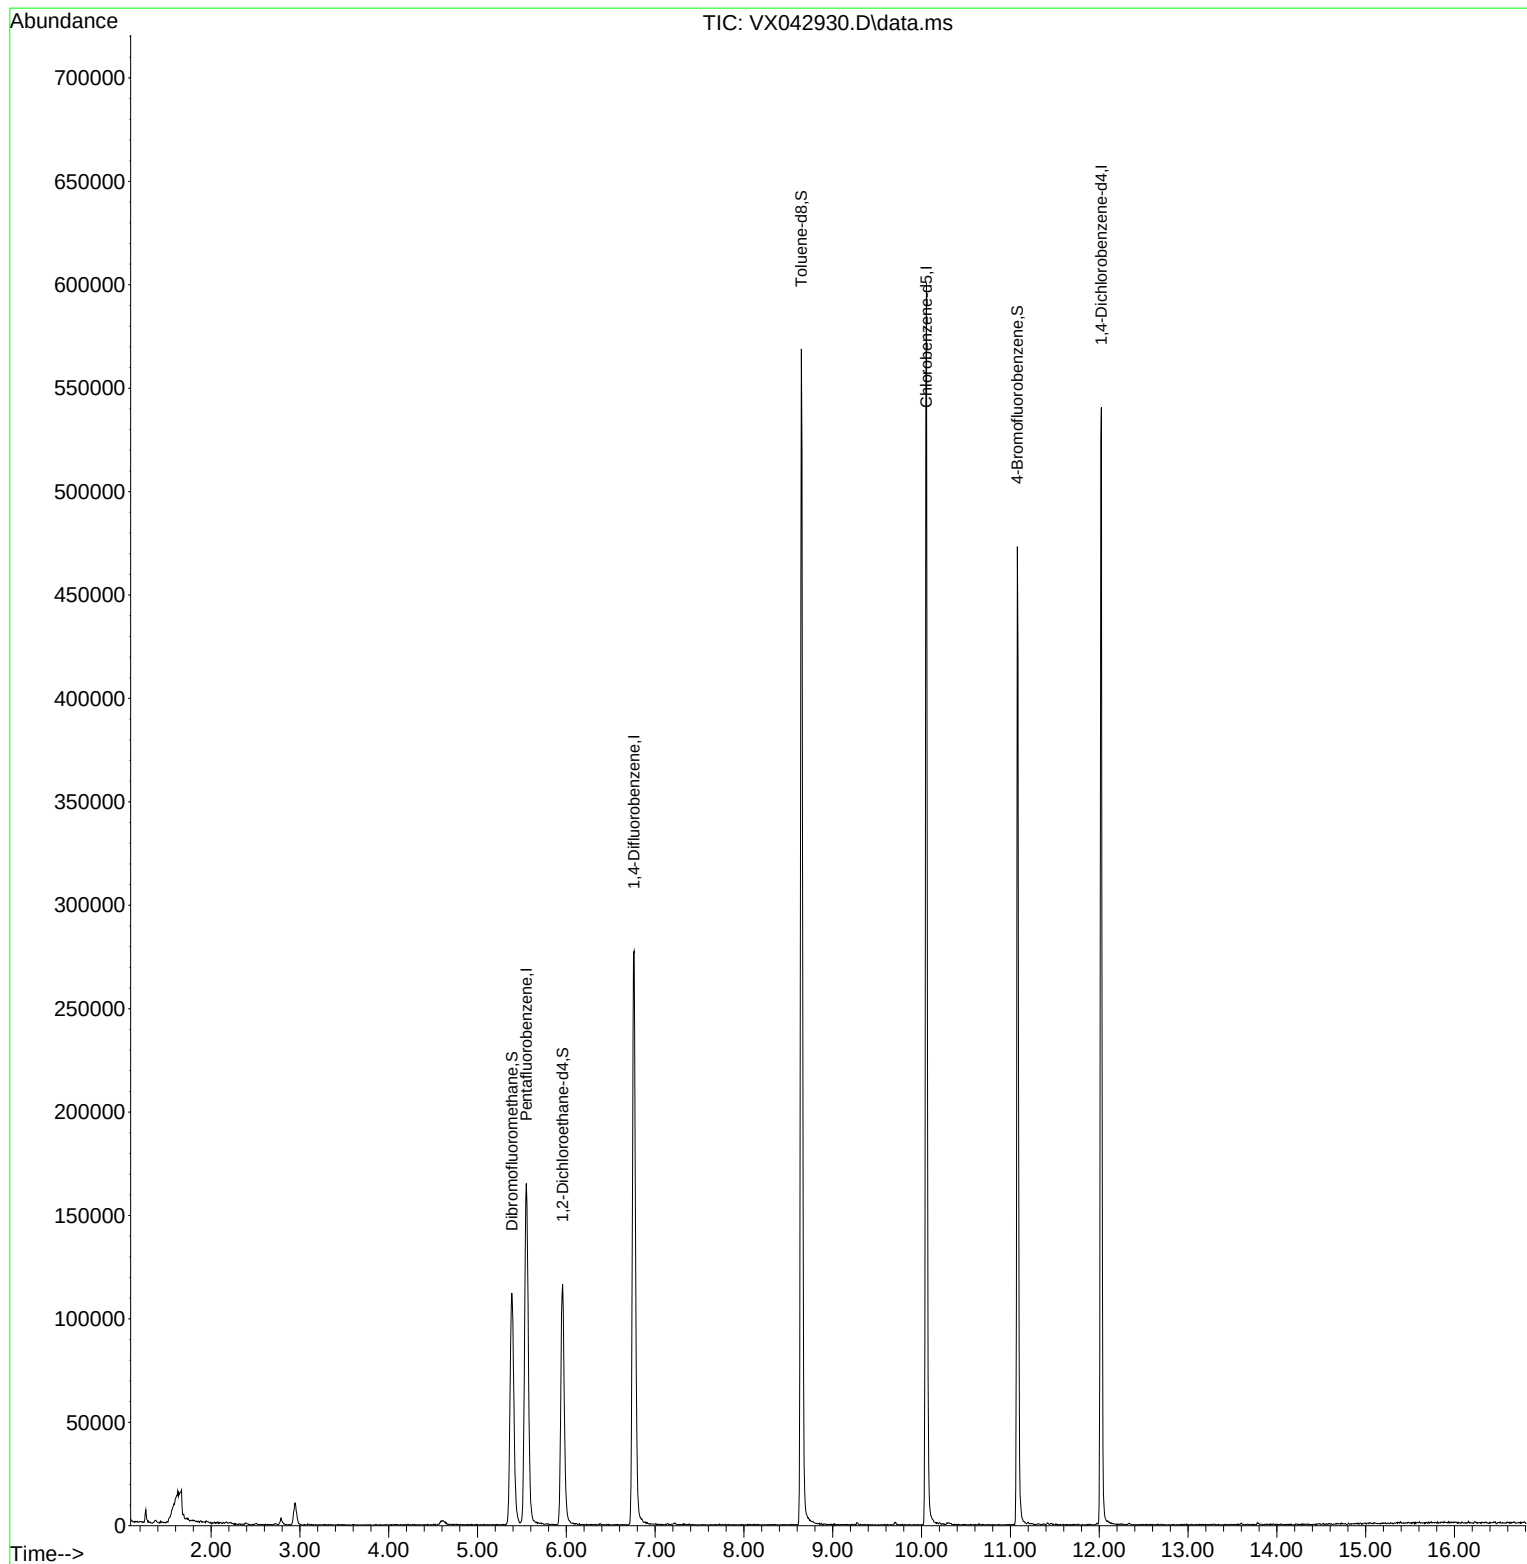


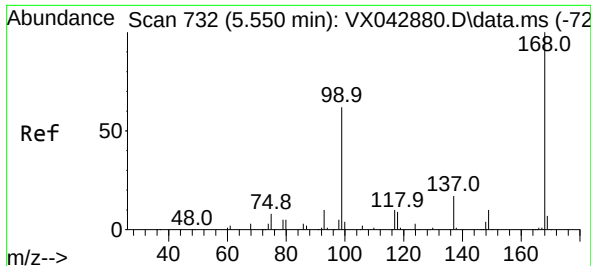

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 712
Delta R.T. -0.000 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09




Instrument :
MSVOA_X
ClientSampleId :
VX0807WBL03


Tgt Ion:168 Resp: 158861
Ion Ratio Lower Upper
168 100
99 60.0 56.6 85.0

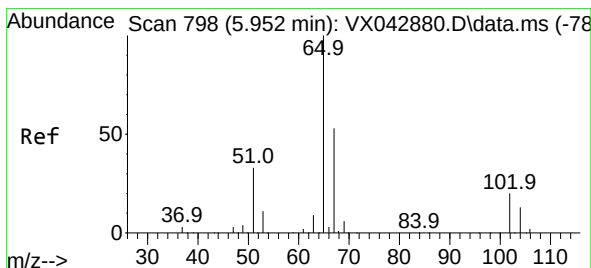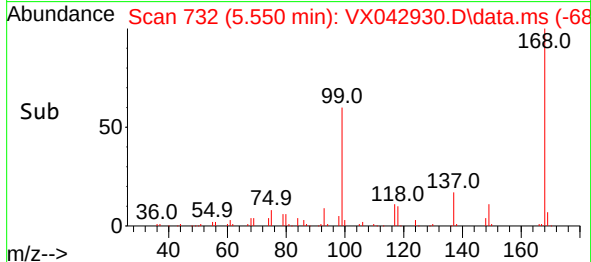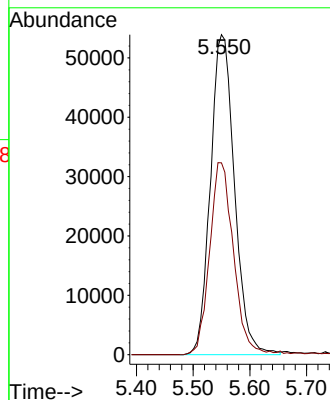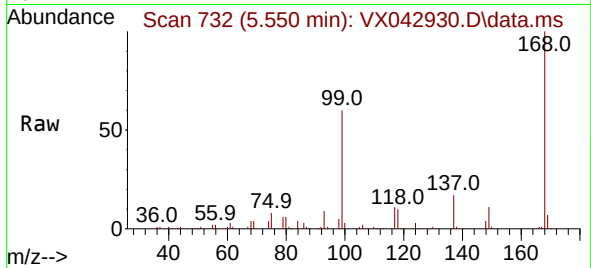

#33
1,2-Dichloroethane-d4
Concen: 55.332 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09

Tgt Ion: 65 Resp: 120671
Ion Ratio Lower Upper
65 100
67 50.9 0.0 100.2


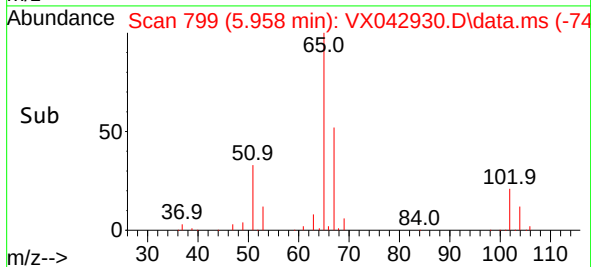
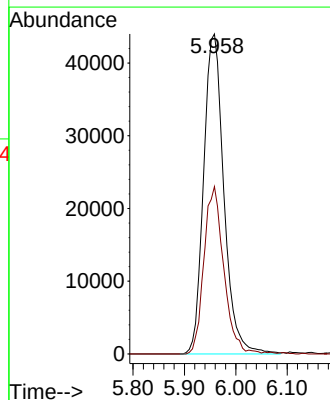
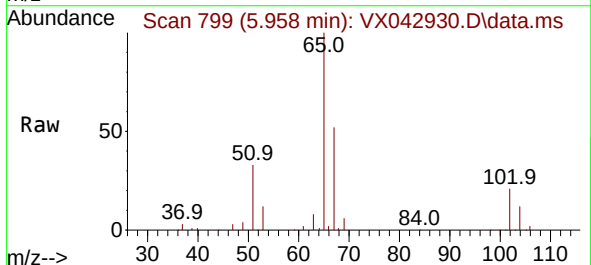


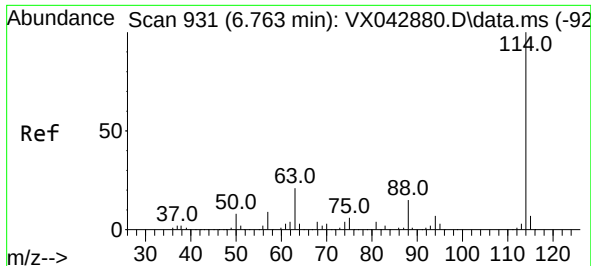

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09




Instrument :
MSVOA_X
ClientSampleId :
VX0807WBL03


Tgt Ion:114 Resp: 297458
Ion Ratio Lower Upper
114 100
63 18.8 0.0 45.0
88 15.9 0.0 36.6

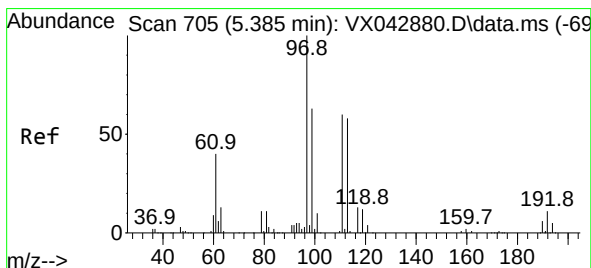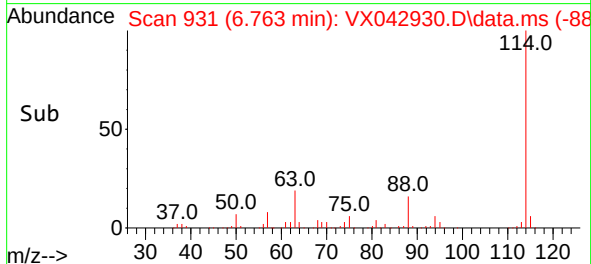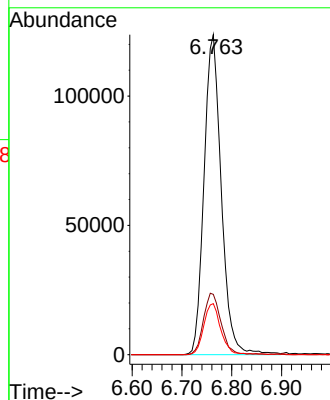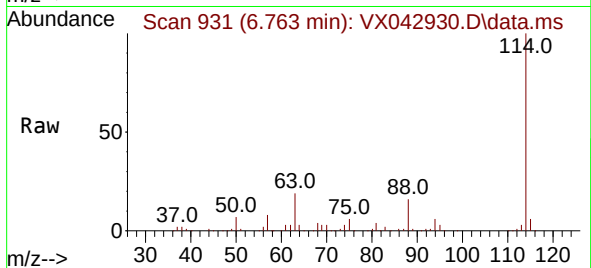

#35
Dibromofluoromethane
Concen: 52.521 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09

Tgt Ion:113 Resp: 102149
Ion Ratio Lower Upper
113 100
111 103.1 82.9 124.3
192 19.3 13.3 19.9


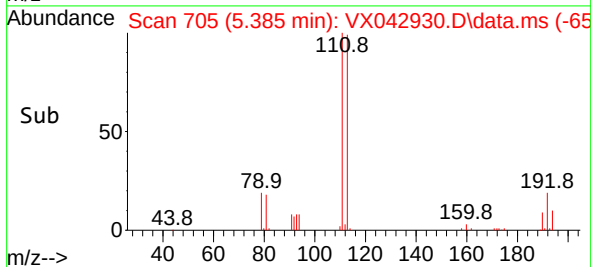
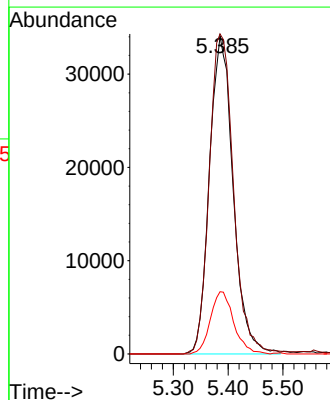
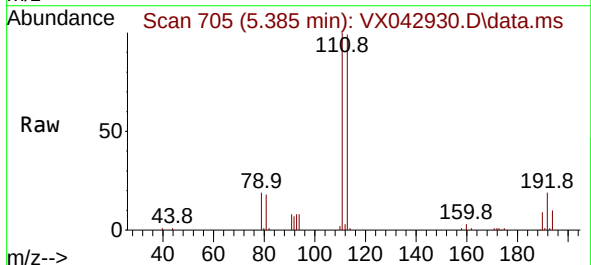


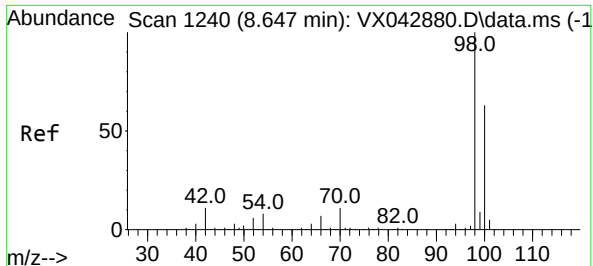

#50
Toluene-d8
Concen: 51.800 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09




Instrument :
MSVOA_X
ClientSampleId :
VX0807WBL03


Tgt Ion: 98 Resp: 357654
Ion Ratio Lower Upper
98 100
100 64.0 53.1 79.7

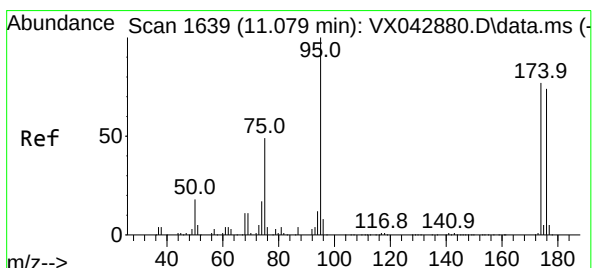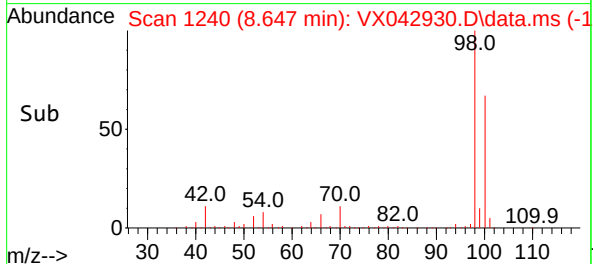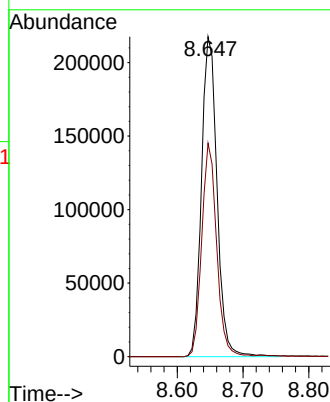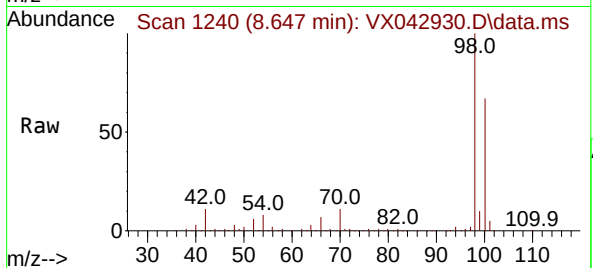

#62
4-Bromofluorobenzene
Concen: 52.556 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09

Tgt Ion: 95 Resp: 130397
Ion Ratio Lower Upper
95 100
174 79.8 0.0 135.6
176 76.2 0.0 131.0


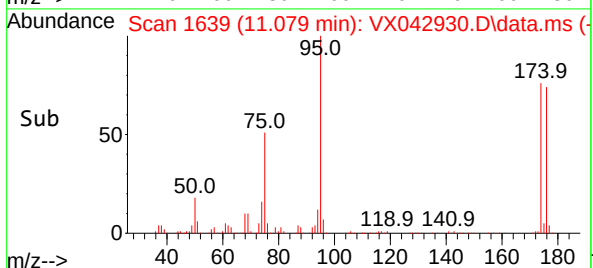
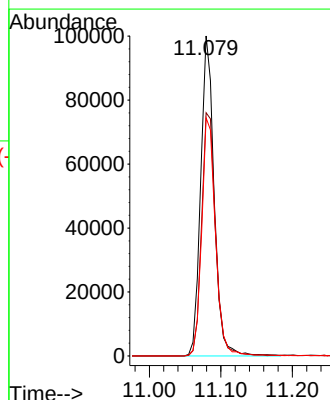
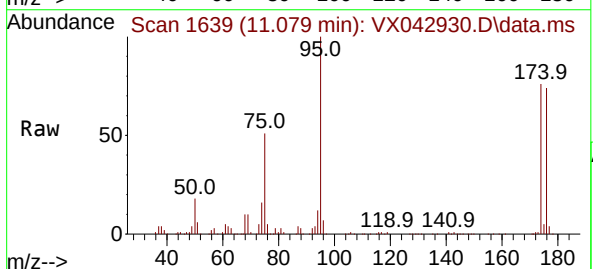


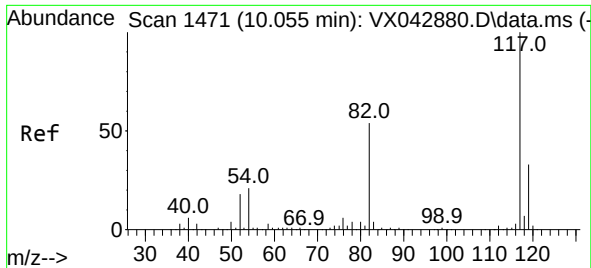

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09

Instrument :
MSVOA_X
ClientSampleId :
VX0807WBL03

Tgt Ion:117 Resp: 284079
Ion Ratio Lower Upper
117 100
82 56.0 46.2 69.4
119 32.8 25.5 38.3

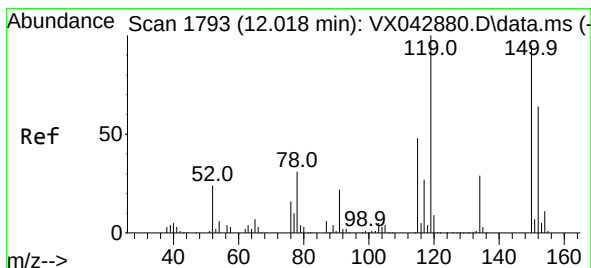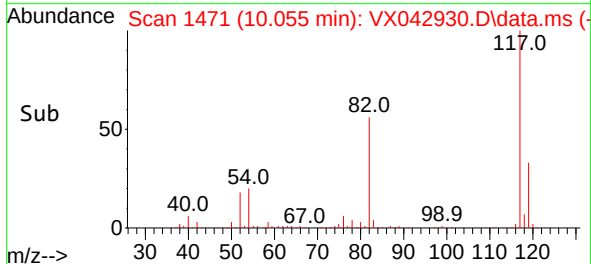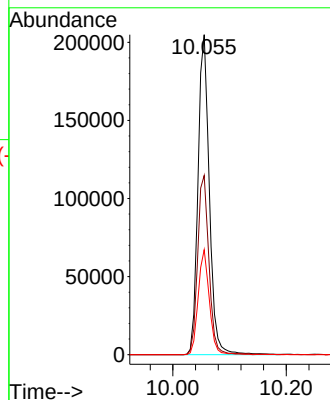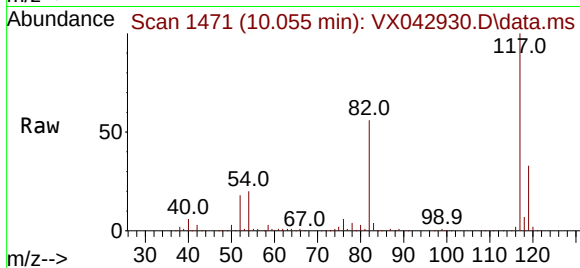

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX042930.D
Acq: 07 Aug 2024 23:09

Tgt Ion:152 Resp: 117506
Ion Ratio Lower Upper
152 100
115 59.7 43.3 129.9
150 157.9 0.0 345.0

