

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080818\
 Data File : VX003923.D
 Acq On : 08 Aug 2018 15:05
 Operator : JC/MD
 Sample : J4379-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FB-08072018

Quant Time: Aug 09 03:13:46 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 07 07:45:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	327364	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	509365	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	481770	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	278218	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.07	65	220765	50.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.74%	
35) Dibromofluoromethane	5.50	113	190093	49.26	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.52%	
50) Toluene-d8	8.71	98	723339	48.20	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.40%	
62) 4-Bromofluorobenzene	11.14	95	258869	53.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.62%	

Target Compounds


						Qvalue
5) Bromomethane	1.64	94	987	Below Cal		84
6) Chloroethane	1.79	64	6096	2.12 ug/l	#	58
9) 1,1,2-Trichlorotrifluoroet	2.37	101	790	0.21 ug/l	#	95
10) Methyl Iodide	2.51	142	1250	0.27 ug/l		93
11) Tert butyl alcohol	3.07	59	544	0.52 ug/l	#	82
13) Acrolein	2.30	56	546	Below Cal		95
15) Acrylonitrile	3.15	53	877	0.35 ug/l	#	62
16) Acetone	2.45	43	16878	6.54 ug/l		97
17) Carbon Disulfide	2.56	76	3566	0.79 ug/l		99
20) Methylene Chloride	2.86	84	1374	Below Cal		94
21) trans-1,2-Dichloroethene	3.16	96	806	0.20 ug/l		89
25) 2-Butanone	4.70	43	1329	0.34 ug/l		93
29) Tetrahydrofuran	5.16	42	935	0.47 ug/l	#	92
38) Carbon Tetrachloride	5.67	117	29109	5.36 ug/l	#	15
39) Methylcyclohexane	7.46	83	1757	0.26 ug/l		96
48) Methyl methacrylate	7.78	41	3152	0.66 ug/l		93
49) 1,4-Dioxane	7.77	88	43	0.38 ug/l	#	1
68) m/p-Xylenes	10.36	106	2084	0.26 ug/l		98
76) 1,2,3-Trichloropropane	11.14	75	124040	20.18 ug/l	#	36
81) trans-1,4-Dichloro-2-buten	11.14	75	124040	54.69 ug/l	#	9
86) p-Isopropyltoluene	12.07	119	8533	0.49 ug/l		90
87) 1,3-Dichlorobenzene	12.03	146	2139	0.21 ug/l		94
88) 1,4-Dichlorobenzene	12.03	146	2139	Below Cal		93
93) 1,2,4-Trichlorobenzene	13.65	180	1853	0.26 ug/l		98
94) Hexachlorobutadiene	13.79	225	961	0.73 ug/l		99
96) 1,2,3-Trichlorobenzene	14.02	180	1486	0.21 ug/l		92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080818\
Data File : VX003923.D
Acq On : 08 Aug 2018 15:05
Operator : JC/MD
Sample : J4379-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FB-08072018

Quant Time: Aug 09 03:13:46 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 07 07:45:48 2018
Response via : Initial Calibration

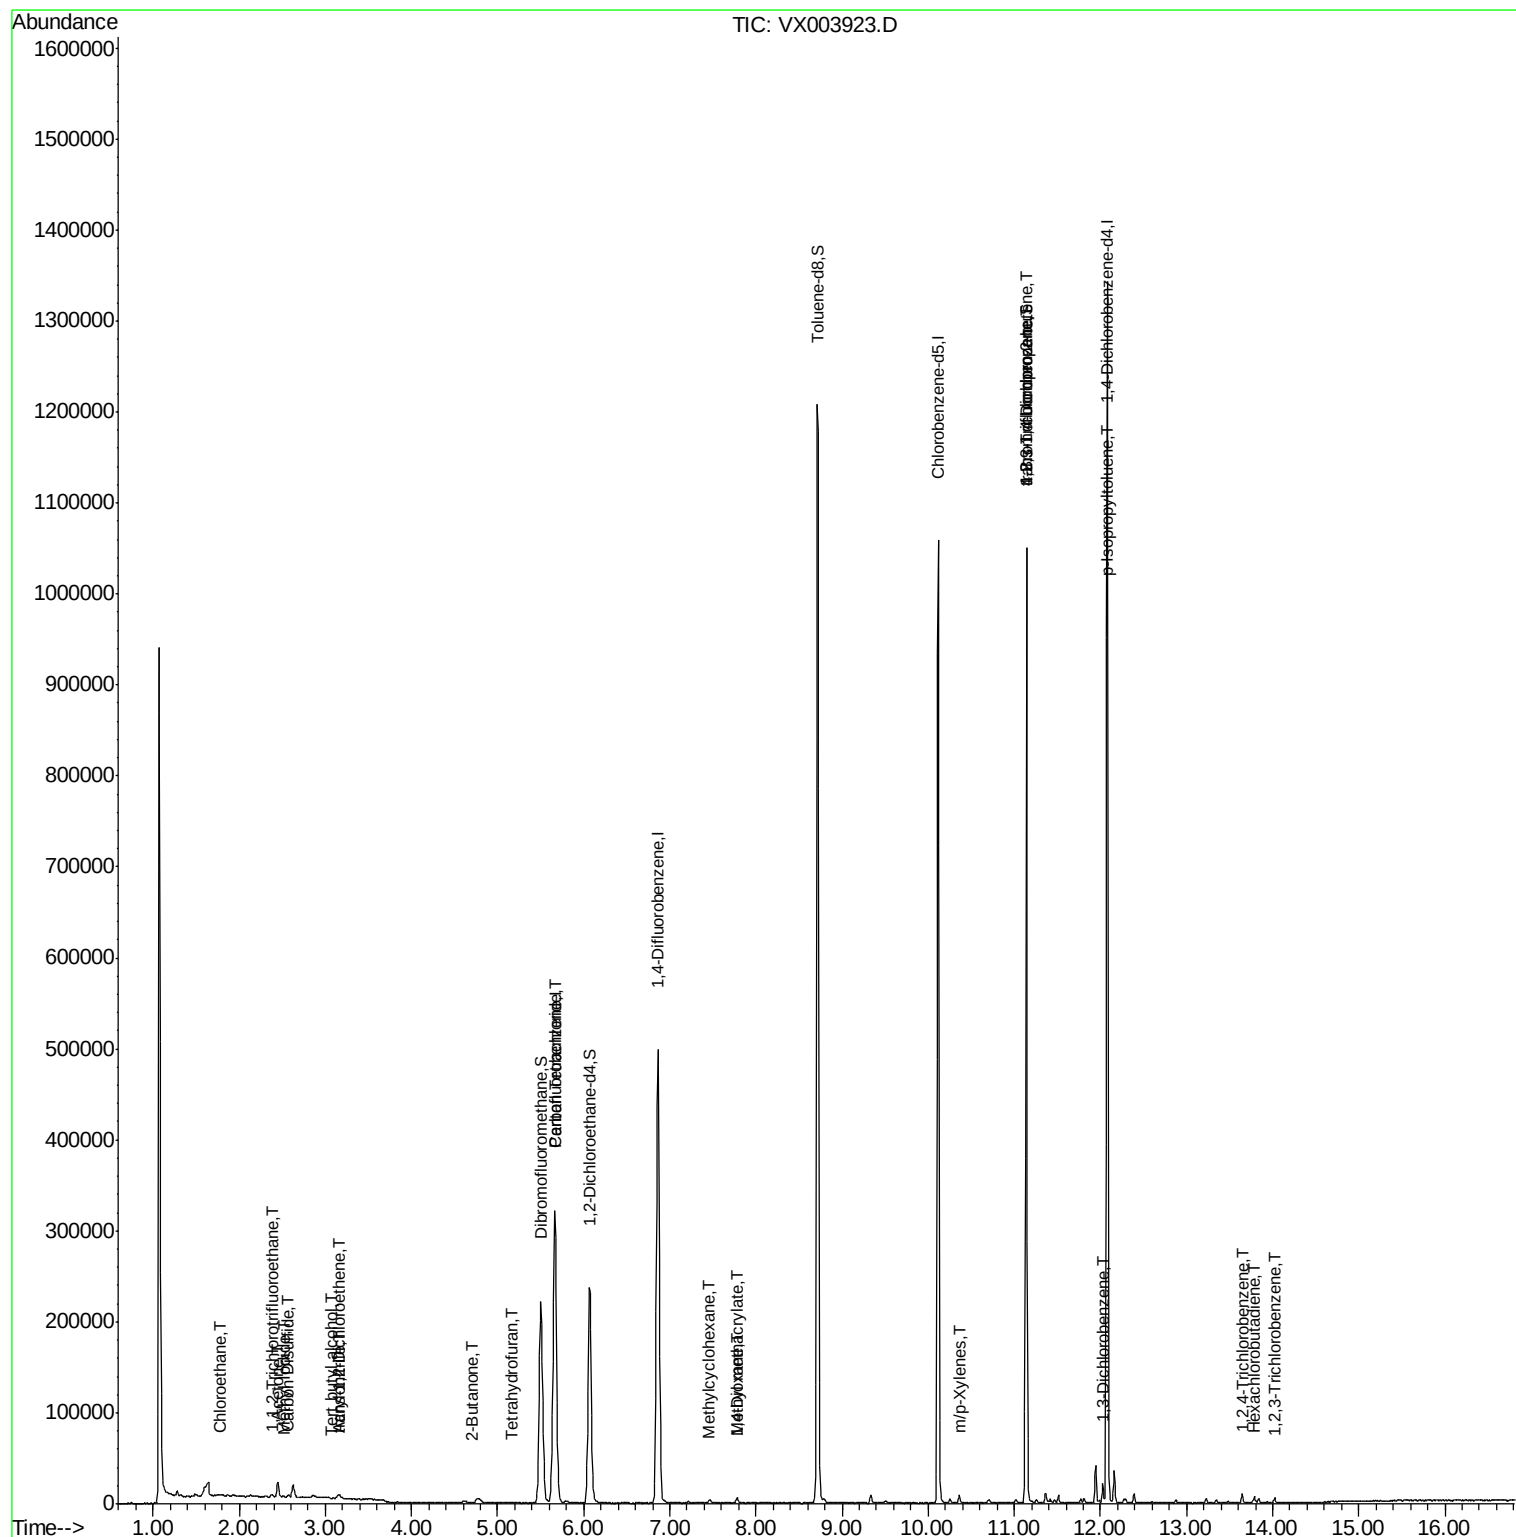

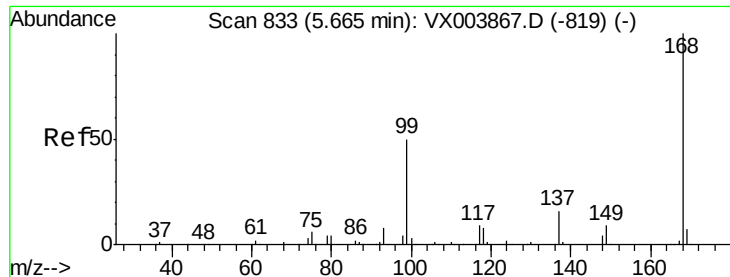

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampleId :


FB-08072018

Tot Ion:168 Resp: 327364

Ion Ratio Lower Upper

168 100

99 50.1 40.1 60.1

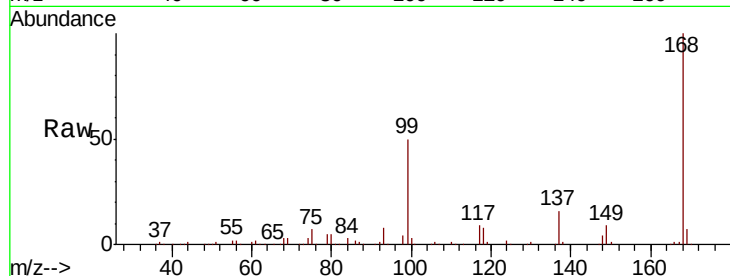

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67



100000

50000

0

Time-->

5.50 5.60 5.70 5.80 5.90

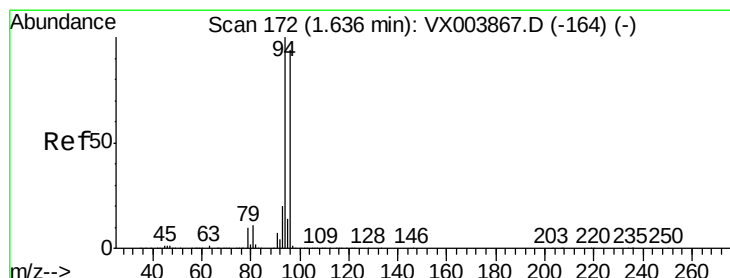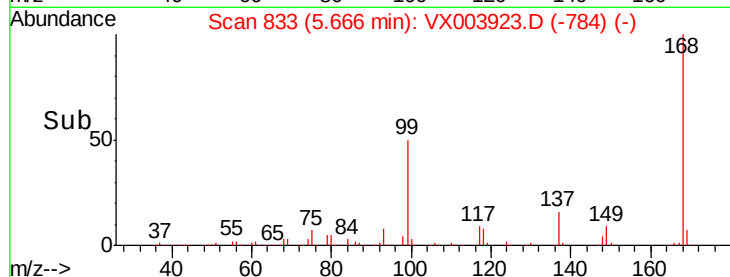

#5

Bromomethane

Concen: Below Cal

RT: 1.64 min Scan# 173

Delta R.T. 0.01 min

Lab File: VX003923.D


Acq: 08 Aug 2018 15:05

Tgt Ion: 94 Resp: 987

Ion Ratio Lower Upper

94 100

96 78.4 75.2 112.8

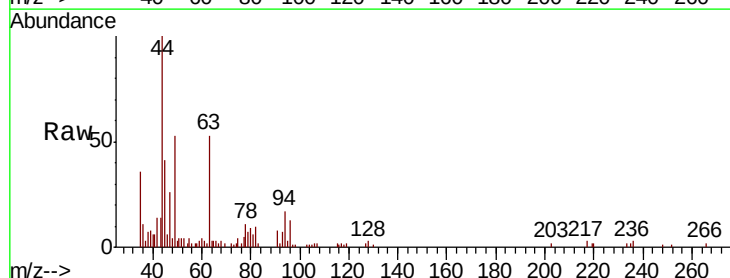

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

1.64

600


400


200

0

Time-->

1.60 1.65 1.70

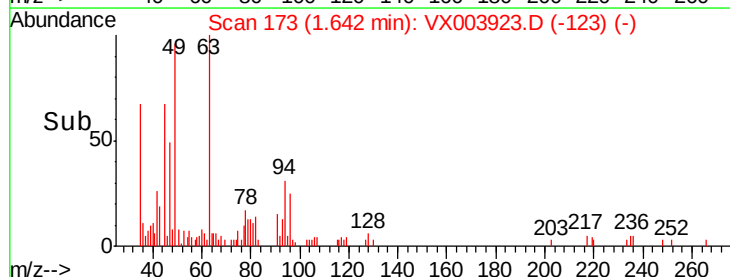

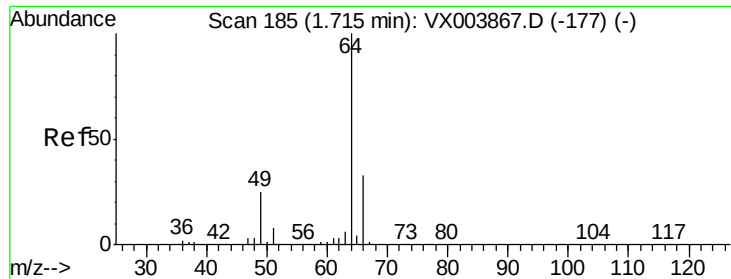

#6

Chloroethane

Concen: 2.12 ug/l

RT: 1.79 min Scan# 197

Delta R.T. 0.07 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampleId :





FB-08072018

Tot Ion: 64 Resp: 6096

Ion Ratio Lower Upper

64 100

66 9.5 26.5 39.7#

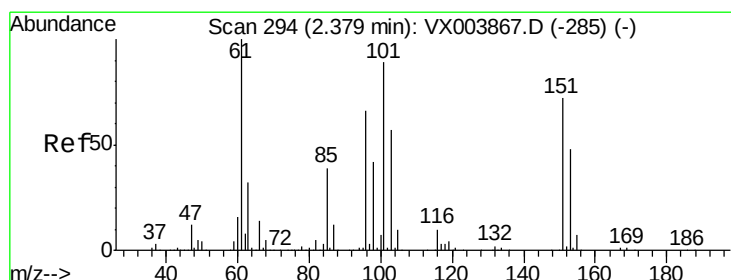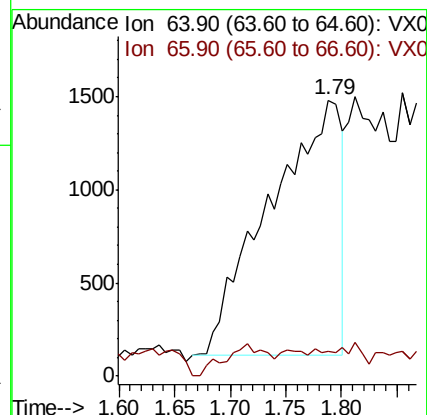

#9

1,1,2-Trichlorotrifluoroethane

Concen: 0.21 ug/l

RT: 2.37 min Scan# 293

Delta R.T. -0.01 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05




Tgt Ion:101 Resp: 790


Ion Ratio Lower Upper

101 100

85 51.6 34.2 51.4#

151 82.0 65.0 97.4



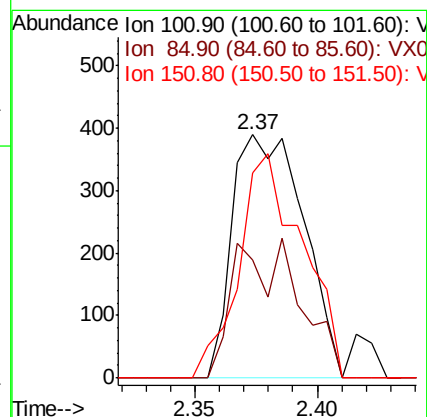





#10
Methyl Iodide
Concen: 0.27 ug/l
RT: 2.51 min Scan# 316
Delta R.T. 0.01 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05




Instrument :
MSVOA_X
ClientSampleId :
FB-08072018


Tot Ion:142 Resp: 1250
Ion Ratio Lower Upper
142 100
127 46.8 33.1 49.7
141 13.8 11.1 16.7

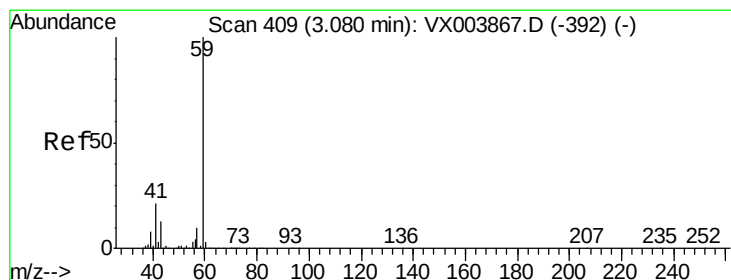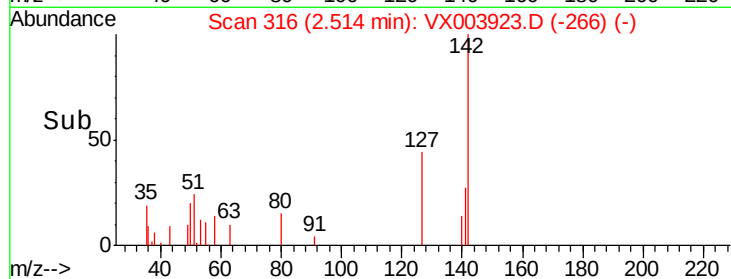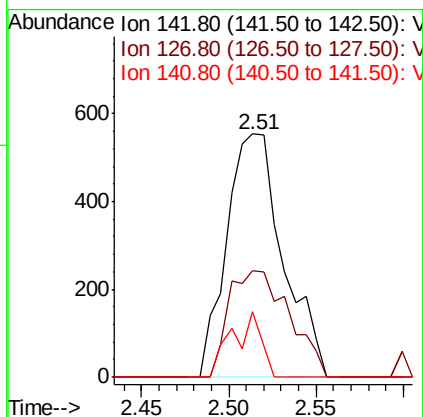

#11
Tert butyl alcohol
Concen: 0.52 ug/l
RT: 3.07 min Scan# 408
Delta R.T. -0.01 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05

Tgt Ion: 59 Resp: 544
Ion Ratio Lower Upper
59 100
57 3.5 8.1 12.1#

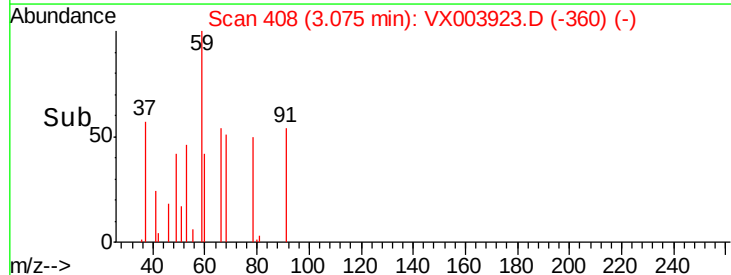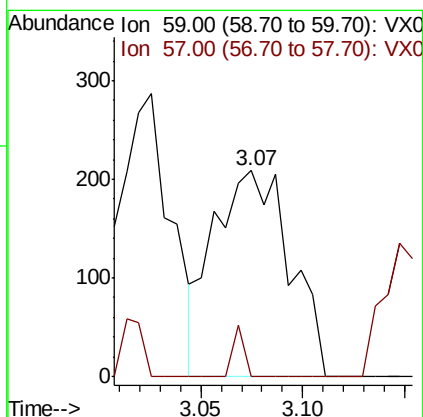



#13

Acrolein

Concen: Below Cal

RT: 2.30 min Scan# 281

Delta R.T. 0.01 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampleId :





FB-08072018

Tot Ion: 56 Resp: 546

Ion Ratio Lower Upper

56 100

55 74.2 56.1 84.1

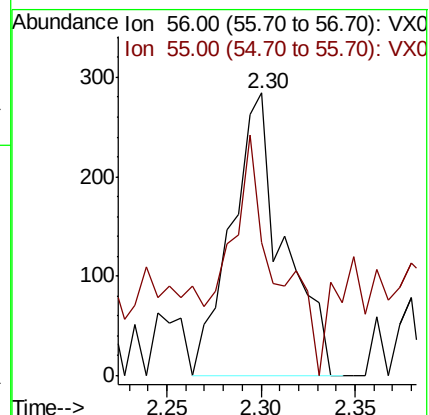

#15

Acrylonitrile

Concen: 0.35 ug/l

RT: 3.15 min Scan# 421

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05




Tgt Ion: 53 Resp: 877


Ion Ratio Lower Upper

53 100

52 123.6 65.3 97.9#

51 44.6 27.9 41.9#

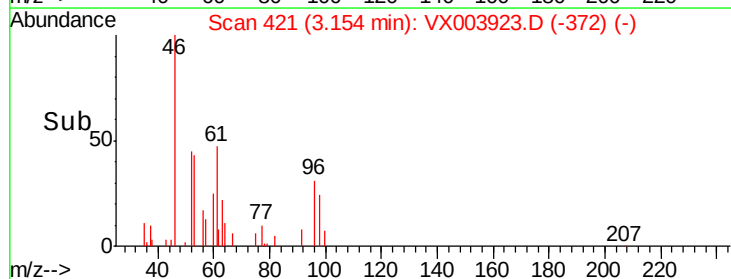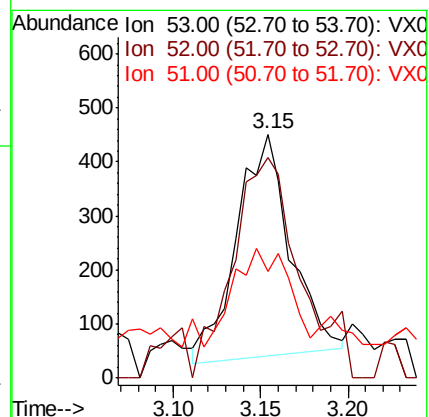



#16

Acetone

Concen: 6.54 ug/l

RT: 2.45 min Scan# 305

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampled :





FB-08072018

Tot Ion: 43 Resp: 16878

Ion Ratio Lower Upper

43 100

58 34.6 26.4 39.6

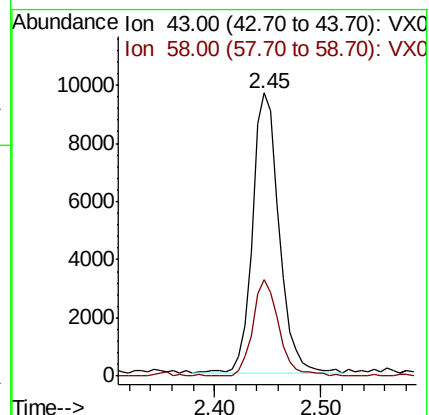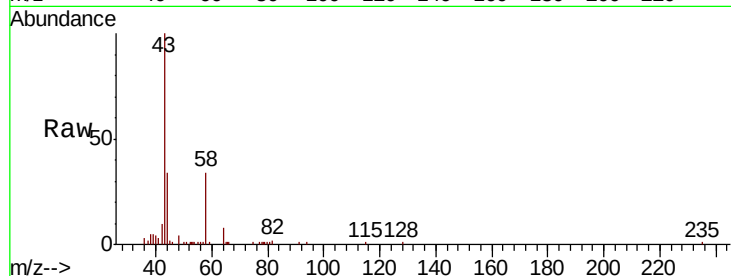

#17

Carbon Disulfide

Concen: 0.79 ug/l

RT: 2.56 min Scan# 324

Delta R.T. 0.00 min

Lab File: VX003923.D




Acq: 08 Aug 2018 15:05


Tgt Ion: 76 Resp: 3566

Ion Ratio Lower Upper

76 100

78 9.8 7.5 11.3

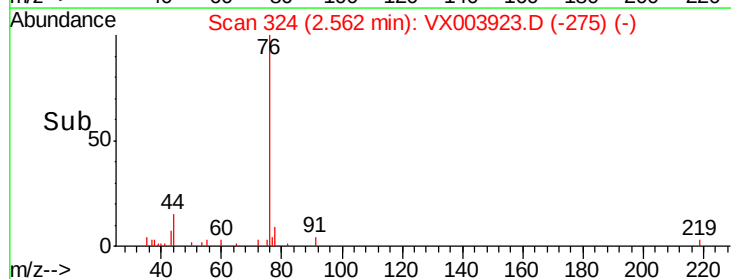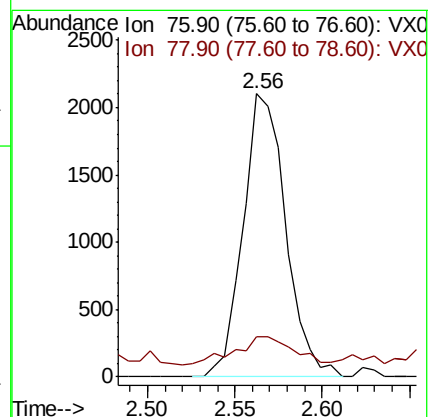


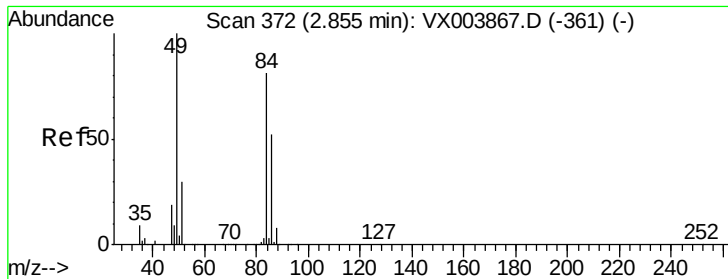




#20
Methylene Chloride
Concen: Below Cal
RT: 2.86 min Scan# 372
Delta R.T. 0.00 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05

Instrument :
MSVOA_X
ClientSampled :
FB-08072018

Tot Ion:	84	Resp:	1374
Ion	Ratio	Lower	Upper
84	100		
49	132.2	98.9	148.3
51	34.5	29.9	44.9
86	60.8	51.0	76.6

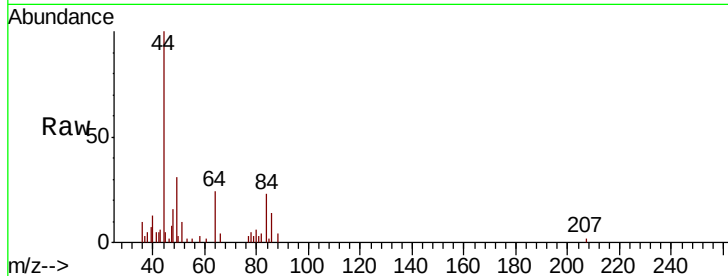


Abundance Ion 83.90 (83.60 to 84.60): VX0
Ion 48.90 (48.60 to 49.60): VX0
Ion 50.90 (50.60 to 51.60): VX0
Ion 85.90 (85.60 to 86.60): VX0

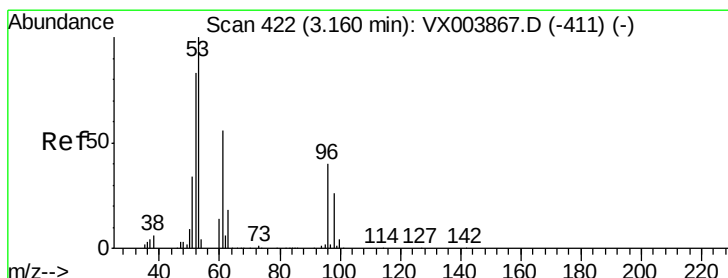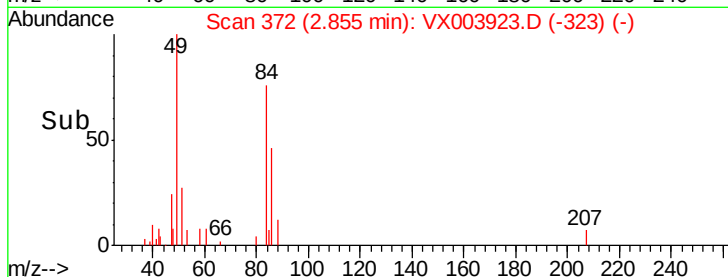
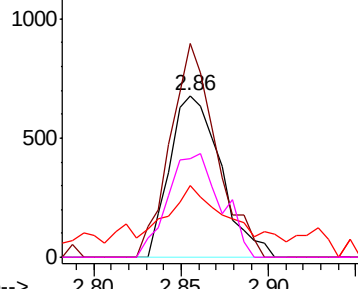



#21
trans-1,2-Dichloroethene
Concen: 0.20 ug/l
RT: 3.16 min Scan# 422
Delta R.T. 0.00 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05

Tgt Ion:	96	Resp:	806
Ion	Ratio	Lower	Upper
96	100		
61	126.5	111.8	167.6
98	74.0	51.8	77.6

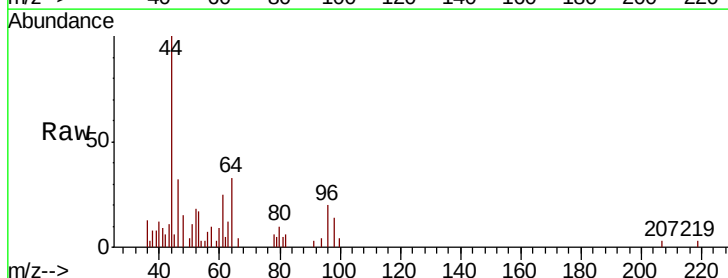

Abundance Ion 95.90 (95.60 to 96.60): VX0
Ion 60.90 (60.60 to 61.60): VX0
Ion 97.90 (97.60 to 98.60): VX0

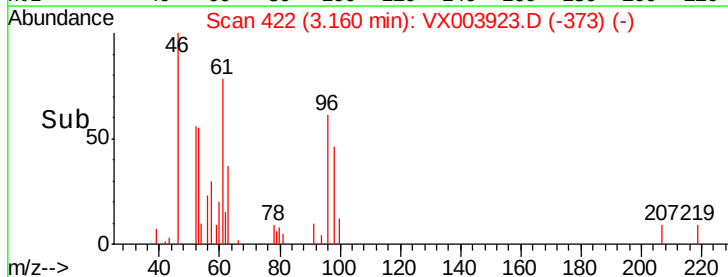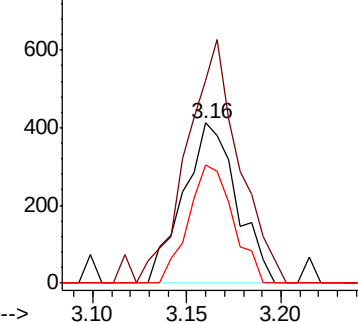



#25

2-Butanone

Concen: 0.34 ug/l

RT: 4.70 min Scan# 675

Delta R.T. -0.01 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampleId :


FB-08072018

Tot Ion: 43 Resp: 1329

Ion Ratio Lower Upper

43 100

72 30.4 21.4 32.0

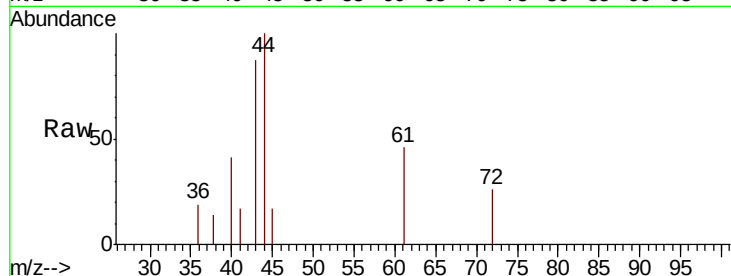

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

4.70

400

300



200

100

0

Time-->

4.65 4.70 4.75



#29

Tetrahydrofuran

Concen: 0.47 ug/l

RT: 5.16 min Scan# 750

Delta R.T. -0.01 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05


Tgt Ion: 42 Resp: 935

Ion Ratio Lower Upper

42 100

72 45.6 37.7 56.5

71 34.7 35.0 52.6#



Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

400

300


200


100

0

Time-->

5.10 5.15 5.20 5.25



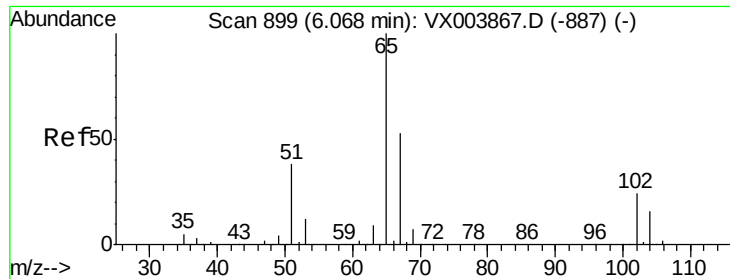

#33

1,2-Dichloroethane-d4

Concen: 50.87 ug/l

RT: 6.07 min Scan# 899

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampleId :


FB-08072018

Tot Ion: 65 Resp: 220765

Ion Ratio Lower Upper




65 100

67 53.5 0.0 105.8

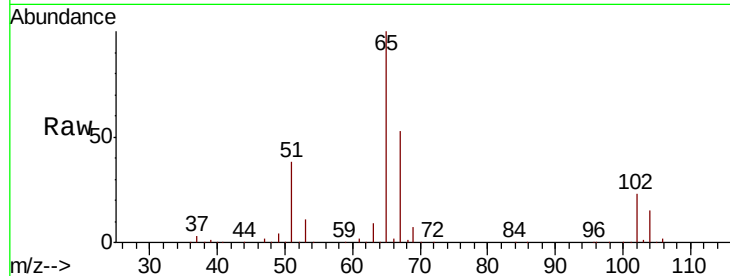

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

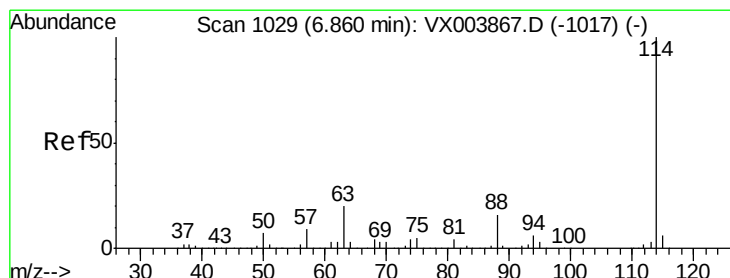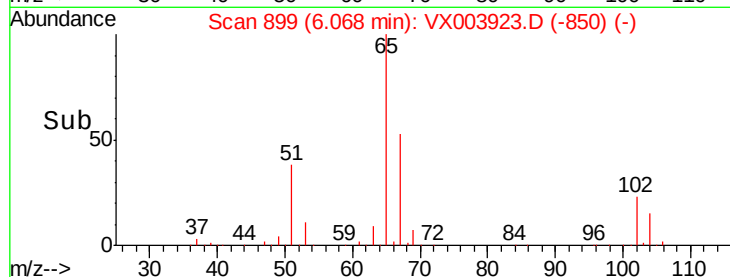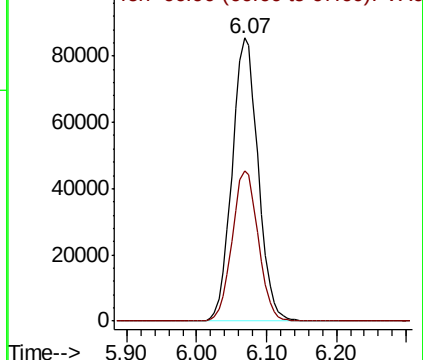

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.86 min Scan# 1029

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05


Tgt Ion: 114 Resp: 509365

Ion Ratio Lower Upper

114 100

63 20.0 0.0 39.0



88 15.7 0.0 32.0

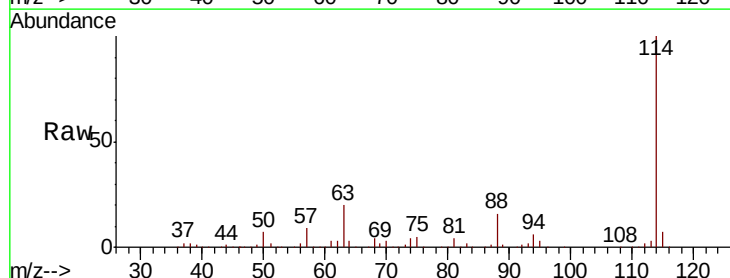


Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0



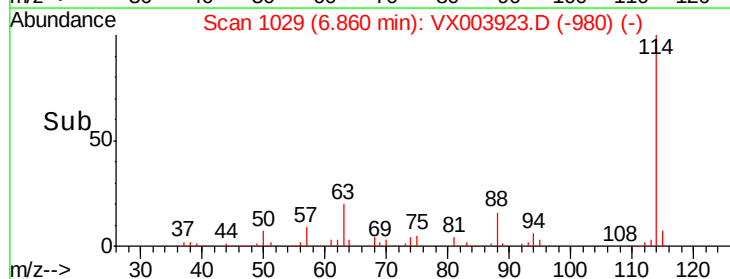
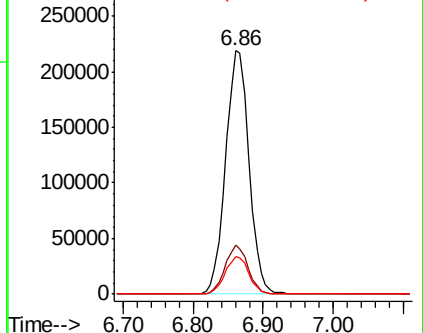


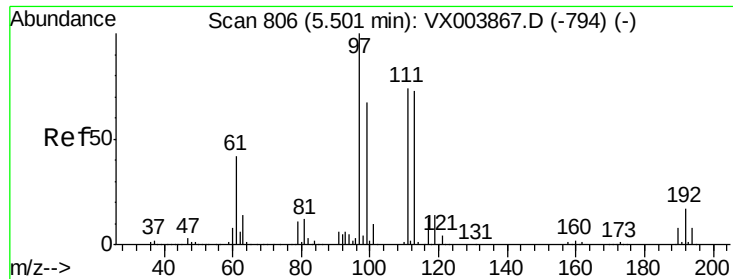

#35
 Dibromofluoromethane
 Concen: 49.26 ug/l
 RT: 5.50 min Scan# 806
 Delta R.T. 0.00 min
 Lab File: VX003923.D
 Acq: 08 Aug 2018 15:05




Instrument :
 MSVOA_X
 ClientSampleId :
 FB-08072018


Tot Ion:113 Resp: 190093
 Ion Ratio Lower Upper
 113 100
 111 102.0 82.0 123.0
 192 23.9 19.0 28.4

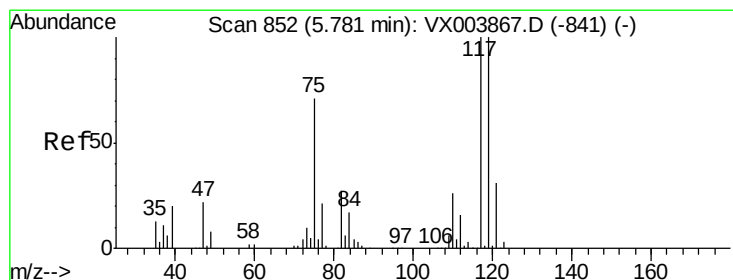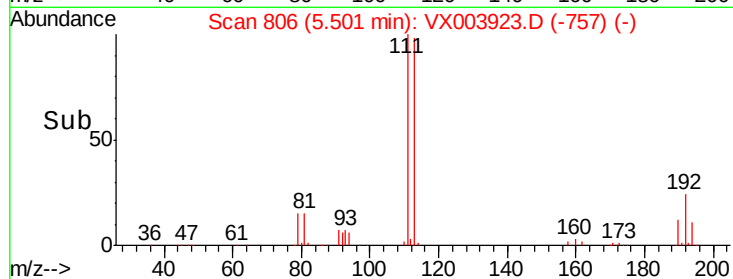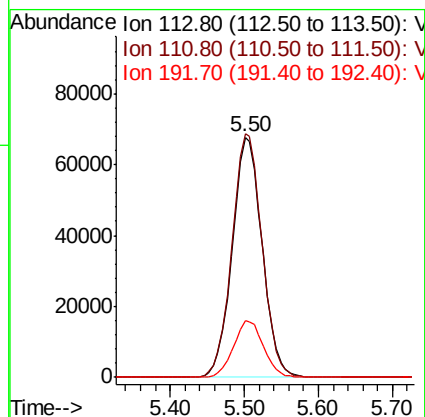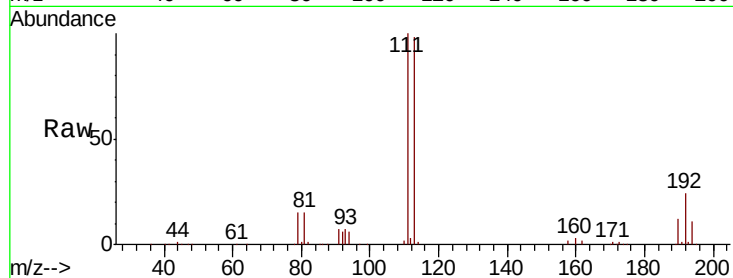

#38
 Carbon Tetrachloride
 Concen: 5.36 ug/l
 RT: 5.67 min Scan# 833
 Delta R.T. -0.12 min
 Lab File: VX003923.D
 Acq: 08 Aug 2018 15:05

Tgt Ion:117 Resp: 29109
 Ion Ratio Lower Upper
 117 100
 119 6.1 79.5 119.3#
 121 0.0 25.0 37.4#

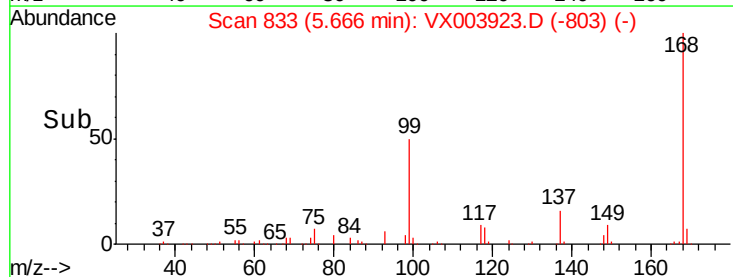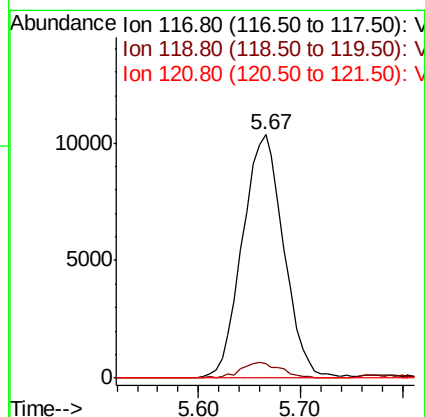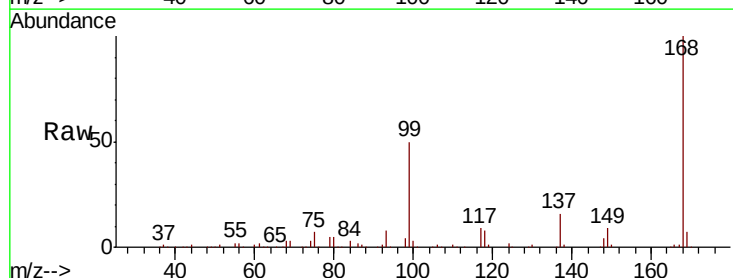


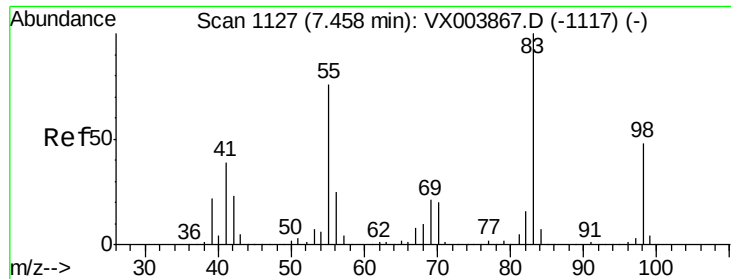




#39
Methylcyclohexane
Concen: 0.26 ug/l
RT: 7.46 min Scan# 1127
Delta R.T. 0.00 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05

Instrument :
MSVOA_X
ClientSampleId :
FB-08072018

Tot Ion: 83 Resp: 1757
Ion Ratio Lower Upper
83 100
55 80.3 61.0 91.6
98 45.8 38.6 57.8

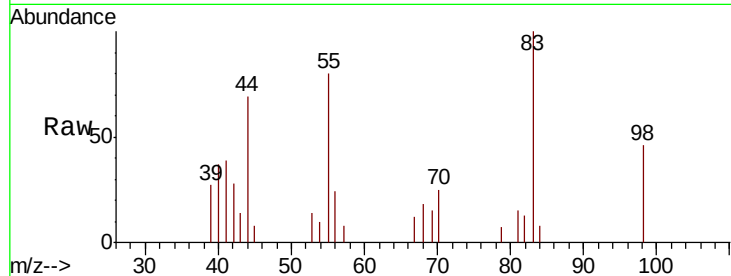


Abundance Ion 83.00 (82.70 to 83.70): VX0
Ion 55.00 (54.70 to 55.70): VX0
Ion 98.00 (97.70 to 98.70): VX0


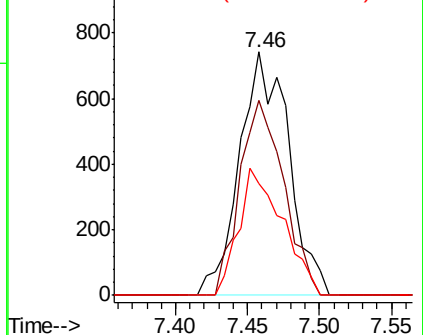



#48
Methyl methacrylate
Concen: 0.66 ug/l
RT: 7.78 min Scan# 1180
Delta R.T. 0.00 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05

Tgt Ion: 41 Resp: 3152
Ion Ratio Lower Upper
41 100
69 76.2 68.8 103.2
39 51.2 42.3 63.5



Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0

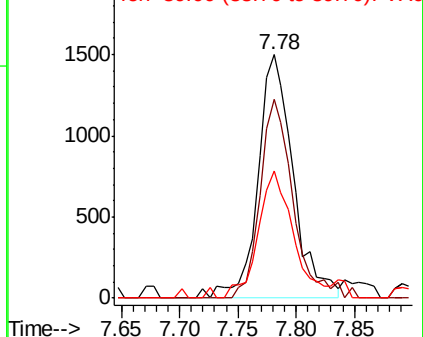







#49
 1,4-Dioxane
 Concen: 0.38 ug/l
 RT: 7.77 min Scan# 1179
 Delta R.T. 0.02 min
 Lab File: VX003923.D
 Acq: 08 Aug 2018 15:05

Instrument :
 MSVOA_X
 ClientSampled :
 FB-08072018

Tot Ion: 88 Resp: 43
 Ion Ratio Lower Upper
 88 100
 43 409.3 23.8 35.8#
 58 120.9 55.4 83.0#

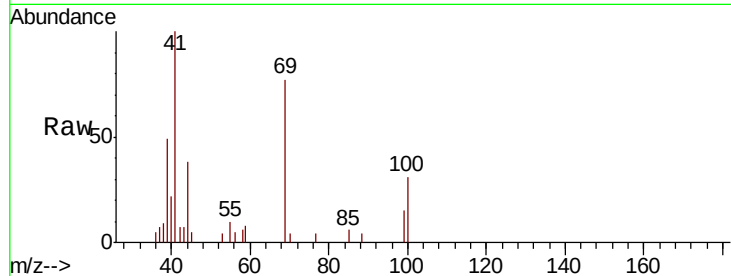


Abundance Ion 88.00 (87.70 to 88.70): VX0
 Ion 43.00 (42.70 to 43.70): VX0
 Ion 58.00 (57.70 to 58.70): VX0


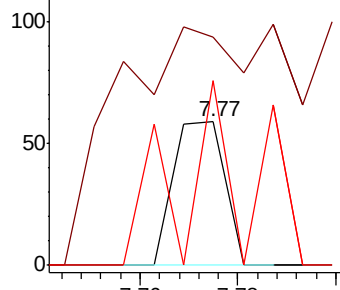



#50
 Toluene-d8
 Concen: 48.20 ug/l
 RT: 8.71 min Scan# 1333
 Delta R.T. -0.01 min
 Lab File: VX003923.D
 Acq: 08 Aug 2018 15:05

Tgt Ion: 98 Resp: 723339
 Ion Ratio Lower Upper
 98 100
 100 66.1 53.3 79.9



Abundance Ion 98.00 (97.70 to 98.70): VX0
 Ion 100.00 (99.70 to 100.70): VX0



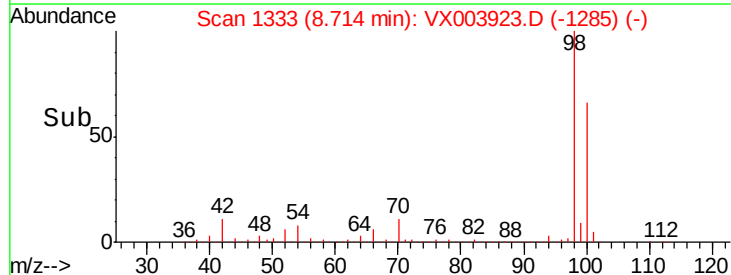
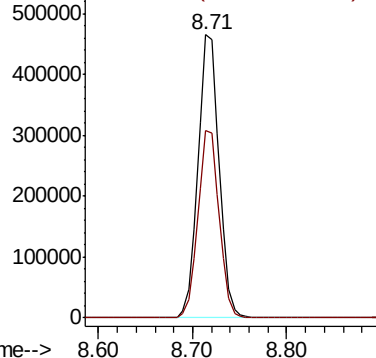


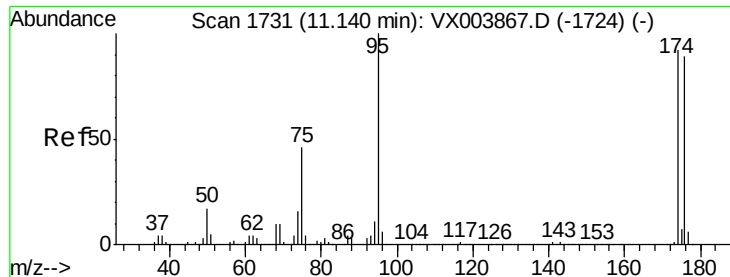

#62
4-Bromofluorobenzene
Concen: 53.31 ug/l
RT: 11.14 min Scan# 1731
Delta R.T. 0.00 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05




Instrument :
MSVOA_X
ClientSampleId :
FB-08072018


Tot Ion: 95 Resp: 258869
Ion Ratio Lower Upper
95 100
174 90.6 0.0 182.8
176 87.6 0.0 179.0

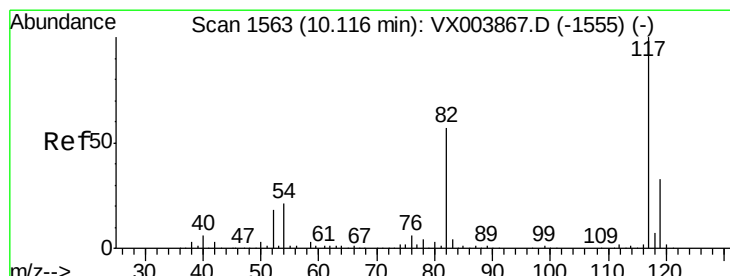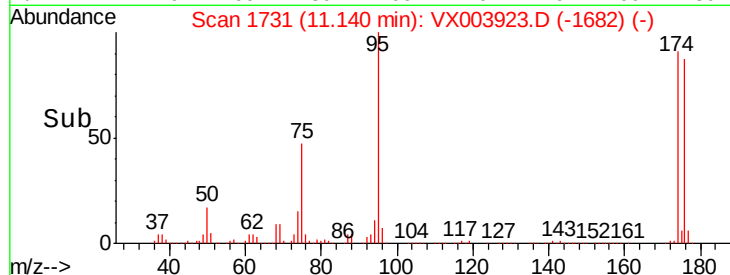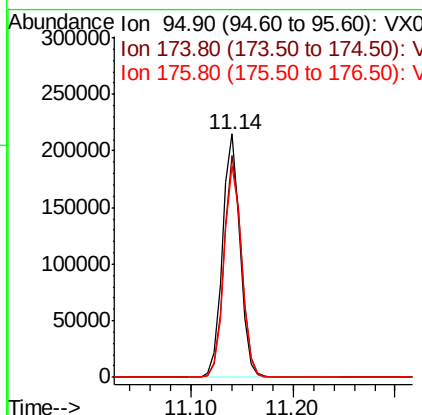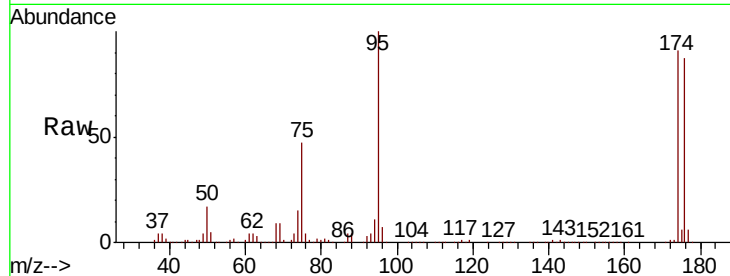

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX003923.D
Acq: 08 Aug 2018 15:05

Tgt Ion: 117 Resp: 481770
Ion Ratio Lower Upper
117 100
82 53.7 45.4 68.0
119 32.9 26.6 40.0

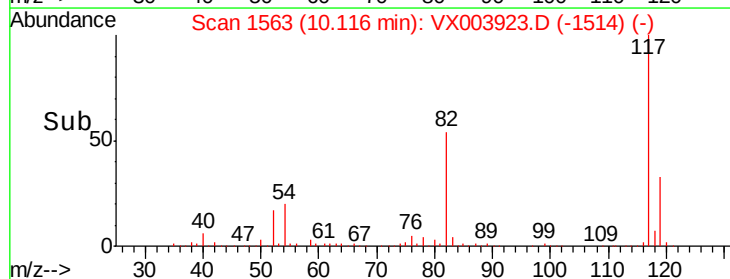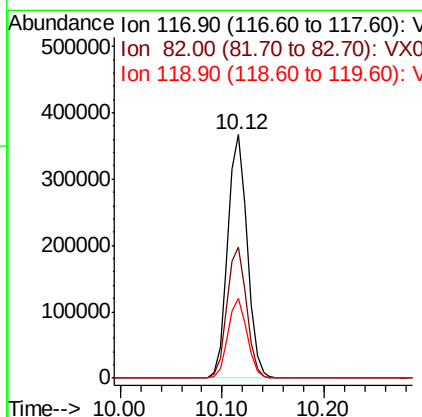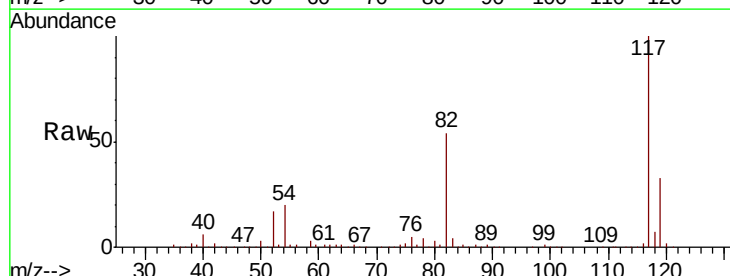



#68

m/p-Xvlenes

Concen: 0.26 ug/l

RT: 10.36 min Scan# 1603

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampleId :


FB-08072018

Tot Ion:106 Resp: 2084

Ion Ratio Lower Upper




106 100

91 199.7 162.3 243.5

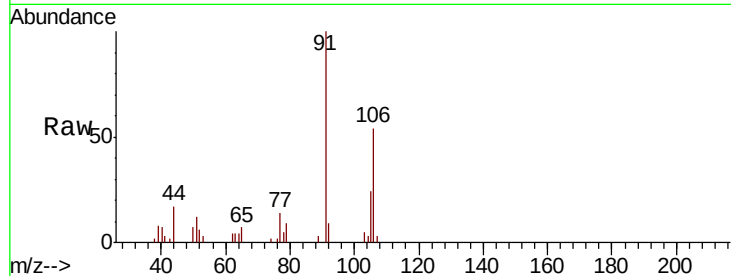

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VX0

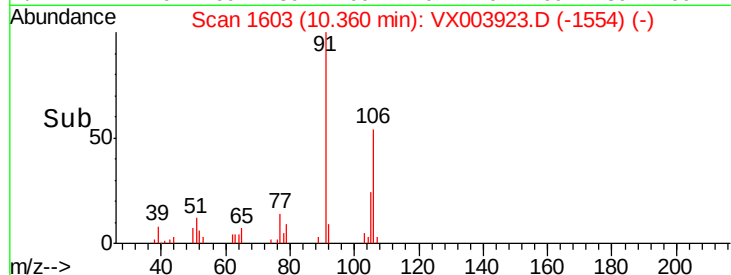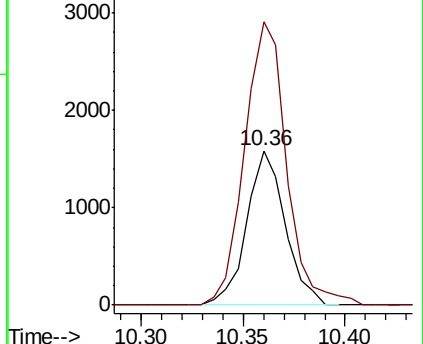

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 12.08 min Scan# 1885

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05


Tgt Ion:152 Resp: 278218

Ion Ratio Lower Upper

152 100

115 54.6 39.1 117.3



150 155.2 0.0 349.2

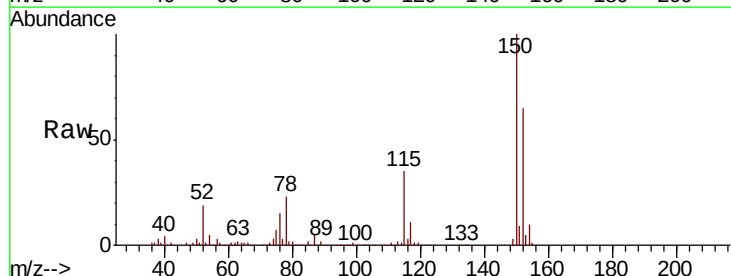


Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

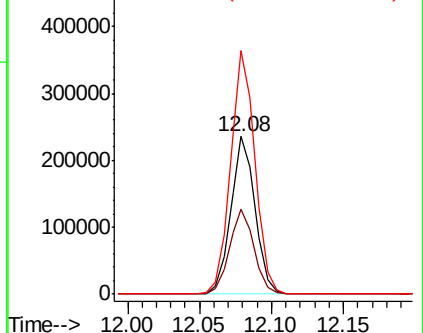

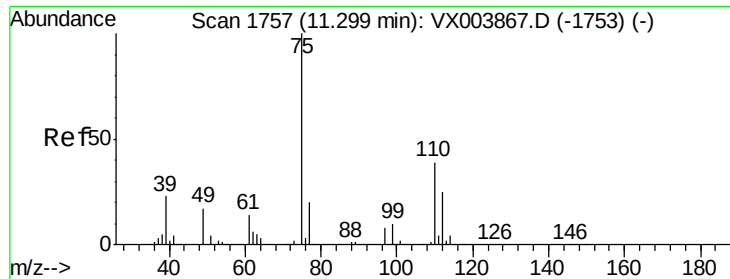

#76

1,2,3-Trichloropropane

Concen: 20.18 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. -0.16 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampled :


FB-08072018

Tot Ion: 75 Resp: 124040

Ion Ratio Lower Upper

75 100

77 1.3 20.8 62.5#

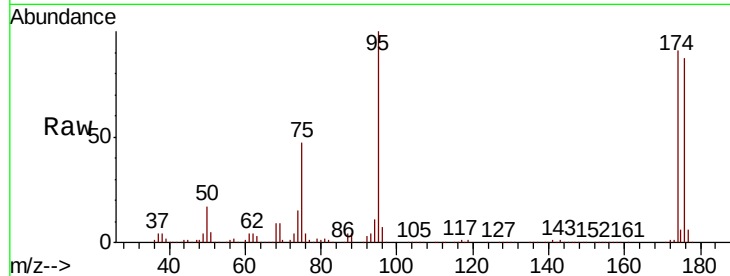

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

11.14

100000

80000

60000



40000

20000

0

Time-->

11.10 11.20

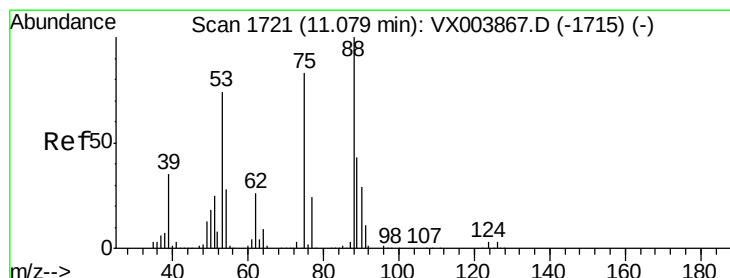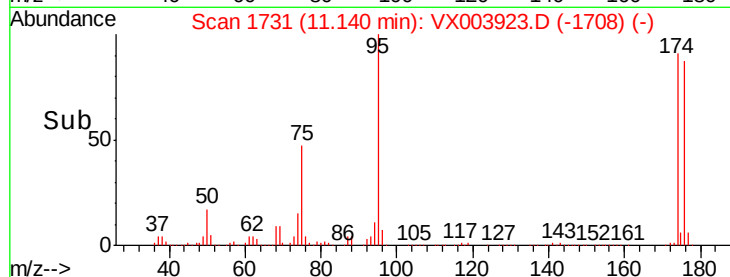

#81

trans-1,4-Dichloro-2-butene

Concen: 54.69 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.06 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05


Tgt Ion: 75 Resp: 124040

Ion Ratio Lower Upper

75 100

53 0.2 80.3 120.5#

89 0.0 37.8 56.8#

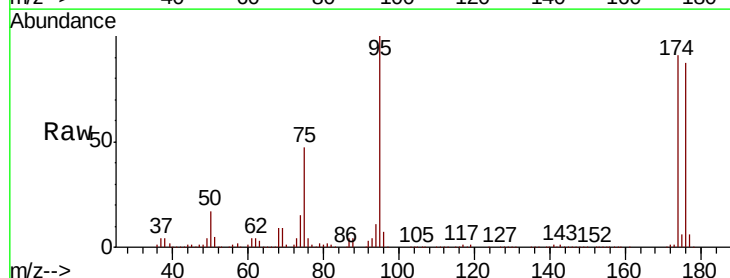

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

11.14


100000


50000

0

Time-->

11.10 11.20

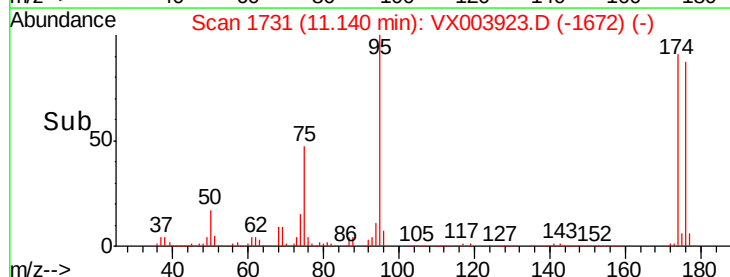



#86

p-Isopropyltoluene

Concen: 0.49 ug/l

RT: 12.07 min Scan# 1883

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05

Instrument :

MSVOA_X

ClientSampleId :

FB-08072018


Tot Ion:119 Resp: 8533

Ion Ratio Lower Upper

119 100

134 27.9 13.3 39.8




91 30.3 10.9 32.7

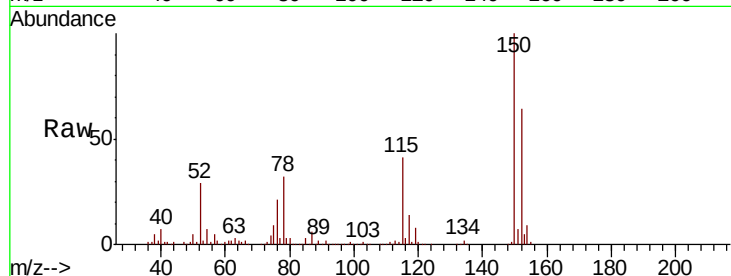

Abundance Ion 119.00 (118.70 to 119.70): V

Ion 134.00 (133.70 to 134.70): V

Ion 91.00 (90.70 to 91.70): V

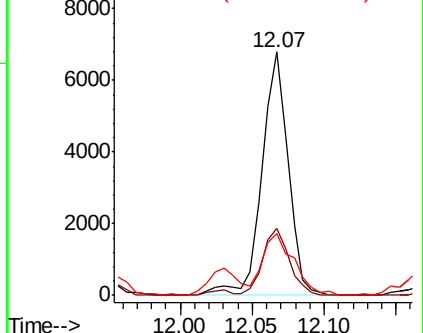

#87

1,3-Dichlorobenzene

Concen: 0.21 ug/l

RT: 12.03 min Scan# 1877

Delta R.T. 0.00 min

Lab File: VX003923.D

Acq: 08 Aug 2018 15:05


Tgt Ion:146 Resp: 2139

Ion Ratio Lower Upper

146 100

111 41.2 18.8 56.4



148 59.5 31.9 95.5




Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

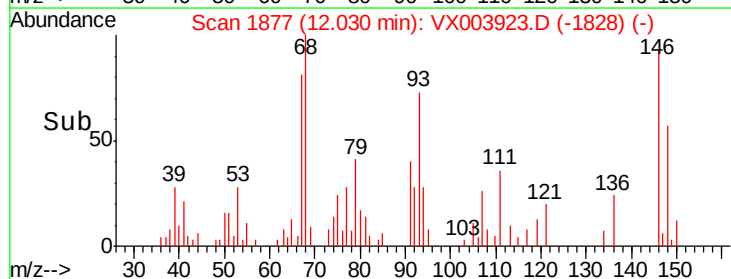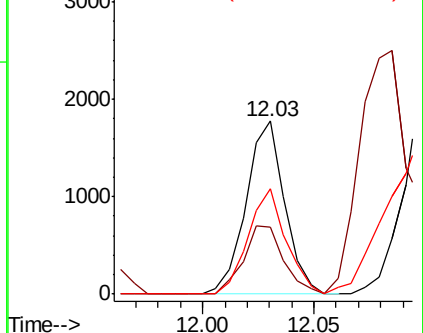


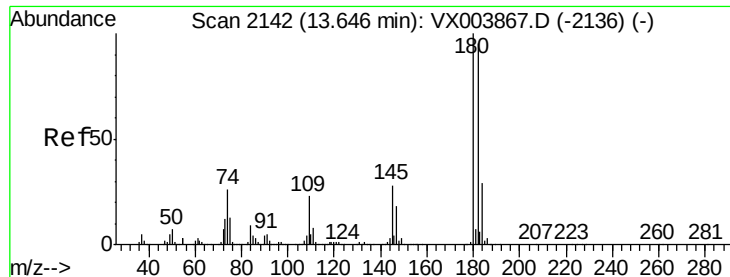

#93
 1,2,4-Trichlorobenzene
 Concen: 0.26 ug/l
 RT: 13.65 min Scan# 2143
 Delta R.T. 0.01 min
 Lab File: VX003923.D
 Acq: 08 Aug 2018 15:05

Instrument :
 MSVOA_X
 ClientSampleId :
 FB-08072018

Tot Ion	Ratio	Lower	Upper
180	100		
182	94.2	47.7	143.1
145	30.3	13.9	41.6



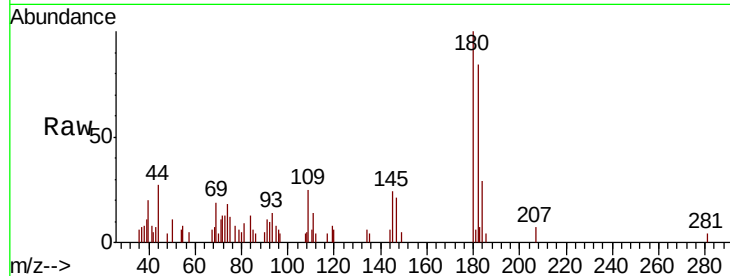


Abundance

Ion 179.80 (179.50 to 180.50): V


Ion 181.80 (181.50 to 182.50): V

Ion 144.80 (144.50 to 145.50): V

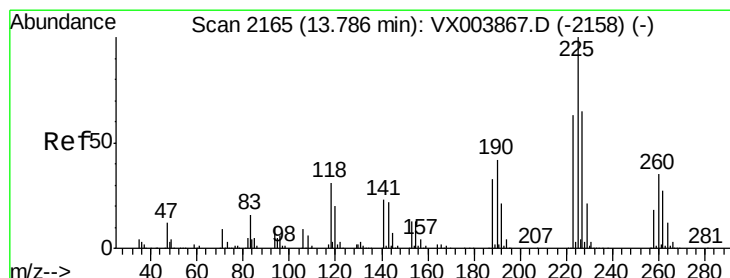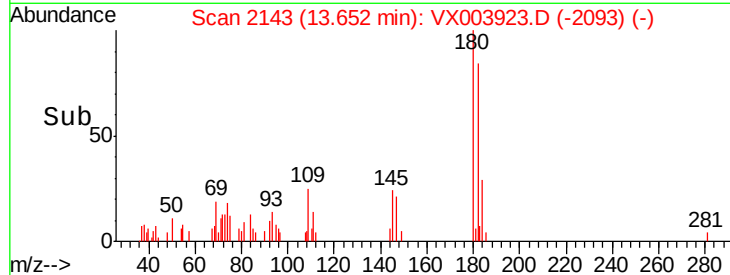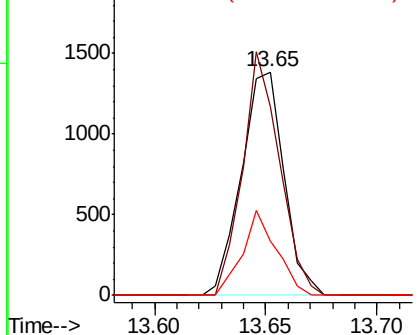

#94
 Hexachlorobutadiene
 Concen: 0.73 ug/l
 RT: 13.79 min Scan# 2165
 Delta R.T. 0.00 min
 Lab File: VX003923.D
 Acq: 08 Aug 2018 15:05

Tgt Ion	Ratio	Lower	Upper
225	100		
223	64.7	31.4	94.0
227	64.2	32.1	96.5


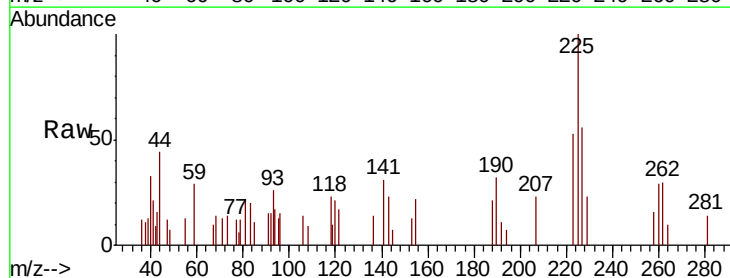



Abundance

Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

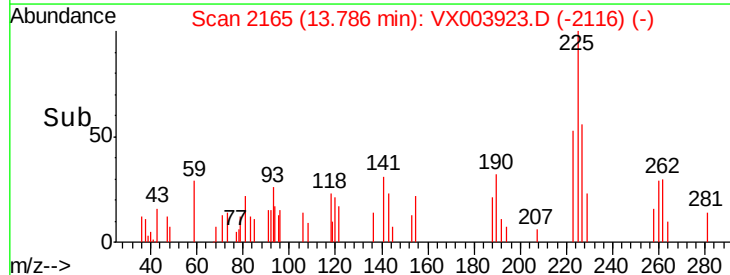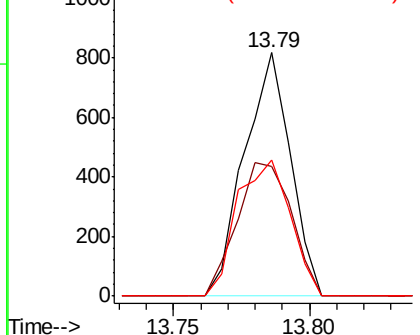

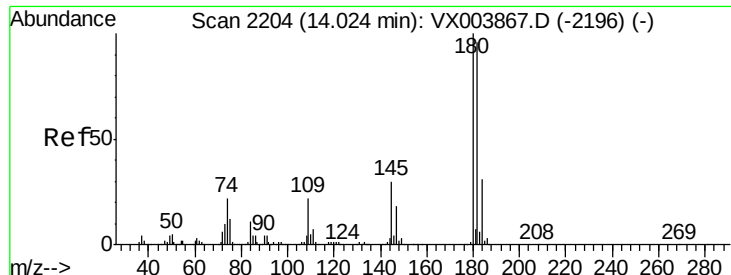

#96
 1,2,3-Trichlorobenzene
 Concen: 0.21 ug/l
 RT: 14.02 min Scan# 2203
 Delta R.T. -0.01 min
 Lab File: VX003923.D
 Acq: 08 Aug 2018 15:05

Instrument :
 MSVOA_X
 ClientSampleId :
 FB-08072018

Tot Ion	Ratio	Lower	Upper
180	100		
182	87.8	48.1	144.4
145	32.4	14.9	44.7

