

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080819\
 Data File : VX011392.D
 Acq On : 08 Aug 2019 15:15
 Operator : JC/SP
 Sample : K3613-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AU-05-080719-A

Quant Time: Aug 09 04:25:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 02 01:55:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.66	168	190127	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	282553	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	258423	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.07	152	119039	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	100938	52.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.44%	
35) Dibromofluoromethane	5.49	113	85871	46.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.10%	
50) Toluene-d8	8.71	98	340510	48.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.80%	
62) 4-Bromofluorobenzene	11.13	95	113230	45.55	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.10%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
6) Chloroethane	1.71	64	306	Below Cal	#	63
8) Diethyl Ether	2.18	74	242	0.210	ug/l	66
11) Tert butyl alcohol	3.01	59	1742	4.585	ug/l #	72
13) Acrolein	2.29	56	27	Below Cal	#	1
16) Acetone	2.43	43	8201	8.999	ug/l	88
18) Methyl Acetate	2.76	43	675	0.324	ug/l #	38
20) Methylene Chloride	2.85	84	35570	17.822	ug/l	98
25) 2-Butanone	4.68	43	1197	0.923	ug/l #	64
29) Tetrahydrofuran	5.15	42	244	0.307	ug/l #	44
30) Chloroform	5.21	83	1023	0.315	ug/l	91
31) Cyclohexane	5.65	56	3757	1.524	ug/l #	1
36) 1,1-Dichloropropene	5.65	75	12644	5.125	ug/l #	46
38) Carbon Tetrachloride	5.66	117	17726	7.142	ug/l #	14
43) Isopropyl Acetate	6.44	43	9479	2.396	ug/l	98
48) Methyl methacrylate	7.67	41	4891	2.627	ug/l #	10
49) 1,4-Dioxane	7.87	88	237	4.391	ug/l #	1
51) 4-Methyl-2-Pentanone	8.61	43	47762	18.707	ug/l #	49
53) t-1,3-Dichloropropene	9.12	75	23	2.846	ug/l #	43
54) cis-1,3-Dichloropropene	8.61	75	23643	8.589	ug/l #	67
57) 1,3-Dichloropropane	9.54	76	5589	1.766	ug/l #	44
59) 2-Hexanone	9.54	43	69048	34.915	ug/l #	51
64) Tetrachloroethene	9.34	164	723	0.329	ug/l #	80
76) 1,2,3-Trichloropropane	11.13	75	57923	26.719	ug/l #	36
80) 1,3,5-Trimethylbenzene	11.51	105	1417	0.208	ug/l	97
81) trans-1,4-Dichloro-2-buten	11.13	75	57923	69.414	ug/l #	10
95) Naphthalene	13.83	128	3403	0.438	ug/l #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX080819\
Data File : VX011392.D
Acq On : 08 Aug 2019 15:15
Operator : JC/SP
Sample : K3613-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AU-05-080719-A

Quant Time: Aug 09 04:25:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 02 01:55:00 2019
Response via : Initial Calibration

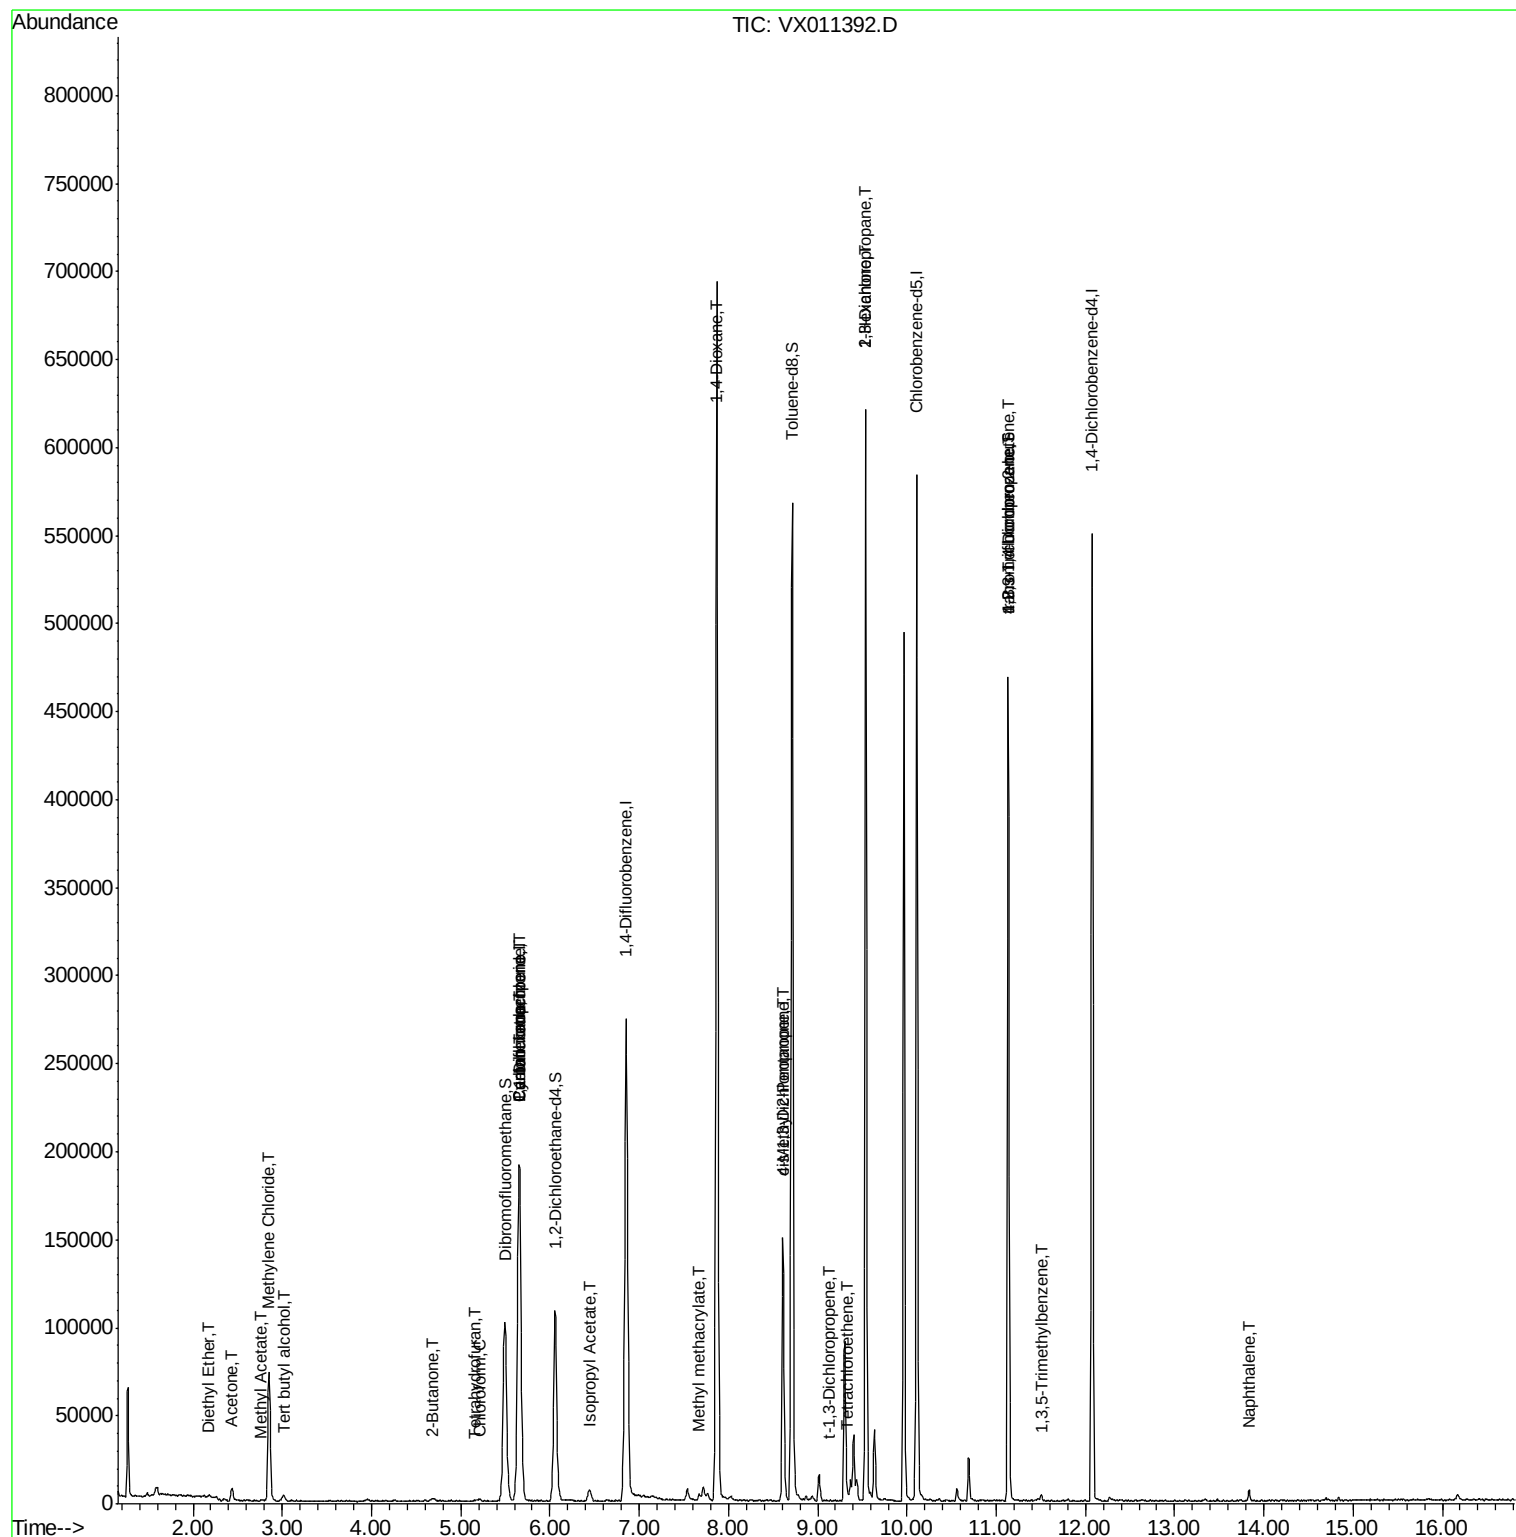



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.66 min Scan# 739

Delta R.T. 0.01 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :


AU-05-080719-A

Tgt Ion: 168 Resp: 190127

Ion Ratio Lower Upper

168 100

99 50.7 38.5 57.7

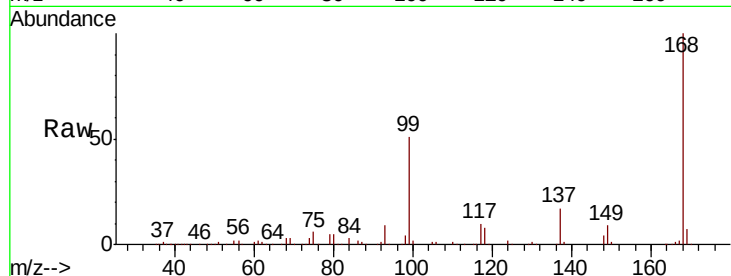

Abundance Ion 167.90 (167.60 to 168.60): VX011392.D (-689) (-)

Ion 98.90 (98.60 to 99.60): VX011392.D (-689) (-)

5.66



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#6

Chloroethane

Concen: Below Cal

RT: 1.71 min Scan# 91

Delta R.T. -0.01 min

Lab File: VX011392.D


Acq: 08 Aug 2019 15:15

Tgt Ion: 64 Resp: 306

Ion Ratio Lower Upper

64 100

66 10.8 25.1 37.7#



Abundance Ion 63.90 (63.60 to 64.60): VX011392.D (-43) (-)

Ion 65.90 (65.60 to 66.60): VX011392.D (-43) (-)

1.71


600


400

200

0

Time--> 1.66 1.68 1.70 1.72



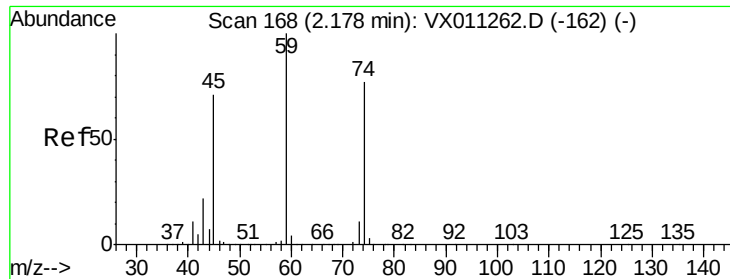

#8

Diethyl Ether

Concen: 0.210 ug/l

RT: 2.18 min Scan# 168

Delta R.T. 0.00 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :


AU-05-080719-A

Tgt Ion: 74 Resp: 242

Ion Ratio Lower Upper




74 100

45 124.8 46.1 138.3



Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

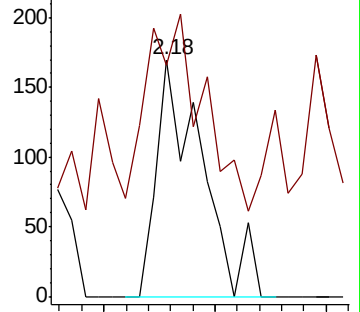

#11

Tert butyl alcohol

Concen: 4.585 ug/l

RT: 3.01 min Scan# 305

Delta R.T. -0.02 min

Lab File: VX011392.D


Acq: 08 Aug 2019 15:15

Tgt Ion: 59 Resp: 1742

Ion Ratio Lower Upper



59 100


57 0.0 8.3 12.5#



Abundance Ion 59.00 (58.70 to 59.70): VX0

Ion 57.00 (56.70 to 57.70): VX0

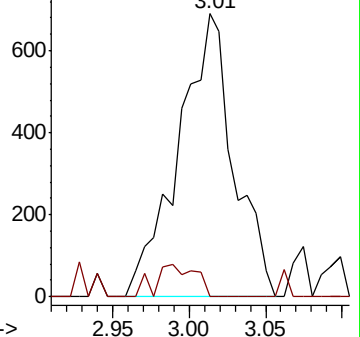

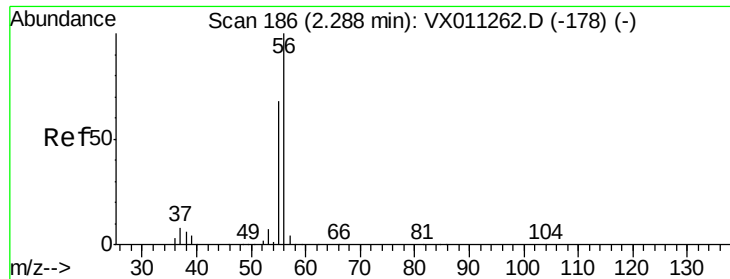

#13

Acrolein

Concen: Below Cal

RT: 2.29 min Scan# 186

Delta R.T. 0.00 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :


AU-05-080719-A

Tgt Ion: 56 Resp: 27

Ion Ratio Lower Upper




56 100

55 414.8 56.0 84.0#



Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

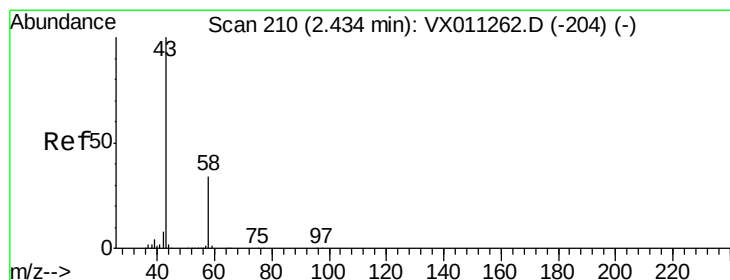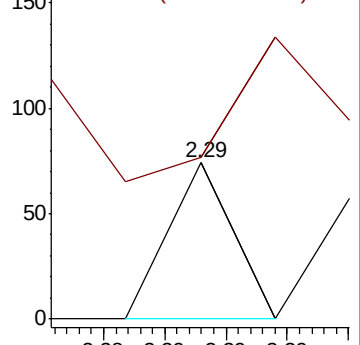

#16

Acetone

Concen: 8.999 ug/l

RT: 2.43 min Scan# 210

Delta R.T. 0.00 min

Lab File: VX011392.D


Acq: 08 Aug 2019 15:15

Tgt Ion: 43 Resp: 8201

Ion Ratio Lower Upper



43 100


58 27.5 27.4 41.0



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0




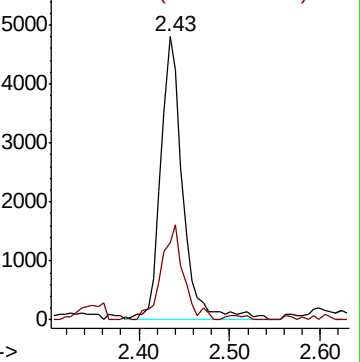




#18
Methyl Acetate
Concen: 0.324 ug/l
RT: 2.76 min Scan# 263
Delta R.T. -0.01 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15




Instrument :
MSVOA_X
ClientSampleId :
AU-05-080719-A


Tgt Ion: 43 Resp: 675
Ion Ratio Lower Upper
43 100
74 57.9 21.0 31.6#

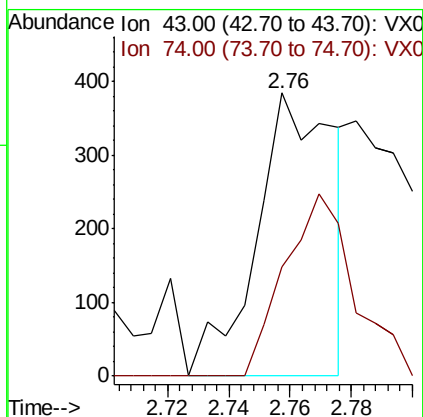

#20
Methylene Chloride
Concen: 17.822 ug/l
RT: 2.85 min Scan# 278
Delta R.T. 0.00 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15

Tgt Ion: 84 Resp: 35570
Ion Ratio Lower Upper
84 100
49 111.6 89.3 133.9
51 35.4 28.3 42.5
86 62.1 54.5 81.7

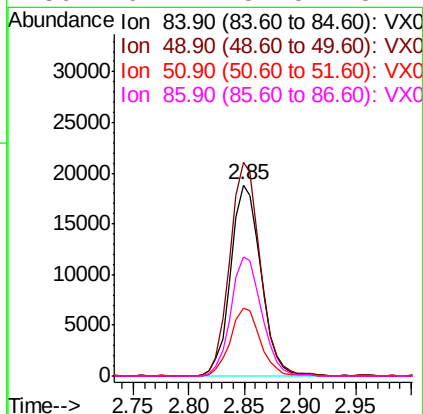

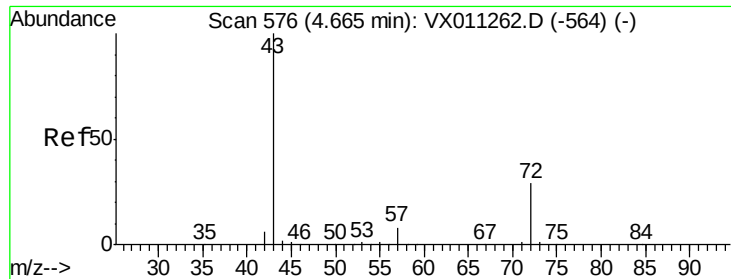

#25

2-Butanone

Concen: 0.923 ug/l

RT: 4.68 min Scan# 579

Delta R.T. 0.02 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampled :





AU-05-080719-A

Tgt Ion: 43 Resp: 1197

Ion Ratio Lower Upper

43 100

72 9.6 23.2 34.8#

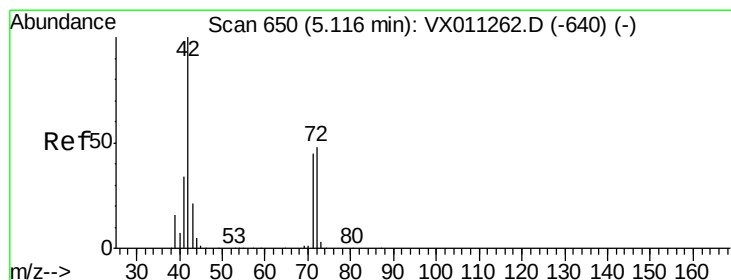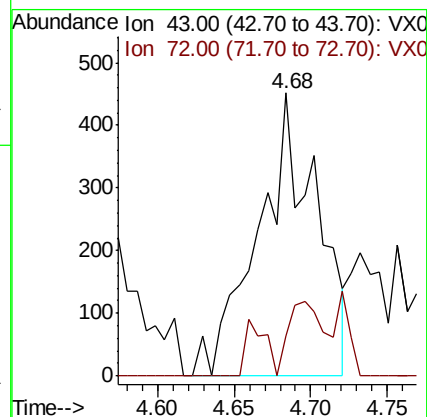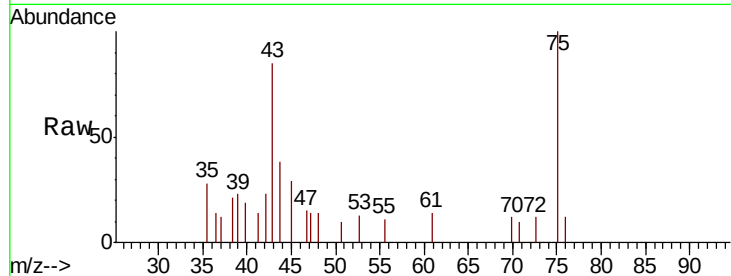

#29

Tetrahydrofuran

Concen: 0.307 ug/l

RT: 5.15 min Scan# 655

Delta R.T. 0.03 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15




Tgt Ion: 42 Resp: 244


Ion Ratio Lower Upper

42 100

72 0.0 39.9 59.9#

71 20.5 36.9 55.3#



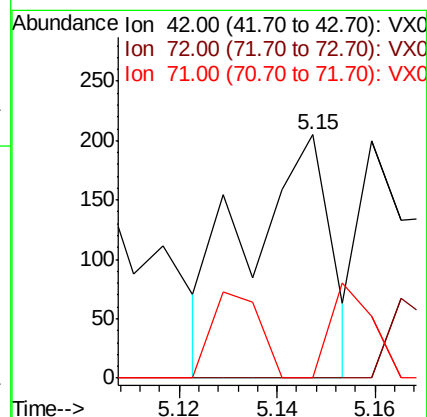



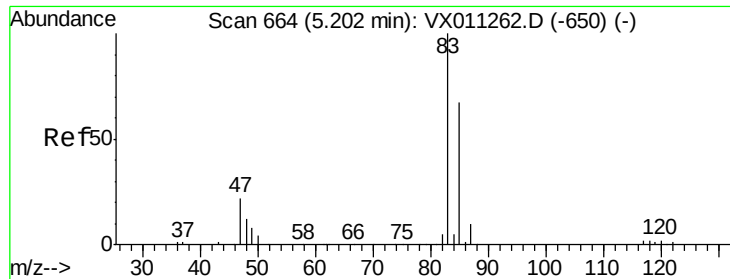

#30
Chloroform
Concen: 0.315 ug/l
RT: 5.21 min Scan# 666
Delta R.T. 0.01 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15




Instrument :
MSVOA_X
ClientSampleId :
AU-05-080719-A


Tgt Ion: 83 Resp: 1023
Ion Ratio Lower Upper
83 100
85 73.9 53.4 80.0

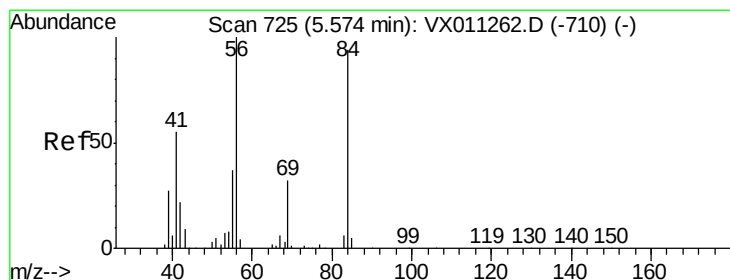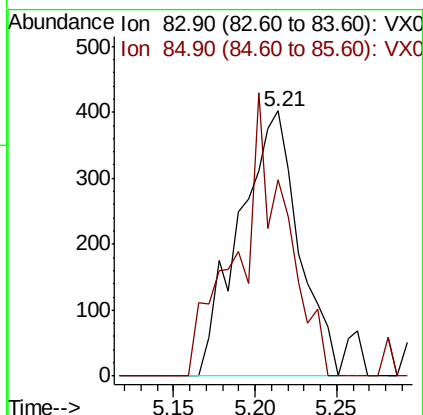

#31
Cyclohexane
Concen: 1.524 ug/l
RT: 5.65 min Scan# 738
Delta R.T. 0.08 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15

Tgt Ion: 56 Resp: 3757
Ion Ratio Lower Upper
56 100
69 176.0 25.5 38.3#
84 146.7 75.0 112.4#



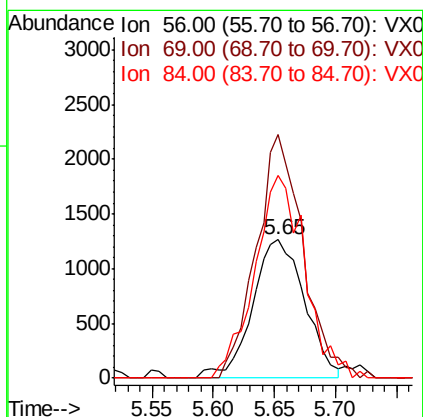



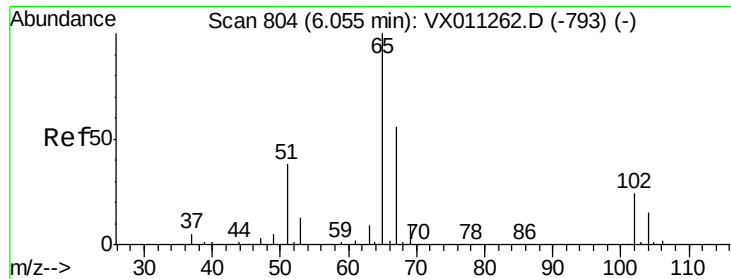

#33
 1,2-Dichloroethane-d4
 Concen: 52.718 ug/l
 RT: 6.06 min Scan# 804
 Delta R.T. 0.00 min
 Lab File: VX011392.D
 Acq: 08 Aug 2019 15:15




Instrument :
 MSVOA_X
 ClientSampleId :
 AU-05-080719-A


Tgt Ion: 65 Resp: 100938
 Ion Ratio Lower Upper
 65 100
 67 51.7 0.0 110.6

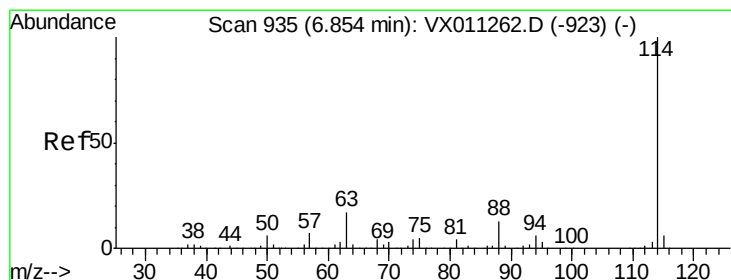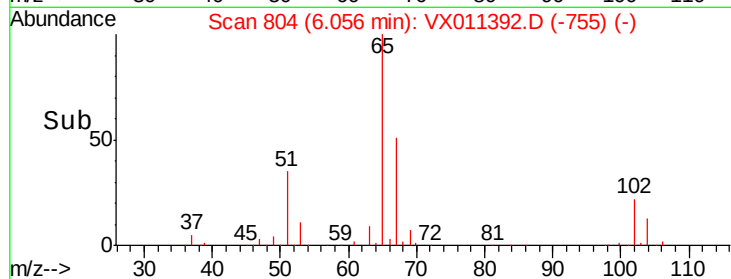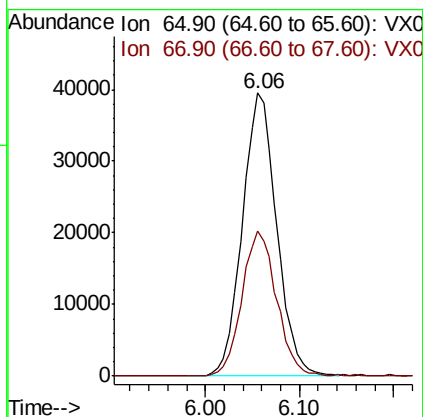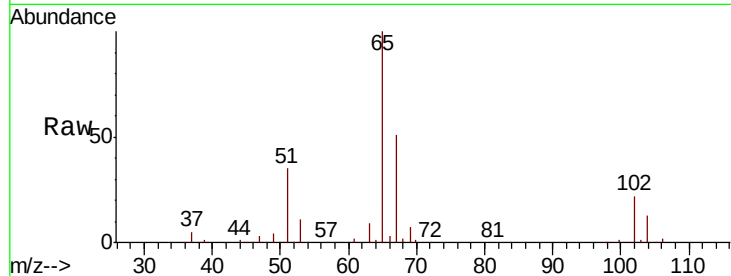

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.85 min Scan# 935
 Delta R.T. 0.00 min
 Lab File: VX011392.D
 Acq: 08 Aug 2019 15:15

Tgt Ion: 114 Resp: 282553
 Ion Ratio Lower Upper
 114 100
 63 18.4 0.0 34.0
 88 14.7 0.0 26.4

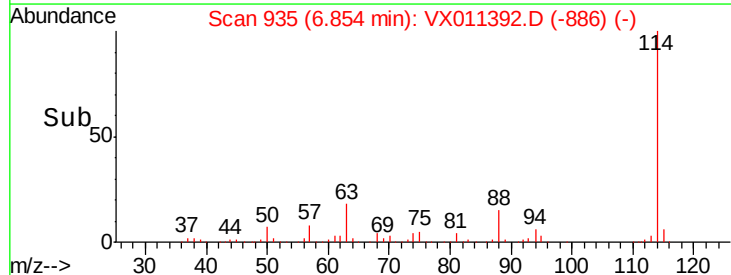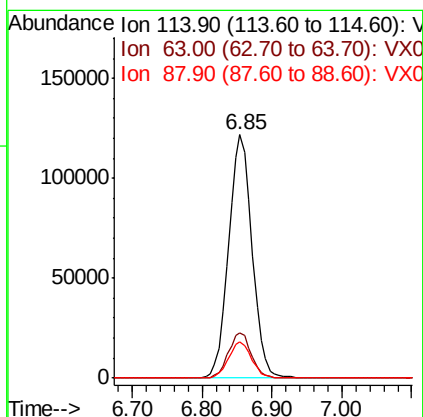

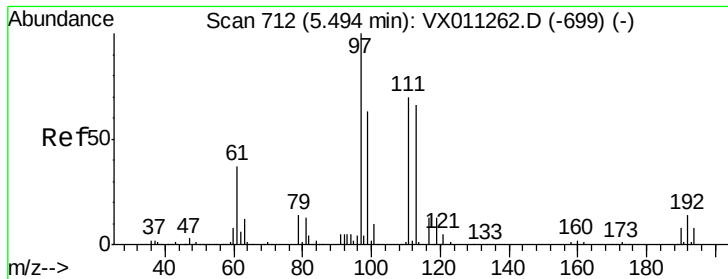

#35

Dibromofluoromethane

Concen: 46.549 ug/l

RT: 5.49 min Scan# 712

Delta R.T. 0.00 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :

AU-05-080719-A


Tgt Ion:113 Resp: 85871

Ion Ratio Lower Upper




113 100

111 102.2 81.9 122.9

192 21.5 17.8 26.8

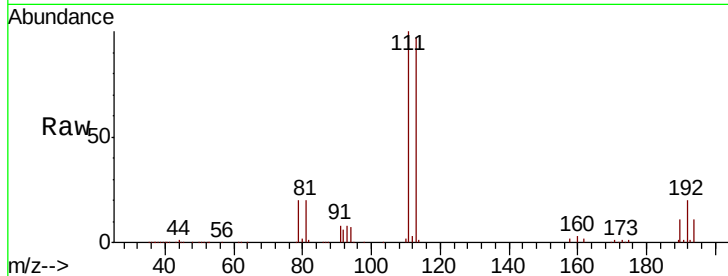

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

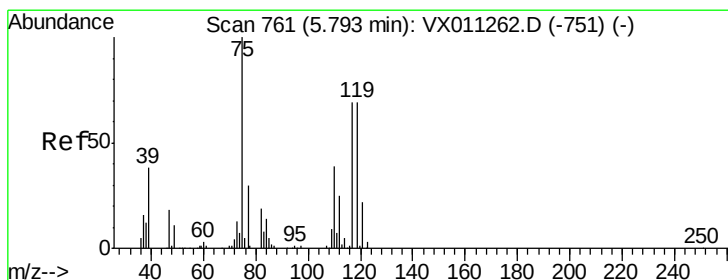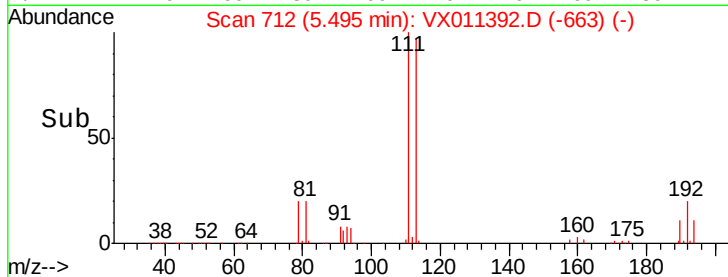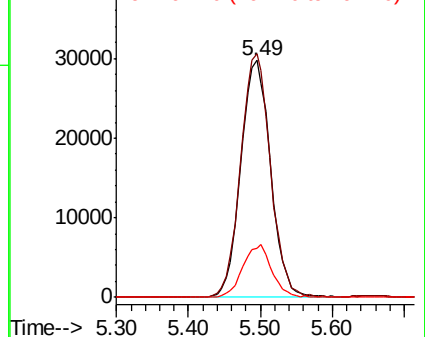

#36

1,1-Dichloropropene

Concen: 5.125 ug/l

RT: 5.65 min Scan# 738

Delta R.T. -0.14 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15


Tgt Ion: 75 Resp: 12644

Ion Ratio Lower Upper



75 100


110 7.8 20.0 59.9#

77 0.3 24.8 37.2#

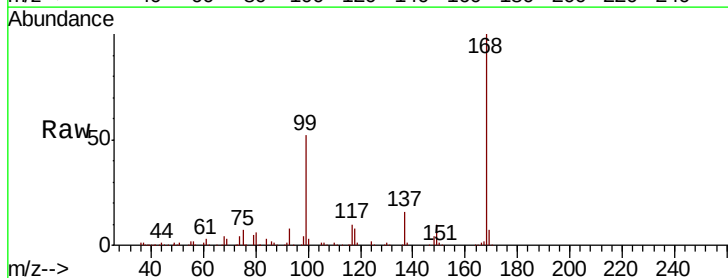

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 109.90 (109.60 to 110.60): V
Ion 76.90 (76.60 to 77.60): VX0



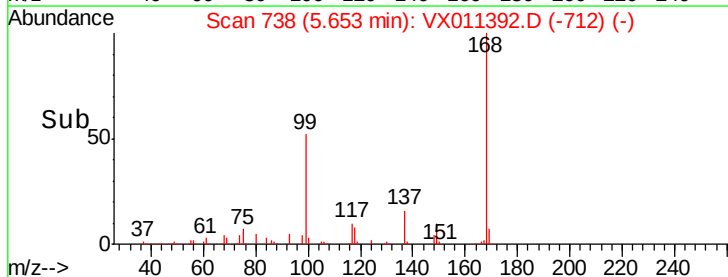
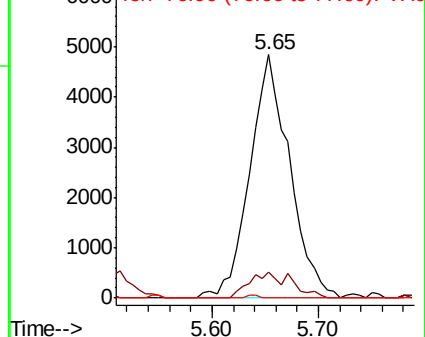




#38
Carbon Tetrachloride
Concen: 7.142 ug/l
RT: 5.66 min Scan# 739
Delta R.T. -0.12 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15




Instrument :
MSVOA_X
ClientSampleId :
AU-05-080719-A


Tgt Ion:117 Resp: 17726
Ion Ratio Lower Upper
117 100
119 3.8 79.0 118.4#
121 0.0 25.9 38.9#

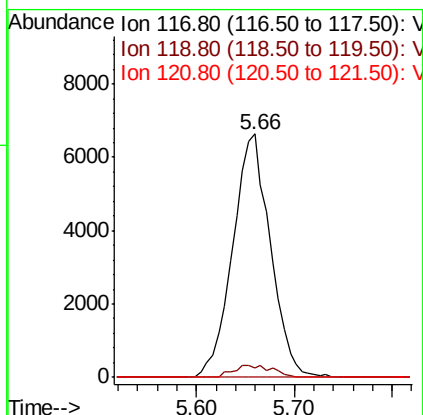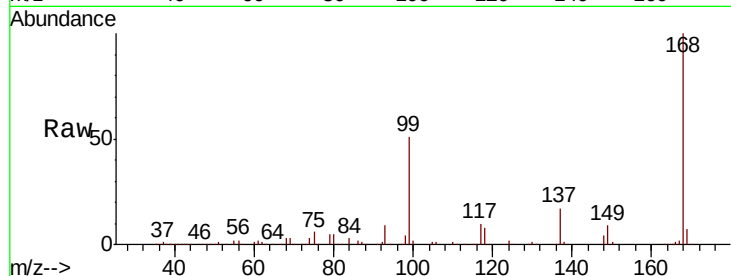

#43
Isopropyl Acetate
Concen: 2.396 ug/l
RT: 6.44 min Scan# 867
Delta R.T. 0.00 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15

Tgt Ion: 43 Resp: 9479
Ion Ratio Lower Upper
43 100
61 21.4 16.5 24.7
87 16.3 12.1 18.1

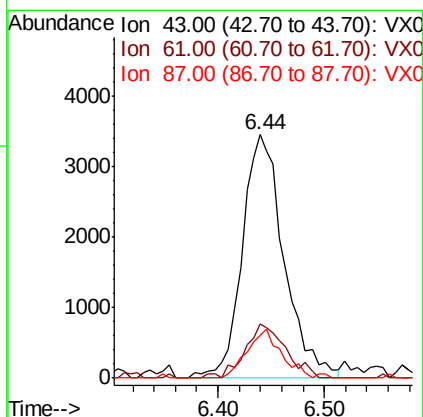

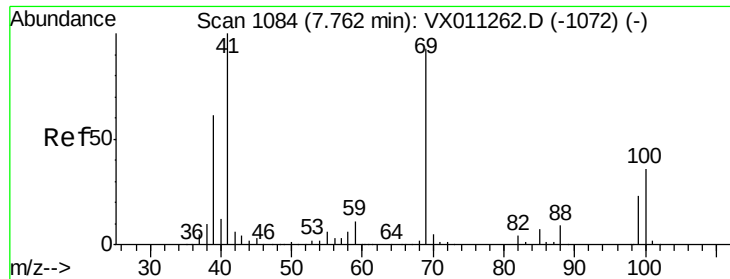

#48

Methyl methacrylate

Concen: 2.627 ug/l

RT: 7.67 min Scan# 1069

Delta R.T. -0.09 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :

AU-05-080719-A


Tgt Ion: 41 Resp: 4891

Ion Ratio Lower Upper

41 100

69 0.4 74.5 111.7#




39 0.0 48.6 72.8#



Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

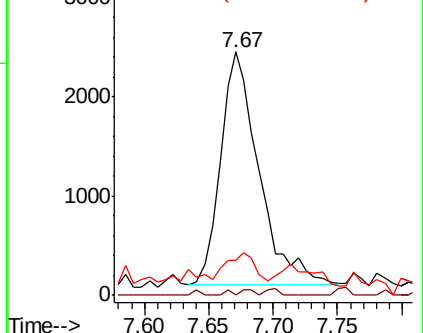

#49

1,4-Dioxane

Concen: 4.391 ug/l

RT: 7.87 min Scan# 1101

Delta R.T. 0.13 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15


Tgt Ion: 88 Resp: 237

Ion Ratio Lower Upper

88 100

43 264175.5 22.2 33.2#



58 1420.7 47.8 71.8#




Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

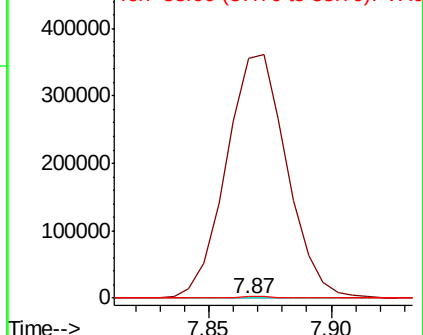

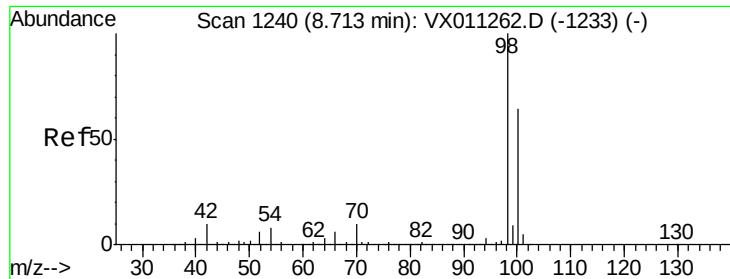

#50

Toluene-d8

Concen: 48.901 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :


AU-05-080719-A

Tgt Ion: 98 Resp: 340510

Ion Ratio Lower Upper




98 100

100 63.7 51.7 77.5



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX0

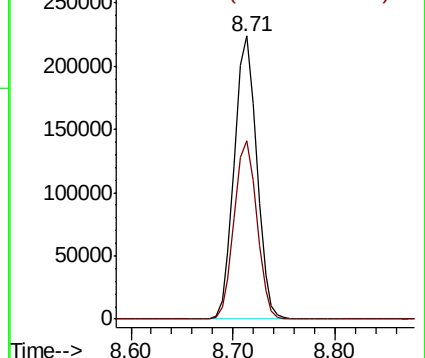

#51

4-Methyl-2-Pentanone

Concen: 18.707 ug/l

RT: 8.61 min Scan# 1223

Delta R.T. -0.03 min

Lab File: VX011392.D


Acq: 08 Aug 2019 15:15

Tgt Ion: 43 Resp: 47762

Ion Ratio Lower Upper



43 100


58 8.7 32.3 48.5#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0



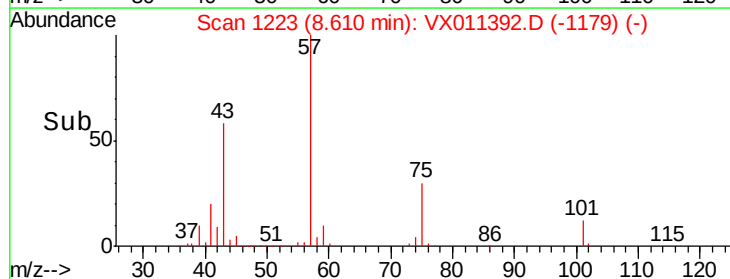
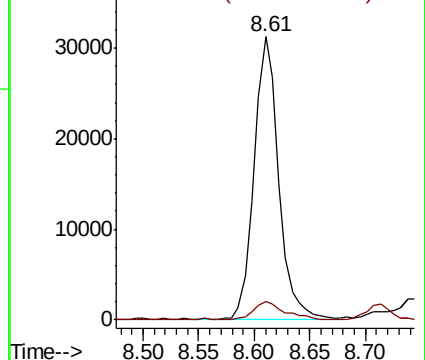




#53
 t-1,3-Dichloropropene
 Concen: 2.846 ug/l
 RT: 9.12 min Scan# 1307
 Delta R.T. 0.09 min
 Lab File: VX011392.D
 Acq: 08 Aug 2019 15:15




Instrument :
 MSVOA_X
 ClientSampleId :
 AU-05-080719-A


Tgt Ion: 75 Resp: 23
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.4 38.0#

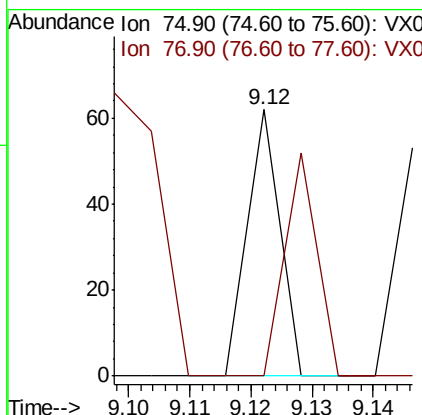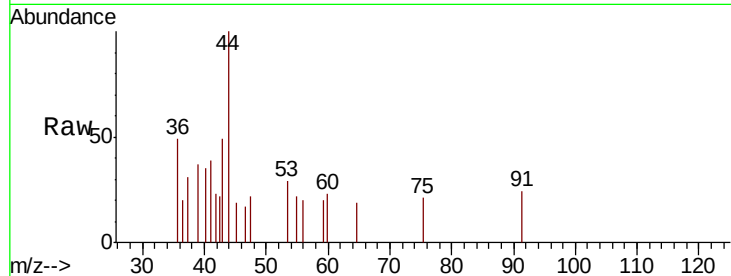

#54
 cis-1,3-Dichloropropene
 Concen: 8.589 ug/l
 RT: 8.61 min Scan# 1223
 Delta R.T. 0.18 min
 Lab File: VX011392.D
 Acq: 08 Aug 2019 15:15

Tgt Ion: 75 Resp: 23643
 Ion Ratio Lower Upper
 75 100
 77 0.7 25.0 37.6#
 39 33.1 35.3 52.9#



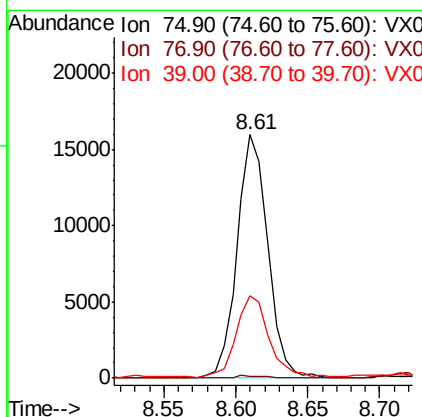
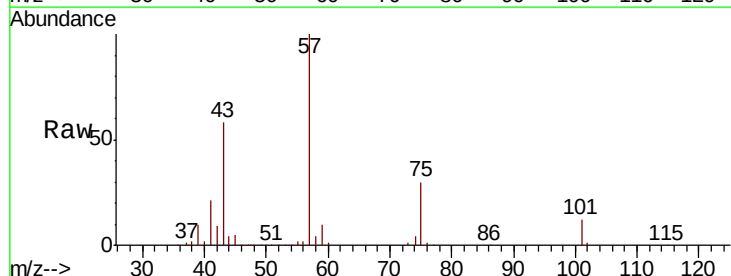


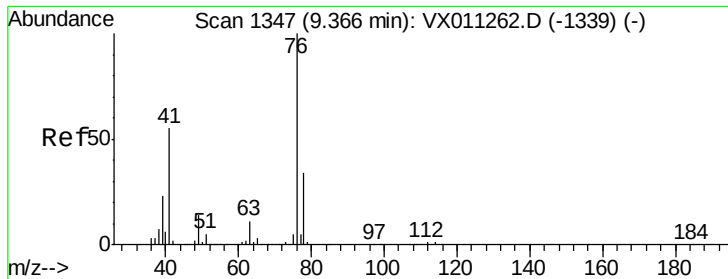

#57
 1,3-Dichloropropane
 Concen: 1.766 ug/l
 RT: 9.54 min Scan# 1375
 Delta R.T. 0.17 min
 Lab File: VX011392.D
 Acq: 08 Aug 2019 15:15




Instrument :
 MSVOA_X
 ClientSampleId :
 AU-05-080719-A


Tgt Ion: 76 Resp: 5589
 Ion Ratio Lower Upper
 76 100
 78 1.5 26.6 40.0#

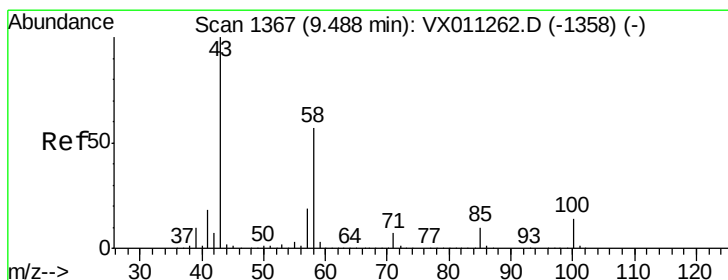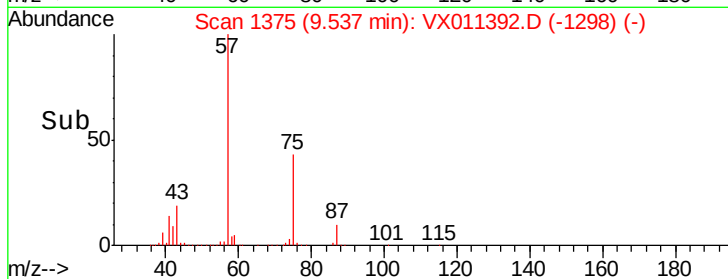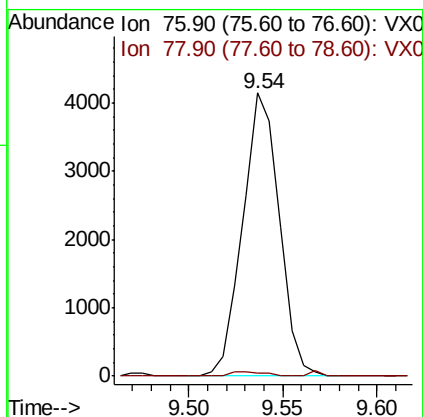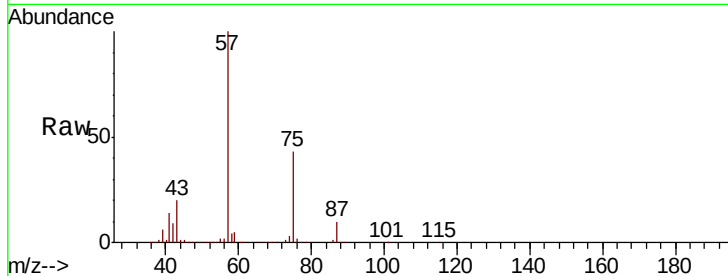

#59
 2-Hexanone
 Concen: 34.915 ug/l
 RT: 9.54 min Scan# 1375
 Delta R.T. 0.05 min
 Lab File: VX011392.D
 Acq: 08 Aug 2019 15:15

Tgt Ion: 43 Resp: 69048
 Ion Ratio Lower Upper
 43 100
 58 20.3 28.2 84.6#


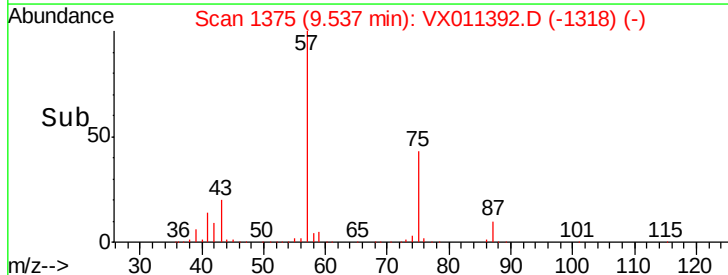
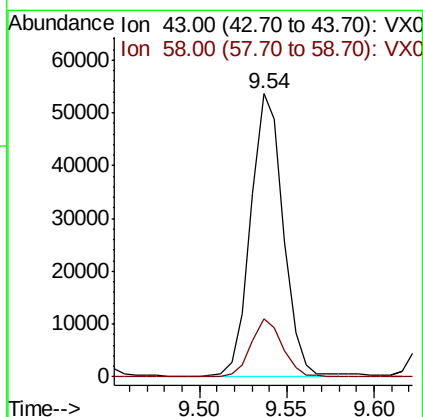
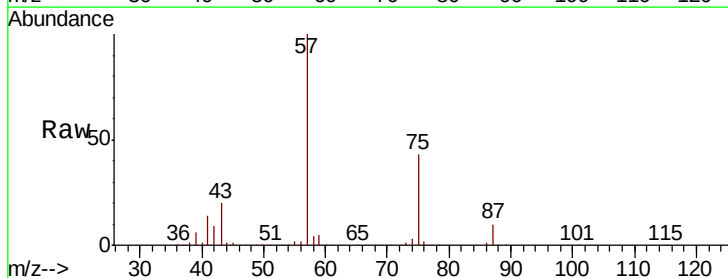




#62
4-Bromofluorobenzene
Concen: 45.545 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.00 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15




Instrument :
MSVOA_X
ClientSampleId :
AU-05-080719-A


Tgt Ion: 95 Resp: 113230
Ion Ratio Lower Upper
95 100
174 90.8 0.0 191.2
176 88.1 0.0 184.8

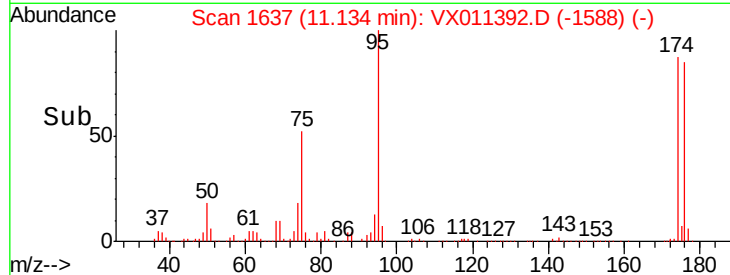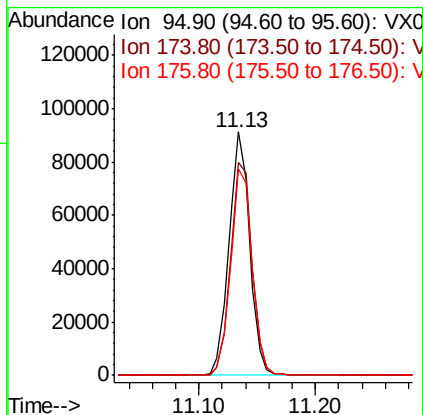

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. 0.00 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15

Tgt Ion: 117 Resp: 258423
Ion Ratio Lower Upper
117 100
82 53.5 42.2 63.2
119 33.5 26.6 39.8

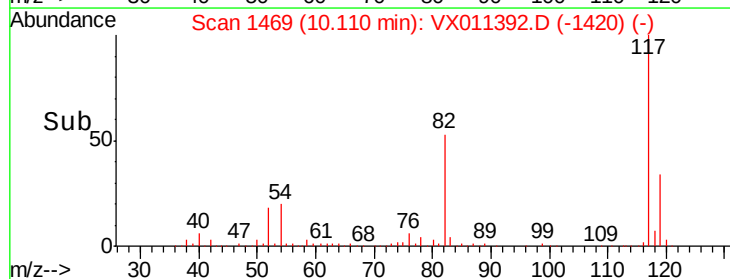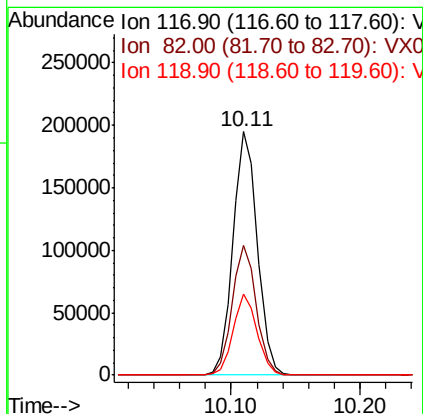



#64

Tetrachloroethene

Concen: 0.329 ug/l

RT: 9.34 min Scan# 1342

Delta R.T. 0.00 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :

AU-05-080719-A

Tgt Ion:164 Resp: 723


Ion Ratio Lower Upper

164 100

166 107.5 107.5 161.3

129 99.6 71.0 106.4

131 64.4 69.8 104.6#






Abundance Ion 163.80 (163.50 to 164.50): V

Ion 165.80 (165.50 to 166.50): V

Ion 128.80 (128.50 to 129.50): V

Ion 130.80 (130.50 to 131.50): V

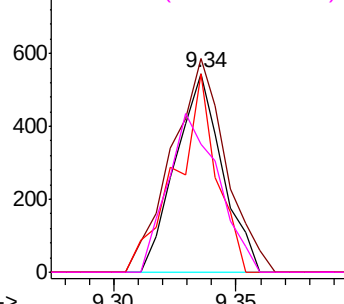

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.07 min Scan# 1791

Delta R.T. -0.01 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15


Tgt Ion:152 Resp: 119039

Ion Ratio Lower Upper

152 100

115 54.4 40.0 119.9



150 155.0 0.0 350.4




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

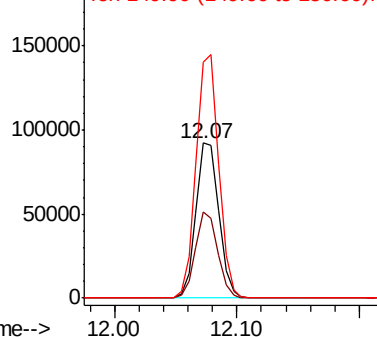

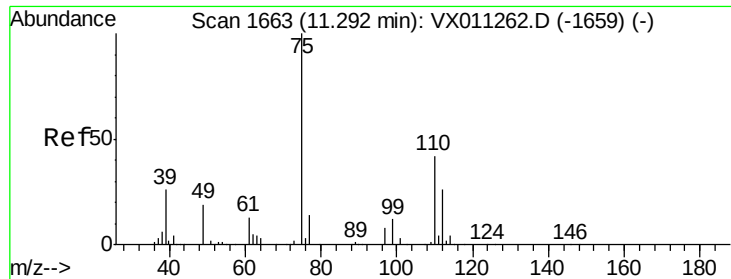

#76

1,2,3-Trichloropropane

Concen: 26.719 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX011392.D

Acq: 08 Aug 2019 15:15

Instrument :

MSVOA_X

ClientSampleId :


AU-05-080719-A

Tgt Ion: 75 Resp: 57923

Ion Ratio Lower Upper




75 100

77 1.5 21.1 63.4#

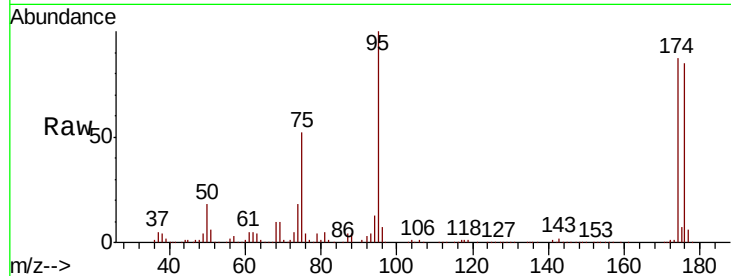

Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0

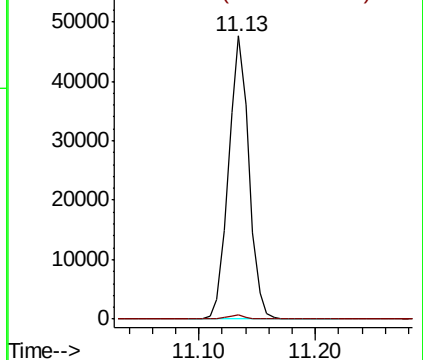

#80

1,3,5-Trimethylbenzene

Concen: 0.208 ug/l

RT: 11.51 min Scan# 1698

Delta R.T. 0.00 min

Lab File: VX011392.D


Acq: 08 Aug 2019 15:15

Tgt Ion: 105 Resp: 1417

Ion Ratio Lower Upper



105 100


120 48.0 25.1 75.2



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V




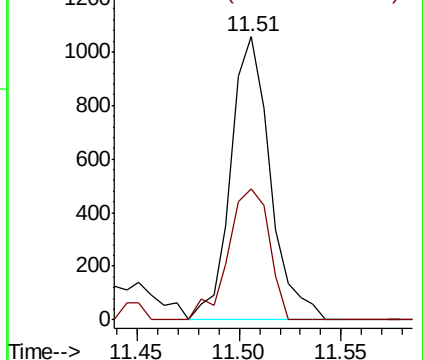


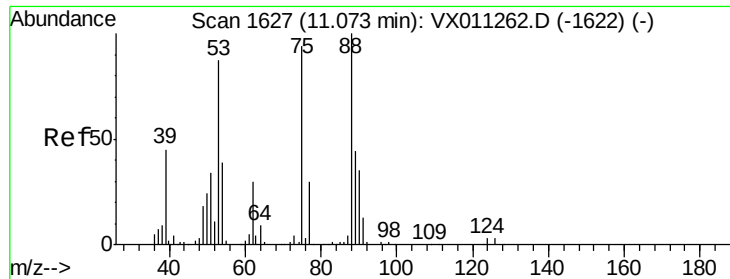

#81
trans-1,4-Dichloro-2-butene
Concen: 69.414 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. 0.06 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15

Instrument :
MSVOA_X
ClientSampleId :
AU-05-080719-A

Tgt Ion: 75 Resp: 57923
Ion Ratio Lower Upper
75 100
53 0.3 78.2 117.4#
89 0.1 37.9 56.9#

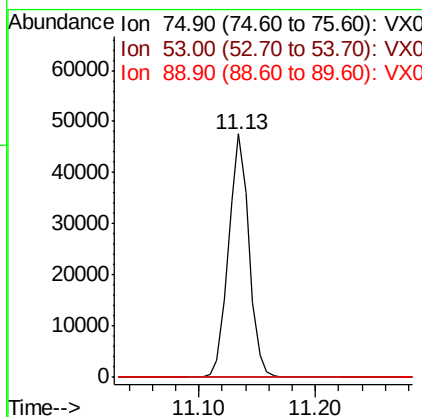

#95
Naphthalene
Concen: 0.438 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. 0.00 min
Lab File: VX011392.D
Acq: 08 Aug 2019 15:15

Tgt Ion: 128 Resp: 3403
Ion Ratio Lower Upper
128 100
127 12.0 10.4 15.6
129 15.4 8.9 13.3#

