

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030508.D
 Acq On : 08 Aug 2022 13:20
 Operator : JC/MD
 Sample : N4021-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030508.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	114255	120355	11.68%	1.496%
2	1.660	91	94	106	rVB	92169	118820	11.53%	1.476%
3	2.142	172	173	176	rBV3	973	1046	0.10%	0.013%
4	2.300	193	199	210	rVB	190924	306362	29.74%	3.807%
5	2.508	229	233	236	rBV4	869	1355	0.13%	0.017%
6	2.605	247	249	252	rBV2	592	702	0.07%	0.009%
7	2.788	276	279	286	rVB2	2250	3673	0.36%	0.046%
8	2.947	300	305	311	rVB4	1436	3518	0.34%	0.044%
9	3.038	319	320	324	rVB	522	488	0.05%	0.006%
10	3.215	346	349	351	rBV	710	804	0.08%	0.010%
11	3.416	380	382	383	rBV	397	264	0.03%	0.003%
12	3.447	386	387	389	rBV	578	426	0.04%	0.005%
13	3.581	404	409	411	rBV2	314	371	0.04%	0.005%
14	3.715	428	431	435	rBV2	229	462	0.04%	0.006%
15	3.818	446	448	449	rVB	393	267	0.03%	0.003%
16	3.843	449	452	453	rBV	491	510	0.05%	0.006%
17	4.276	521	523	527	rBV	243	263	0.03%	0.003%
18	4.465	545	554	569	rBV	94790	275101	26.71%	3.418%
19	4.727	595	597	599	rVB2	570	434	0.04%	0.005%
20	5.056	639	651	666	rBV	133394	421456	40.91%	5.237%
21	5.215	676	677	680	rVV3	688	557	0.05%	0.007%
22	5.245	680	682	686	rVB3	590	643	0.06%	0.008%
23	5.306	688	692	694	rVB	523	608	0.06%	0.008%
24	5.458	714	717	718	rBV	301	267	0.03%	0.003%
25	5.501	722	724	727	rVB2	339	309	0.03%	0.004%
26	5.550	727	732	739	rBV3	1304	3285	0.32%	0.041%
27	5.970	789	801	816	rBV2	350920	1030147	100.00%	12.801%
28	6.257	846	848	851	rBV	266	239	0.02%	0.003%
29	6.513	888	890	892	rBV2	300	253	0.02%	0.003%
30	6.684	917	918	920	rBV2	422	344	0.03%	0.004%
31	6.763	922	931	945	rVV	285535	683315	66.33%	8.491%
32	6.982	965	967	969	rBV2	344	251	0.02%	0.003%
33	7.111	981	988	998	rVB4	11790	28341	2.75%	0.352%
34	7.312	1011	1021	1031	rBV	213054	473646	45.98%	5.886%
35	7.476	1046	1048	1049	rBV2	595	297	0.03%	0.004%
36	7.531	1055	1057	1059	rBV2	348	312	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030508.D
 Acq On : 08 Aug 2022 13:20
 Operator : JC/MD
 Sample : N4021-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.592	1064	1067	1069	rBV2	503	684	0.07%	0.008%
38	7.641	1072	1075	1078	rBV	265	389	0.04%	0.005%
39	7.671	1078	1080	1082	rBV	308	248	0.02%	0.003%
40	7.714	1085	1087	1089	rVB2	499	345	0.03%	0.004%
41	7.885	1111	1115	1117	rBV	310	422	0.04%	0.005%
42	7.946	1122	1125	1127	rBV2	596	743	0.07%	0.009%
43	8.177	1160	1163	1165	rBV2	297	345	0.03%	0.004%
44	8.324	1181	1187	1201	rBV	141871	245224	23.80%	3.047%
45	8.488	1211	1214	1218	rVV4	709	879	0.09%	0.011%
46	8.653	1234	1241	1252	rBV	502964	800088	77.67%	9.942%
47	8.757	1257	1258	1262	rVB3	1218	871	0.08%	0.011%
48	8.952	1284	1290	1301	rBV	111070	160381	15.57%	1.993%
49	9.086	1310	1312	1313	rBV	312	236	0.02%	0.003%
50	9.153	1321	1323	1325	rVV2	415	363	0.04%	0.005%
51	9.269	1340	1342	1344	rBV3	826	842	0.08%	0.010%
52	9.385	1356	1361	1372	rBV	424453	602312	58.47%	7.484%
53	9.653	1403	1405	1408	rVB2	501	420	0.04%	0.005%
54	9.769	1421	1424	1425	rBV	408	368	0.04%	0.005%
55	9.830	1432	1434	1437	rBV	303	398	0.04%	0.005%
56	9.964	1454	1456	1457	rBV	317	248	0.02%	0.003%
57	10.055	1465	1471	1484	rBV	610620	793739	77.05%	9.863%
58	10.147	1484	1486	1490	rVV3	1029	887	0.09%	0.011%
59	10.177	1490	1491	1494	rVB	597	348	0.03%	0.004%
60	10.348	1517	1519	1521	rBV	494	258	0.03%	0.003%
61	10.403	1526	1528	1529	rBV2	377	318	0.03%	0.004%
62	10.427	1530	1532	1537	rVV2	295	390	0.04%	0.005%
63	10.732	1579	1582	1583	rBV2	311	426	0.04%	0.005%
64	10.848	1599	1601	1603	rBV	331	244	0.02%	0.003%
65	10.927	1612	1614	1617	rVB	458	385	0.04%	0.005%
66	10.963	1617	1620	1621	rBV2	477	451	0.04%	0.006%
67	11.012	1626	1628	1631	rBV	320	242	0.02%	0.003%
68	11.061	1634	1636	1638	rBV2	348	419	0.04%	0.005%
69	11.195	1652	1658	1664	rBV	381811	485258	47.11%	6.030%
70	11.482	1704	1705	1706	rBV	480	250	0.02%	0.003%
71	11.518	1710	1711	1713	rBV	278	253	0.02%	0.003%
72	11.628	1727	1729	1731	rBV	374	342	0.03%	0.004%
73	11.683	1736	1738	1741	rVB2	547	497	0.05%	0.006%
74	11.713	1741	1743	1745	rBV2	489	492	0.05%	0.006%
75	11.756	1748	1750	1752	rVV	480	334	0.03%	0.004%
76	11.847	1763	1765	1766	rBV	441	374	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030508.D
 Acq On : 08 Aug 2022 13:20
 Operator : JC/MD
 Sample : N4021-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.976	1785	1786	1788	rBV2	664	530	0.05%	0.007%
78	12.024	1789	1794	1805	rVV	621129	753607	73.16%	9.364%
79	12.225	1825	1827	1829	rBV2	688	631	0.06%	0.008%
80	12.323	1837	1843	1851	rBV	540820	701531	68.10%	8.717%
81	12.774	1915	1917	1919	rBV	312	253	0.02%	0.003%
82	12.829	1924	1926	1927	rBV2	421	326	0.03%	0.004%
83	12.975	1949	1950	1955	rVB2	669	732	0.07%	0.009%
84	13.036	1957	1960	1961	rBV2	330	339	0.03%	0.004%
85	13.122	1973	1974	1977	rVB2	613	494	0.05%	0.006%
86	13.207	1986	1988	1990	rBV2	520	541	0.05%	0.007%
87	13.262	1995	1997	1998	rVV	421	248	0.02%	0.003%
88	13.365	2012	2014	2015	rBV	417	293	0.03%	0.004%
89	13.402	2018	2020	2022	rVB2	576	303	0.03%	0.004%
90	13.542	2041	2043	2044	rBV2	441	420	0.04%	0.005%
91	13.615	2051	2055	2057	rBV	630	836	0.08%	0.010%
92	14.091	2132	2133	2135	rBV2	569	381	0.04%	0.005%
93	14.189	2147	2149	2151	rBV2	607	563	0.05%	0.007%
94	14.402	2182	2184	2185	rVB	542	287	0.03%	0.004%
95	14.420	2185	2187	2188	rBV	451	329	0.03%	0.004%
96	14.579	2211	2213	2216	rVB2	767	521	0.05%	0.006%
97	14.609	2216	2218	2222	rBV2	559	881	0.09%	0.011%
98	14.719	2234	2236	2237	rBV	459	240	0.02%	0.003%
99	15.548	2370	2372	2374	rBV	756	389	0.04%	0.005%
100	15.621	2381	2384	2389	rBV4	804	1762	0.17%	0.022%




Sum of corrected areas: 8047641

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030508.D
Acq On : 08 Aug 2022 13:20
Operator : JC/MD
Sample : N4021-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

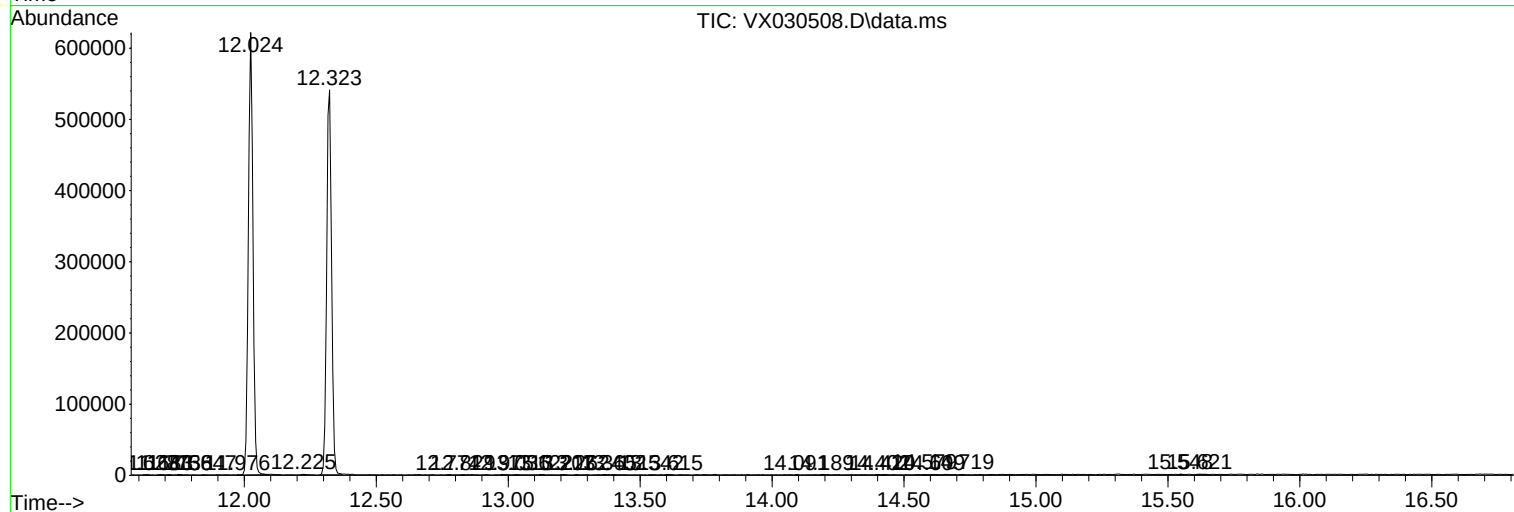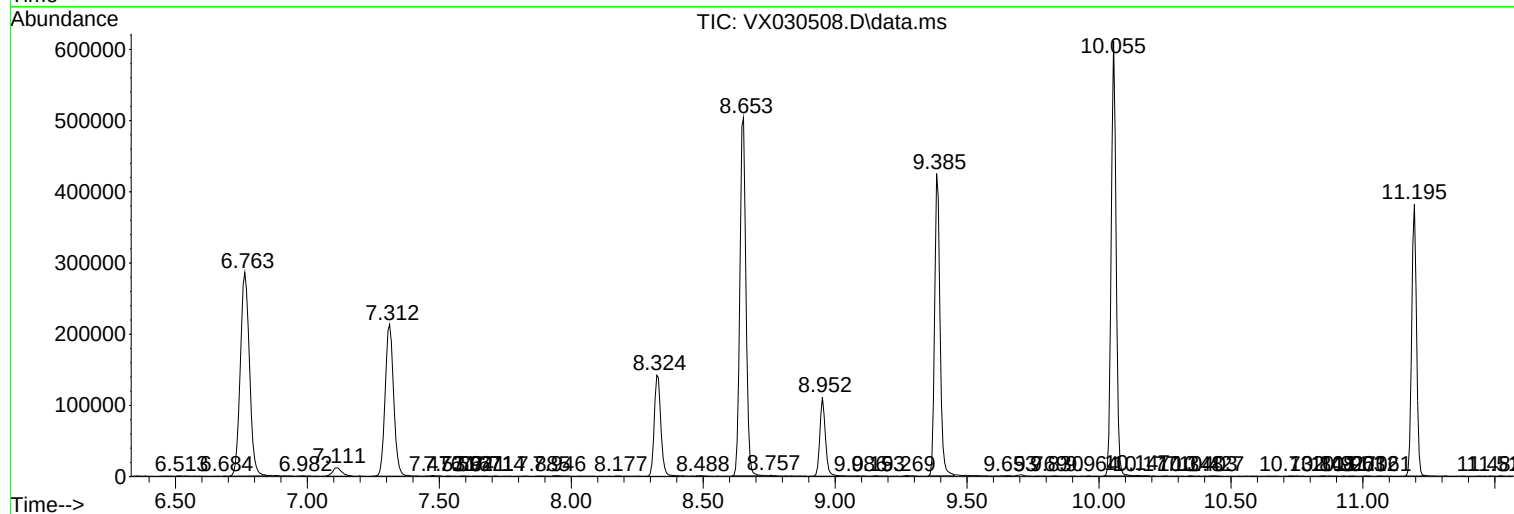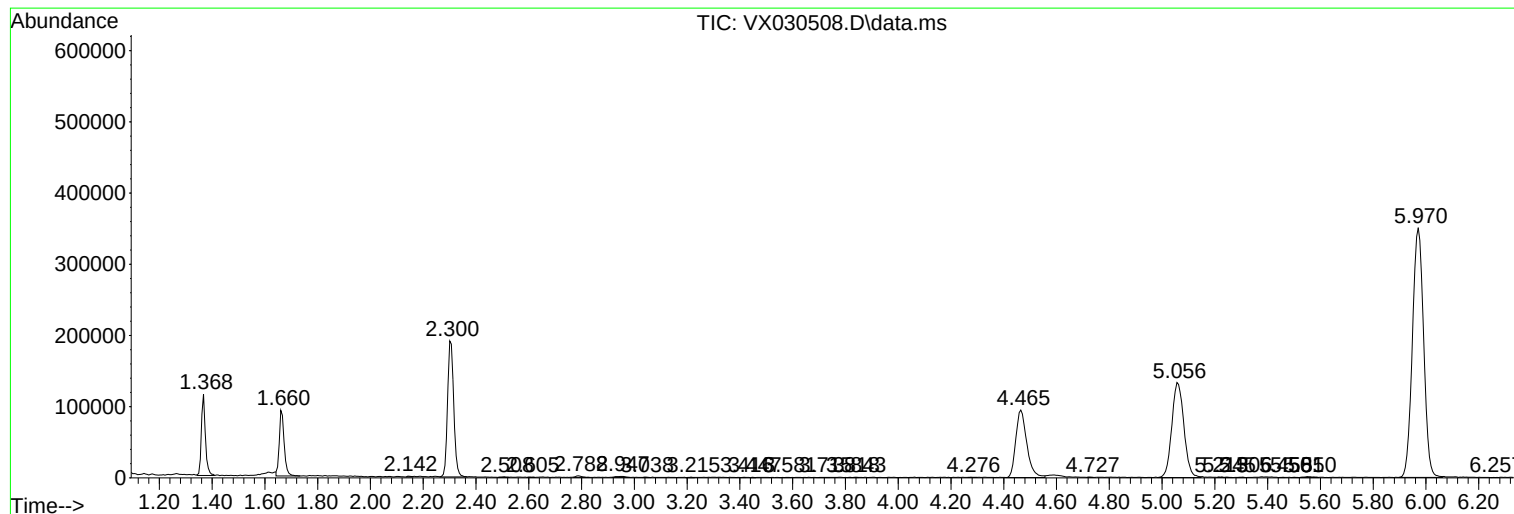

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030508.D
Acq On : 08 Aug 2022 13:20
Operator : JC/MD
Sample : N4021-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030508.D
Acq On : 08 Aug 2022 13:20
Operator : JC/MD
Sample : N4021-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------