

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030509.D
 Acq On : 08 Aug 2022 13:48
 Operator : JC/MD
 Sample : N4066-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030509.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	42	47	58	rVB2	395314	463955	11.10%	3.777%
2	1.666	91	95	103	rVB2	85797	129069	3.09%	1.051%
3	2.306	194	200	208	rVB	203230	314045	7.52%	2.557%
4	2.562	239	242	244	rBV2	340	389	0.01%	0.003%
5	2.733	268	270	271	rBV2	356	326	0.01%	0.003%
6	2.983	307	311	313	rBV2	627	694	0.02%	0.006%
7	3.093	322	329	341	rBV2	29402	62514	1.50%	0.509%
8	3.264	354	357	361	rVB2	375	395	0.01%	0.003%
9	3.324	365	367	370	rVB2	311	338	0.01%	0.003%
10	3.349	370	371	377	rVB2	481	761	0.02%	0.006%
11	3.556	402	405	406	rBV2	333	372	0.01%	0.003%
12	3.702	428	429	431	rBV2	374	340	0.01%	0.003%
13	3.885	457	459	460	rBV2	392	354	0.01%	0.003%
14	3.922	462	465	466	rBV2	307	375	0.01%	0.003%
15	4.190	506	509	510	rBV	308	421	0.01%	0.003%
16	4.312	527	529	531	rVB2	561	471	0.01%	0.004%
17	4.489	546	558	574	rVV2	1470730	4178069	100.00%	34.014%
18	4.916	626	628	630	rBV3	362	442	0.01%	0.004%
19	5.062	638	652	669	rBV2	124489	406325	9.73%	3.308%
20	5.269	685	686	690	rBV2	382	460	0.01%	0.004%
21	5.312	690	693	696	rVB3	671	797	0.02%	0.006%
22	5.348	696	699	700	rBV	524	384	0.01%	0.003%
23	5.397	700	707	712	rVV6	1180	2520	0.06%	0.021%
24	5.562	729	734	740	rVB6	2147	4799	0.11%	0.039%
25	5.836	776	779	780	rBV	506	402	0.01%	0.003%
26	5.970	789	801	821	rVV3	329475	981536	23.49%	7.991%
27	6.184	834	836	838	rVB2	493	367	0.01%	0.003%
28	6.245	844	846	850	rBV2	415	637	0.02%	0.005%
29	6.275	850	851	854	rVB	327	346	0.01%	0.003%
30	6.367	865	866	868	rVV2	415	358	0.01%	0.003%
31	6.525	887	892	893	rBV4	470	590	0.01%	0.005%
32	6.556	893	897	901	rVB2	582	891	0.02%	0.007%
33	6.641	910	911	913	rBV2	550	348	0.01%	0.003%
34	6.763	920	931	944	rBV	296654	704696	16.87%	5.737%
35	6.995	966	969	971	rBV	549	674	0.02%	0.005%
36	7.129	981	991	1000	rBV5	23739	59052	1.41%	0.481%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030509.D
 Acq On : 08 Aug 2022 13:48
 Operator : JC/MD
 Sample : N4066-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1012	1021	1033	rBV	208928	446803	10.69%	3.637%
38	7.665	1077	1079	1084	rVB3	385	606	0.01%	0.005%
39	7.811	1101	1103	1106	rBV	307	425	0.01%	0.003%
40	7.927	1121	1122	1124	rBV2	545	404	0.01%	0.003%
41	8.092	1146	1149	1150	rBV	506	466	0.01%	0.004%
42	8.250	1170	1175	1181	rBV3	2964	4847	0.12%	0.039%
43	8.330	1181	1188	1201	rVV	138865	233618	5.59%	1.902%
44	8.458	1207	1209	1211	rBV2	363	396	0.01%	0.003%
45	8.574	1225	1228	1230	rBV2	351	325	0.01%	0.003%
46	8.653	1234	1241	1252	rBV	482860	760878	18.21%	6.194%
47	8.842	1270	1272	1273	rBV	436	352	0.01%	0.003%
48	8.952	1284	1290	1300	rBV	104065	154041	3.69%	1.254%
49	9.159	1322	1324	1328	rVB2	409	511	0.01%	0.004%
50	9.275	1340	1343	1351	rVB4	2115	3350	0.08%	0.027%
51	9.348	1351	1355	1356	rBV2	463	607	0.01%	0.005%
52	9.384	1356	1361	1376	rBV	396612	578049	13.84%	4.706%
53	9.525	1382	1384	1385	rBV2	711	460	0.01%	0.004%
54	9.543	1385	1387	1389	rVB2	849	635	0.02%	0.005%
55	9.817	1428	1432	1436	rBV3	534	594	0.01%	0.005%
56	10.055	1465	1471	1481	rBV	617767	812725	19.45%	6.616%
57	10.341	1516	1518	1520	rBV2	451	377	0.01%	0.003%
58	10.457	1535	1537	1542	rVB2	496	675	0.02%	0.005%
59	10.530	1547	1549	1553	rBV2	572	626	0.01%	0.005%
60	10.799	1590	1593	1594	rBV	403	382	0.01%	0.003%
61	10.841	1597	1600	1602	rVV2	349	440	0.01%	0.004%
62	10.860	1602	1603	1609	rVB2	471	642	0.02%	0.005%
63	10.963	1618	1620	1622	rVB	635	387	0.01%	0.003%
64	10.994	1622	1625	1627	rBV2	445	598	0.01%	0.005%
65	11.104	1641	1643	1644	rBV	408	326	0.01%	0.003%
66	11.195	1652	1658	1666	rBV	374010	473593	11.34%	3.856%
67	11.299	1671	1675	1676	rBV2	536	607	0.01%	0.005%
68	11.408	1691	1693	1696	rVB2	384	350	0.01%	0.003%
69	11.512	1708	1710	1711	rVB2	472	331	0.01%	0.003%
70	11.530	1711	1713	1715	rBV2	404	420	0.01%	0.003%
71	11.573	1718	1720	1724	rVV2	383	336	0.01%	0.003%
72	11.713	1741	1743	1745	rVB2	766	481	0.01%	0.004%
73	11.762	1749	1751	1754	rVV2	491	435	0.01%	0.004%
74	11.805	1756	1758	1759	rVV	476	389	0.01%	0.003%
75	11.957	1780	1783	1786	rBV3	506	550	0.01%	0.004%
76	12.024	1788	1794	1805	rBV	649205	779557	18.66%	6.346%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030509.D
 Acq On : 08 Aug 2022 13:48
 Operator : JC/MD
 Sample : N4066-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.323	1837	1843	1852	rBV	558719	690804	16.53%	5.624%
78	12.652	1895	1897	1899	rBV2	434	339	0.01%	0.003%
79	12.713	1905	1907	1909	rVB	587	388	0.01%	0.003%
80	12.859	1927	1931	1933	rBV3	573	519	0.01%	0.004%
81	13.030	1957	1959	1960	rBV	681	495	0.01%	0.004%
82	13.237	1992	1993	1995	rBV	689	360	0.01%	0.003%
83	13.286	2000	2001	2004	rVB	620	329	0.01%	0.003%
84	13.378	2011	2016	2018	rBV	573	1223	0.03%	0.010%
85	13.457	2026	2029	2033	rVB2	418	561	0.01%	0.005%
86	13.506	2035	2037	2043	rBV2	493	762	0.02%	0.006%
87	13.554	2043	2045	2050	rBV2	367	576	0.01%	0.005%
88	13.780	2080	2082	2083	rBV	546	326	0.01%	0.003%
89	13.884	2096	2099	2100	rVV	503	454	0.01%	0.004%
90	13.926	2102	2106	2109	rBV3	465	581	0.01%	0.005%
91	13.969	2112	2113	2117	rVB2	525	443	0.01%	0.004%
92	13.999	2117	2118	2120	rBV	543	342	0.01%	0.003%
93	14.066	2128	2129	2132	rVB2	615	396	0.01%	0.003%
94	14.585	2213	2214	2216	rBV	541	401	0.01%	0.003%
95	14.615	2216	2219	2222	rBV2	604	901	0.02%	0.007%
96	14.896	2263	2265	2266	rBV	964	509	0.01%	0.004%
97	15.786	2408	2411	2412	rBV2	761	693	0.02%	0.006%
98	16.103	2462	2463	2465	rBV2	753	444	0.01%	0.004%
99	16.529	2531	2533	2535	rBV	598	429	0.01%	0.003%
100	16.596	2543	2544	2547	rBV2	890	996	0.02%	0.008%




Sum of corrected areas: 12283377

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030509.D
Acq On : 08 Aug 2022 13:48
Operator : JC/MD
Sample : N4066-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

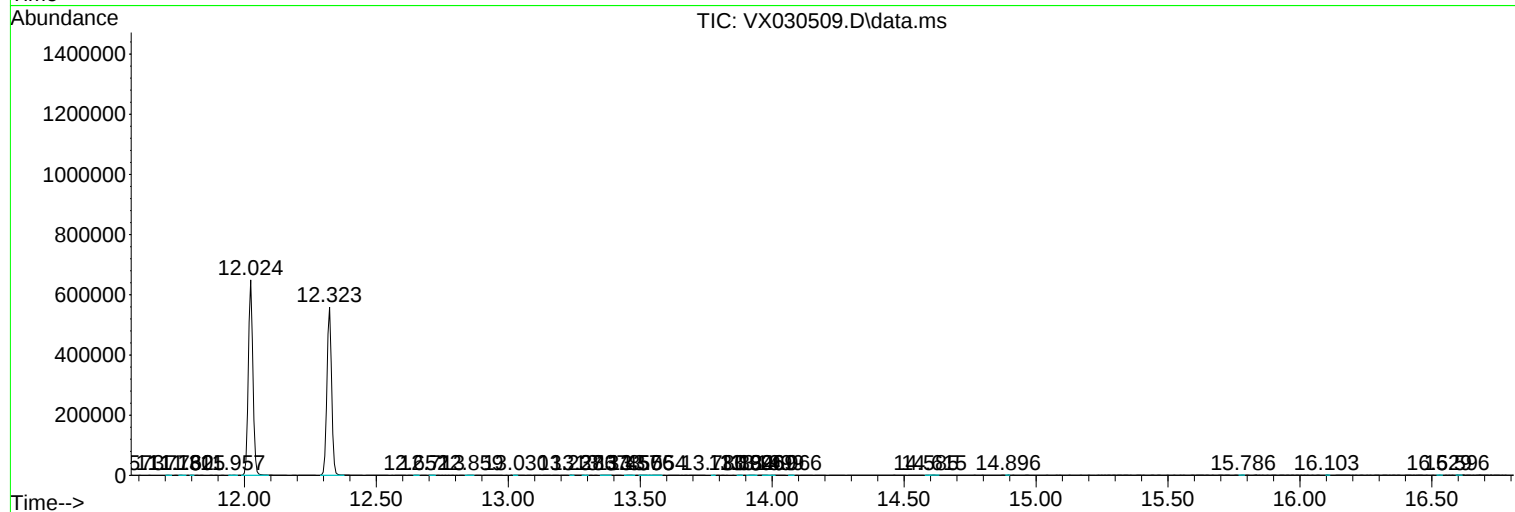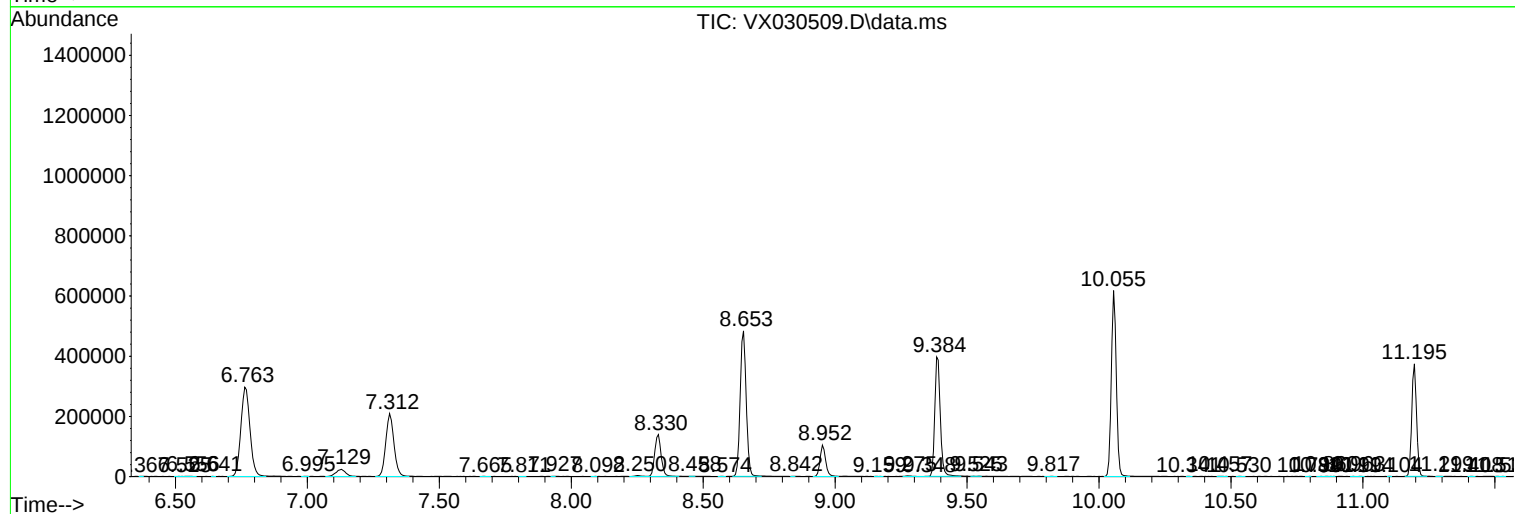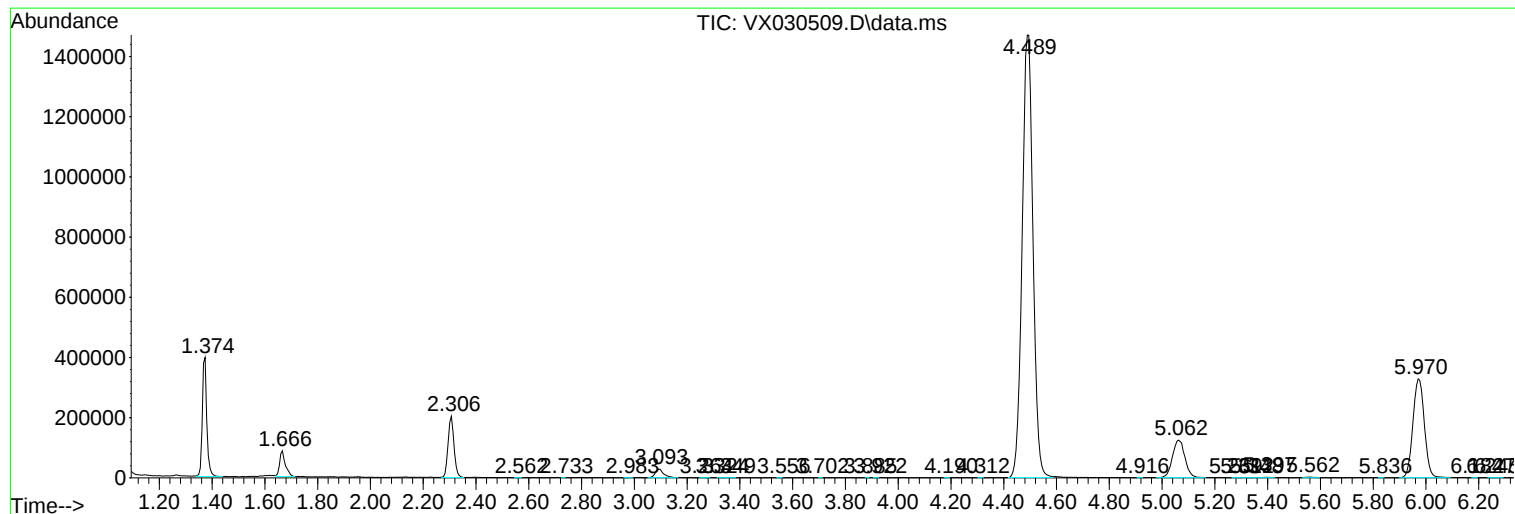

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030509.D
Acq On : 08 Aug 2022 13:48
Operator : JC/MD
Sample : N4066-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030509.D
Acq On : 08 Aug 2022 13:48
Operator : JC/MD
Sample : N4066-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc