

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030512.D
 Acq On : 08 Aug 2022 15:05
 Operator : JC/MD
 Sample : VIBLK663
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB	100103	107075	11.57%	1.463%
2	1.666	91	95	103	rVB	77716	99092	10.70%	1.354%
3	2.306	194	200	210	rVB	171245	259220	28.00%	3.542%
4	2.471	225	227	229	rVB	599	467	0.05%	0.006%
5	2.642	253	255	257	rBV2	454	454	0.05%	0.006%
6	2.697	263	264	267	rVB2	478	391	0.04%	0.005%
7	2.788	276	279	284	rVB5	2344	3486	0.38%	0.048%
8	2.947	297	305	311	rBV	5508	13158	1.42%	0.180%
9	3.050	319	322	323	rVB	428	351	0.04%	0.005%
10	3.093	326	329	331	rVV2	463	622	0.07%	0.008%
11	3.294	360	362	366	rVB2	463	478	0.05%	0.007%
12	3.434	383	385	387	rBV	475	365	0.04%	0.005%
13	3.593	407	411	412	rBV2	327	430	0.05%	0.006%
14	3.654	419	421	424	rVB2	551	513	0.06%	0.007%
15	3.721	429	432	434	rBV2	525	641	0.07%	0.009%
16	4.013	477	480	481	rBV	499	393	0.04%	0.005%
17	4.154	500	503	505	rBV2	324	343	0.04%	0.005%
18	4.227	514	515	519	rVB2	436	439	0.05%	0.006%
19	4.471	546	555	567	rBV2	87686	255926	27.64%	3.497%
20	4.946	632	633	635	rVB	683	334	0.04%	0.005%
21	4.971	635	637	640	rBV2	527	474	0.05%	0.006%
22	5.068	640	653	670	rVV2	117983	376305	40.64%	5.142%
23	5.221	676	678	681	rBV4	689	961	0.10%	0.013%
24	5.342	697	698	700	rBV	357	351	0.04%	0.005%
25	5.477	719	720	722	rBV	453	370	0.04%	0.005%
26	5.556	725	733	742	rBV4	2608	7001	0.76%	0.096%
27	5.781	767	770	772	rVB	491	425	0.05%	0.006%
28	5.818	772	776	778	rBV2	521	834	0.09%	0.011%
29	5.977	790	802	818	rBV3	326995	925844	100.00%	12.651%
30	6.269	846	850	853	rVB2	386	631	0.07%	0.009%
31	6.348	860	863	865	rVB	371	360	0.04%	0.005%
32	6.385	865	869	870	rBV	297	332	0.04%	0.005%
33	6.574	896	900	901	rBV2	289	351	0.04%	0.005%
34	6.647	909	912	915	rBV2	310	379	0.04%	0.005%
35	6.672	915	916	920	rVB2	438	458	0.05%	0.006%
36	6.763	922	931	949	rVV	276678	674268	72.83%	9.214%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030512.D
 Acq On : 08 Aug 2022 15:05
 Operator : JC/MD
 Sample : VIBLK663
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.921	955	957	958	rVB2	800	468	0.05%	0.006%
38	6.940	958	960	961	rBV	409	354	0.04%	0.005%
39	7.049	976	978	980	rBV2	380	345	0.04%	0.005%
40	7.117	981	989	1000	rVB4	11833	27768	3.00%	0.379%
41	7.312	1012	1021	1036	rBV	187303	417388	45.08%	5.703%
42	7.482	1046	1049	1052	rBV3	666	951	0.10%	0.013%
43	7.543	1057	1059	1063	rVB3	369	383	0.04%	0.005%
44	7.714	1086	1087	1091	rVB2	549	538	0.06%	0.007%
45	7.757	1091	1094	1096	rBV2	521	518	0.06%	0.007%
46	7.842	1107	1108	1113	rVB2	463	366	0.04%	0.005%
47	7.952	1124	1126	1129	rBV3	411	420	0.05%	0.006%
48	8.244	1171	1174	1178	rBV	466	887	0.10%	0.012%
49	8.330	1181	1188	1197	rBV	127723	210923	22.78%	2.882%
50	8.653	1234	1241	1254	rBV	444210	696272	75.20%	9.514%
51	8.952	1285	1290	1301	rVV	89539	139294	15.05%	1.903%
52	9.134	1317	1320	1323	rVB2	551	541	0.06%	0.007%
53	9.183	1326	1328	1330	rVB	663	409	0.04%	0.006%
54	9.238	1336	1337	1340	rBV2	280	353	0.04%	0.005%
55	9.281	1340	1344	1348	rBV4	3165	4588	0.50%	0.063%
56	9.391	1356	1362	1375	rBV	373384	541400	58.48%	7.398%
57	9.586	1392	1394	1398	rBV4	693	880	0.10%	0.012%
58	9.683	1407	1410	1411	rBV2	718	719	0.08%	0.010%
59	9.708	1411	1414	1419	rVB4	2504	3538	0.38%	0.048%
60	9.775	1423	1425	1426	rBV	379	399	0.04%	0.005%
61	9.921	1447	1449	1454	rVB2	408	681	0.07%	0.009%
62	9.964	1454	1456	1458	rBV2	308	341	0.04%	0.005%
63	10.055	1465	1471	1482	rBV	561440	759296	82.01%	10.376%
64	10.226	1496	1499	1501	rBV2	329	506	0.05%	0.007%
65	10.750	1581	1585	1587	rBV2	340	554	0.06%	0.008%
66	10.787	1590	1591	1596	rVB2	406	439	0.05%	0.006%
67	10.860	1602	1603	1607	rVB	513	559	0.06%	0.008%
68	11.195	1652	1658	1666	rBV	351280	431128	46.57%	5.891%
69	11.372	1686	1687	1692	rVB2	530	592	0.06%	0.008%
70	11.445	1697	1699	1701	rVB	540	454	0.05%	0.006%
71	11.469	1701	1703	1705	rBV2	344	346	0.04%	0.005%
72	11.549	1713	1716	1722	rBV2	461	967	0.10%	0.013%
73	11.695	1736	1740	1741	rVB2	482	430	0.05%	0.006%
74	11.713	1741	1743	1747	rBV2	480	661	0.07%	0.009%
75	11.914	1773	1776	1779	rBV2	474	582	0.06%	0.008%
76	11.945	1779	1781	1783	rBV	340	347	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030512.D
 Acq On : 08 Aug 2022 15:05
 Operator : JC/MD
 Sample : VIBLK663
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK663

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1803	rVV	568228	700398	75.65%	9.571%
78	12.231	1826	1828	1832	rVB2	687	707	0.08%	0.010%
79	12.323	1837	1843	1851	rBV	495098	625626	67.57%	8.549%
80	12.469	1865	1867	1869	rVB2	488	349	0.04%	0.005%
81	12.677	1899	1901	1904	rBV	369	410	0.04%	0.006%
82	12.762	1914	1915	1920	rVB	500	558	0.06%	0.008%
83	12.847	1927	1929	1931	rBV2	507	530	0.06%	0.007%
84	12.890	1934	1936	1938	rBV	486	433	0.05%	0.006%
85	12.945	1943	1945	1947	rBV	521	398	0.04%	0.005%
86	13.000	1952	1954	1956	rBV	486	553	0.06%	0.008%
87	13.298	2000	2003	2004	rBV	464	366	0.04%	0.005%
88	13.384	2012	2017	2020	rBV	549	972	0.10%	0.013%
89	13.750	2074	2077	2078	rBV	800	552	0.06%	0.008%
90	13.859	2092	2095	2098	rBV2	406	649	0.07%	0.009%
91	14.073	2128	2130	2132	rBV2	547	666	0.07%	0.009%
92	14.115	2134	2137	2138	rBV	288	347	0.04%	0.005%
93	14.225	2152	2155	2157	rVB2	464	517	0.06%	0.007%
94	14.243	2157	2158	2160	rBV	388	336	0.04%	0.005%
95	14.457	2192	2193	2195	rVV2	501	352	0.04%	0.005%
96	14.609	2216	2218	2220	rVV	544	361	0.04%	0.005%
97	14.786	2245	2247	2250	rBV2	739	735	0.08%	0.010%
98	15.280	2326	2328	2329	rBV2	673	470	0.05%	0.006%
99	16.444	2517	2519	2520	rBV	714	357	0.04%	0.005%
100	16.737	2565	2567	2568	rBV	614	404	0.04%	0.006%




Sum of corrected areas: 7318153

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030512.D
Acq On : 08 Aug 2022 15:05
Operator : JC/MD
Sample : VIBLK663
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXL080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

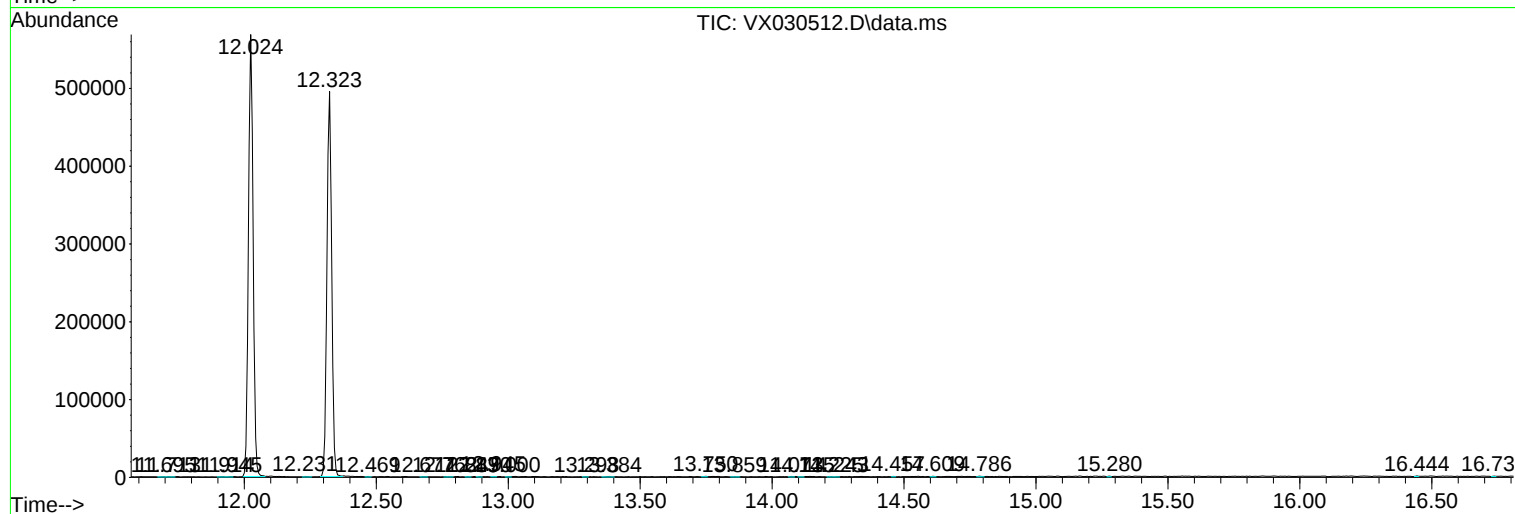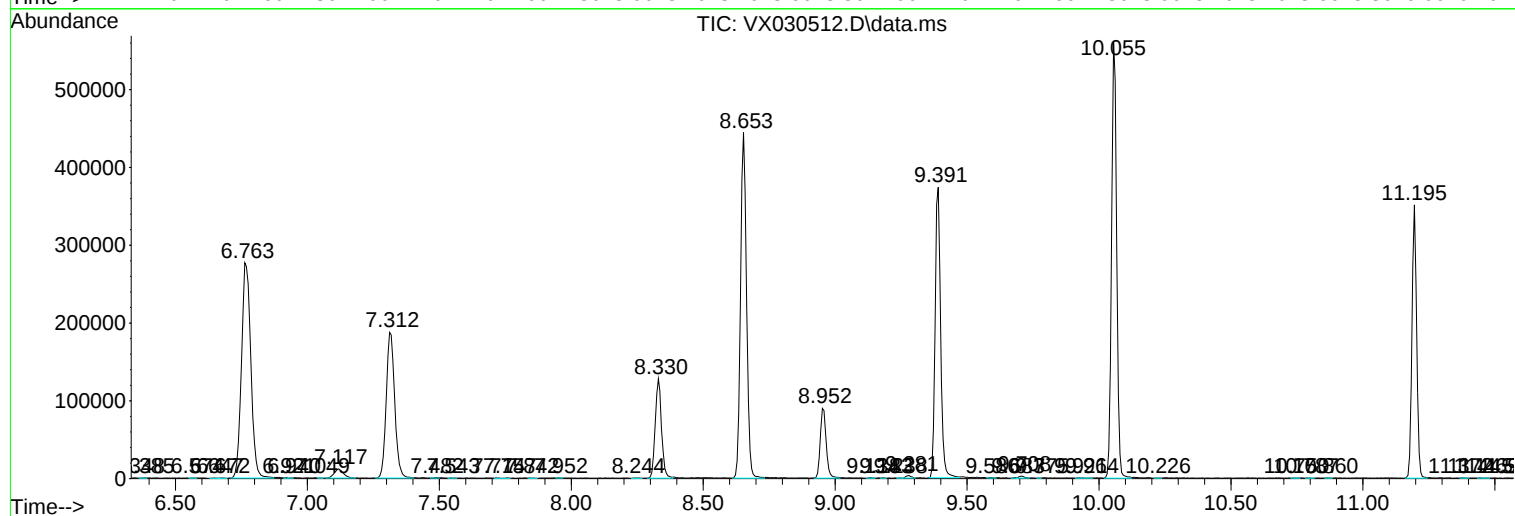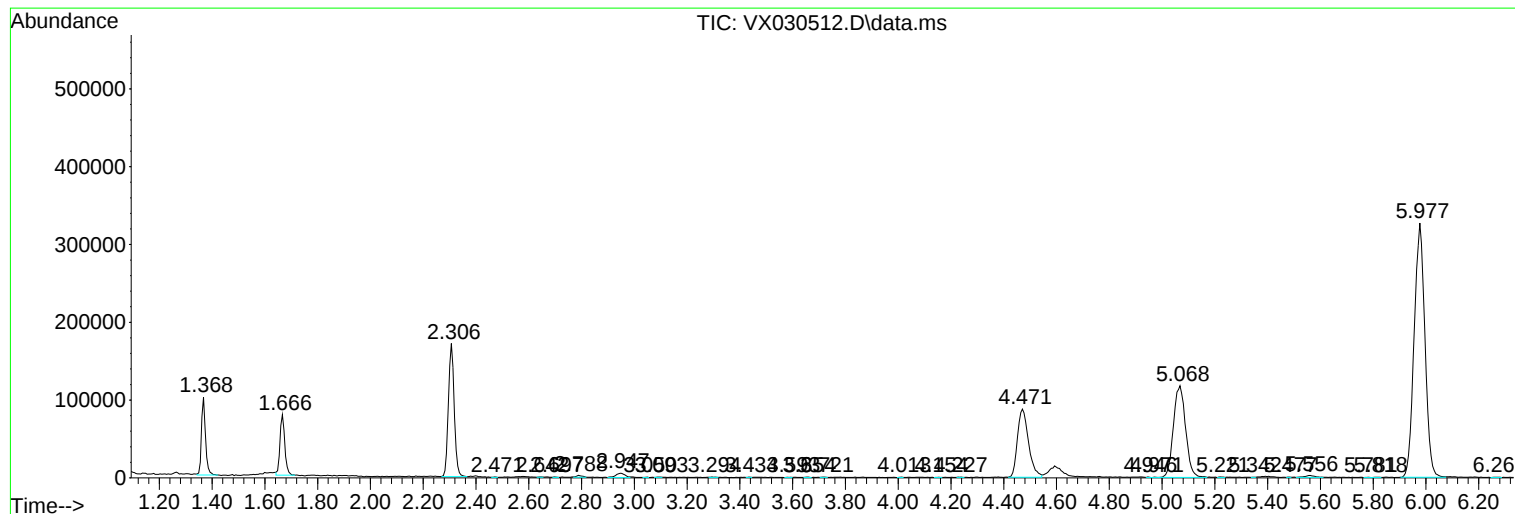

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030512.D
Acq On : 08 Aug 2022 15:05
Operator : JC/MD
Sample : VIBLK663
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030512.D
Acq On : 08 Aug 2022 15:05
Operator : JC/MD
Sample : VIBLK663
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK663

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc