

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030513.D
 Acq On : 08 Aug 2022 15:29
 Operator : JC/MD
 Sample : N4066-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	43	46	56	rVB2	288457	345249	2.54%	1.147%
2	1.666	91	95	103	rVB	79328	106248	0.78%	0.353%
3	2.306	194	200	210	rVB	196076	304529	2.24%	1.012%
4	2.508	230	233	239	rVB3	769	1160	0.01%	0.004%
5	2.556	239	241	243	rBV2	522	447	0.00%	0.001%
6	2.873	292	293	298	rVB	426	527	0.00%	0.002%
7	3.093	320	329	338	rBV	32041	60661	0.45%	0.202%
8	3.349	369	371	372	rVB	556	321	0.00%	0.001%
9	3.367	372	374	376	rBV2	336	316	0.00%	0.001%
10	3.446	385	387	388	rBV	439	332	0.00%	0.001%
11	3.605	411	413	415	rVB2	532	335	0.00%	0.001%
12	3.635	417	418	423	rBV2	291	391	0.00%	0.001%
13	3.818	444	448	451	rBV3	588	859	0.01%	0.003%
14	3.849	451	453	456	rBV2	429	550	0.00%	0.002%
15	3.904	456	462	463	rBV	335	347	0.00%	0.001%
16	3.952	468	470	473	rBV	469	392	0.00%	0.001%
17	4.050	484	486	488	rBV	305	305	0.00%	0.001%
18	4.087	491	492	495	rBV	291	345	0.00%	0.001%
19	4.172	504	506	508	rVB	392	282	0.00%	0.001%
20	4.251	517	519	522	rVB2	323	315	0.00%	0.001%
21	4.495	545	559	577	rBV2	1591430	4341344	31.98%	14.423%
22	5.068	640	653	670	rBV2	133088	402481	2.97%	1.337%
23	5.306	690	692	694	rBV2	502	565	0.00%	0.002%
24	5.641	745	747	751	rVB	642	569	0.00%	0.002%
25	5.684	751	754	757	rBV	389	474	0.00%	0.002%
26	5.726	760	761	764	rBV2	446	365	0.00%	0.001%
27	5.794	770	772	774	rVB	398	330	0.00%	0.001%
28	5.842	779	780	782	rBV	334	291	0.00%	0.001%
29	5.897	786	789	791	rBV	354	296	0.00%	0.001%
30	5.976	791	802	816	rBV3	343926	990431	7.30%	3.291%
31	6.263	847	849	850	rBV	635	442	0.00%	0.001%
32	6.543	892	895	896	rBV2	353	343	0.00%	0.001%
33	6.562	896	898	901	rVV2	491	547	0.00%	0.002%
34	6.769	922	932	947	rBV	314617	740750	5.46%	2.461%
35	6.915	954	956	957	rVB2	662	460	0.00%	0.002%
36	7.135	978	992	1013	rBV	6375942	13574190	100.00%	45.098%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030513.D
 Acq On : 08 Aug 2022 15:29
 Operator : JC/MD
 Sample : N4066-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.312	1014	1021	1039	rVB	206088	460344	3.39%	1.529%
38	7.702	1084	1085	1088	rVB2	659	556	0.00%	0.002%
39	7.830	1104	1106	1109	rVB3	412	439	0.00%	0.001%
40	7.939	1122	1124	1126	rBV3	883	830	0.01%	0.003%
41	8.092	1148	1149	1151	rBV2	413	326	0.00%	0.001%
42	8.116	1151	1153	1155	rVV2	527	474	0.00%	0.002%
43	8.244	1172	1174	1177	rVB2	584	595	0.00%	0.002%
44	8.330	1181	1188	1199	rBV	137792	229298	1.69%	0.762%
45	8.488	1212	1214	1217	rBV3	609	731	0.01%	0.002%
46	8.653	1234	1241	1252	rVV	487331	767107	5.65%	2.549%
47	8.787	1261	1263	1264	rVB	688	334	0.00%	0.001%
48	8.860	1272	1275	1280	rBV4	623	1006	0.01%	0.003%
49	8.958	1285	1291	1301	rBV	101104	153690	1.13%	0.511%
50	9.220	1332	1334	1336	rBV3	380	415	0.00%	0.001%
51	9.281	1336	1344	1356	rBV	2796552	4206197	30.99%	13.974%
52	9.390	1356	1362	1374	rVB	411690	586040	4.32%	1.947%
53	9.659	1404	1406	1408	rBV3	622	475	0.00%	0.002%
54	9.726	1415	1417	1418	rBV2	557	354	0.00%	0.001%
55	9.811	1429	1431	1432	rBV2	381	345	0.00%	0.001%
56	9.872	1437	1441	1444	rBV3	425	772	0.01%	0.003%
57	10.055	1465	1471	1482	rBV	621411	837778	6.17%	2.783%
58	10.274	1505	1507	1509	rBV2	577	522	0.00%	0.002%
59	10.311	1511	1513	1515	rVV	738	615	0.00%	0.002%
60	10.354	1518	1520	1523	rVB2	628	720	0.01%	0.002%
61	10.384	1523	1525	1528	rBV2	531	688	0.01%	0.002%
62	10.415	1528	1530	1533	rBV2	476	481	0.00%	0.002%
63	10.512	1543	1546	1547	rBV	396	335	0.00%	0.001%
64	10.530	1547	1549	1551	rVB2	443	381	0.00%	0.001%
65	10.555	1551	1553	1554	rBV	369	403	0.00%	0.001%
66	10.683	1573	1574	1577	rBV	369	443	0.00%	0.001%
67	11.036	1630	1632	1635	rVB3	438	317	0.00%	0.001%
68	11.085	1637	1640	1641	rBV2	780	586	0.00%	0.002%
69	11.195	1653	1658	1666	rVV	381646	476412	3.51%	1.583%
70	11.341	1680	1682	1684	rBV2	387	421	0.00%	0.001%
71	11.402	1689	1692	1694	rBV2	392	440	0.00%	0.001%
72	11.445	1697	1699	1701	rBV2	418	474	0.00%	0.002%
73	11.475	1703	1704	1708	rBV2	544	645	0.00%	0.002%
74	11.561	1715	1718	1719	rBV2	384	438	0.00%	0.001%
75	11.603	1722	1725	1729	rVV2	340	533	0.00%	0.002%
76	11.756	1749	1750	1754	rVB3	549	479	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030513.D
 Acq On : 08 Aug 2022 15:29
 Operator : JC/MD
 Sample : N4066-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1804	rBV	642679	783245	5.77%	2.602%
78	12.323	1837	1843	1850	rBV	556573	693801	5.11%	2.305%
79	12.451	1863	1864	1866	rBV	568	453	0.00%	0.002%
80	12.475	1866	1868	1870	rVB	793	520	0.00%	0.002%
81	12.865	1930	1932	1933	rBV2	521	400	0.00%	0.001%
82	12.969	1947	1949	1951	rBV2	483	538	0.00%	0.002%
83	13.128	1972	1975	1979	rBV2	320	527	0.00%	0.002%
84	13.426	2021	2024	2025	rBV	429	447	0.00%	0.001%
85	13.487	2031	2034	2035	rBV	383	320	0.00%	0.001%
86	13.743	2074	2076	2078	rBV2	538	377	0.00%	0.001%
87	13.890	2097	2100	2102	rBV2	406	557	0.00%	0.002%
88	13.981	2113	2115	2117	rBV	599	384	0.00%	0.001%
89	14.054	2126	2127	2129	rBV	490	382	0.00%	0.001%
90	14.115	2135	2137	2138	rBV2	374	333	0.00%	0.001%
91	14.170	2143	2146	2148	rBV3	459	458	0.00%	0.002%
92	14.402	2181	2184	2187	rBV4	551	727	0.01%	0.002%
93	14.457	2191	2193	2195	rVB2	579	384	0.00%	0.001%
94	14.896	2263	2265	2266	rBV	547	308	0.00%	0.001%
95	14.969	2275	2277	2278	rBV2	504	467	0.00%	0.002%
96	15.274	2325	2327	2328	rBV2	707	612	0.00%	0.002%
97	15.517	2366	2367	2370	rBV	856	618	0.00%	0.002%
98	15.627	2383	2385	2387	rBV2	663	480	0.00%	0.002%
99	15.889	2426	2428	2432	rBV3	1041	1195	0.01%	0.004%
100	16.517	2530	2531	2533	rBV2	655	447	0.00%	0.001%




Sum of corrected areas: 30099208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030513.D
Acq On : 08 Aug 2022 15:29
Operator : JC/MD
Sample : N4066-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

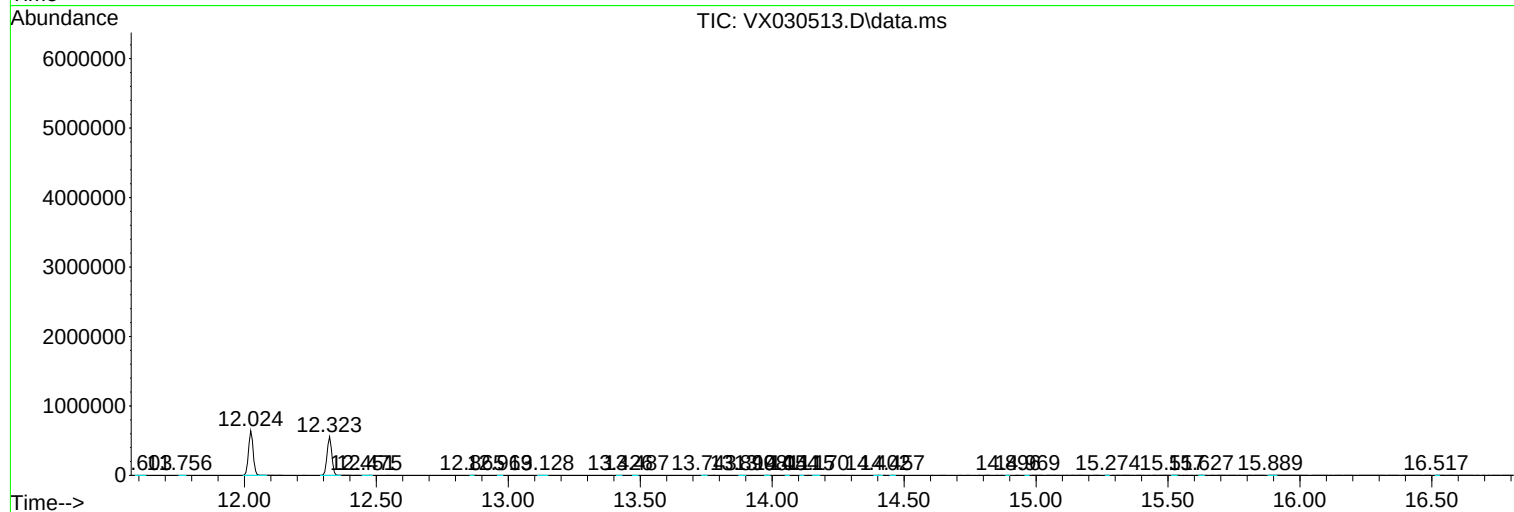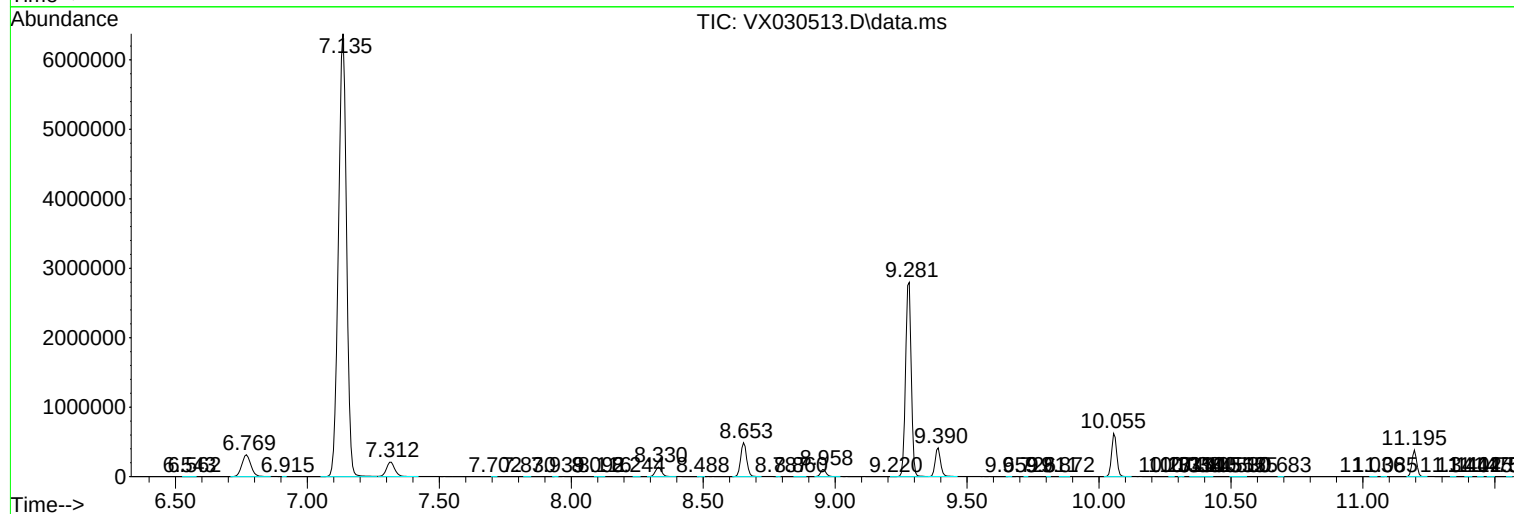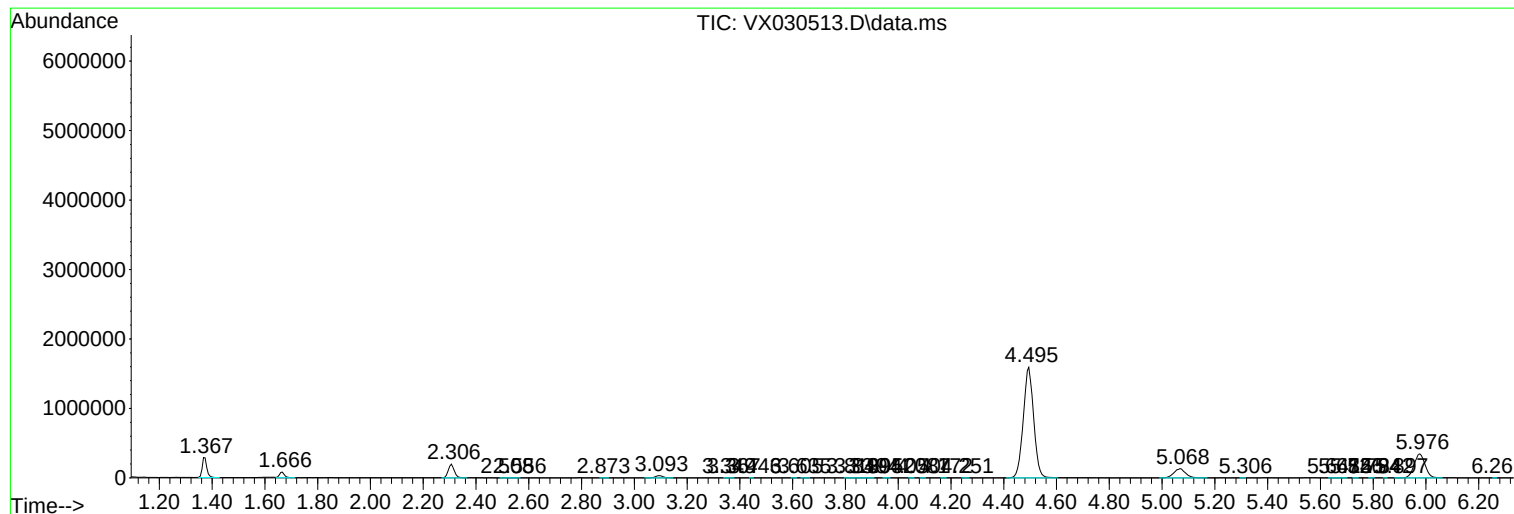

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030513.D
Acq On : 08 Aug 2022 15:29
Operator : JC/MD
Sample : N4066-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030513.D
Acq On : 08 Aug 2022 15:29
Operator : JC/MD
Sample : N4066-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc