

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030514.D
 Acq On : 08 Aug 2022 15:52
 Operator : JC/MD
 Sample : VIBLK664
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	56	rVB	114019	115473	11.48%	1.434%
2	1.666	91	95	104	rVB	84233	107328	10.67%	1.333%
3	1.995	147	149	150	rBV2	789	420	0.04%	0.005%
4	2.087	162	164	167	rVB3	1075	962	0.10%	0.012%
5	2.306	194	200	211	rVB	195170	299168	29.73%	3.715%
6	2.501	229	232	233	rBV	659	641	0.06%	0.008%
7	2.568	238	243	245	rBV3	1034	1650	0.16%	0.020%
8	2.788	276	279	286	rVB2	2007	3395	0.34%	0.042%
9	2.898	295	297	299	rBV2	359	316	0.03%	0.004%
10	2.946	299	305	311	rBV2	4768	10710	1.06%	0.133%
11	3.172	341	342	344	rVV	708	360	0.04%	0.004%
12	3.190	344	345	348	rVB2	594	403	0.04%	0.005%
13	3.568	406	407	410	rVB2	447	332	0.03%	0.004%
14	3.678	422	425	429	rVB2	408	485	0.05%	0.006%
15	3.715	429	431	432	rBV	451	325	0.03%	0.004%
16	3.843	450	452	455	rVB2	353	313	0.03%	0.004%
17	3.873	455	457	461	rBV2	436	660	0.07%	0.008%
18	4.074	488	490	491	rBV2	431	384	0.04%	0.005%
19	4.190	506	509	512	rVV2	412	534	0.05%	0.007%
20	4.471	546	555	568	rBV2	94901	282402	28.06%	3.506%
21	4.849	616	617	619	rBV2	562	429	0.04%	0.005%
22	4.989	637	640	641	rBV3	504	614	0.06%	0.008%
23	5.068	641	653	669	rVV3	127486	400873	39.84%	4.977%
24	5.367	701	702	703	rBV	740	494	0.05%	0.006%
25	5.397	703	707	708	rVV3	802	1192	0.12%	0.015%
26	5.464	716	718	721	rBV2	396	601	0.06%	0.007%
27	5.519	725	727	728	rVV2	523	419	0.04%	0.005%
28	5.568	728	735	740	rVV6	2243	5569	0.55%	0.069%
29	5.629	743	745	750	rVB	407	468	0.05%	0.006%
30	5.885	786	787	790	rVB2	558	460	0.05%	0.006%
31	5.976	790	802	817	rBV2	347369	1006267	100.00%	12.494%
32	6.141	827	829	830	rBV	558	439	0.04%	0.005%
33	6.537	892	894	895	rBV	477	301	0.03%	0.004%
34	6.623	906	908	910	rBV	411	337	0.03%	0.004%
35	6.702	919	921	923	rBV	301	316	0.03%	0.004%
36	6.769	923	932	945	rBV	307909	737188	73.26%	9.153%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030514.D
 Acq On : 08 Aug 2022 15:52
 Operator : JC/MD
 Sample : VIBLK664
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.122	979	990	1002	rBV5	28772	73052	7.26%	0.907%
38	7.311	1013	1021	1034	rVV	204010	451819	44.90%	5.610%
39	7.482	1046	1049	1050	rBV3	406	437	0.04%	0.005%
40	7.696	1082	1084	1089	rVB3	403	590	0.06%	0.007%
41	7.830	1100	1106	1110	rBV2	469	761	0.08%	0.009%
42	7.939	1122	1124	1125	rVV	701	436	0.04%	0.005%
43	7.958	1125	1127	1132	rVB2	886	758	0.08%	0.009%
44	8.000	1132	1134	1136	rBV	335	307	0.03%	0.004%
45	8.049	1139	1142	1143	rBV	384	411	0.04%	0.005%
46	8.177	1161	1163	1165	rVB2	312	297	0.03%	0.004%
47	8.220	1165	1170	1171	rBV2	358	409	0.04%	0.005%
48	8.244	1171	1174	1175	rVB	367	318	0.03%	0.004%
49	8.330	1181	1188	1199	rBV	136380	225682	22.43%	2.802%
50	8.580	1226	1229	1230	rBV	789	671	0.07%	0.008%
51	8.653	1234	1241	1251	rBV	506291	767556	76.28%	9.530%
52	8.842	1269	1272	1274	rVB3	573	654	0.06%	0.008%
53	8.878	1274	1278	1281	rBV4	467	719	0.07%	0.009%
54	8.951	1285	1290	1303	rVV	102387	152601	15.17%	1.895%
55	9.281	1338	1344	1351	rVB2	11481	18011	1.79%	0.224%
56	9.390	1356	1362	1374	rBV	408386	592588	58.89%	7.358%
57	9.579	1391	1393	1395	rBV2	566	575	0.06%	0.007%
58	9.707	1409	1414	1418	rBV3	4015	5862	0.58%	0.073%
59	9.762	1421	1423	1427	rBV2	470	510	0.05%	0.006%
60	9.823	1431	1433	1436	rVV	395	498	0.05%	0.006%
61	10.055	1466	1471	1485	rVV	595387	831161	82.60%	10.320%
62	10.280	1506	1508	1513	rVB2	528	661	0.07%	0.008%
63	10.463	1536	1538	1541	rVB2	340	415	0.04%	0.005%
64	10.506	1541	1545	1547	rBV2	556	751	0.07%	0.009%
65	10.573	1553	1556	1559	rBV2	394	401	0.04%	0.005%
66	10.622	1563	1564	1567	rBV2	410	449	0.04%	0.006%
67	10.866	1601	1604	1607	rVB	489	564	0.06%	0.007%
68	10.933	1614	1615	1617	rVB2	472	340	0.03%	0.004%
69	10.982	1622	1623	1628	rBV2	447	673	0.07%	0.008%
70	11.140	1647	1649	1652	rBV2	393	342	0.03%	0.004%
71	11.195	1652	1658	1665	rBV	366106	462337	45.95%	5.741%
72	11.555	1716	1717	1720	rVB3	388	375	0.04%	0.005%
73	11.585	1720	1722	1725	rBV2	392	520	0.05%	0.006%
74	11.664	1733	1735	1737	rVB	551	404	0.04%	0.005%
75	11.701	1740	1741	1744	rBV2	284	296	0.03%	0.004%
76	11.957	1780	1783	1784	rBV	300	299	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030514.D
 Acq On : 08 Aug 2022 15:52
 Operator : JC/MD
 Sample : VIBLK664
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VIBLK664

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1802	rBV	628003	770852	76.61%	9.571%
78	12.164	1815	1817	1819	rVB	672	336	0.03%	0.004%
79	12.189	1819	1821	1823	rVB2	449	383	0.04%	0.005%
80	12.219	1823	1826	1829	rBV2	811	1105	0.11%	0.014%
81	12.323	1837	1843	1853	rBV	566241	692324	68.80%	8.596%
82	12.408	1855	1857	1859	rVB2	959	798	0.08%	0.010%
83	12.914	1938	1940	1943	rVB3	489	389	0.04%	0.005%
84	12.969	1943	1949	1950	rBV2	421	606	0.06%	0.008%
85	13.036	1956	1960	1962	rBV2	440	596	0.06%	0.007%
86	13.201	1986	1987	1990	rVB2	551	388	0.04%	0.005%
87	13.585	2048	2050	2055	rVB2	586	609	0.06%	0.008%
88	13.621	2055	2056	2059	rBV	438	433	0.04%	0.005%
89	13.890	2099	2100	2102	rBV2	705	522	0.05%	0.006%
90	13.969	2110	2113	2114	rBV2	549	508	0.05%	0.006%
91	14.115	2135	2137	2139	rBV	448	367	0.04%	0.005%
92	14.176	2145	2147	2149	rBV	520	475	0.05%	0.006%
93	14.359	2174	2177	2178	rBV	513	564	0.06%	0.007%
94	15.237	2319	2321	2325	rBV3	498	698	0.07%	0.009%
95	15.682	2392	2394	2395	rBV2	783	467	0.05%	0.006%
96	15.908	2429	2431	2432	rBV2	695	454	0.05%	0.006%
97	16.078	2458	2459	2461	rBV2	689	486	0.05%	0.006%
98	16.401	2508	2512	2515	rBV3	746	1358	0.13%	0.017%
99	16.566	2538	2539	2542	rBV2	913	777	0.08%	0.010%
100	16.621	2546	2548	2550	rBV2	724	563	0.06%	0.007%




Sum of corrected areas: 8053796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030514.D
Acq On : 08 Aug 2022 15:52
Operator : JC/MD
Sample : VIBLK664
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

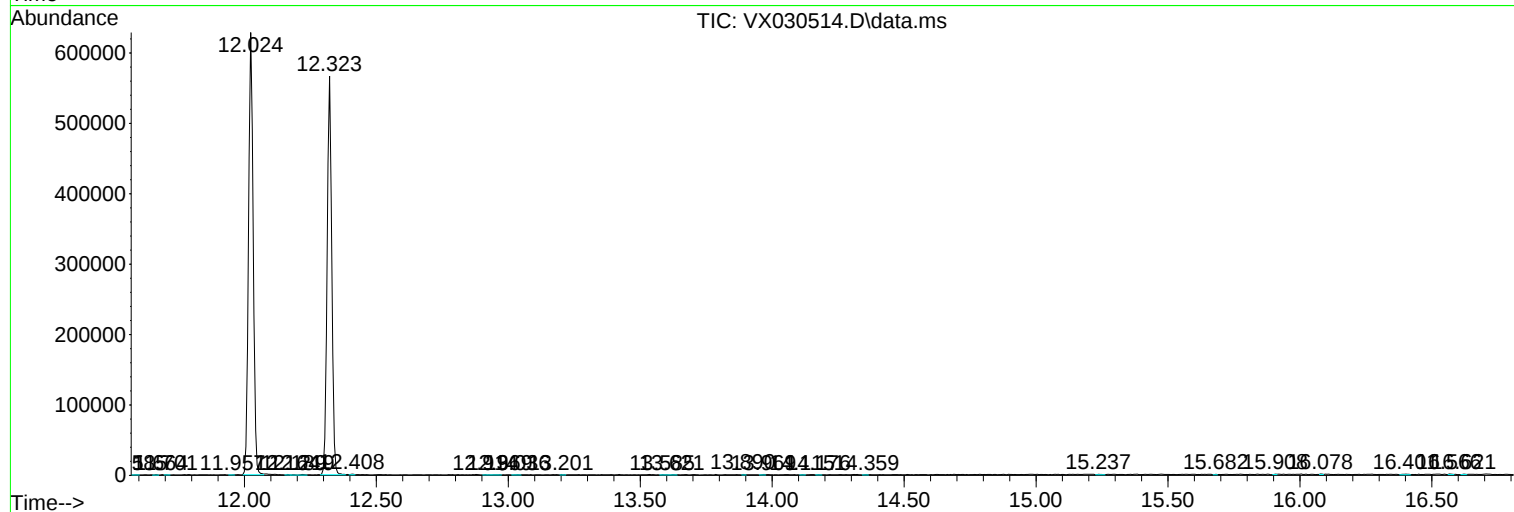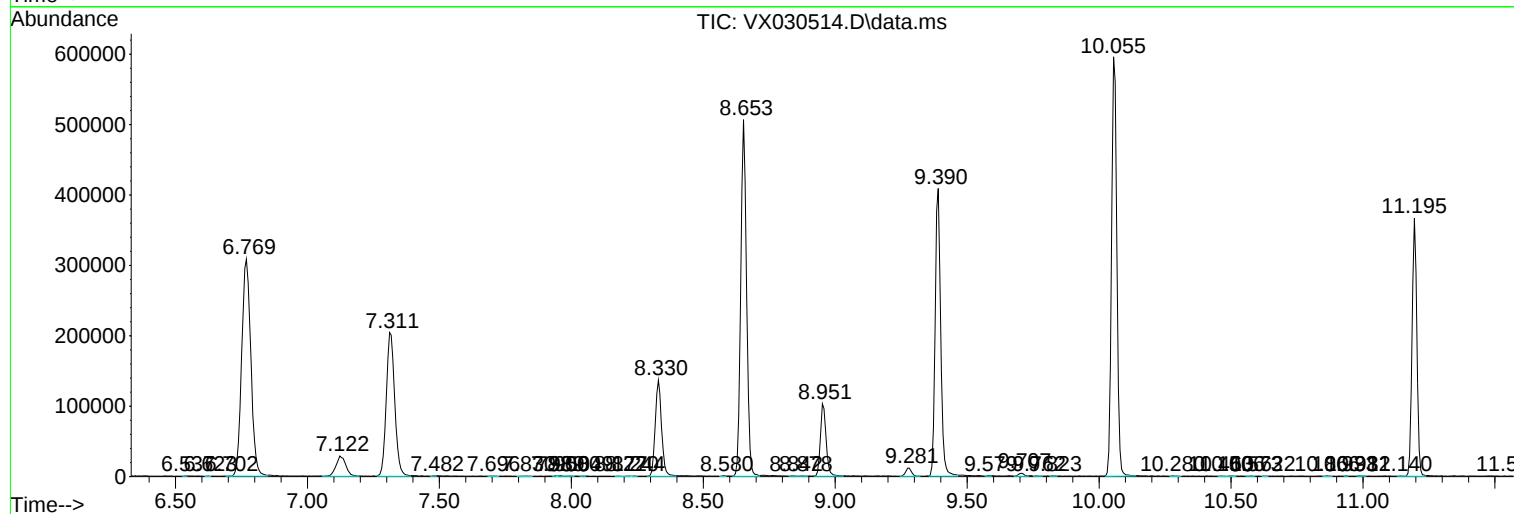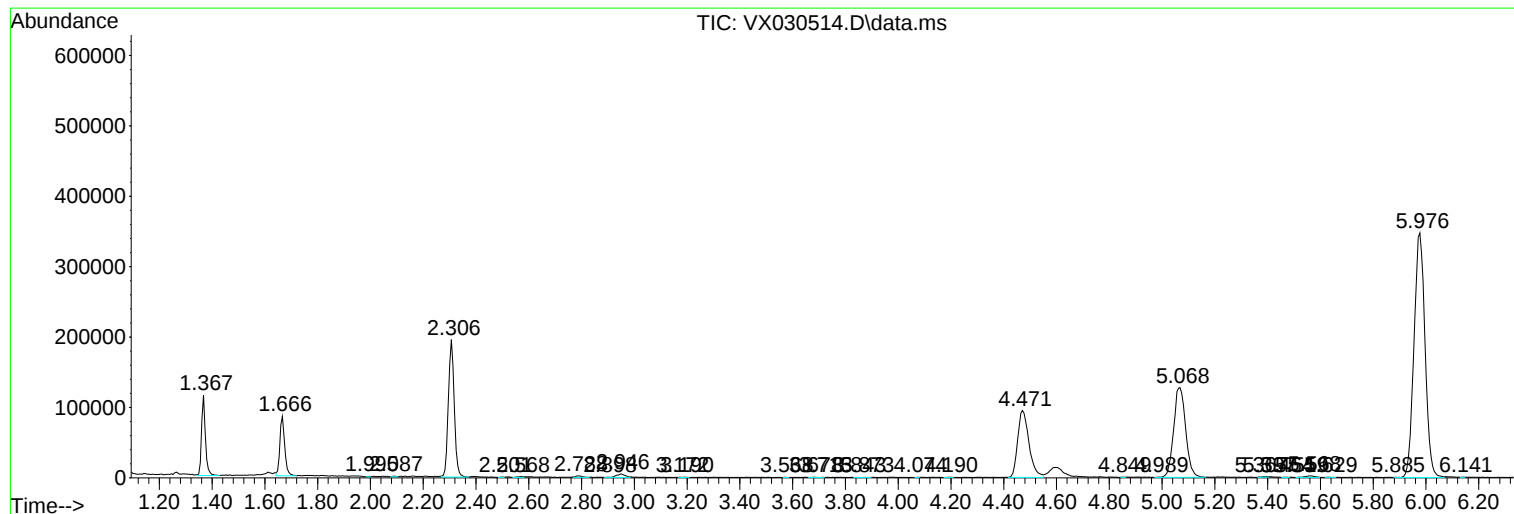

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030514.D
Acq On : 08 Aug 2022 15:52
Operator : JC/MD
Sample : VIBLK664
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030514.D
Acq On : 08 Aug 2022 15:52
Operator : JC/MD
Sample : VIBLK664
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VIBLK664

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------