

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030515.D
 Acq On : 08 Aug 2022 16:16
 Operator : JC/MD
 Sample : N4066-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	56	rVB2	303020	351872	2.59%	1.164%
2	1.666	91	95	102	rVB	89036	107166	0.79%	0.354%
3	2.306	194	200	209	rVB	212865	336278	2.47%	1.112%
4	2.483	225	229	232	rBV2	401	828	0.01%	0.003%
5	2.508	232	233	236	rVB	683	396	0.00%	0.001%
6	2.593	245	247	248	rVB	514	315	0.00%	0.001%
7	2.782	273	278	279	rBV3	931	1318	0.01%	0.004%
8	2.843	286	288	289	rBV2	567	377	0.00%	0.001%
9	2.941	300	304	307	rVB	440	546	0.00%	0.002%
10	2.971	307	309	310	rBV2	455	327	0.00%	0.001%
11	3.093	320	329	338	rBV2	30890	60155	0.44%	0.199%
12	3.221	345	350	351	rBV2	541	840	0.01%	0.003%
13	3.319	365	366	369	rBV2	372	499	0.00%	0.002%
14	3.343	369	370	374	rVB2	672	493	0.00%	0.002%
15	3.440	379	386	388	rBV2	527	1240	0.01%	0.004%
16	3.666	420	423	425	rBV2	291	315	0.00%	0.001%
17	3.727	430	433	435	rBV2	354	388	0.00%	0.001%
18	3.806	443	446	447	rBV2	438	477	0.00%	0.002%
19	4.154	500	503	509	rBV2	393	595	0.00%	0.002%
20	4.385	539	541	544	rVB2	457	487	0.00%	0.002%
21	4.495	546	559	576	rBV2	1577823	4404196	32.39%	14.564%
22	4.904	624	626	628	rBV	453	361	0.00%	0.001%
23	4.971	635	637	640	rBV2	258	412	0.00%	0.001%
24	5.068	640	653	670	rVV	132149	407561	3.00%	1.348%
25	5.324	693	695	700	rVB2	687	890	0.01%	0.003%
26	5.397	700	707	713	rBV5	1892	4534	0.03%	0.015%
27	5.556	728	733	734	rBV3	1606	2099	0.02%	0.007%
28	5.977	790	802	816	rBV2	337401	991613	7.29%	3.279%
29	6.190	835	837	840	rBV3	504	474	0.00%	0.002%
30	6.312	856	857	859	rVV	619	426	0.00%	0.001%
31	6.361	862	865	868	rBV	575	601	0.00%	0.002%
32	6.440	876	878	882	rBV3	395	436	0.00%	0.001%
33	6.483	884	885	887	rBV	378	312	0.00%	0.001%
34	6.556	895	897	899	rBV2	566	533	0.00%	0.002%
35	6.598	902	904	905	rBV	471	397	0.00%	0.001%
36	6.769	922	932	945	rBV2	299418	733986	5.40%	2.427%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030515.D
 Acq On : 08 Aug 2022 16:16
 Operator : JC/MD
 Sample : N4066-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.135	981	992	1013	rBV	6422071	13595701	100.00%	44.960%
38	7.318	1014	1022	1038	rVB	206392	457645	3.37%	1.513%
39	7.873	1112	1113	1116	rVB3	647	329	0.00%	0.001%
40	7.921	1119	1121	1122	rBV	502	375	0.00%	0.001%
41	7.940	1122	1124	1131	rVB2	961	1375	0.01%	0.005%
42	8.141	1154	1157	1159	rBV	511	755	0.01%	0.002%
43	8.238	1170	1173	1175	rBV2	660	830	0.01%	0.003%
44	8.330	1179	1188	1199	rBV	138025	228727	1.68%	0.756%
45	8.482	1211	1213	1214	rBV	536	461	0.00%	0.002%
46	8.653	1230	1241	1253	rBV	495537	772633	5.68%	2.555%
47	8.958	1283	1291	1300	rBV	99419	153082	1.13%	0.506%
48	9.153	1319	1323	1325	rBV2	541	561	0.00%	0.002%
49	9.281	1336	1344	1356	rBV	2796125	4182954	30.77%	13.833%
50	9.391	1357	1362	1374	rVB	414207	592168	4.36%	1.958%
51	9.531	1383	1385	1386	rBV2	753	378	0.00%	0.001%
52	9.726	1415	1417	1420	rBV2	479	585	0.00%	0.002%
53	9.817	1430	1432	1434	rBV3	490	573	0.00%	0.002%
54	9.915	1444	1448	1449	rBV2	435	467	0.00%	0.002%
55	9.982	1457	1459	1461	rBV3	579	687	0.01%	0.002%
56	10.055	1465	1471	1483	rBV	614499	841906	6.19%	2.784%
57	10.281	1507	1508	1510	rVB2	553	342	0.00%	0.001%
58	10.299	1510	1511	1514	rBV2	636	770	0.01%	0.003%
59	10.390	1523	1526	1527	rVB2	411	346	0.00%	0.001%
60	10.512	1545	1546	1549	rVV	761	504	0.00%	0.002%
61	10.537	1549	1550	1552	rVV2	353	312	0.00%	0.001%
62	10.579	1556	1557	1560	rBV2	462	519	0.00%	0.002%
63	10.714	1576	1579	1580	rVB3	559	352	0.00%	0.001%
64	10.732	1580	1582	1584	rBV	374	378	0.00%	0.001%
65	11.067	1635	1637	1639	rBV	450	490	0.00%	0.002%
66	11.195	1651	1658	1666	rBV	387467	477829	3.51%	1.580%
67	11.341	1679	1682	1684	rBV2	441	482	0.00%	0.002%
68	11.409	1691	1693	1696	rBV	442	303	0.00%	0.001%
69	11.512	1708	1710	1713	rVB3	410	444	0.00%	0.001%
70	11.591	1722	1723	1727	rVB	609	583	0.00%	0.002%
71	11.628	1727	1729	1732	rBV2	445	731	0.01%	0.002%
72	11.707	1739	1742	1743	rBV2	638	702	0.01%	0.002%
73	11.744	1746	1748	1749	rBV	469	399	0.00%	0.001%
74	11.780	1752	1754	1755	rBV2	584	427	0.00%	0.001%
75	11.884	1769	1771	1773	rVV	479	456	0.00%	0.002%
76	11.927	1776	1778	1780	rBV2	550	614	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030515.D
 Acq On : 08 Aug 2022 16:16
 Operator : JC/MD
 Sample : N4066-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.024	1789	1794	1803	rVV	666624	797451	5.87%	2.637%
78	12.189	1820	1821	1822	rBV	565	312	0.00%	0.001%
79	12.323	1837	1843	1853	rBV	572165	699270	5.14%	2.312%
80	12.719	1907	1908	1910	rVB2	613	310	0.00%	0.001%
81	12.756	1912	1914	1915	rBV	506	297	0.00%	0.001%
82	12.841	1925	1928	1934	rBV2	412	616	0.00%	0.002%
83	12.914	1939	1940	1943	rBV3	552	424	0.00%	0.001%
84	13.201	1985	1987	1990	rBV2	424	437	0.00%	0.001%
85	13.256	1995	1996	1999	rBV	396	474	0.00%	0.002%
86	13.323	2006	2007	2011	rBV	451	491	0.00%	0.002%
87	13.408	2019	2021	2024	rBV2	425	492	0.00%	0.002%
88	13.494	2033	2035	2036	rBV	483	319	0.00%	0.001%
89	13.622	2052	2056	2058	rBV2	564	681	0.01%	0.002%
90	13.926	2104	2106	2107	rBV	686	352	0.00%	0.001%
91	14.091	2131	2133	2135	rVB2	428	345	0.00%	0.001%
92	14.597	2215	2216	2219	rBV	637	565	0.00%	0.002%
93	14.627	2219	2221	2222	rVB	731	417	0.00%	0.001%
94	14.646	2222	2224	2227	rBV2	741	773	0.01%	0.003%
95	15.024	2284	2286	2288	rVB2	690	479	0.00%	0.002%
96	15.536	2369	2370	2372	rVB2	712	395	0.00%	0.001%
97	16.158	2471	2472	2477	rVB3	682	545	0.00%	0.002%
98	16.261	2488	2489	2490	rVB	896	327	0.00%	0.001%
99	16.725	2564	2565	2567	rBV	700	665	0.00%	0.002%
100	16.767	2570	2572	2573	rBV	517	345	0.00%	0.001%




Sum of corrected areas: 30239700

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030515.D
Acq On : 08 Aug 2022 16:16
Operator : JC/MD
Sample : N4066-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

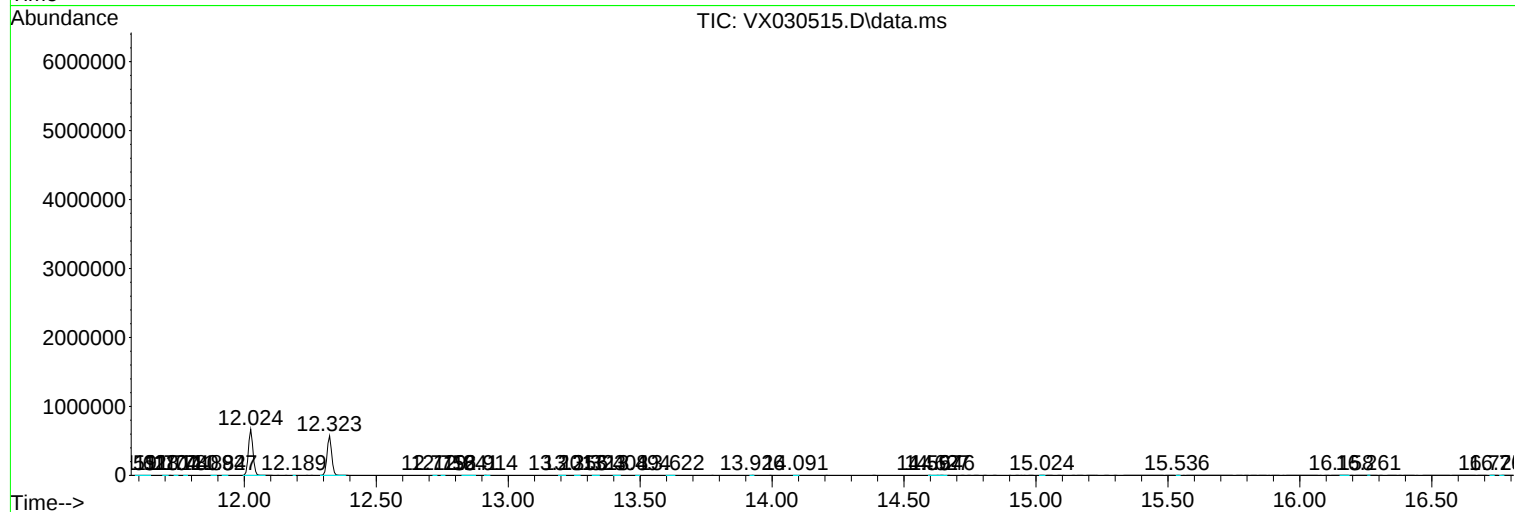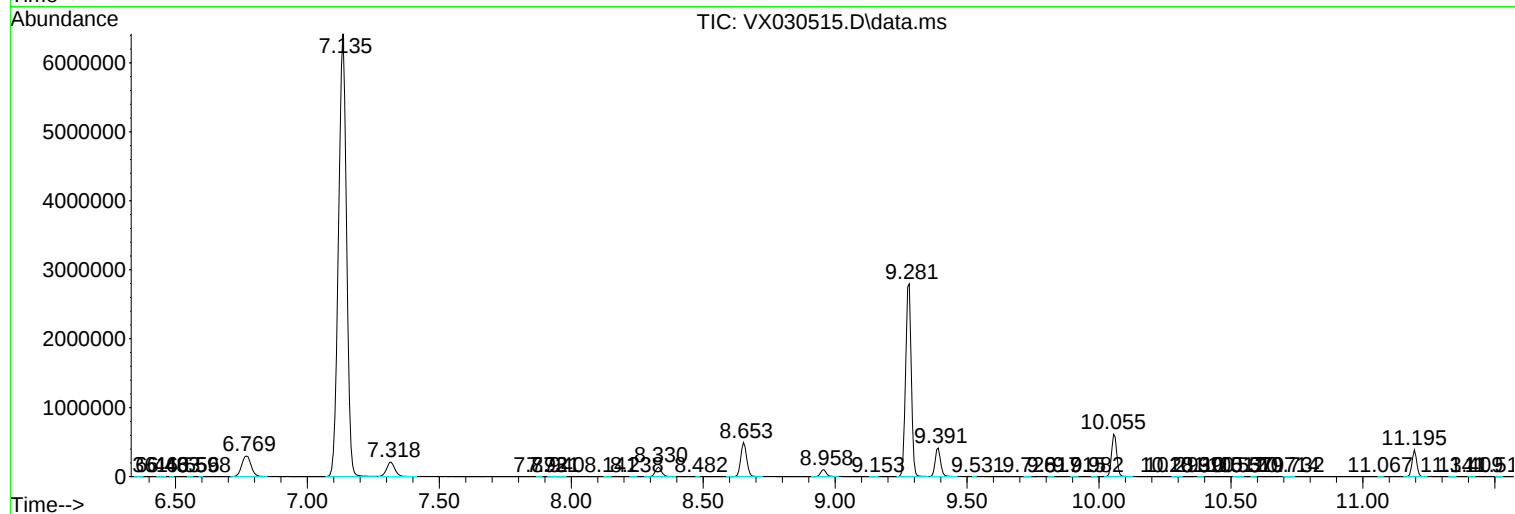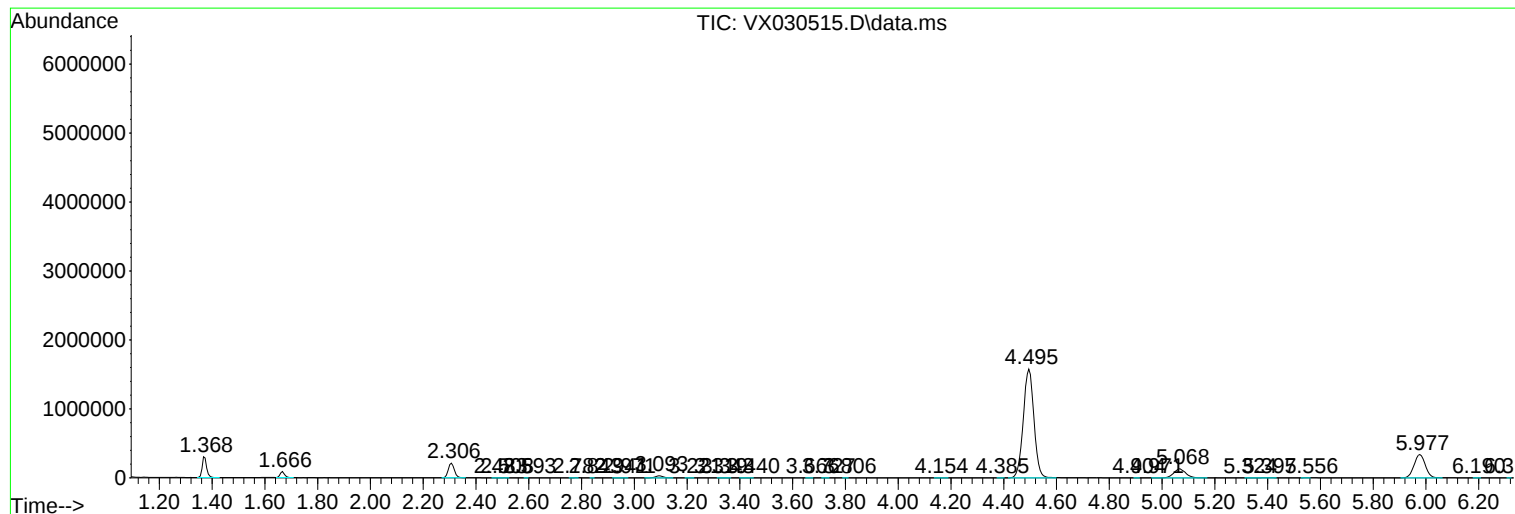

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030515.D
Acq On : 08 Aug 2022 16:16
Operator : JC/MD
Sample : N4066-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030515.D
Acq On : 08 Aug 2022 16:16
Operator : JC/MD
Sample : N4066-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc