

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030517.D
 Acq On : 08 Aug 2022 17:22
 Operator : JC/MD
 Sample : N4066-05DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB2	135638	148676	15.70%	1.641%
2	1.666	91	95	102	rVB	78954	103081	10.88%	1.138%
3	2.130	169	171	177	rBV2	1067	1380	0.15%	0.015%
4	2.307	193	200	209	rVB	177099	283194	29.90%	3.127%
5	2.715	265	267	269	rVV2	487	318	0.03%	0.004%
6	2.788	273	279	285	rBV4	3249	6568	0.69%	0.073%
7	2.861	289	291	294	rVB	824	614	0.06%	0.007%
8	2.886	294	295	297	rBV	428	361	0.04%	0.004%
9	2.947	298	305	311	rVB3	4385	9255	0.98%	0.102%
10	3.093	321	329	336	rVV	11958	21094	2.23%	0.233%
11	3.239	350	353	354	rBV2	475	503	0.05%	0.006%
12	3.380	375	376	380	rVB2	468	424	0.04%	0.005%
13	3.428	382	384	386	rBV	396	346	0.04%	0.004%
14	3.508	394	397	399	rBV	362	355	0.04%	0.004%
15	3.806	443	446	449	rBV2	413	608	0.06%	0.007%
16	3.873	456	457	465	rVB	341	468	0.05%	0.005%
17	3.995	475	477	478	rBV	344	317	0.03%	0.003%
18	4.075	486	490	491	rBV	394	307	0.03%	0.003%
19	4.093	491	493	496	rVB2	435	408	0.04%	0.005%
20	4.142	499	501	504	rBV2	315	328	0.03%	0.004%
21	4.251	517	519	522	rVB2	388	308	0.03%	0.003%
22	4.337	531	533	537	rBV2	597	695	0.07%	0.008%
23	4.379	537	540	545	rVB2	386	635	0.07%	0.007%
24	4.483	545	557	568	rBV3	216363	718903	75.91%	7.937%
25	4.830	613	614	616	rVB	679	338	0.04%	0.004%
26	4.855	616	618	622	rVB3	396	381	0.04%	0.004%
27	5.056	639	651	670	rBV	127440	400326	42.27%	4.420%
28	5.245	680	682	684	rVB	478	332	0.04%	0.004%
29	5.294	687	690	693	rBV2	445	563	0.06%	0.006%
30	5.349	697	699	701	rBV2	537	436	0.05%	0.005%
31	5.367	701	702	705	rBV3	643	735	0.08%	0.008%
32	5.465	716	718	723	rVB2	290	537	0.06%	0.006%
33	5.501	723	724	726	rBV2	417	324	0.03%	0.004%
34	5.550	726	732	734	rBV4	1272	2656	0.28%	0.029%
35	5.818	774	776	781	rVB2	315	370	0.04%	0.004%
36	5.861	781	783	786	rBV2	491	540	0.06%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030517.D
 Acq On : 08 Aug 2022 17:22
 Operator : JC/MD
 Sample : N4066-05DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	5.971	789	801	816	rBV2	324923	947045	100.00%	10.456%
38	6.330	857	860	861	rVB	423	338	0.04%	0.004%
39	6.361	863	865	867	rVB3	659	491	0.05%	0.005%
40	6.385	867	869	871	rBV	668	642	0.07%	0.007%
41	6.763	921	931	942	rBV	319047	753205	79.53%	8.316%
42	7.129	980	991	1002	rBV3	137298	312923	33.04%	3.455%
43	7.245	1008	1010	1012	rBV3	699	543	0.06%	0.006%
44	7.312	1012	1021	1035	rVV	201844	443750	46.86%	4.899%
45	7.482	1046	1049	1050	rBV2	917	792	0.08%	0.009%
46	7.739	1087	1091	1092	rBV2	349	502	0.05%	0.006%
47	7.934	1119	1123	1124	rBV3	494	675	0.07%	0.007%
48	8.025	1135	1138	1139	rBV2	322	339	0.04%	0.004%
49	8.129	1153	1155	1156	rBV2	498	384	0.04%	0.004%
50	8.330	1180	1188	1196	rBV	132020	222362	23.48%	2.455%
51	8.458	1207	1209	1211	rVB2	560	330	0.03%	0.004%
52	8.488	1211	1214	1220	rVB4	760	1455	0.15%	0.016%
53	8.653	1233	1241	1249	rBV	474474	728235	76.90%	8.040%
54	8.952	1283	1290	1300	rBV	99643	151289	15.97%	1.670%
55	9.147	1319	1322	1325	rVB2	344	379	0.04%	0.004%
56	9.196	1328	1330	1332	rBV	482	309	0.03%	0.003%
57	9.275	1337	1343	1352	rVB	253628	374233	39.52%	4.132%
58	9.385	1356	1361	1371	rBV	414709	587965	62.08%	6.491%
59	9.702	1410	1413	1419	rVV3	1606	2506	0.26%	0.028%
60	9.939	1450	1452	1455	rVB	430	306	0.03%	0.003%
61	9.970	1455	1457	1458	rBV	343	344	0.04%	0.004%
62	10.055	1465	1471	1483	rBV	650724	855918	90.38%	9.450%
63	10.201	1494	1495	1499	rVB2	462	361	0.04%	0.004%
64	10.256	1501	1504	1505	rBV2	545	643	0.07%	0.007%
65	10.555	1551	1553	1554	rBV2	350	326	0.03%	0.004%
66	10.598	1558	1560	1563	rVV	356	319	0.03%	0.004%
67	10.683	1571	1574	1576	rVV2	489	459	0.05%	0.005%
68	10.768	1586	1588	1589	rVB2	434	304	0.03%	0.003%
69	10.811	1593	1595	1598	rVB	794	713	0.08%	0.008%
70	10.848	1598	1601	1602	rBV	357	417	0.04%	0.005%
71	10.909	1609	1611	1612	rBV	492	372	0.04%	0.004%
72	11.085	1638	1640	1642	rBV	738	545	0.06%	0.006%
73	11.195	1652	1658	1668	rVV	358886	453767	47.91%	5.010%
74	11.305	1675	1676	1678	rBV	565	353	0.04%	0.004%
75	11.396	1689	1691	1693	rBV2	574	632	0.07%	0.007%
76	11.518	1709	1711	1712	rBV	487	351	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030517.D
 Acq On : 08 Aug 2022 17:22
 Operator : JC/MD
 Sample : N4066-05DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E25DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.585	1720	1722	1724	rBV2	443	321	0.03%	0.004%
78	11.646	1731	1732	1734	rBV2	528	339	0.04%	0.004%
79	11.707	1740	1742	1744	rBV2	349	431	0.05%	0.005%
80	11.957	1781	1783	1785	rBV2	364	344	0.04%	0.004%
81	12.024	1789	1794	1802	rVV	666089	817574	86.33%	9.026%
82	12.189	1819	1821	1823	rBV	494	512	0.05%	0.006%
83	12.274	1833	1835	1837	rBV2	371	388	0.04%	0.004%
84	12.323	1837	1843	1853	rBV	537953	674651	71.24%	7.449%
85	12.689	1902	1903	1905	rBV2	326	322	0.03%	0.004%
86	12.835	1925	1927	1928	rBV	565	304	0.03%	0.003%
87	13.305	2002	2004	2005	rBV	456	334	0.04%	0.004%
88	13.548	2042	2044	2047	rBV2	329	392	0.04%	0.004%
89	13.603	2049	2053	2054	rBV	364	376	0.04%	0.004%
90	13.695	2066	2068	2071	rVB2	810	631	0.07%	0.007%
91	13.719	2071	2072	2074	rBV	475	408	0.04%	0.005%
92	13.914	2101	2104	2105	rBV2	413	453	0.05%	0.005%
93	14.042	2123	2125	2127	rBV	527	486	0.05%	0.005%
94	14.146	2138	2142	2146	rVB2	288	443	0.05%	0.005%
95	14.225	2152	2155	2157	rBV3	567	777	0.08%	0.009%
96	14.280	2161	2164	2167	rVV	555	748	0.08%	0.008%
97	16.011	2446	2448	2451	rBV3	718	1028	0.11%	0.011%
98	16.389	2508	2510	2511	rVB2	677	427	0.05%	0.005%
99	16.517	2529	2531	2535	rBV3	621	861	0.09%	0.010%
100	16.688	2558	2559	2564	rBV4	834	1439	0.15%	0.016%




Sum of corrected areas: 9057495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030517.D
Acq On : 08 Aug 2022 17:22
Operator : JC/MD
Sample : N4066-05DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

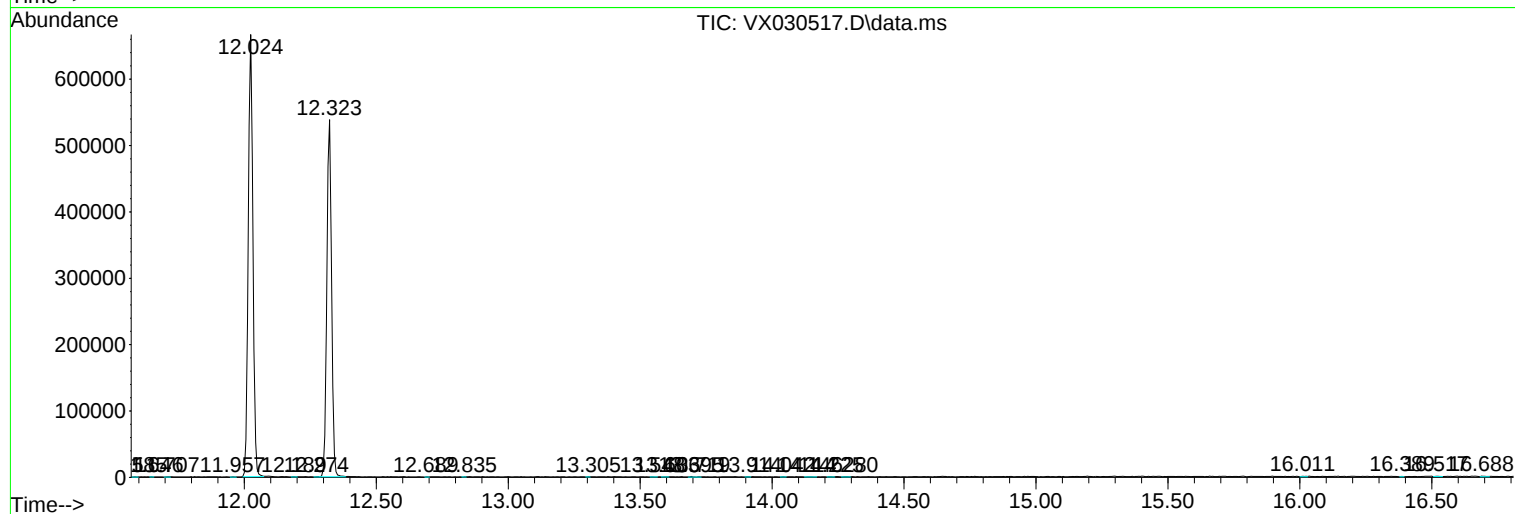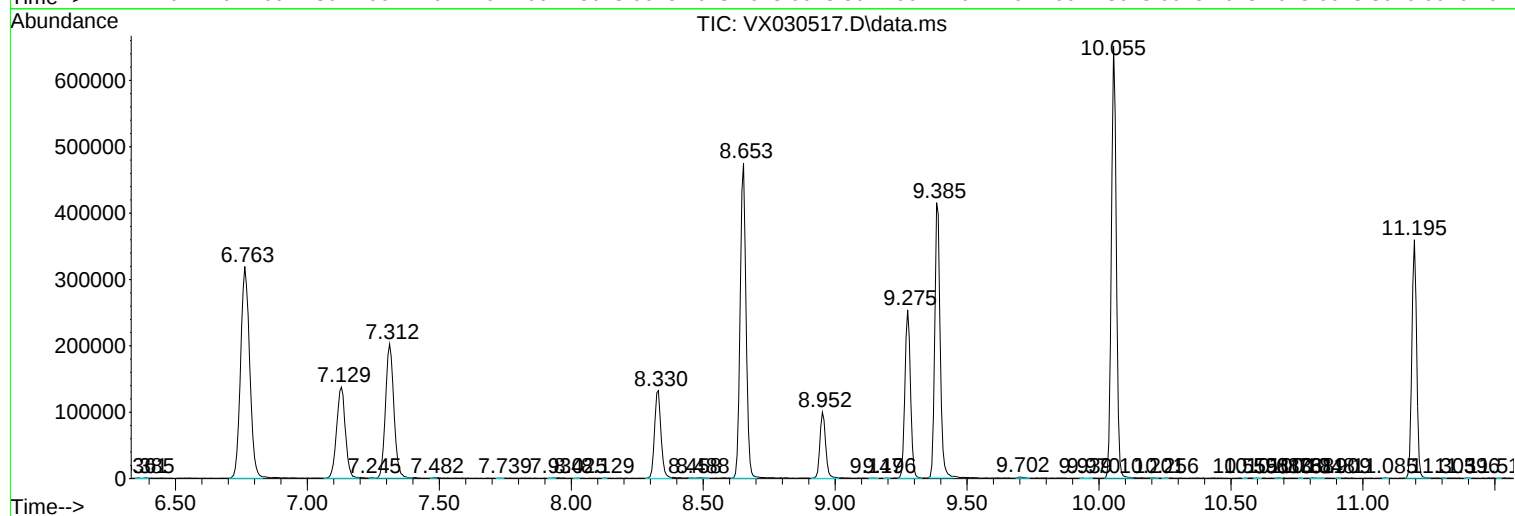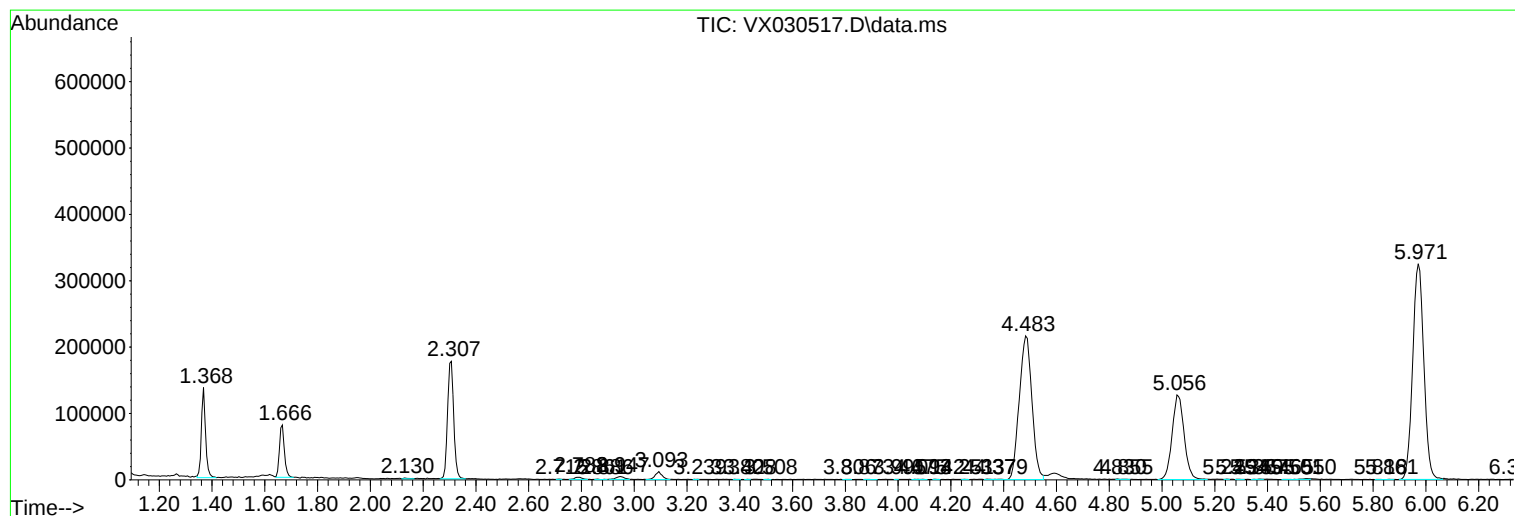

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030517.D
Acq On : 08 Aug 2022 17:22
Operator : JC/MD
Sample : N4066-05DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030517.D
Acq On : 08 Aug 2022 17:22
Operator : JC/MD
Sample : N4066-05DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E25DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc