

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030518.D
 Acq On : 08 Aug 2022 17:46
 Operator : JC/MD
 Sample : N4066-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	55	rVB2	121709	131475	9.96%	1.308%
2	1.660	91	94	105	rVB	89146	109212	8.28%	1.087%
3	2.306	193	200	209	rVB	175644	276087	20.92%	2.747%
4	2.453	222	224	228	rVB2	519	548	0.04%	0.005%
5	2.502	230	232	236	rVB3	526	632	0.05%	0.006%
6	2.575	239	244	245	rBV3	1341	1940	0.15%	0.019%
7	2.788	273	279	287	rBV5	3526	7436	0.56%	0.074%
8	2.947	297	305	312	rBV2	9790	22899	1.74%	0.228%
9	3.093	322	329	335	rBV5	3129	6379	0.48%	0.063%
10	3.142	335	337	339	rVB2	377	380	0.03%	0.004%
11	3.172	339	342	343	rBV2	417	501	0.04%	0.005%
12	3.239	351	353	356	rBV3	460	586	0.04%	0.006%
13	3.355	368	372	373	rVB2	363	353	0.03%	0.004%
14	3.611	412	414	417	rVB	407	347	0.03%	0.003%
15	4.141	497	501	502	rBV	293	373	0.03%	0.004%
16	4.172	505	506	510	rVB2	583	472	0.04%	0.005%
17	4.282	521	524	528	rVB2	372	576	0.04%	0.006%
18	4.337	528	533	537	rBV2	644	1052	0.08%	0.010%
19	4.391	539	542	544	rVB2	390	487	0.04%	0.005%
20	4.489	544	558	569	rBV4	191578	653994	49.56%	6.508%
21	5.068	638	653	671	rBV2	136073	407233	30.86%	4.052%
22	5.385	701	705	706	rBV3	1160	1455	0.11%	0.014%
23	5.562	727	734	739	rBV5	2681	5814	0.44%	0.058%
24	5.678	750	753	754	rVB	581	425	0.03%	0.004%
25	5.970	789	801	818	rBV2	332522	979169	74.20%	9.744%
26	6.172	833	834	837	rVB3	436	375	0.03%	0.004%
27	6.251	845	847	850	rBV	423	357	0.03%	0.004%
28	6.458	879	881	883	rVV	390	406	0.03%	0.004%
29	6.476	883	884	887	rVV2	631	474	0.04%	0.005%
30	6.543	891	895	896	rBV2	685	699	0.05%	0.007%
31	6.562	896	898	901	rVV2	856	723	0.05%	0.007%
32	6.598	903	904	909	rBV2	374	529	0.04%	0.005%
33	6.763	919	931	947	rBV2	308117	740884	56.14%	7.372%
34	7.062	978	980	982	rBV2	297	385	0.03%	0.004%
35	7.129	982	991	1012	rVV	606828	1319661	100.00%	13.132%
36	7.312	1013	1021	1039	rVB	202330	450670	34.15%	4.485%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030518.D
 Acq On : 08 Aug 2022 17:46
 Operator : JC/MD
 Sample : N4066-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.434	1039	1041	1043	rBV3	625	436	0.03%	0.004%
38	7.470	1044	1047	1048	rBV2	654	644	0.05%	0.006%
39	7.653	1073	1077	1079	rVB2	352	440	0.03%	0.004%
40	7.738	1089	1091	1092	rBV	539	361	0.03%	0.004%
41	7.763	1092	1095	1097	rVV2	545	437	0.03%	0.004%
42	7.933	1121	1123	1125	rVV3	400	456	0.03%	0.005%
43	8.092	1144	1149	1152	rVB2	615	806	0.06%	0.008%
44	8.135	1152	1156	1157	rBV2	366	433	0.03%	0.004%
45	8.232	1169	1172	1173	rBV	501	349	0.03%	0.003%
46	8.275	1176	1179	1180	rBV	438	330	0.03%	0.003%
47	8.330	1181	1188	1199	rBV	135533	224756	17.03%	2.237%
48	8.439	1204	1206	1207	rVB2	696	441	0.03%	0.004%
49	8.580	1225	1229	1233	rVB5	668	1232	0.09%	0.012%
50	8.653	1233	1241	1257	rBV	484469	743198	56.32%	7.396%
51	8.799	1262	1265	1266	rBV	496	510	0.04%	0.005%
52	8.903	1279	1282	1283	rBV2	385	436	0.03%	0.004%
53	8.952	1283	1290	1301	rBV	99181	151315	11.47%	1.506%
54	9.116	1315	1317	1321	rVB2	533	694	0.05%	0.007%
55	9.177	1325	1327	1329	rBV3	502	584	0.04%	0.006%
56	9.195	1329	1330	1333	rVB	597	392	0.03%	0.004%
57	9.275	1337	1343	1356	rBV	264409	393670	29.83%	3.917%
58	9.391	1356	1362	1372	rBV	423060	598034	45.32%	5.951%
59	9.701	1410	1413	1419	rVB2	3420	5373	0.41%	0.053%
60	9.762	1419	1423	1424	rVB	625	748	0.06%	0.007%
61	10.055	1466	1471	1482	rBV	612595	834936	63.27%	8.308%
62	10.543	1549	1551	1553	rBV2	333	376	0.03%	0.004%
63	10.579	1556	1557	1559	rBV2	400	335	0.03%	0.003%
64	10.640	1564	1567	1568	rBV2	359	382	0.03%	0.004%
65	10.793	1590	1592	1593	rVV	445	329	0.02%	0.003%
66	10.872	1603	1605	1607	rVB	546	395	0.03%	0.004%
67	11.195	1653	1658	1665	rBV	374354	466208	35.33%	4.639%
68	11.384	1688	1689	1692	rBV2	349	339	0.03%	0.003%
69	11.677	1735	1737	1739	rBV2	293	352	0.03%	0.004%
70	11.756	1748	1750	1751	rBV	545	395	0.03%	0.004%
71	12.024	1788	1794	1804	rBV	634903	788023	59.71%	7.842%
72	12.122	1808	1810	1814	rVB3	610	703	0.05%	0.007%
73	12.323	1837	1843	1854	rVV	578174	690290	52.31%	6.869%
74	12.500	1870	1872	1876	rVB2	490	512	0.04%	0.005%
75	12.579	1882	1885	1887	rBV	565	632	0.05%	0.006%
76	12.677	1898	1901	1903	rBV2	491	623	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030518.D
 Acq On : 08 Aug 2022 17:46
 Operator : JC/MD
 Sample : N4066-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E26DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.725	1907	1909	1910	rBV2	381	322	0.02%	0.003%
78	12.890	1934	1936	1937	rVB	531	361	0.03%	0.004%
79	12.908	1937	1939	1941	rBV2	689	691	0.05%	0.007%
80	13.122	1973	1974	1976	rVB2	561	345	0.03%	0.003%
81	13.146	1976	1978	1980	rBV2	545	440	0.03%	0.004%
82	13.201	1985	1987	1991	rVB2	606	703	0.05%	0.007%
83	13.262	1995	1997	1999	rBV2	331	418	0.03%	0.004%
84	13.420	2019	2023	2026	rVB2	628	822	0.06%	0.008%
85	13.475	2029	2032	2033	rBV	379	497	0.04%	0.005%
86	13.579	2047	2049	2052	rBV3	630	760	0.06%	0.008%
87	13.829	2088	2090	2091	rBV	566	476	0.04%	0.005%
88	13.951	2108	2110	2112	rVV	616	458	0.03%	0.005%
89	13.993	2115	2117	2120	rVV2	426	438	0.03%	0.004%
90	14.134	2137	2140	2143	rVB3	839	851	0.06%	0.008%
91	14.158	2143	2144	2145	rBV	791	349	0.03%	0.003%
92	14.256	2156	2160	2162	rBV2	779	1101	0.08%	0.011%
93	14.585	2213	2214	2217	rVB2	675	471	0.04%	0.005%
94	14.731	2236	2238	2239	rBV	610	368	0.03%	0.004%
95	14.835	2254	2255	2257	rBV2	489	429	0.03%	0.004%
96	15.194	2312	2314	2315	rBV2	537	409	0.03%	0.004%
97	15.249	2321	2323	2325	rBV3	741	743	0.06%	0.007%
98	16.048	2452	2454	2458	rBV2	704	1017	0.08%	0.010%
99	16.280	2490	2492	2495	rVV3	568	505	0.04%	0.005%
100	16.639	2548	2551	2552	rBV2	528	429	0.03%	0.004%




Sum of corrected areas: 10049296

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030518.D
Acq On : 08 Aug 2022 17:46
Operator : JC/MD
Sample : N4066-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

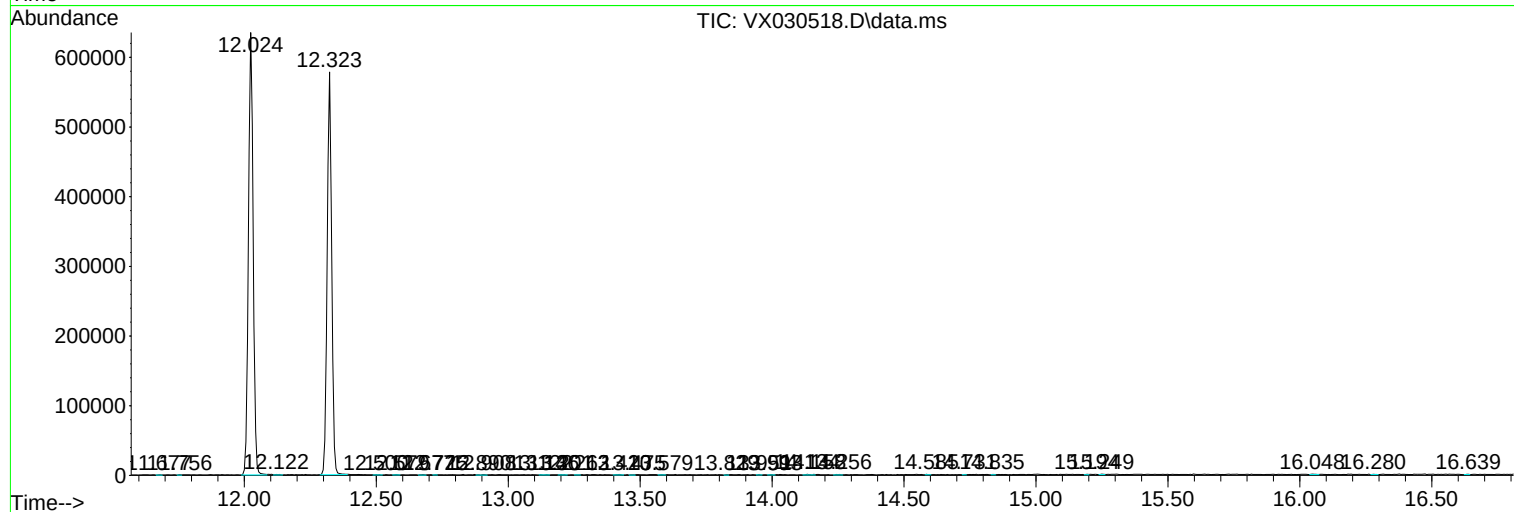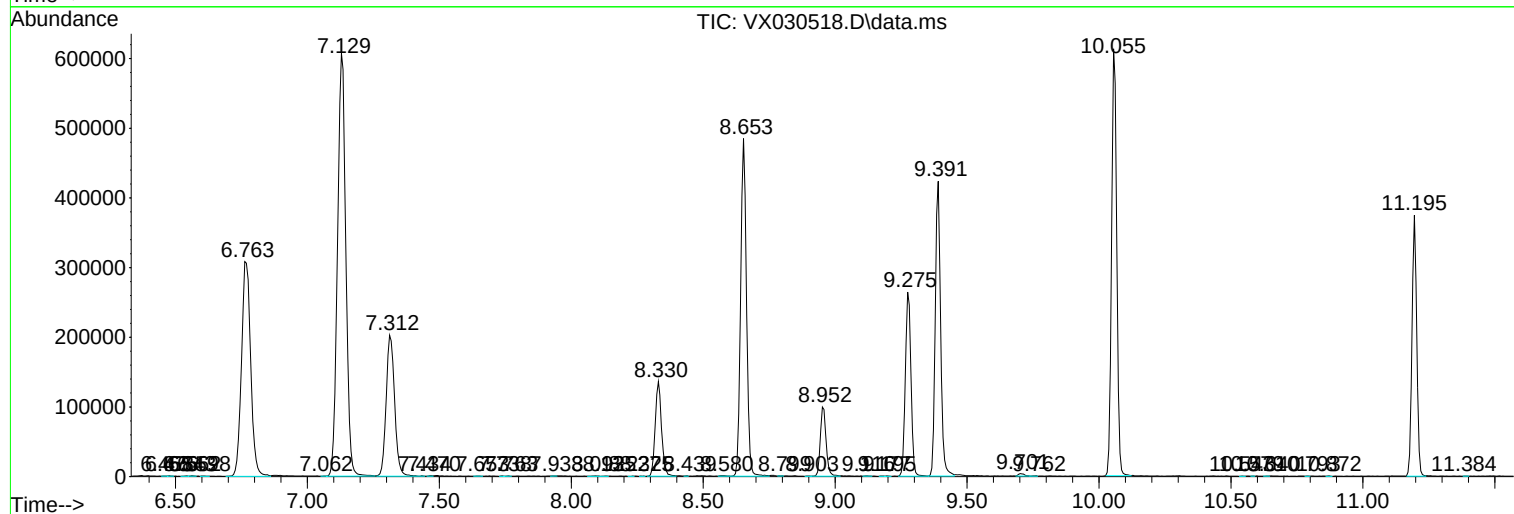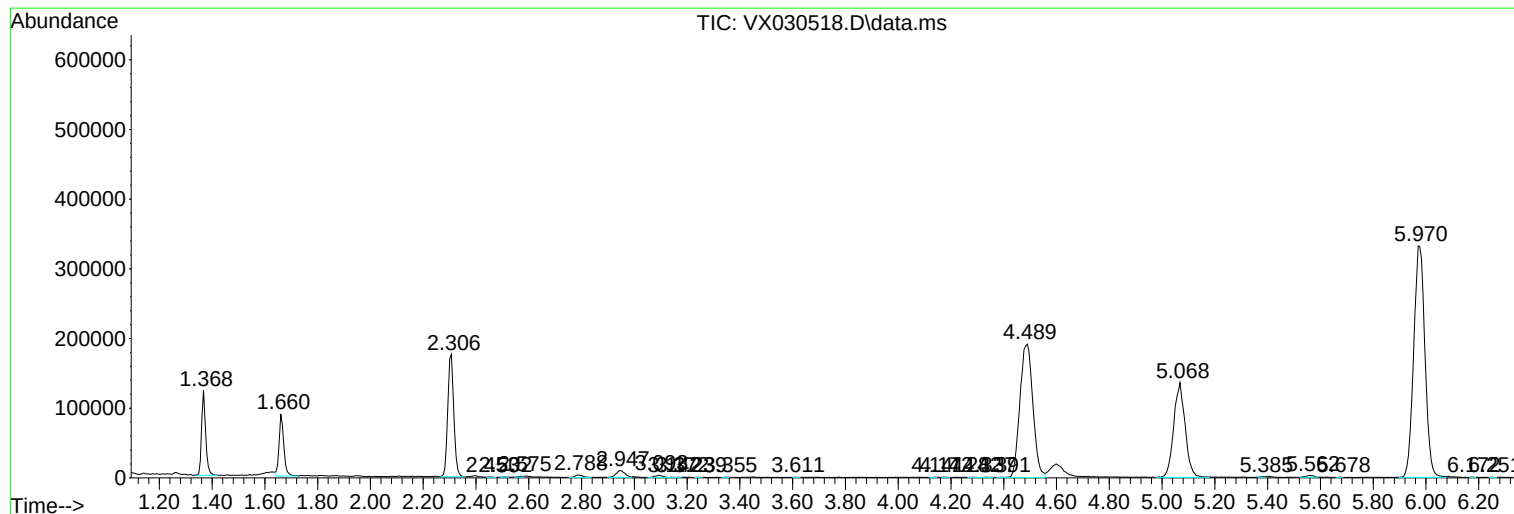

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030518.D
Acq On : 08 Aug 2022 17:46
Operator : JC/MD
Sample : N4066-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030518.D
Acq On : 08 Aug 2022 17:46
Operator : JC/MD
Sample : N4066-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E26DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc