

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030519.D
 Acq On : 08 Aug 2022 18:10
 Operator : JC/MD
 Sample : N4066-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.367	42	46	57	rVB2	124148	131832	11.45%	1.389%
2	1.666	91	95	104	rVB	78621	108406	9.41%	1.142%
3	2.306	194	200	210	rVB	176228	270198	23.46%	2.847%
4	2.721	264	268	270	rBV2	402	533	0.05%	0.006%
5	2.794	276	280	286	rVB4	3483	5817	0.51%	0.061%
6	2.946	298	305	313	rBV2	6909	15428	1.34%	0.163%
7	3.093	324	329	336	rVB2	3244	5540	0.48%	0.058%
8	3.245	353	354	357	rVB2	443	454	0.04%	0.005%
9	3.275	357	359	361	rBV	454	507	0.04%	0.005%
10	3.422	381	383	384	rBV	385	342	0.03%	0.004%
11	3.696	425	428	431	rBV2	319	493	0.04%	0.005%
12	3.800	443	445	449	rVB2	391	498	0.04%	0.005%
13	3.849	451	453	456	rVB2	474	448	0.04%	0.005%
14	3.946	462	469	471	rBV3	476	878	0.08%	0.009%
15	4.166	504	505	507	rBV2	492	303	0.03%	0.003%
16	4.190	507	509	513	rVV2	375	507	0.04%	0.005%
17	4.324	529	531	534	rVB	543	549	0.05%	0.006%
18	4.489	546	558	569	rBV2	184597	619601	53.80%	6.529%
19	5.068	641	653	668	rBV2	127620	386909	33.60%	4.077%
20	5.330	691	696	700	rBV2	474	865	0.08%	0.009%
21	5.391	700	706	707	rBV3	1235	2147	0.19%	0.023%
22	5.562	729	734	741	rVB4	2044	5127	0.45%	0.054%
23	5.653	746	749	751	rBV2	321	369	0.03%	0.004%
24	5.769	766	768	770	rVB2	472	399	0.03%	0.004%
25	5.976	790	802	825	rBV3	323492	944095	81.98%	9.948%
26	6.324	854	859	860	rBV	427	505	0.04%	0.005%
27	6.342	860	862	863	rVV	503	298	0.03%	0.003%
28	6.409	871	873	876	rVB2	347	321	0.03%	0.003%
29	6.452	878	880	881	rBV	623	471	0.04%	0.005%
30	6.622	905	908	910	rBV2	426	473	0.04%	0.005%
31	6.696	916	920	922	rBV2	491	490	0.04%	0.005%
32	6.769	922	932	947	rBV	299650	697565	60.58%	7.350%
33	6.982	965	967	971	rVB2	403	523	0.05%	0.006%
34	7.019	971	973	974	rBV	589	454	0.04%	0.005%
35	7.135	981	992	1004	rBV	522801	1151568	100.00%	12.134%
36	7.317	1013	1022	1034	rBV	195844	433062	37.61%	4.563%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030519.D
 Acq On : 08 Aug 2022 18:10
 Operator : JC/MD
 Sample : N4066-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.622	1070	1072	1075	rBV2	370	457	0.04%	0.005%
38	7.701	1083	1085	1086	rVB	480	346	0.03%	0.004%
39	7.720	1086	1088	1092	rBV2	467	695	0.06%	0.007%
40	7.756	1092	1094	1095	rVB	547	335	0.03%	0.004%
41	7.769	1095	1096	1099	rBV	464	537	0.05%	0.006%
42	7.866	1110	1112	1114	rBV2	423	318	0.03%	0.003%
43	7.897	1115	1117	1120	rVB2	433	392	0.03%	0.004%
44	8.025	1133	1138	1140	rBV2	782	1284	0.11%	0.014%
45	8.049	1140	1142	1145	rVV2	486	658	0.06%	0.007%
46	8.073	1145	1146	1149	rVV2	642	568	0.05%	0.006%
47	8.116	1152	1153	1157	rVV2	413	399	0.03%	0.004%
48	8.232	1171	1172	1176	rVB2	455	473	0.04%	0.005%
49	8.329	1180	1188	1198	rBV	133828	221233	19.21%	2.331%
50	8.415	1201	1202	1205	rVB2	904	611	0.05%	0.006%
51	8.476	1211	1212	1214	rBV2	538	449	0.04%	0.005%
52	8.573	1226	1228	1230	rBV	398	382	0.03%	0.004%
53	8.598	1230	1232	1234	rVB2	781	599	0.05%	0.006%
54	8.653	1234	1241	1252	rBV	461875	717528	62.31%	7.561%
55	8.762	1257	1259	1262	rVV2	1117	1295	0.11%	0.014%
56	8.793	1262	1264	1267	rVB2	861	790	0.07%	0.008%
57	8.957	1285	1291	1299	rBV	95946	146292	12.70%	1.542%
58	9.274	1337	1343	1355	rVB	239918	356422	30.95%	3.756%
59	9.390	1356	1362	1375	rBV	417889	590038	51.24%	6.217%
60	9.658	1404	1406	1409	rVB2	654	584	0.05%	0.006%
61	9.707	1409	1414	1421	rBV5	3699	6435	0.56%	0.068%
62	9.774	1421	1425	1430	rBV3	862	1378	0.12%	0.015%
63	10.055	1466	1471	1486	rVB	592386	818655	71.09%	8.626%
64	10.158	1486	1488	1493	rBV2	679	951	0.08%	0.010%
65	10.299	1509	1511	1516	rVB3	703	949	0.08%	0.010%
66	10.427	1530	1532	1534	rBV	488	443	0.04%	0.005%
67	10.786	1590	1591	1593	rVB	660	374	0.03%	0.004%
68	10.805	1593	1594	1597	rBV2	375	438	0.04%	0.005%
69	11.195	1652	1658	1668	rBV	360321	457424	39.72%	4.820%
70	11.359	1683	1685	1687	rVB	504	362	0.03%	0.004%
71	11.530	1711	1713	1714	rBV2	343	305	0.03%	0.003%
72	11.926	1776	1778	1780	rVB	397	321	0.03%	0.003%
73	11.951	1780	1782	1783	rBV2	321	327	0.03%	0.003%
74	12.024	1789	1794	1801	rBV	614948	739014	64.17%	7.787%
75	12.231	1825	1828	1832	rBV4	596	723	0.06%	0.008%
76	12.323	1837	1843	1851	rBV	504284	619602	53.81%	6.529%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030519.D
 Acq On : 08 Aug 2022 18:10
 Operator : JC/MD
 Sample : N4066-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 F5E27DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	12.426	1858	1860	1861	rBV2	378	328	0.03%	0.003%
78	12.579	1883	1885	1887	rBV2	485	496	0.04%	0.005%
79	12.627	1891	1893	1896	rVB2	803	613	0.05%	0.006%
80	12.707	1905	1906	1909	rBV2	458	329	0.03%	0.003%
81	12.896	1935	1937	1939	rBV2	314	360	0.03%	0.004%
82	13.109	1970	1972	1975	rBV2	320	309	0.03%	0.003%
83	13.133	1975	1976	1982	rVB2	542	761	0.07%	0.008%
84	13.298	2001	2003	2005	rBV2	479	365	0.03%	0.004%
85	13.353	2011	2012	2014	rBV	349	336	0.03%	0.004%
86	13.377	2014	2016	2018	rVV2	556	443	0.04%	0.005%
87	13.700	2067	2069	2070	rVB	691	386	0.03%	0.004%
88	13.737	2073	2075	2077	rBV	515	361	0.03%	0.004%
89	13.963	2111	2112	2117	rVB2	278	326	0.03%	0.003%
90	14.316	2168	2170	2173	rVB2	439	518	0.04%	0.005%
91	14.651	2222	2225	2227	rBV2	705	698	0.06%	0.007%
92	14.676	2227	2229	2230	rVB2	527	338	0.03%	0.004%
93	14.859	2257	2259	2264	rVB2	939	1141	0.10%	0.012%
94	15.371	2341	2343	2344	rBV	671	443	0.04%	0.005%
95	15.444	2354	2355	2356	rBV	782	328	0.03%	0.003%
96	15.499	2362	2364	2367	rBV3	575	678	0.06%	0.007%
97	15.682	2392	2394	2395	rVB	796	365	0.03%	0.004%
98	15.700	2395	2397	2400	rBV	647	677	0.06%	0.007%
99	16.194	2475	2478	2479	rBV	765	832	0.07%	0.009%
100	16.541	2534	2535	2537	rBV	658	434	0.04%	0.005%




Sum of corrected areas: 9490226

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030519.D
Acq On : 08 Aug 2022 18:10
Operator : JC/MD
Sample : N4066-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

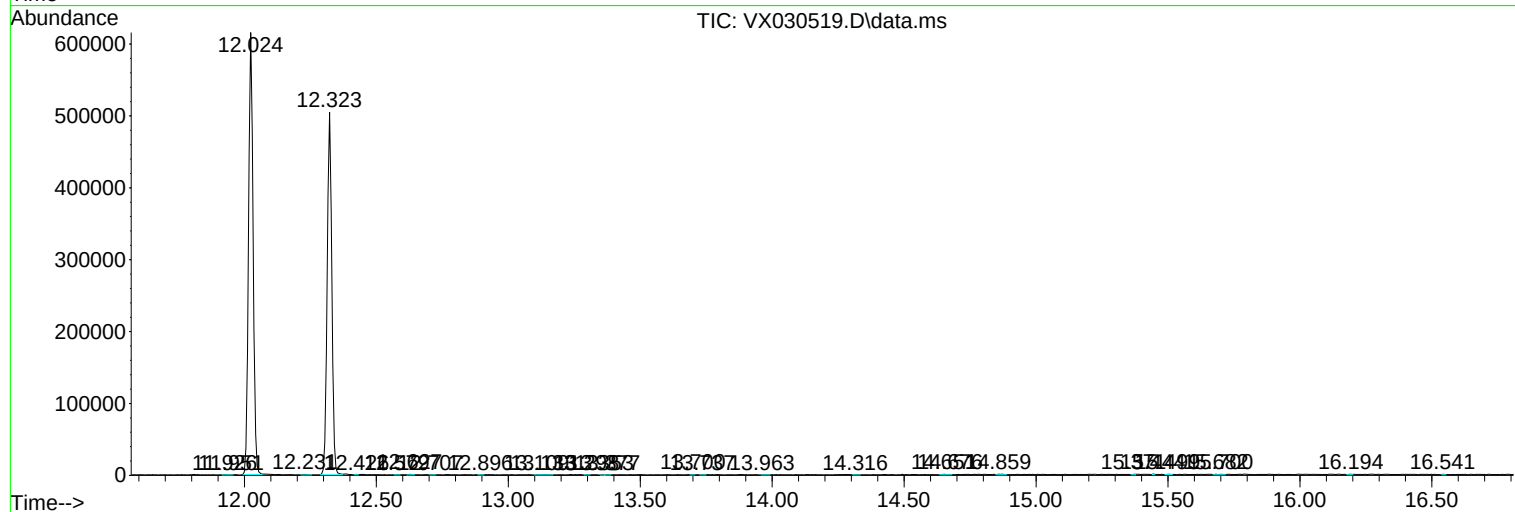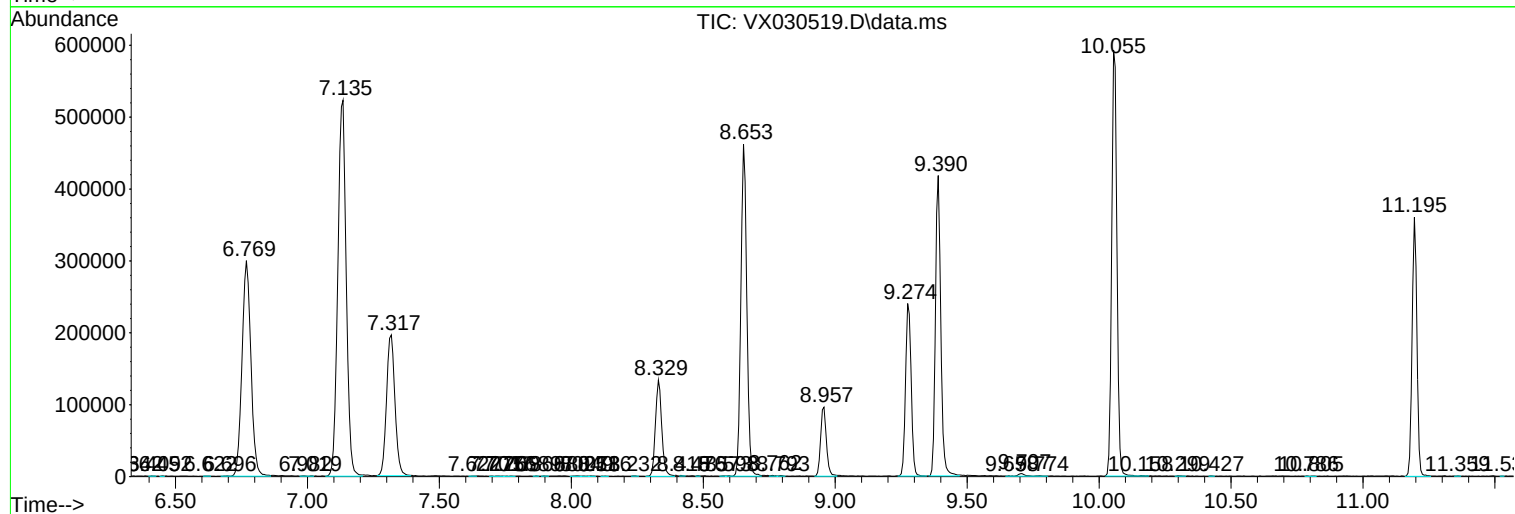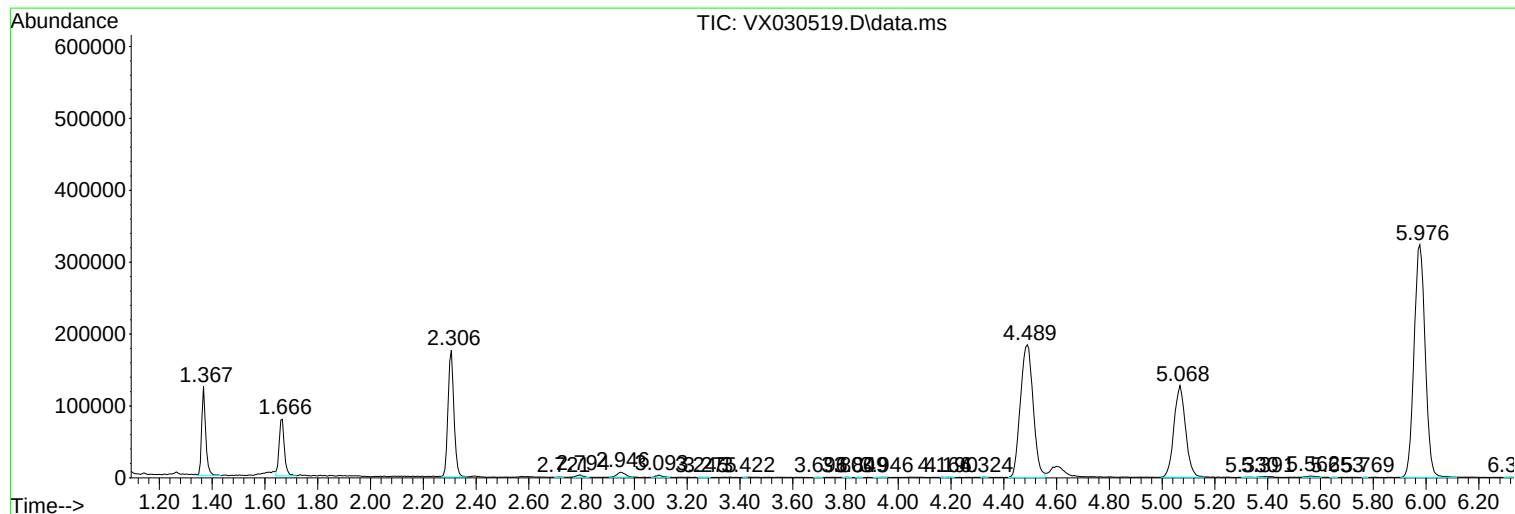

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030519.D
Acq On : 08 Aug 2022 18:10
Operator : JC/MD
Sample : N4066-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030519.D
Acq On : 08 Aug 2022 18:10
Operator : JC/MD
Sample : N4066-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
F5E27DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc