

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030520.D
 Acq On : 08 Aug 2022 18:33
 Operator : JC/MD
 Sample : N4066-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	54	rVB	103487	108580	11.47%	1.393%
2	1.666	91	95	105	rVB	83849	106451	11.24%	1.365%
3	2.307	194	200	209	rVB	161358	252447	26.66%	3.238%
4	2.398	212	215	219	rVB2	1140	1433	0.15%	0.018%
5	2.465	224	226	230	rBV2	485	628	0.07%	0.008%
6	2.788	275	279	287	rVB2	3694	7389	0.78%	0.095%
7	2.947	297	305	313	rVV3	6036	14682	1.55%	0.188%
8	3.032	317	319	322	rVB2	381	383	0.04%	0.005%
9	3.264	354	357	359	rBV	434	526	0.06%	0.007%
10	3.300	361	363	365	rBV2	579	639	0.07%	0.008%
11	3.349	370	371	375	rVB	318	365	0.04%	0.005%
12	3.733	432	434	438	rBV2	282	386	0.04%	0.005%
13	3.782	440	442	446	rVB2	489	468	0.05%	0.006%
14	4.014	479	480	484	rVB	430	330	0.03%	0.004%
15	4.062	484	488	489	rBV2	347	423	0.04%	0.005%
16	4.123	495	498	499	rBV	479	383	0.04%	0.005%
17	4.294	523	526	528	rBV3	564	584	0.06%	0.007%
18	4.471	546	555	567	rBV	106820	301692	31.86%	3.870%
19	4.940	630	632	634	rVB2	375	332	0.04%	0.004%
20	4.983	637	639	641	rBV2	433	402	0.04%	0.005%
21	5.062	641	652	671	rVV2	130723	405883	42.87%	5.206%
22	5.239	680	681	684	rBV	459	362	0.04%	0.005%
23	5.263	684	685	691	rBV3	403	574	0.06%	0.007%
24	5.519	724	727	729	rVV2	661	826	0.09%	0.011%
25	5.562	729	734	742	rVB5	2587	5685	0.60%	0.073%
26	5.867	780	784	790	rVB3	423	881	0.09%	0.011%
27	5.977	790	802	819	rBV2	326275	946861	100.00%	12.146%
28	6.190	836	837	840	rVB	557	351	0.04%	0.005%
29	6.361	862	865	867	rVB2	592	665	0.07%	0.009%
30	6.385	867	869	871	rBV2	559	695	0.07%	0.009%
31	6.507	888	889	893	rVB	312	367	0.04%	0.005%
32	6.617	905	907	908	rBV2	372	346	0.04%	0.004%
33	6.684	916	918	920	rBV	435	451	0.05%	0.006%
34	6.769	922	932	948	rVV	295610	709124	74.89%	9.096%
35	6.946	959	961	964	rBV	478	418	0.04%	0.005%
36	7.050	975	978	981	rBV2	467	616	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030520.D
 Acq On : 08 Aug 2022 18:33
 Operator : JC/MD
 Sample : N4066-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	7.129	981	991	999	rVV4	15984	42204	4.46%	0.541%
38	7.226	1004	1007	1009	rBV2	363	385	0.04%	0.005%
39	7.318	1012	1022	1036	rBV	203132	451769	47.71%	5.795%
40	7.940	1120	1124	1128	rBV5	1224	2594	0.27%	0.033%
41	8.275	1175	1179	1181	rBV	394	536	0.06%	0.007%
42	8.330	1181	1188	1197	rBV	132448	219099	23.14%	2.810%
43	8.421	1202	1203	1206	rVV2	861	532	0.06%	0.007%
44	8.458	1207	1209	1211	rVV	510	410	0.04%	0.005%
45	8.482	1211	1213	1220	rVB3	1063	1638	0.17%	0.021%
46	8.574	1225	1228	1229	rBV2	334	336	0.04%	0.004%
47	8.653	1234	1241	1251	rBV	441857	681058	71.93%	8.736%
48	8.952	1283	1290	1299	rBV	93021	147219	15.55%	1.888%
49	9.116	1314	1317	1320	rBV	441	550	0.06%	0.007%
50	9.165	1323	1325	1328	rVV	348	515	0.05%	0.007%
51	9.196	1328	1330	1332	rVV2	608	492	0.05%	0.006%
52	9.226	1333	1335	1336	rVV	518	401	0.04%	0.005%
53	9.281	1340	1344	1351	rVB5	4621	7143	0.75%	0.092%
54	9.391	1356	1362	1375	rBV	453812	657775	69.47%	8.437%
55	9.702	1409	1413	1419	rBV5	2540	3676	0.39%	0.047%
56	10.055	1464	1471	1481	rBV	585730	822675	86.88%	10.553%
57	10.512	1545	1546	1547	rBV	666	350	0.04%	0.004%
58	10.573	1554	1556	1559	rVB2	465	410	0.04%	0.005%
59	10.756	1584	1586	1589	rBV	386	334	0.04%	0.004%
60	10.805	1592	1594	1595	rBV	414	333	0.04%	0.004%
61	10.829	1595	1598	1601	rBV2	287	355	0.04%	0.005%
62	10.933	1613	1615	1618	rVV2	796	729	0.08%	0.009%
63	11.098	1640	1642	1645	rVB2	374	339	0.04%	0.004%
64	11.195	1652	1658	1671	rBV	391025	493605	52.13%	6.332%
65	11.421	1691	1695	1698	rBV3	463	824	0.09%	0.011%
66	11.463	1701	1702	1705	rVV	475	345	0.04%	0.004%
67	11.494	1705	1707	1711	rVB2	317	444	0.05%	0.006%
68	11.585	1720	1722	1724	rVB	561	389	0.04%	0.005%
69	11.677	1734	1737	1740	rBV3	450	740	0.08%	0.009%
70	11.762	1748	1751	1752	rBV	855	764	0.08%	0.010%
71	12.024	1789	1794	1803	rBV	603959	734264	77.55%	9.419%
72	12.323	1837	1843	1851	rBV	511894	631541	66.70%	8.101%
73	12.433	1859	1861	1862	rBV	725	358	0.04%	0.005%
74	12.860	1928	1931	1932	rBV	368	331	0.03%	0.004%
75	12.908	1936	1939	1940	rBV2	642	603	0.06%	0.008%
76	12.927	1940	1942	1944	rBV	402	373	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030520.D
 Acq On : 08 Aug 2022 18:33
 Operator : JC/MD
 Sample : N4066-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	13.055	1959	1963	1964	rBV2	500	685	0.07%	0.009%
78	13.158	1978	1980	1983	rVB2	550	597	0.06%	0.008%
79	13.402	2019	2020	2023	rBV2	429	377	0.04%	0.005%
80	13.616	2053	2055	2058	rVV	343	369	0.04%	0.005%
81	13.652	2058	2061	2062	rBV	726	443	0.05%	0.006%
82	13.719	2071	2072	2075	rVB2	506	386	0.04%	0.005%
83	13.786	2080	2083	2086	rBV2	668	1007	0.11%	0.013%
84	13.963	2111	2112	2114	rBV2	634	449	0.05%	0.006%
85	14.085	2130	2132	2135	rBV2	867	675	0.07%	0.009%
86	14.140	2135	2141	2143	rBV4	749	982	0.10%	0.013%
87	14.225	2153	2155	2159	rVB3	686	703	0.07%	0.009%
88	14.274	2159	2163	2164	rBV2	368	570	0.06%	0.007%
89	14.432	2184	2189	2191	rBV2	716	1068	0.11%	0.014%
90	14.463	2191	2194	2195	rBV	372	351	0.04%	0.005%
91	14.762	2242	2243	2246	rBV	695	720	0.08%	0.009%
92	14.877	2260	2262	2264	rBV2	669	638	0.07%	0.008%
93	14.902	2264	2266	2268	rVV2	504	341	0.04%	0.004%
94	15.030	2286	2287	2289	rBV2	476	390	0.04%	0.005%
95	15.097	2295	2298	2301	rBV3	552	716	0.08%	0.009%
96	15.390	2345	2346	2348	rBV2	623	539	0.06%	0.007%
97	15.810	2413	2415	2418	rVB4	863	756	0.08%	0.010%
98	16.304	2494	2496	2499	rVB	683	540	0.06%	0.007%
99	16.444	2518	2519	2520	rBV	661	336	0.04%	0.004%
100	16.591	2539	2543	2547	rBV4	630	1239	0.13%	0.016%




Sum of corrected areas: 7795943

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030520.D
Acq On : 08 Aug 2022 18:33
Operator : JC/MD
Sample : N4066-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

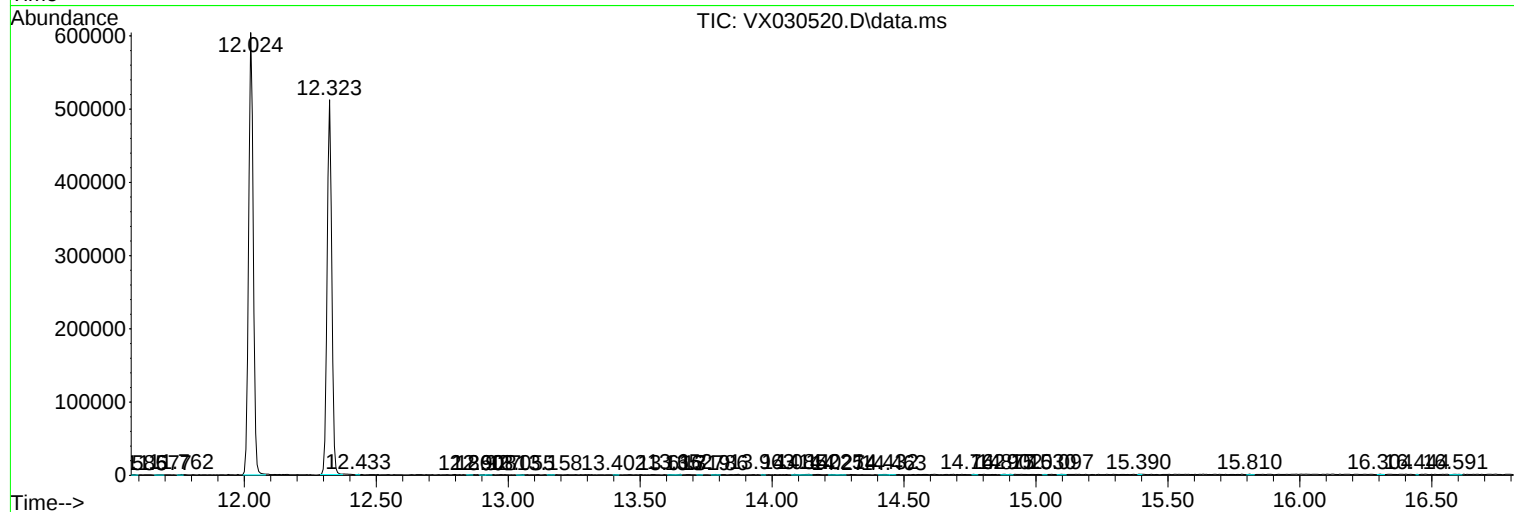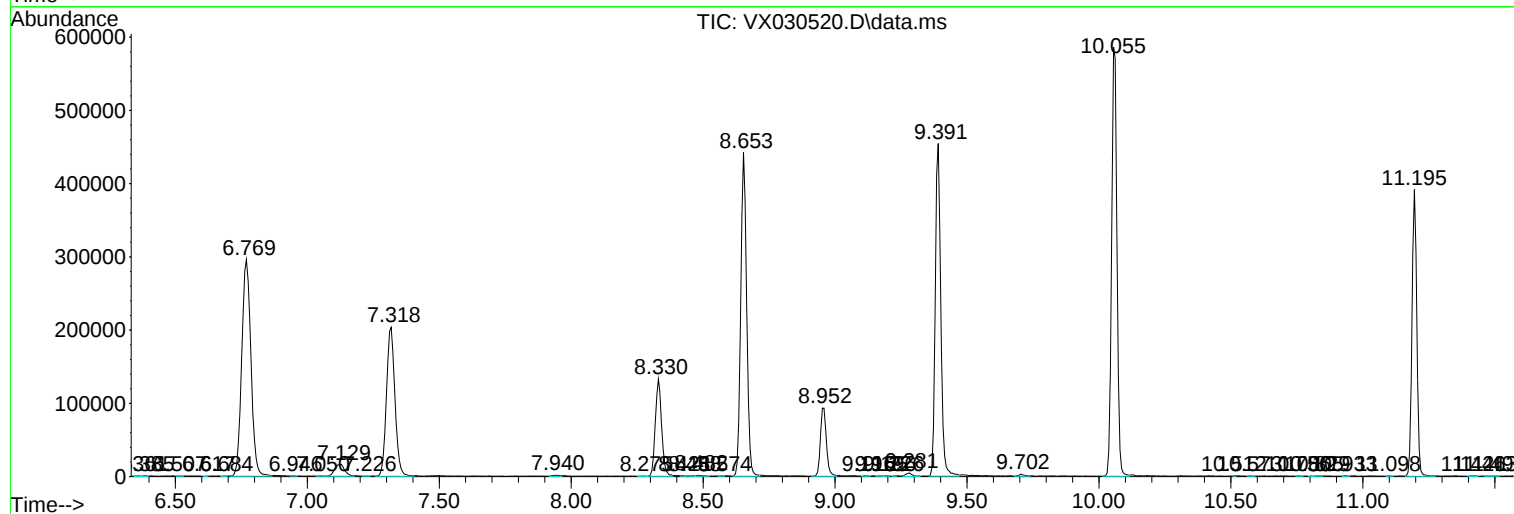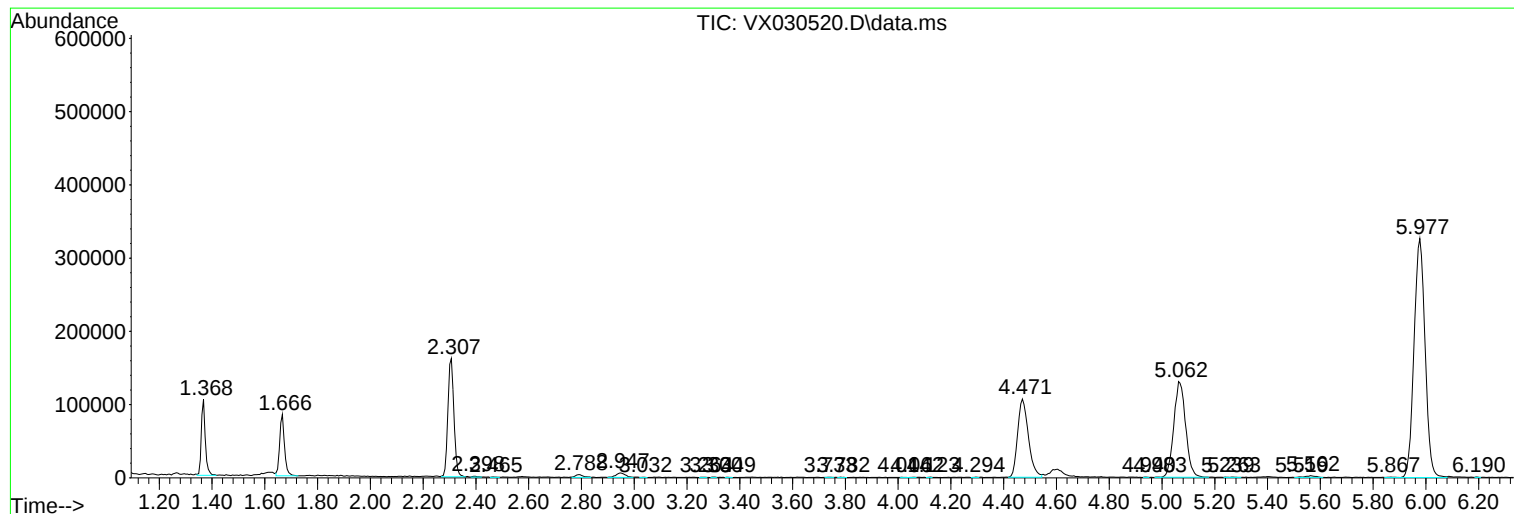

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030520.D
Acq On : 08 Aug 2022 18:33
Operator : JC/MD
Sample : N4066-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
Data File : VX030520.D
Acq On : 08 Aug 2022 18:33
Operator : JC/MD
Sample : N4066-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc