
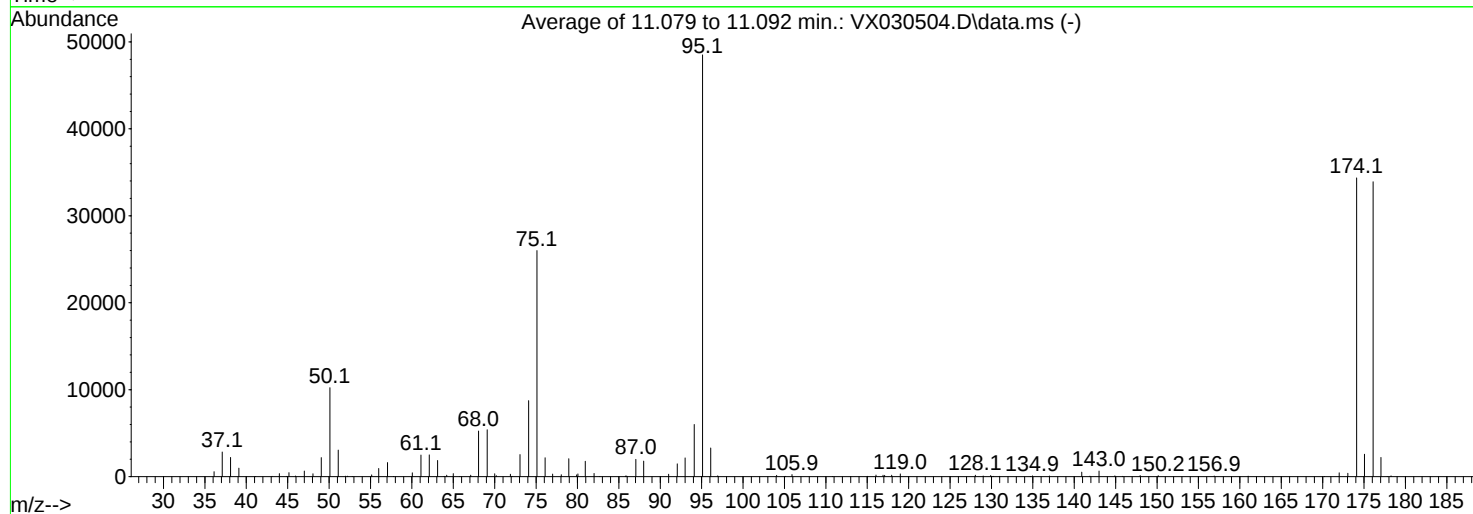


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080822\
 Data File : VX030504.D
 Acq On : 08 Aug 2022 09:09
 Operator : JC/MD
 Sample : BFB673
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB673

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM080422WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 09 00:14:16 2022

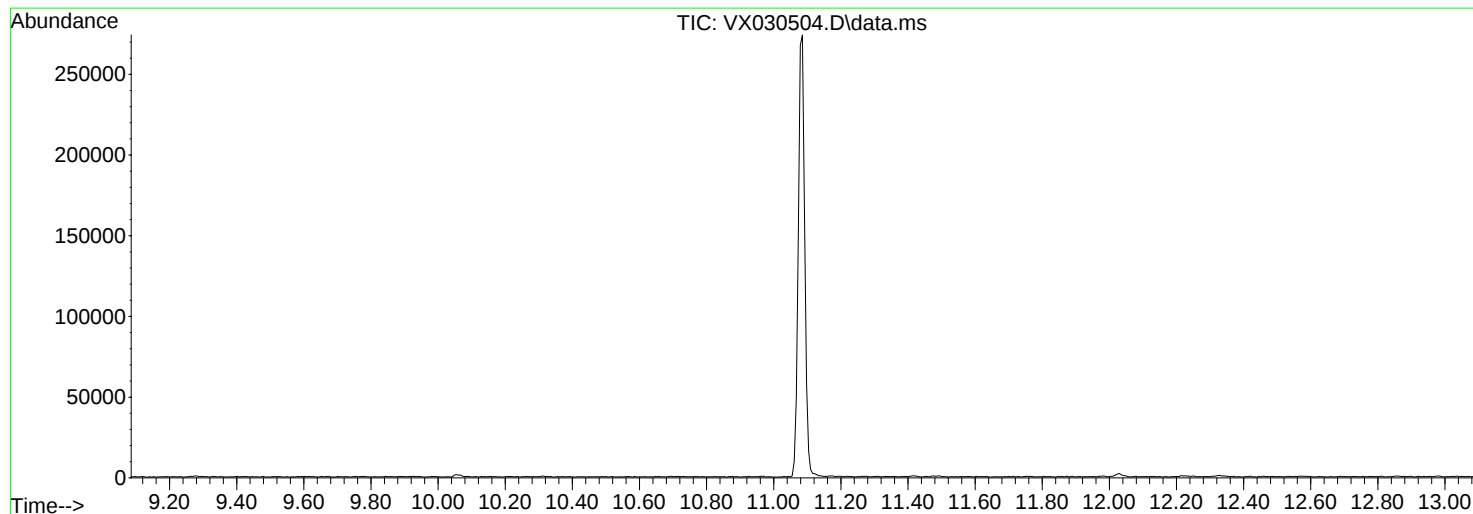

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	10228	PASS
75	95	30	80	53.6	26012	PASS
95	95	100	100	100.0	48512	PASS
96	95	5	9	6.8	3294	PASS
173	174	0.00	2	1.1	379	PASS
174	95	50	120	70.8	34352	PASS
175	174	5	9	7.5	2568	PASS
176	174	95	101	98.7	33917	PASS
177	176	5	9	6.5	2208	PASS

m/z	Abundance
40.00	490.0
43.90	250.0
46.90	56.0
47.80	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673

m/z	Abundance
36.10	784.0
37.10	3695.0
38.10	2971.0
39.10	1092.0
39.90	518.0
43.10	53.0
44.10	817.0
45.10	734.0
45.90	62.0
47.10	688.0
48.00	327.0
49.10	2383.0
50.10	12471.0
51.10	3785.0
52.00	145.0
52.80	54.0
55.10	182.0
56.00	1128.0
57.00	1738.0
57.80	59.0
60.00	577.0
61.10	3066.0
62.10	3142.0
63.10	2229.0
64.20	255.0
65.00	373.0
67.00	167.0
68.00	6437.0
69.10	6590.0
70.00	497.0
71.90	413.0
73.00	3072.0
74.10	11084.0
75.10	32576.0
76.10	2320.0
77.00	365.0
78.00	232.0
78.90	2498.0
79.90	636.0
80.90	1984.0
82.00	421.0
85.80	235.0
87.10	2300.0
88.00	2115.0
91.00	324.0
92.00	1880.0
93.00	2508.0
94.10	7084.0
95.10	54800.0
96.10	3947.0
96.90	134.0
104.10	129.0
106.00	231.0
110.80	87.0
113.00	71.0
115.00	50.0
116.00	224.0
116.90	296.0
118.00	203.0
119.00	346.0
128.10	229.0
129.00	128.0
129.90	197.0
131.00	79.0
134.70	78.0
135.10	80.0
137.00	120.0
140.90	557.0
142.00	96.0
143.00	562.0
144.90	79.0
145.90	74.0
147.90	107.0
150.20	174.0
156.90	118.0
161.00	74.0
172.00	529.0
173.10	488.0
174.10	34016.0
175.00	2693.0
176.10	35480.0
177.10	2288.0
177.80	60.0
178.30	76.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673

m/z	Abundance
36.10	514.0
37.10	3248.0
38.10	2266.0
39.10	1166.0
39.90	338.0
43.10	79.0
44.00	552.0
45.20	623.0
46.00	153.0
47.00	760.0
48.10	435.0
49.00	2733.0
50.10	11680.0
51.10	3523.0
52.20	105.0
55.20	210.0
55.90	962.0
57.10	2011.0
60.10	483.0
61.10	2814.0
62.10	2810.0
63.10	2189.0
64.20	225.0
65.00	518.0
67.10	219.0
68.10	5482.0
69.10	6355.0
70.00	494.0
71.90	400.0
73.10	2891.0
74.10	9430.0
75.10	29104.0
76.10	2561.0
77.00	449.0
78.10	286.0
79.00	2256.0
80.10	530.0
81.00	1880.0
82.00	351.0
82.70	64.0
86.00	121.0
87.00	2390.0
88.00	2295.0
90.90	287.0
92.10	1665.0
93.00	2418.0
94.10	6922.0
95.10	57992.0
96.10	3595.0
97.00	126.0
104.00	255.0
105.10	65.0
105.80	300.0
115.10	75.0
116.00	169.0
117.10	453.0
117.90	184.0
118.90	308.0
128.00	208.0
129.00	119.0
129.90	220.0
130.90	52.0
134.90	171.0
137.00	97.0
140.90	607.0
141.80	87.0
143.00	837.0
144.90	221.0
145.80	55.0
148.00	203.0
150.00	50.0
156.90	117.0
161.00	95.0
172.10	487.0
173.00	466.0
174.10	42472.0
175.10	3395.0
176.10	38984.0
177.00	2518.0
178.20	116.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673

m/z	Abundance
36.10	411.0
37.10	1567.0
38.00	1395.0
39.10	657.0
40.00	376.0
41.10	56.0
44.00	418.0
44.90	142.0
47.10	645.0
48.10	218.0
49.10	1443.0
50.10	6532.0
51.00	1836.0
52.30	58.0
55.10	214.0
56.10	701.0
57.00	1127.0
60.10	250.0
61.10	1585.0
62.10	1578.0
63.10	1151.0
63.90	118.0
64.90	137.0
65.80	65.0
67.20	100.0
68.00	3816.0
69.00	3257.0
70.20	354.0
72.10	137.0
73.10	1678.0
74.00	5699.0
75.10	16355.0
76.00	1614.0
77.10	87.0
78.10	171.0
79.00	1415.0
80.00	407.0
81.00	1447.0
82.00	332.0
85.90	112.0
87.10	1288.0
87.90	934.0
91.10	208.0
92.00	856.0
93.10	1523.0
94.10	3993.0
95.10	32744.0
96.10	2340.0
104.10	74.0
105.10	54.0
105.90	190.0
116.10	168.0
116.90	221.0
117.90	126.0
119.10	297.0
128.00	80.0
130.20	107.0
141.00	369.0
143.00	553.0
148.00	93.0
150.20	84.0
170.20	70.0
171.90	318.0
173.10	182.0
174.10	26568.0
175.10	1615.0
176.10	27288.0
177.00	1819.0
178.20	65.0

Instrument :
MSVOA_X
ClientSampleId :
BFB673