

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080824\
 Data File : VX042972.D
 Acq On : 09 Aug 2024 05:16
 Operator : JC/MD
 Sample : P3469-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-03

Quant Time: Aug 09 05:52:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 07 02:55:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	148227	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	282192	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	254047	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	93244	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	124069	60.972	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	121.940%#
35) Dibromofluoromethane	5.385	113	101267	54.884	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	109.760%
50) Toluene-d8	8.647	98	338694	51.707	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	103.420%
62) 4-Bromofluorobenzene	11.079	95	108862	46.250	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	92.500%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080824\
Data File : VX042972.D
Acq On : 09 Aug 2024 05:16
Operator : JC/MD
Sample : P3469-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-03


Quant Time: Aug 09 05:52:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080724W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 07 02:55:22 2024
Response via : Initial Calibration

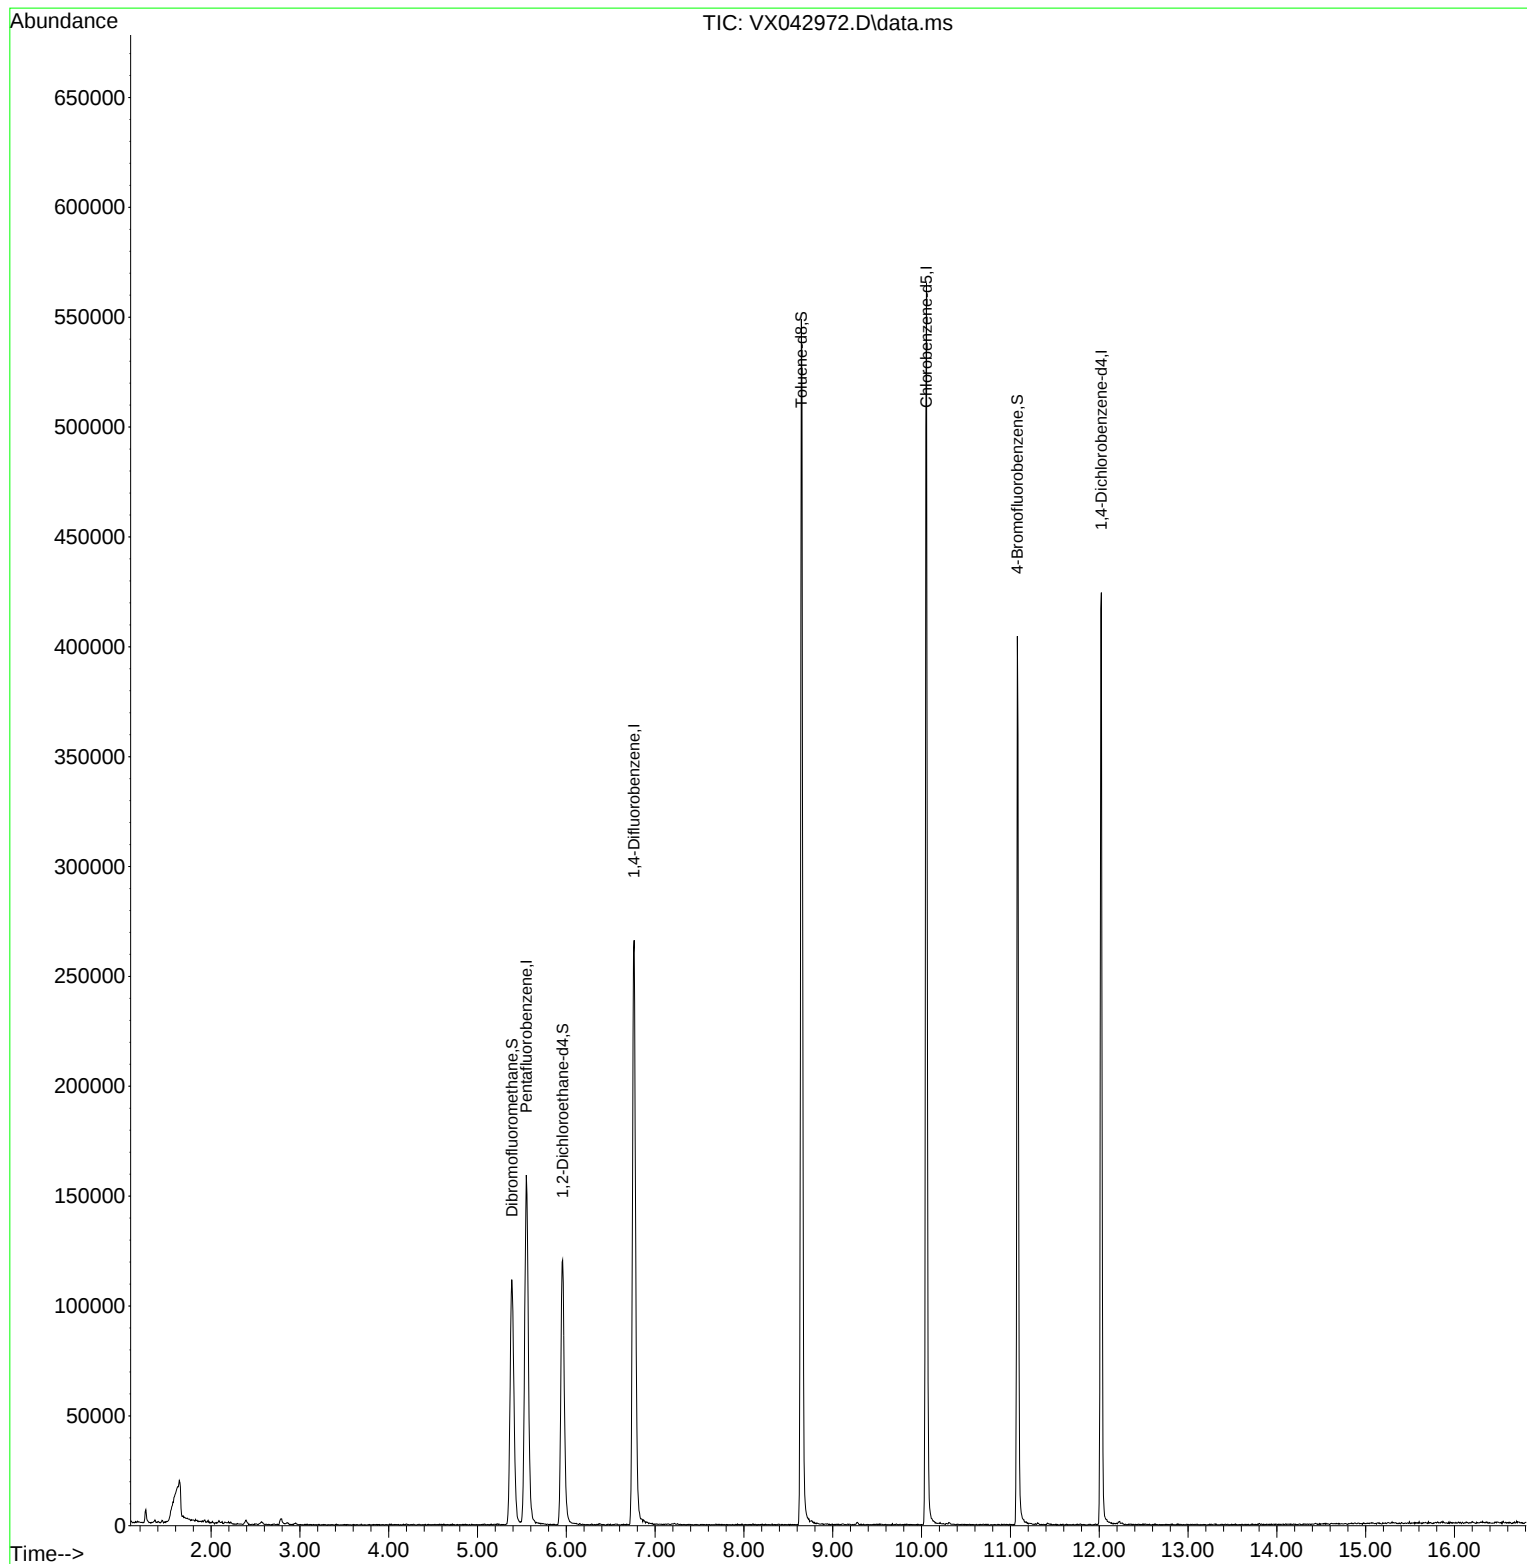



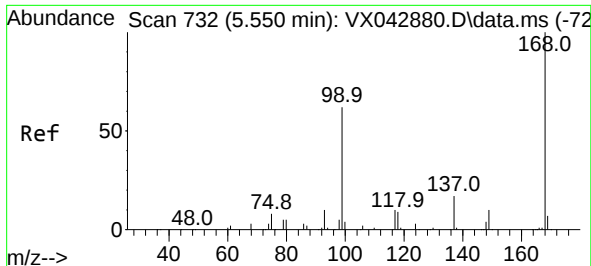


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16

Instrument :
MSVOA_X
ClientSampleId :
TB-03



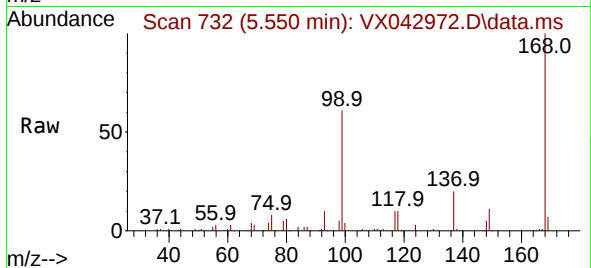



Tgt Ion:168 Resp: 148227
Ion Ratio Lower Upper
168 100
99 61.2 56.6 85.0

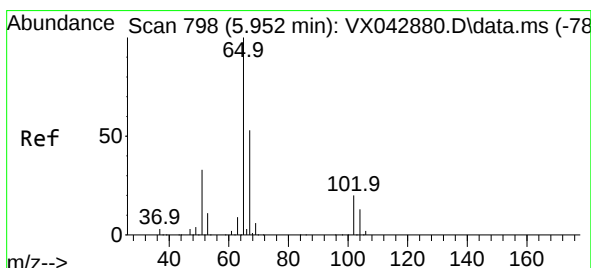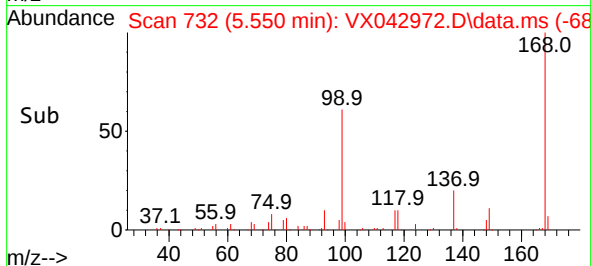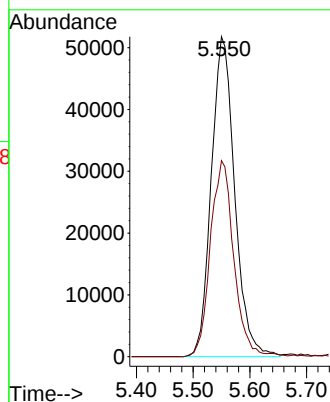

#33
1,2-Dichloroethane-d4
Concen: 60.972 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16

Tgt Ion: 65 Resp: 124069
Ion Ratio Lower Upper
65 100
67 50.9 0.0 100.2


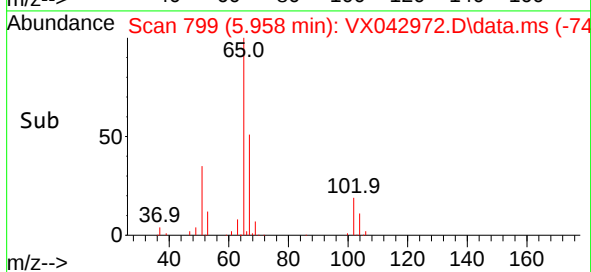
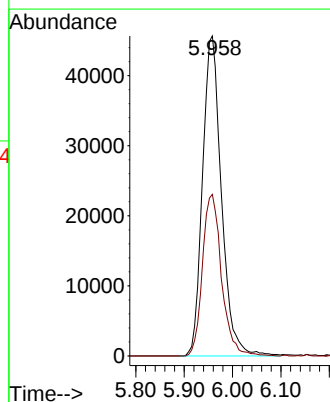
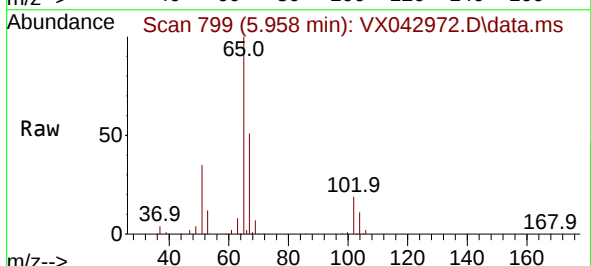


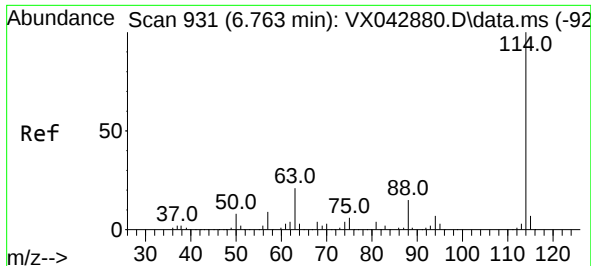

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. -0.000 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16




Instrument :
MSVOA_X
ClientSampleId :
TB-03


Tgt Ion:114 Resp: 282192
Ion Ratio Lower Upper
114 100
63 19.7 0.0 45.0
88 16.9 0.0 36.6

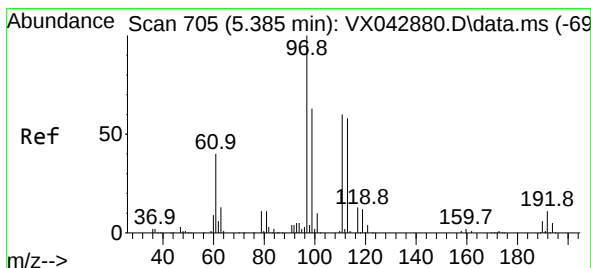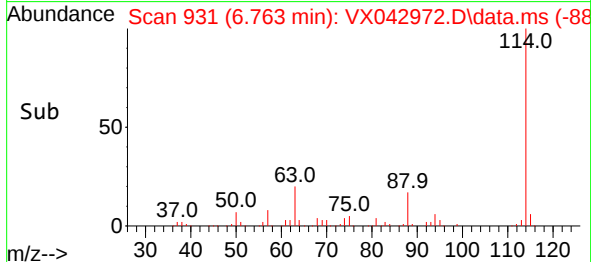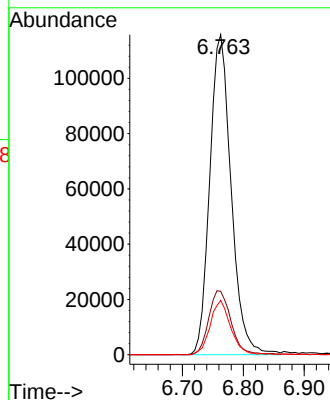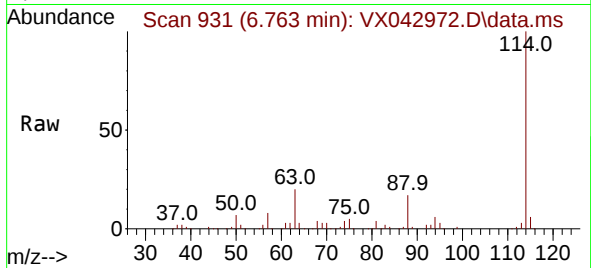

#35
Dibromofluoromethane
Concen: 54.884 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16

Tgt Ion:113 Resp: 101267
Ion Ratio Lower Upper
113 100
111 102.7 82.9 124.3
192 18.1 13.3 19.9


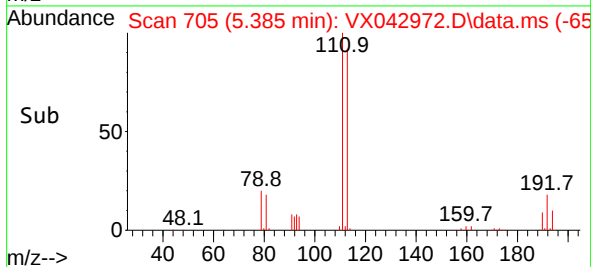
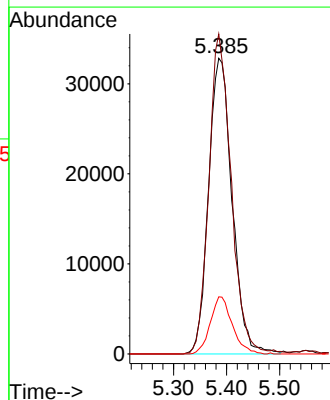
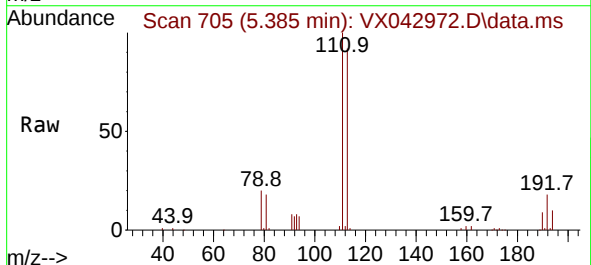


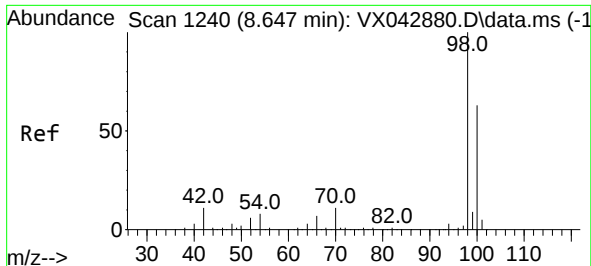

#50
Toluene-d8
Concen: 51.707 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16




Instrument :
MSVOA_X
ClientSampleId :
TB-03


Tgt Ion: 98 Resp: 338694
Ion Ratio Lower Upper
98 100
100 63.6 53.1 79.7

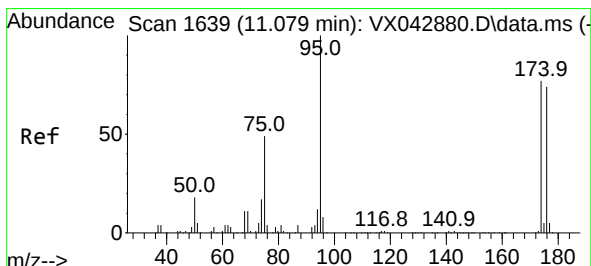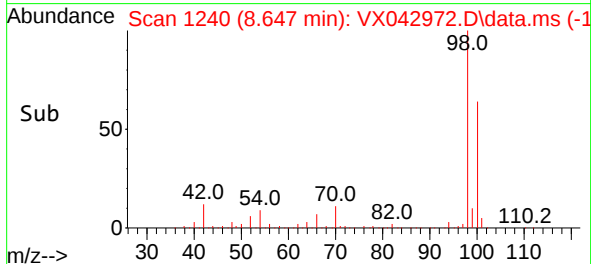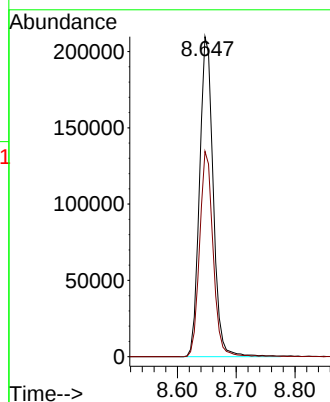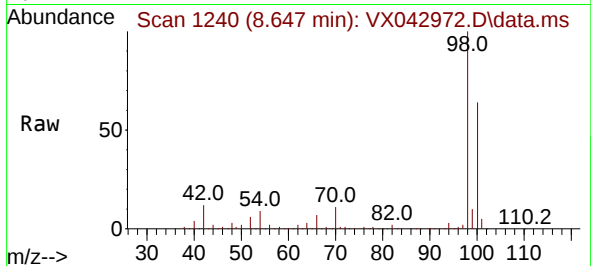

#62
4-Bromofluorobenzene
Concen: 46.250 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16

Tgt Ion: 95 Resp: 108862
Ion Ratio Lower Upper
95 100
174 79.0 0.0 135.6
176 78.2 0.0 131.0


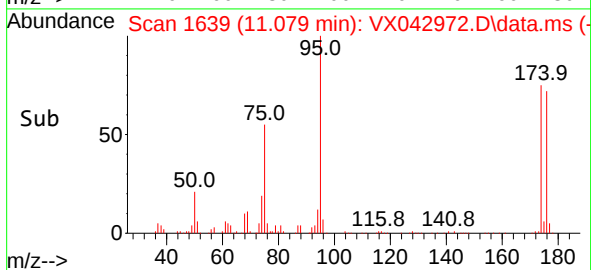
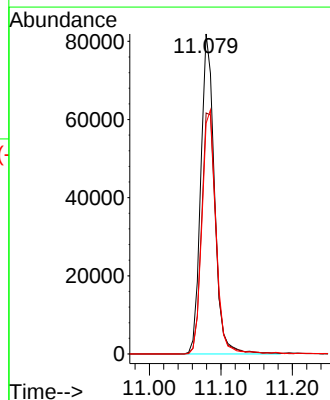
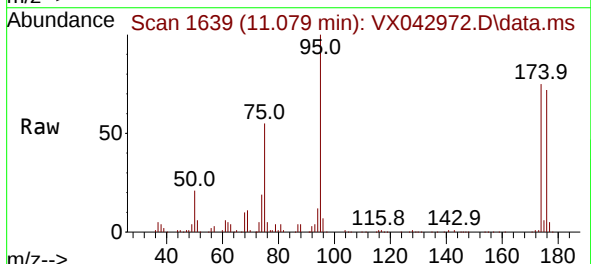


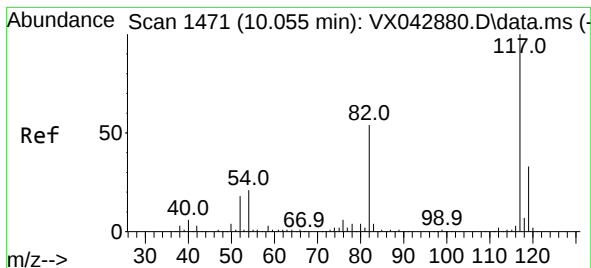

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16

Instrument :
MSVOA_X
ClientSampleId :
TB-03

Tgt Ion:117 Resp: 254047
Ion Ratio Lower Upper
117 100
82 55.2 46.2 69.4
119 32.7 25.5 38.3

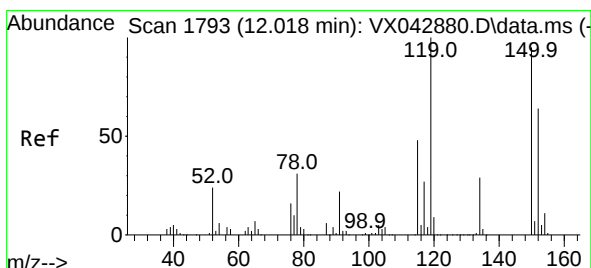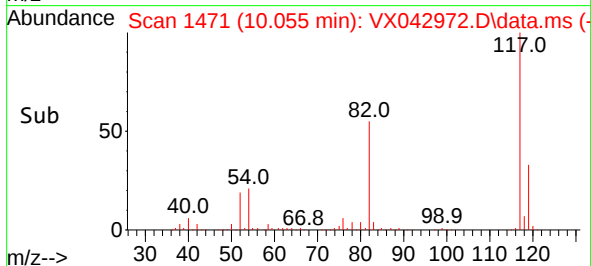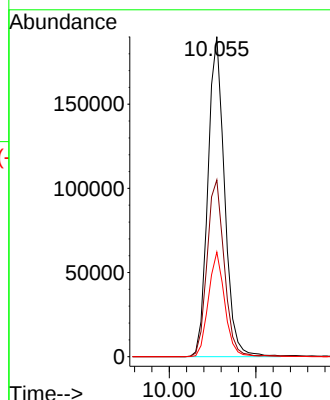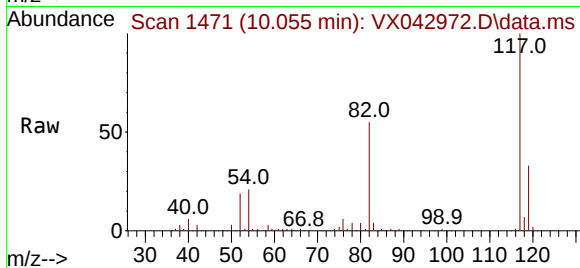

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX042972.D
Acq: 09 Aug 2024 05:16

Tgt Ion:152 Resp: 93244
Ion Ratio Lower Upper
152 100
115 63.2 43.3 129.9
150 155.8 0.0 345.0

