
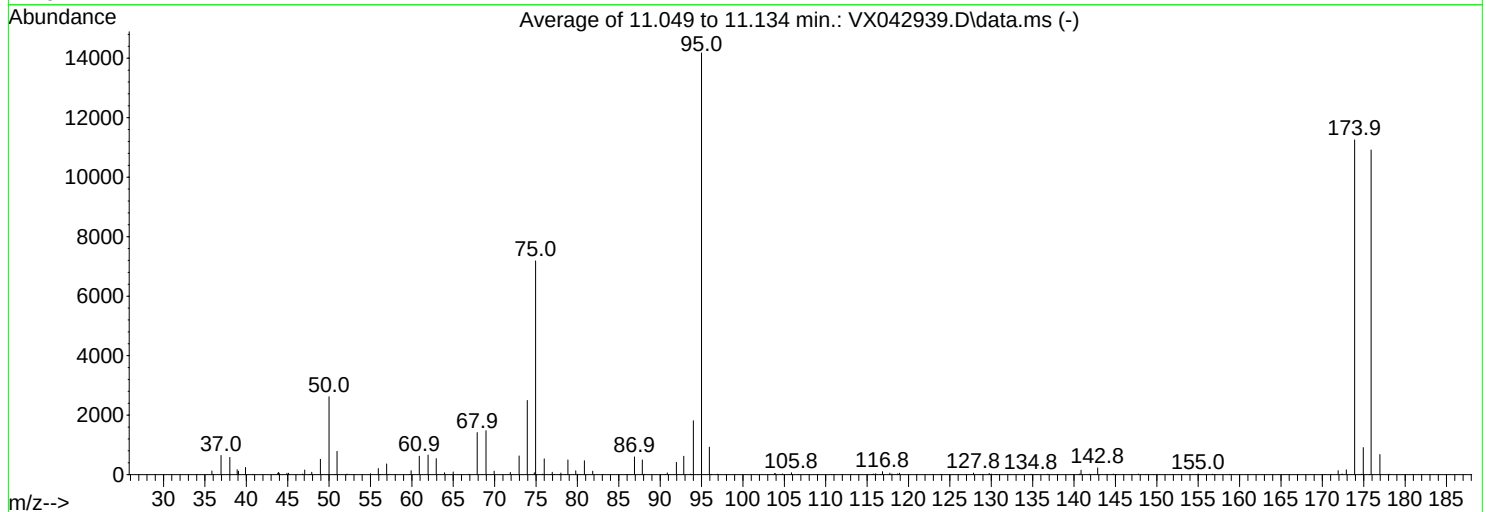


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080824\
Data File : VX042939.D
Acq On : 08 Aug 2024 08:47
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 07 04:53:59 2024

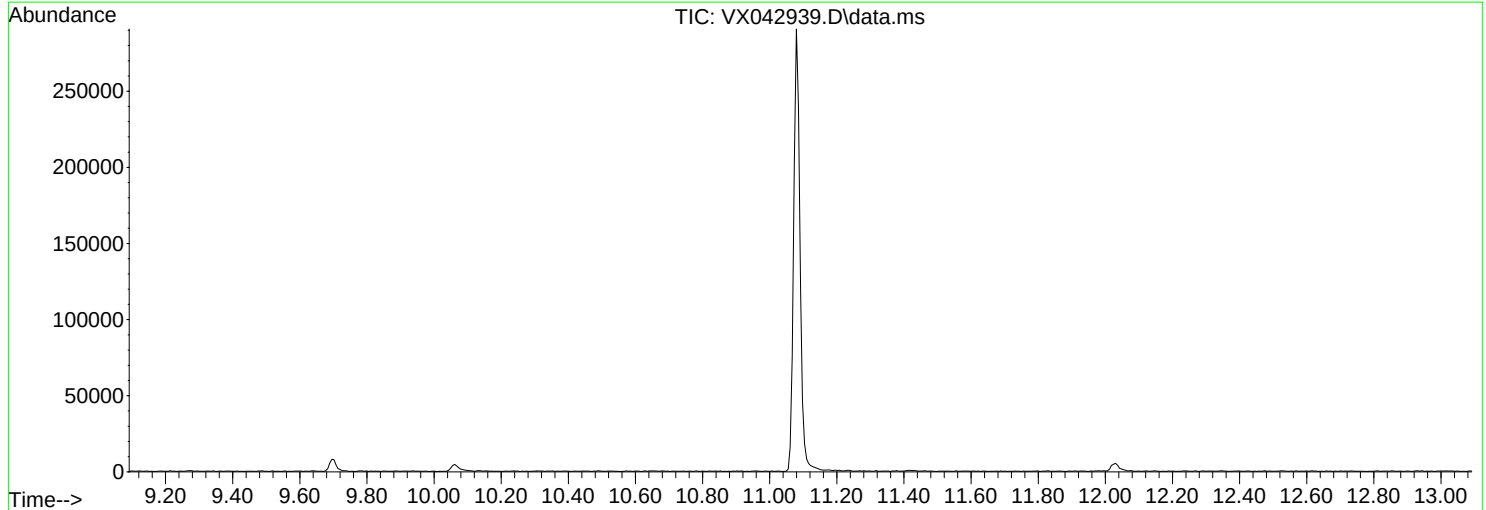

AutoFind: Averaged scan 1634 to 1648; Bkg corrected with scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	2619	PASS
75	95	30	60	50.7	7184	PASS
95	95	100	100	100.0	14180	PASS
96	95	5	9	6.5	927	PASS
173	174	0.00	2	1.4	162	PASS
174	95	50	100	79.4	11252	PASS
175	174	5	9	8.1	907	PASS
176	174	95	101	97.0	10912	PASS
177	176	5	9	6.2	679	PASS