

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080825\
 Data File : VX047277.D
 Acq On : 08 Aug 2025 17:15
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
 Title : SW846 8260

Signal : TIC: VX047277.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.806	275	282	288	rBV2	14482	27903	1.45%	0.337%
2	5.397	695	707	724	rBV2	124354	397863	20.67%	4.805%
3	5.562	724	734	754	rVB2	224787	710408	36.91%	8.579%
4	5.964	789	800	823	rBV	126857	378872	19.68%	4.575%
5	6.769	915	932	949	rBV	458242	1924808	100.00%	23.244%
6	8.653	1234	1241	1255	rBV	567312	948005	49.25%	11.448%
7	10.055	1465	1471	1483	rBV	796354	1114172	57.88%	13.455%
8	11.079	1634	1639	1651	rBV	635221	817357	42.46%	9.870%
9	12.018	1788	1793	1801	rBV	929603	1162262	60.38%	14.035%
10	12.420	1855	1859	1864	rBV	33408	38640	2.01%	0.467%
11	12.762	1909	1915	1920	rBV2	13514	21772	1.13%	0.263%
12	12.890	1929	1936	1942	rVV9	8533	22571	1.17%	0.273%
13	12.975	1946	1950	1954	rVV5	13039	20478	1.06%	0.247%
14	13.268	1994	1998	2001	rBV	51919	65314	3.39%	0.789%
15	13.384	2013	2017	2020	rBV	22033	27765	1.44%	0.335%
16	13.841	2087	2092	2096	rVV	42185	62500	3.25%	0.755%
17	14.036	2120	2124	2128	rBV	135459	141054	7.33%	1.703%
18	14.127	2136	2139	2143	rVB	15668	19607	1.02%	0.237%
19	14.408	2180	2185	2187	rBV3	11661	19351	1.01%	0.234%
20	14.499	2197	2200	2205	rVB2	22772	34936	1.82%	0.422%
21	14.560	2206	2210	2214	rVB2	14542	19446	1.01%	0.235%
22	14.609	2214	2218	2227	rBV	37616	50159	2.61%	0.606%
23	14.755	2237	2242	2245	rBV	108802	127856	6.64%	1.544%
24	15.207	2313	2316	2320	rBV3	17197	20651	1.07%	0.249%
25	15.365	2338	2342	2348	rBV7	14981	25201	1.31%	0.304%
26	15.487	2356	2362	2367	rVB2	32759	49949	2.60%	0.603%
27	15.609	2378	2382	2386	rBV2	19065	31986	1.66%	0.386%




Sum of corrected areas: 8280886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080825\
Data File : VX047277.D
Acq On : 08 Aug 2025 17:15
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

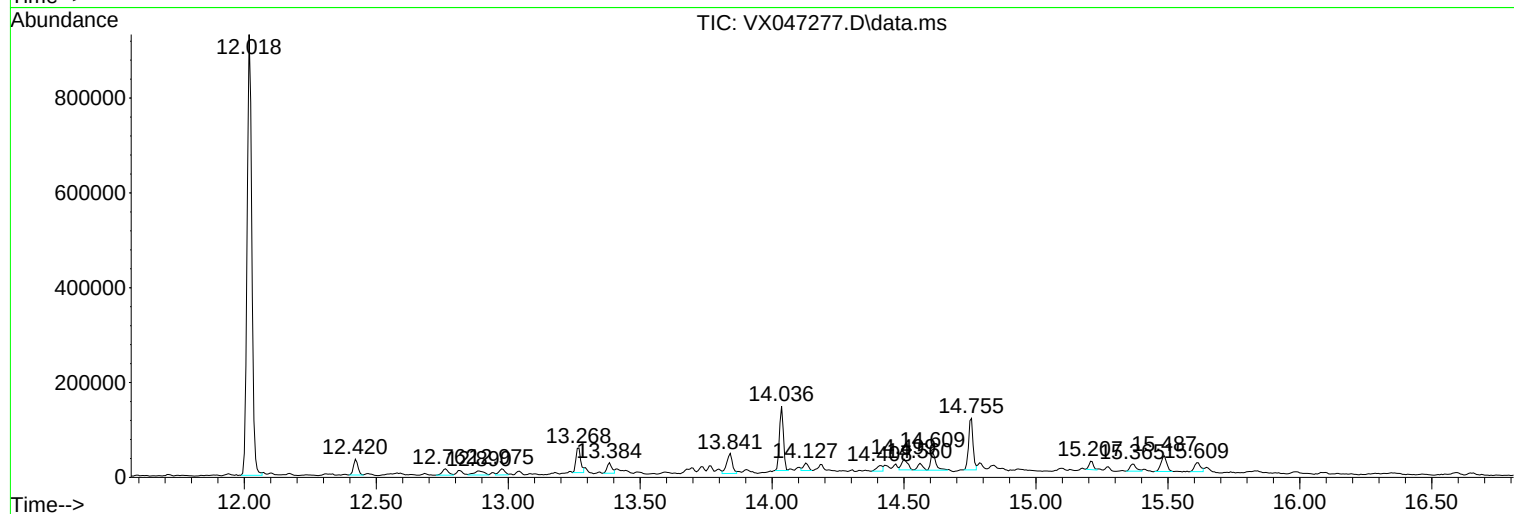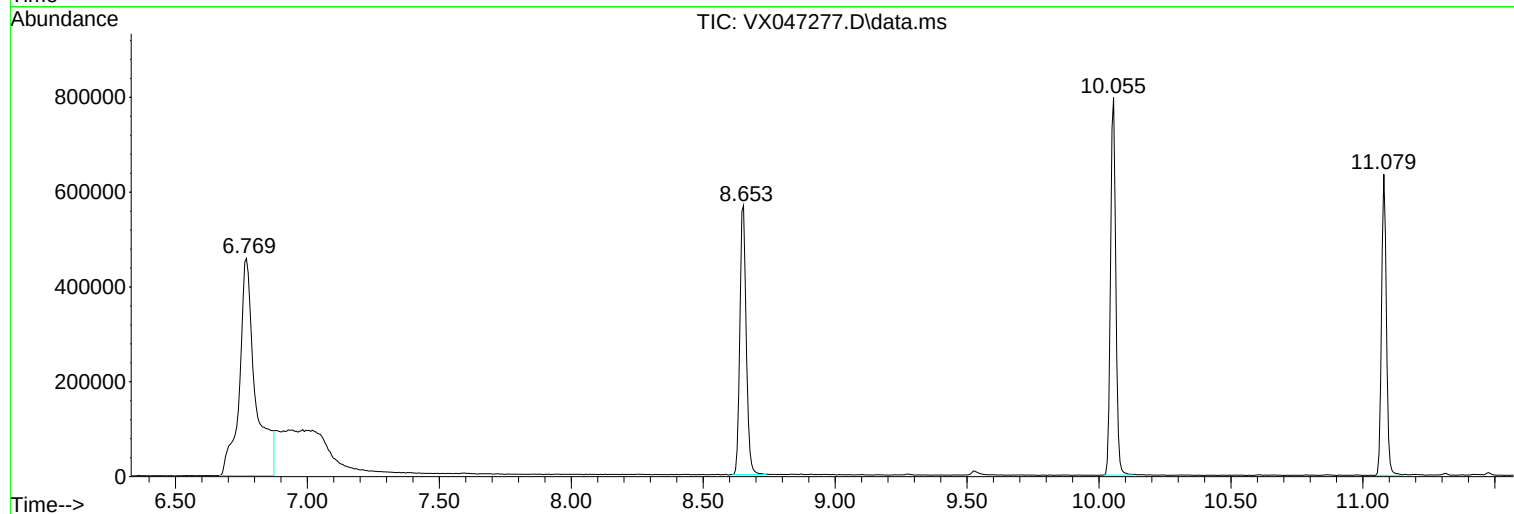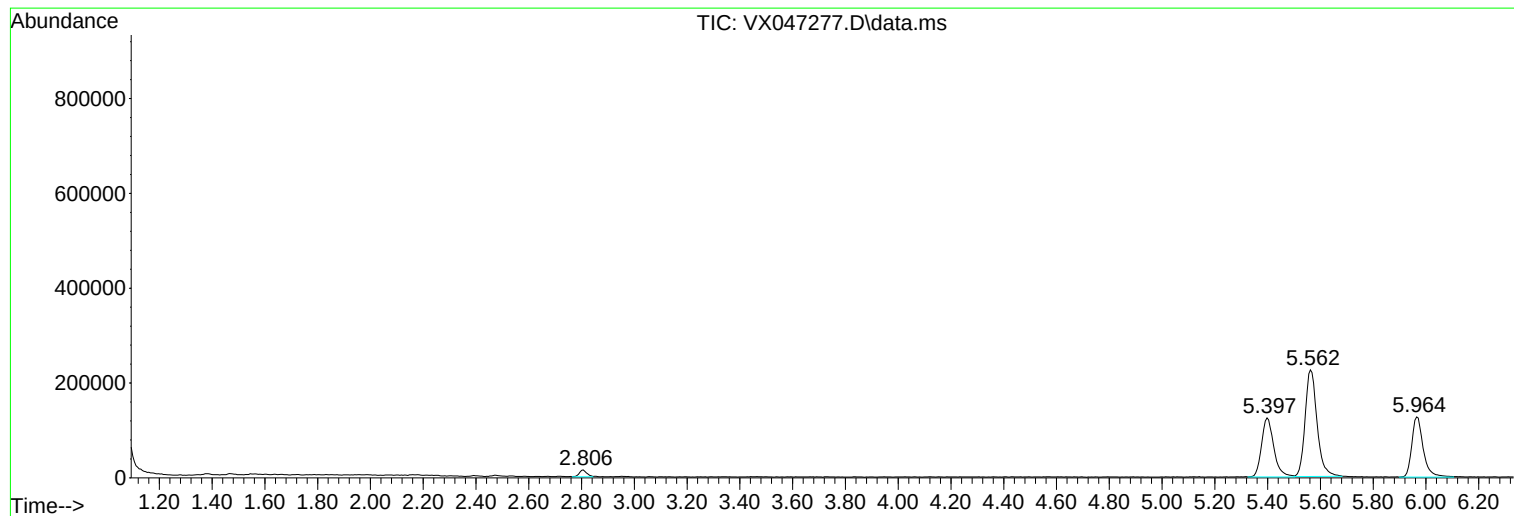

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080825\
Data File : VX047277.D
Acq On : 08 Aug 2025 17:15
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080825\
Data File : VX047277.D
Acq On : 08 Aug 2025 17:15
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------