


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX080918\
Data File : VX003939.D
Acq On : 09 Aug 2018 09:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080618W.M
Title : SW846 8260
Last Update : Tue Aug 07 07:45:48 2018

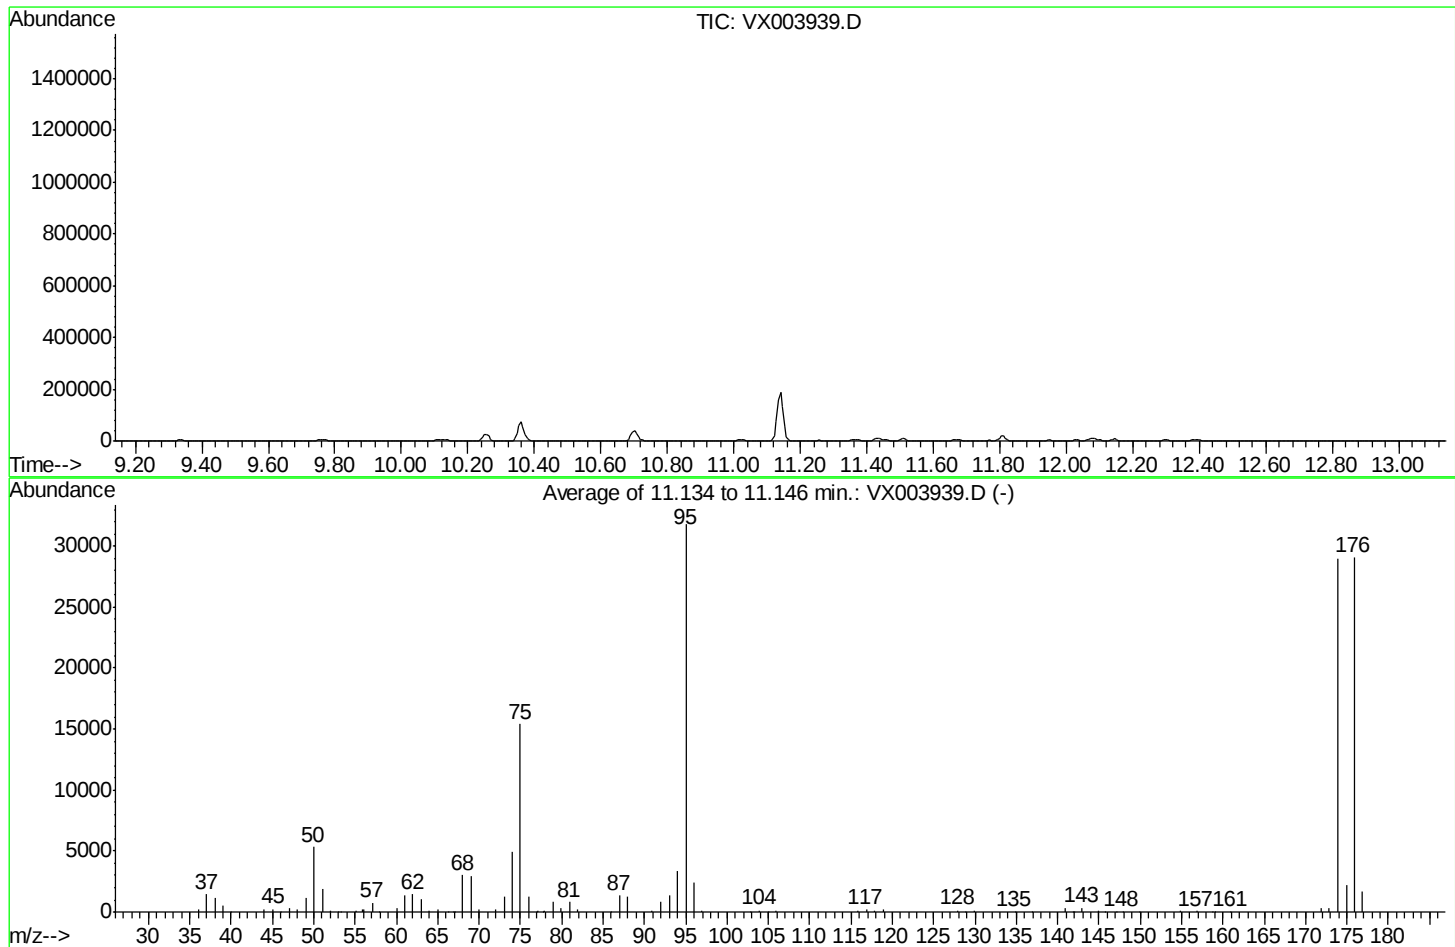

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	5337	PASS
75	95	30	60	48.5	15413	PASS
95	95	100	100	100.0	31776	PASS
96	95	5	9	7.4	2366	PASS
173	174	0.00	2	1.0	276	PASS
174	95	50	100	91.1	28949	PASS
175	174	5	9	7.7	2223	PASS
176	174	95	101	100.3	29050	PASS
177	176	5	9	5.8	1689	PASS