

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX080919\
 Data File : VX011415.D
 Acq On : 09 Aug 2019 17:15
 Operator : JC/SP
 Sample : K4278-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-TB-2019-5

Quant Time: Aug 11 00:03:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 02 01:55:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	216403	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	315983	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	274250	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	128657	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	112599	51.67	ug/l	0.00
Spiked Amount			Recovery	=	103.34%	
35) Dibromofluoromethane	5.49	113	94982	46.04	ug/l	0.00
Spiked Amount			Recovery	=	92.08%	
50) Toluene-d8	8.71	98	361239	46.39	ug/l	0.00
Spiked Amount			Recovery	=	92.78%	
62) 4-Bromofluorobenzene	11.13	95	123140	44.29	ug/l	0.00
Spiked Amount			Recovery	=	88.58%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.64	94	964	0.655	ug/l	91
6) Chloroethane	1.68	64	171	Below Cal	#	51
10) Methyl Iodide	2.51	142	1380	0.551	ug/l #	90
11) Tert butyl alcohol	3.02	59	181	0.439	ug/l #	72
13) Acrolein	2.28	56	317	0.753	ug/l #	78
15) Acrylonitrile	3.14	53	757	0.730	ug/l #	68
16) Acetone	2.43	43	834	0.804	ug/l #	79
17) Carbon Disulfide	2.57	76	2116	0.458	ug/l #	89
20) Methylene Chloride	2.85	84	495	0.218	ug/l #	77
21) trans-1,2-Dichloroethene	3.17	96	535	0.257	ug/l	95
29) Tetrahydrofuran	5.12	42	190	0.210	ug/l #	36
38) Carbon Tetrachloride	5.65	117	20515	7.391	ug/l #	15
39) Methylcyclohexane	7.46	83	773	0.236	ug/l #	81
40) Benzene	6.13	78	1674	0.203	ug/l	98
53) t-1,3-Dichloropropene	9.05	75	316	2.936	ug/l #	43
64) Tetrachloroethene	9.33	164	481	0.207	ug/l #	64
67) Ethyl Benzene	10.25	91	4277	0.434	ug/l	92
76) 1,2,3-Trichloropropane	11.13	75	61348	26.184	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.13	75	61348	68.114	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	3182	0.434	ug/l	100
93) 1,2,4-Trichlorobenzene	13.65	180	842	0.293	ug/l	81
94) Hexachlorobutadiene	13.77	225	296	0.203	ug/l	77
95) Naphthalene	13.83	128	4324	0.515	ug/l #	91
96) 1,2,3-Trichlorobenzene	14.02	180	778	0.266	ug/l	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX080919\
Data File : VX011415.D
Acq On : 09 Aug 2019 17:15
Operator : JC/SP
Sample : K4278-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-TB-2019-5

Quant Time: Aug 11 00:03:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 02 01:55:00 2019
Response via : Initial Calibration

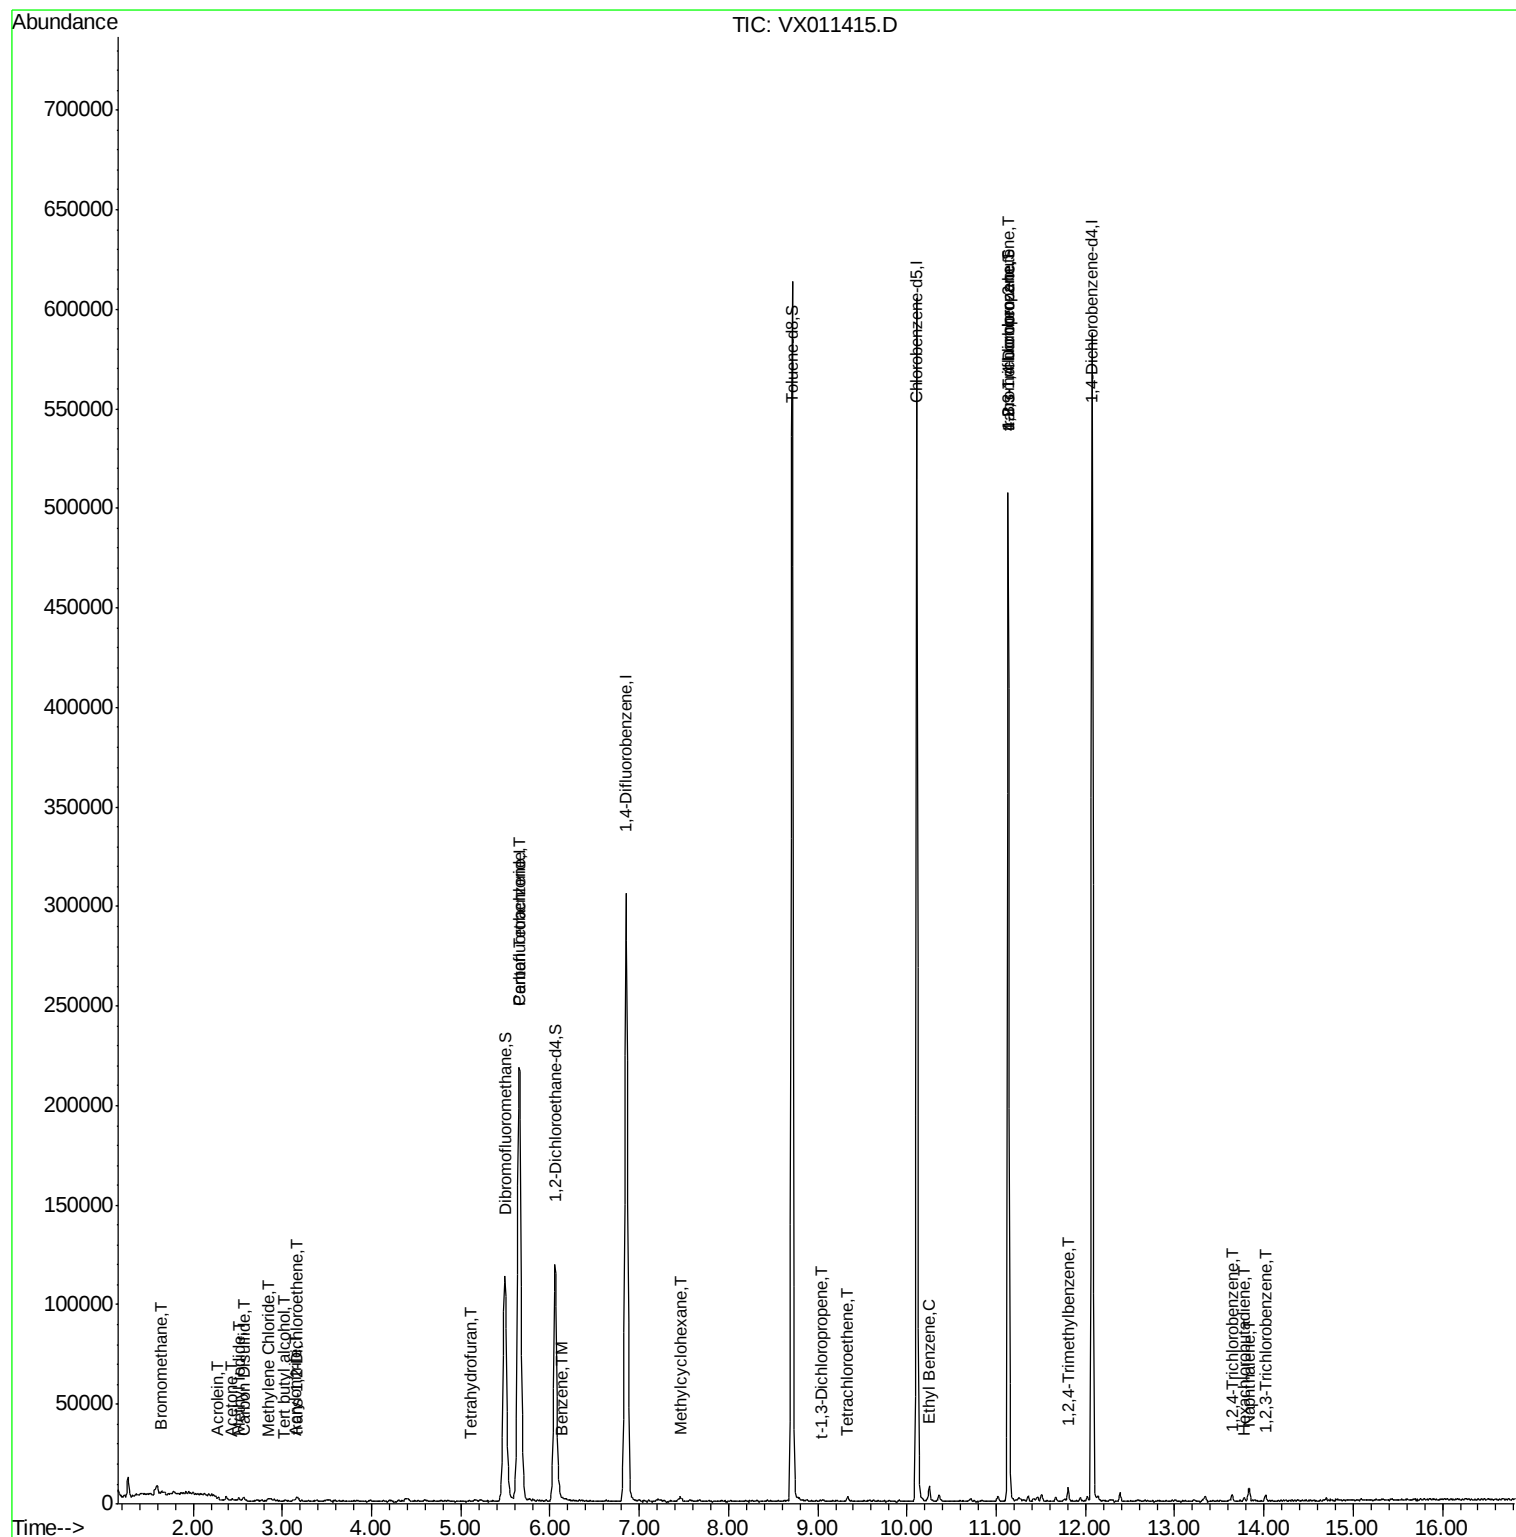



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 738

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :


Z3-TB-2019-5

Tgt Ion:168 Resp: 216403

Ion Ratio Lower Upper




168 100

99 52.9 38.5 57.7

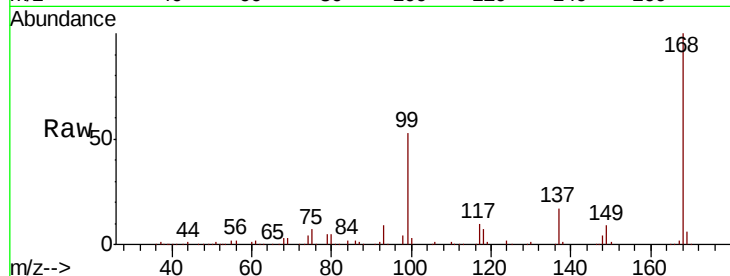

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

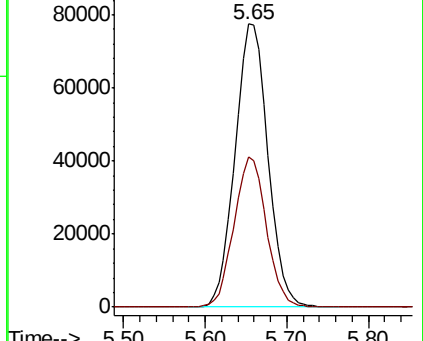

#5

Bromomethane

Concen: 0.655 ug/l

RT: 1.64 min Scan# 80

Delta R.T. 0.01 min

Lab File: VX011415.D


Acq: 09 Aug 2019 17:15

Tgt Ion: 94 Resp: 964

Ion Ratio Lower Upper



94 100


96 84.5 74.6 112.0



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

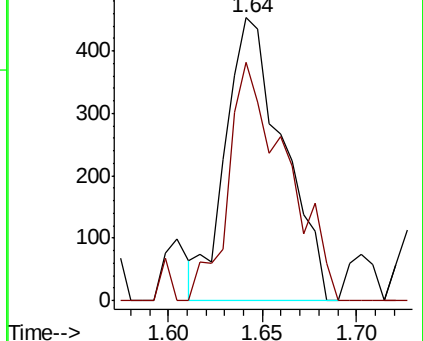



#6

Chloroethane

Concen: Below Cal

RT: 1.68 min Scan# 87

Delta R.T. -0.03 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :


Z3-TB-2019-5

Tgt Ion: 64 Resp: 171

Ion Ratio Lower Upper




64 100

66 58.6 25.1 37.7#

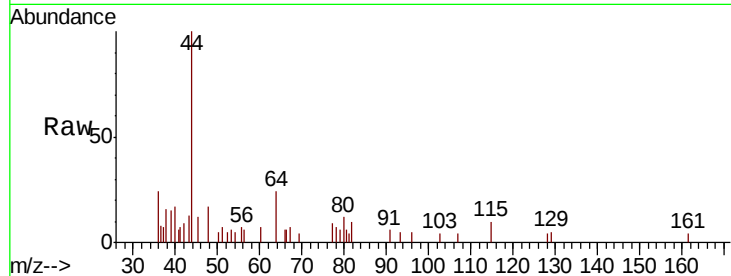

Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

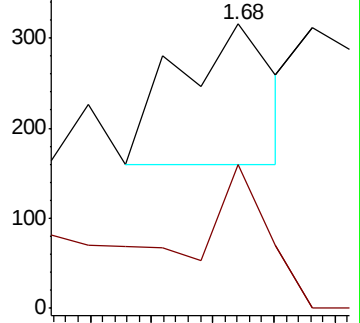

#10

Methyl Iodide

Concen: 0.551 ug/l

RT: 2.51 min Scan# 223

Delta R.T. 0.01 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15


Tgt Ion: 142 Resp: 1380

Ion Ratio Lower Upper

142 100

127 48.2 33.8 50.8



141 8.7 11.4 17.2#




Abundance Ion 141.80 (141.50 to 142.50): V

Ion 126.80 (126.50 to 127.50): V

Ion 140.80 (140.50 to 141.50): V




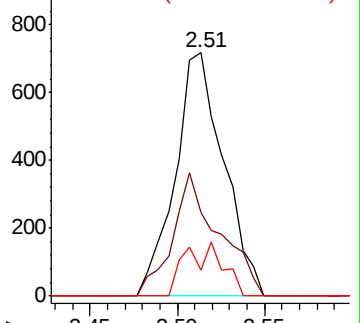




#11
Tert butyl alcohol
Concen: 0.439 ug/l
RT: 3.02 min Scan# 306
Delta R.T. -0.02 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15




Instrument :
MSVOA_X
ClientSampleId :
Z3-TB-2019-5


Tgt Ion: 59 Resp: 181
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

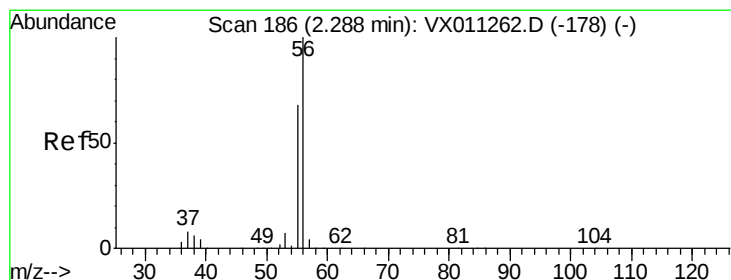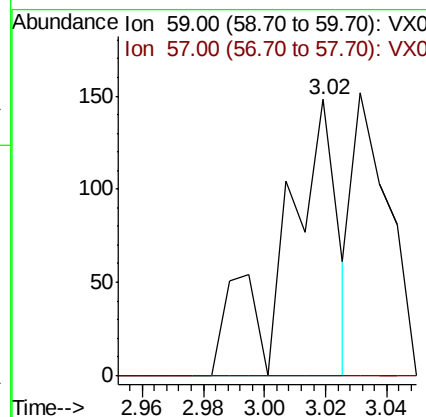

#13
Acrolein
Concen: 0.753 ug/l
RT: 2.28 min Scan# 185
Delta R.T. -0.01 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Tgt Ion: 56 Resp: 317
Ion Ratio Lower Upper
56 100
55 52.1 56.0 84.0#

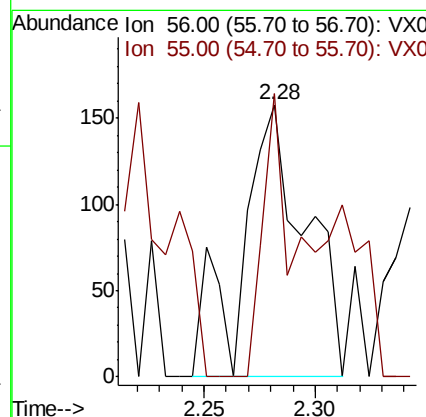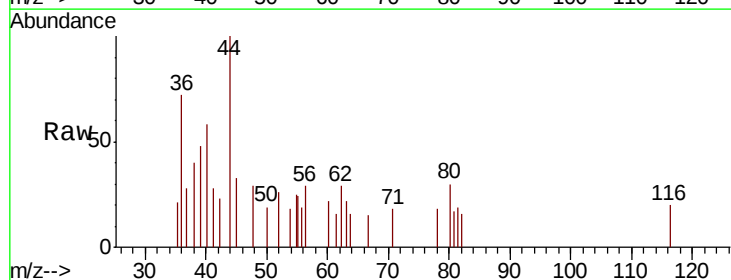



#15

Acrylonitrile

Concen: 0.730 ug/l

RT: 3.14 min Scan# 326

Delta R.T. 0.01 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampled :

Z3-TB-2019-5





Tgt Ion: 53 Resp: 757

Ion Ratio Lower Upper

53 100

52 53.8 65.5 98.3#

51 53.8 27.9 41.9#

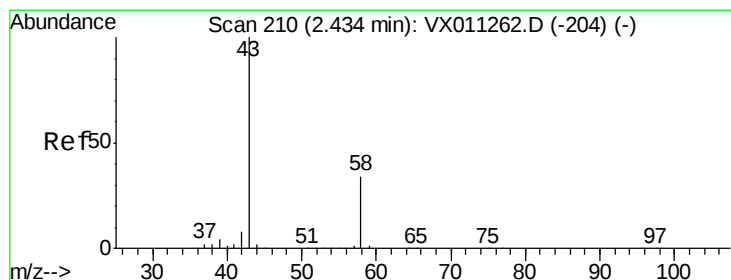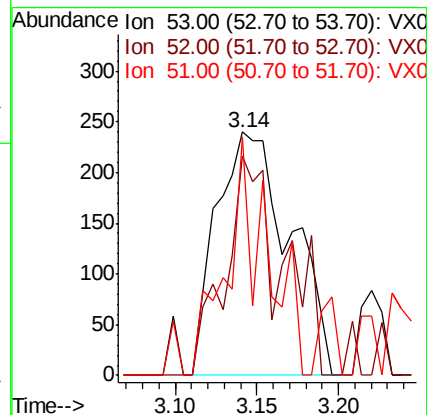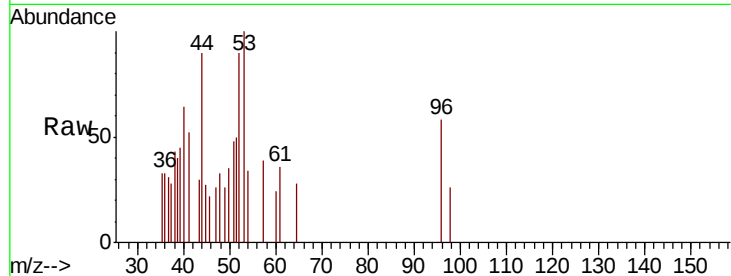

#16

Acetone

Concen: 0.804 ug/l

RT: 2.43 min Scan# 209

Delta R.T. -0.01 min

Lab File: VX011415.D




Acq: 09 Aug 2019 17:15


Tgt Ion: 43 Resp: 834

Ion Ratio Lower Upper

43 100

58 22.2 27.4 41.0#

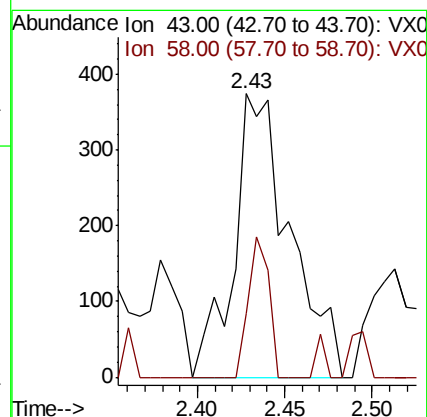



#17

Carbon Disulfide

Concen: 0.458 ug/l

RT: 2.57 min Scan# 232

Delta R.T. 0.01 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampled :


Z3-TB-2019-5

Tgt Ion: 76 Resp: 2116

Ion Ratio Lower Upper




76 100

78 13.2 7.4 11.0#

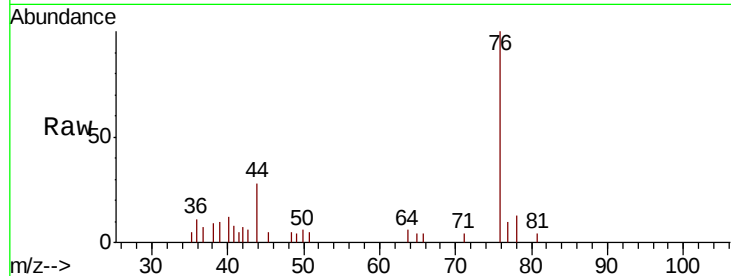

Abundance Ion 75.90 (75.60 to 76.60): VX0

Ion 77.90 (77.60 to 78.60): VX0

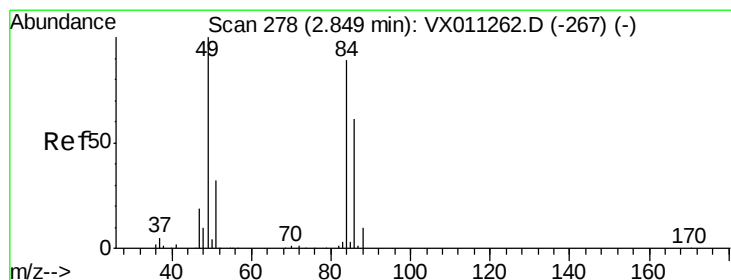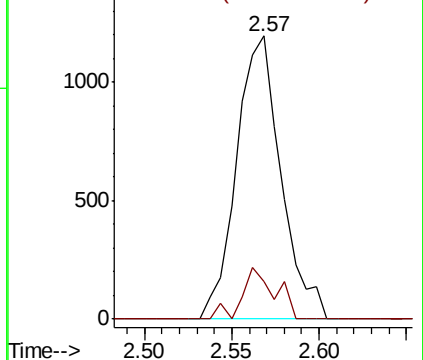

#20

Methylene Chloride

Concen: 0.218 ug/l

RT: 2.85 min Scan# 279

Delta R.T. 0.01 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Tgt Ion: 84 Resp: 495


Ion Ratio Lower Upper

84 100

49 85.0 89.3 133.9#

51 38.9 28.3 42.5

86 91.0 54.5 81.7#






Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

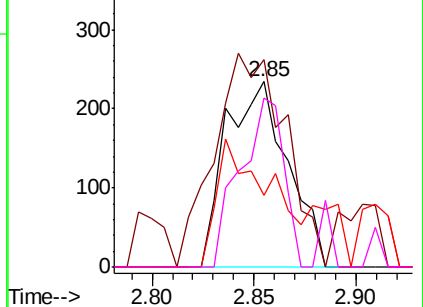

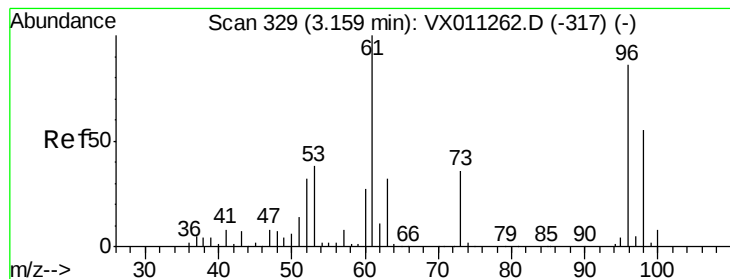

#21

trans-1,2-Dichloroethene

Concen: 0.257 ug/l

RT: 3.17 min Scan# 330

Delta R.T. 0.01 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampled :

Z3-TB-2019-5


Tgt Ion: 96 Resp: 535

Ion Ratio Lower Upper

96 100

61 123.8 92.8 139.2




98 64.5 51.2 76.8



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

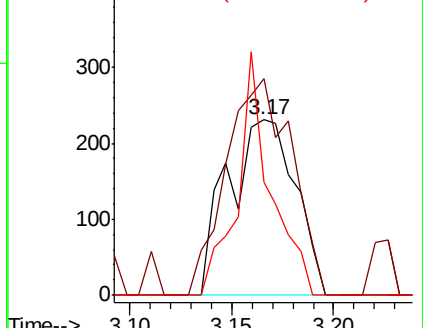

#29

Tetrahydrofuran

Concen: 0.210 ug/l

RT: 5.12 min Scan# 650

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15


Tgt Ion: 42 Resp: 190

Ion Ratio Lower Upper

42 100

72 10.0 39.9 59.9#



71 0.0 36.9 55.3#




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0

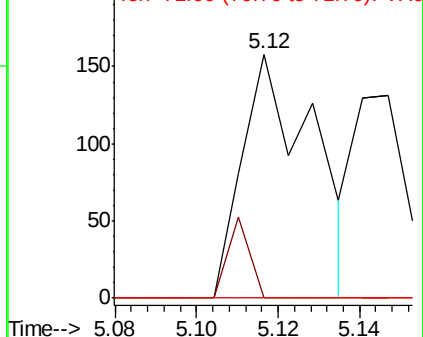

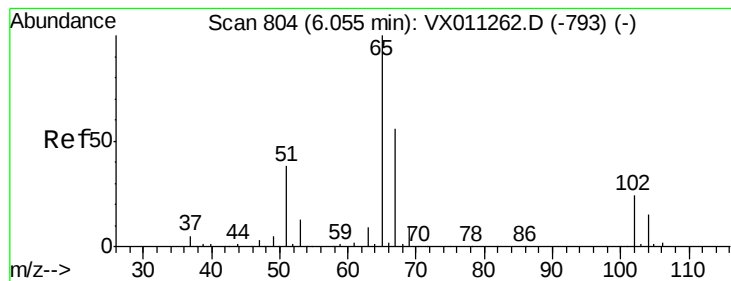

#33

1,2-Dichloroethane-d4

Concen: 51.668 ug/l

RT: 6.06 min Scan# 804

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :


Z3-TB-2019-5

Tgt Ion: 65 Resp: 112599

Ion Ratio Lower Upper

65 100

67 51.6 0.0 110.6



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.06

40000

30000



20000

10000

0

Time-->

5.90 6.00 6.10 6.20

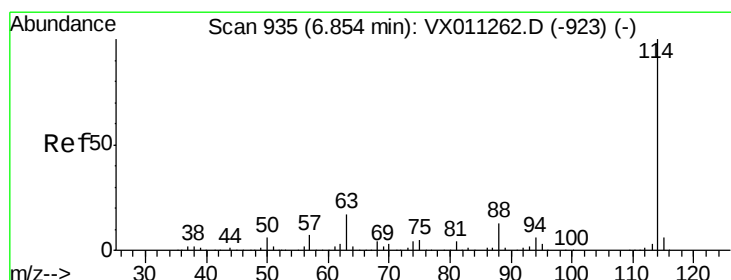

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15


Tgt Ion: 114 Resp: 315983

Ion Ratio Lower Upper

114 100

63 18.3 0.0 34.0

88 14.3 0.0 26.4

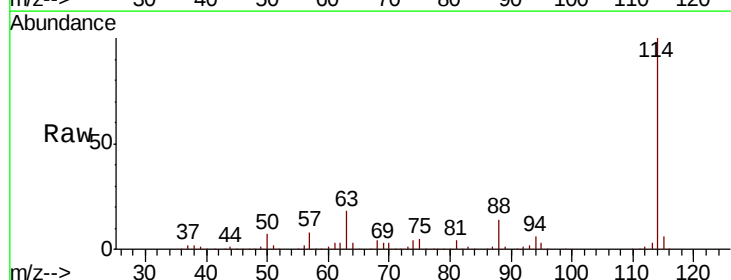

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

6.85

150000


100000


50000

0

Time-->

6.70 6.80 6.90 7.00



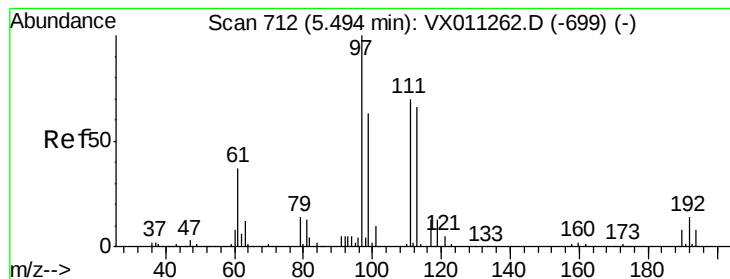

#35

Dibromofluoromethane

Concen: 46.041 ug/l

RT: 5.49 min Scan# 712

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :

Z3-TB-2019-5


Tgt Ion:113 Resp: 94982

Ion Ratio Lower Upper

113 100

111 101.6 81.9 122.9




192 21.7 17.8 26.8



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

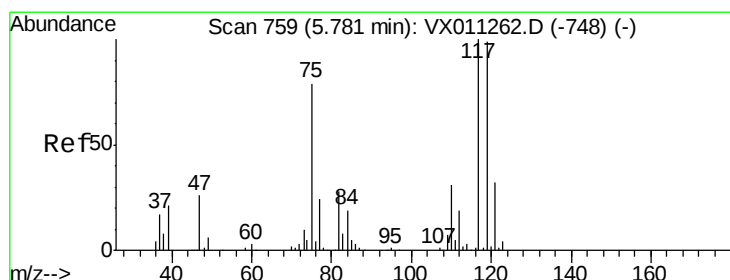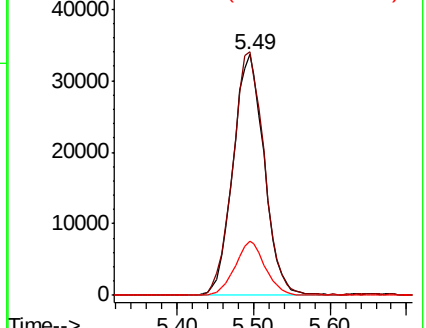

#38

Carbon Tetrachloride

Concen: 7.391 ug/l

RT: 5.65 min Scan# 738

Delta R.T. -0.13 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15


Tgt Ion:117 Resp: 20515

Ion Ratio Lower Upper

117 100

119 5.2 79.0 118.4#



121 0.0 25.9 38.9#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V




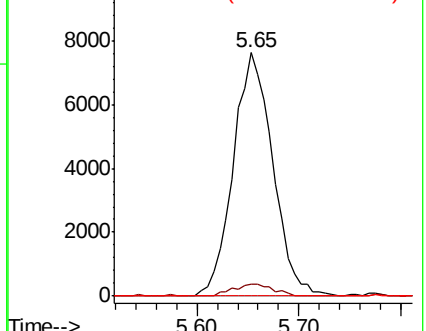


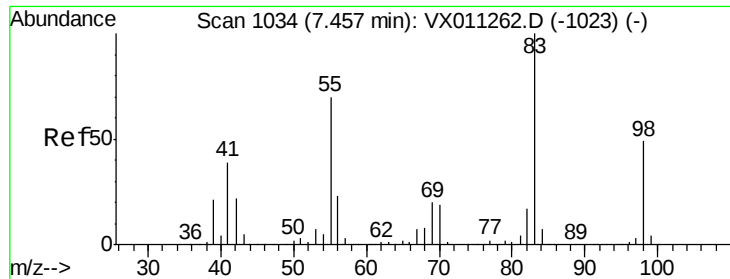

#39
Methylcyclohexane
Concen: 0.236 ug/l
RT: 7.46 min Scan# 1035
Delta R.T. 0.01 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15




Instrument :
MSVOA_X
ClientSampleId :
Z3-TB-2019-5


Tgt Ion: 83 Resp: 773
Ion Ratio Lower Upper
83 100
55 77.0 56.1 84.1
98 24.7 39.0 58.4#

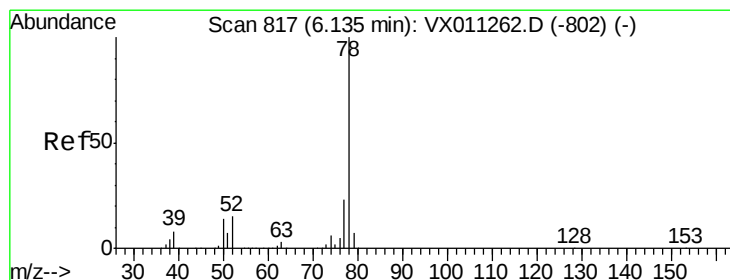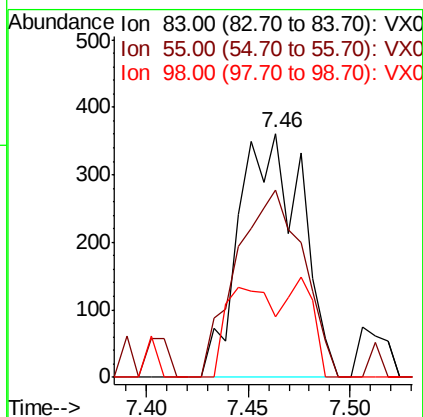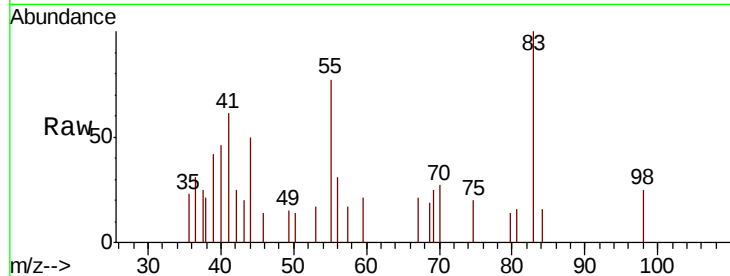

#40
Benzene
Concen: 0.203 ug/l
RT: 6.13 min Scan# 817
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Tgt Ion: 78 Resp: 1674
Ion Ratio Lower Upper
78 100
77 21.7 18.2 27.2



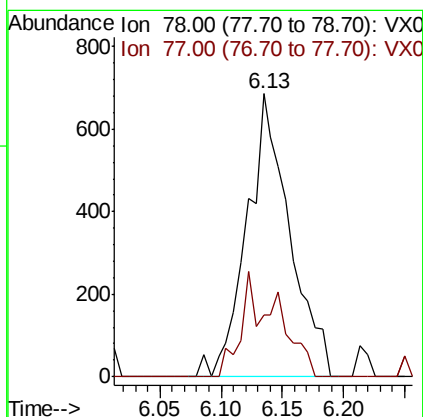



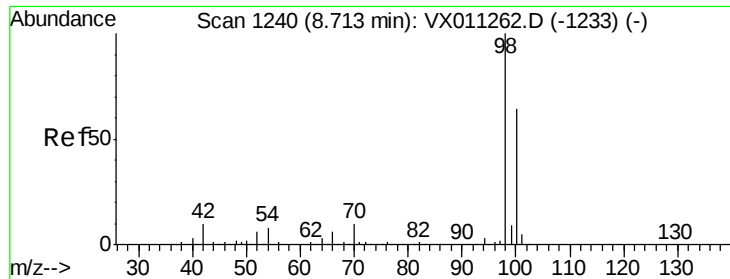

#50
Toluene-d8
Concen: 46.389 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15




Instrument :
MSVOA_X
ClientSampled :
Z3-TB-2019-5


Tgt Ion: 98 Resp: 361239
Ion Ratio Lower Upper
98 100
100 64.4 51.7 77.5

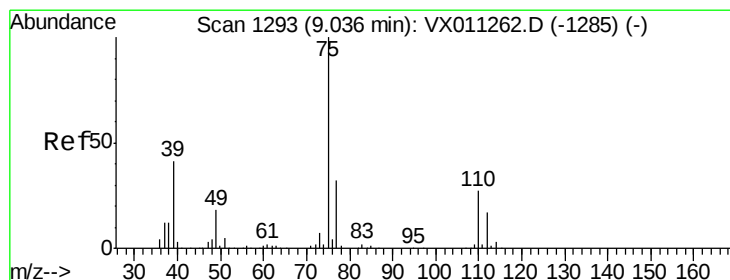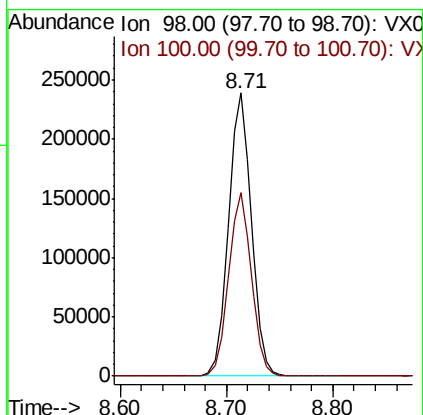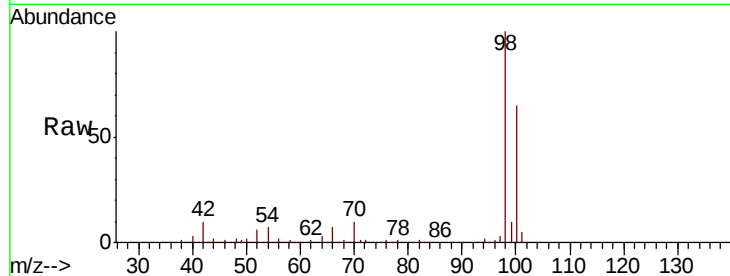

#53
t-1,3-Dichloropropene
Concen: 2.936 ug/l
RT: 9.05 min Scan# 1296
Delta R.T. 0.02 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Tgt Ion: 75 Resp: 316
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#



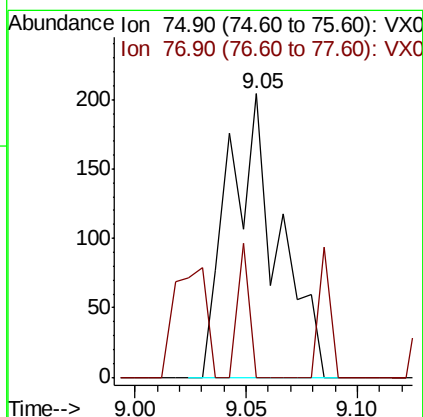





#62
4-Bromofluorobenzene
Concen: 44.291 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15




Instrument :
MSVOA_X
ClientSampleId :
Z3-TB-2019-5


Tgt Ion	Ratio	Lower	Upper
95	100		
174	91.6	0.0	191.2
176	87.9	0.0	184.8

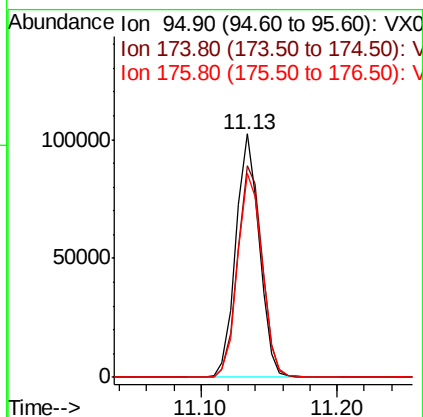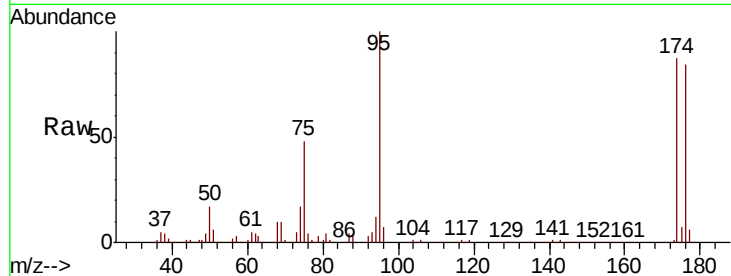

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Tgt Ion	Ratio	Lower	Upper
117	100		
82	52.6	42.2	63.2
119	32.1	26.6	39.8

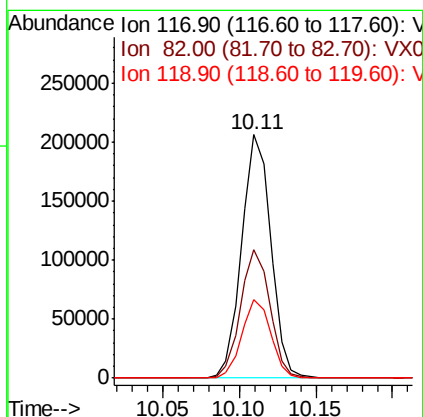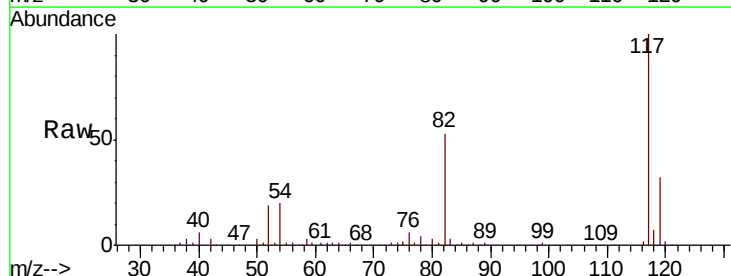



#64

Tetrachloroethene

Concen: 0.207 ug/l

RT: 9.33 min Scan# 1341

Delta R.T. -0.01 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :

Z3-TB-2019-5

Tgt Ion:164 Resp: 481


Ion Ratio Lower Upper

164 100

166 83.1 107.5 161.3#

129 54.9 71.0 106.4#

131 62.8 69.8 104.6#



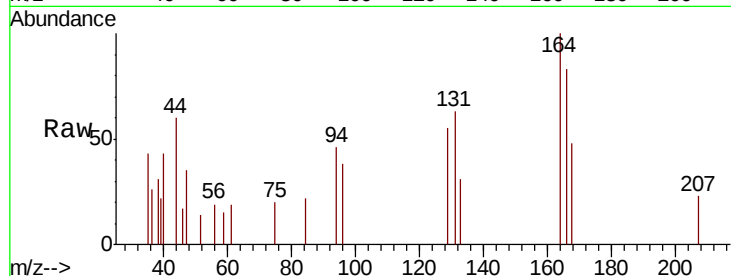


Abundance Ion 163.80 (163.50 to 164.50): V

Ion 165.80 (165.50 to 166.50): V

Ion 128.80 (128.50 to 129.50): V

Ion 130.80 (130.50 to 131.50): V

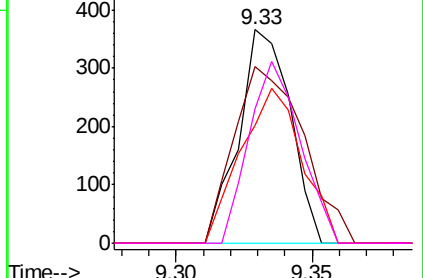

#67

Ethyl Benzene

Concen: 0.434 ug/l

RT: 10.25 min Scan# 1492

Delta R.T. -0.00 min

Lab File: VX011415.D


Acq: 09 Aug 2019 17:15

Tgt Ion: 91 Resp: 4277

Ion Ratio Lower Upper



91 100


106 37.3 26.2 39.4



Abundance Ion 91.00 (90.70 to 91.70): VX0

Ion 106.00 (105.70 to 106.70): V

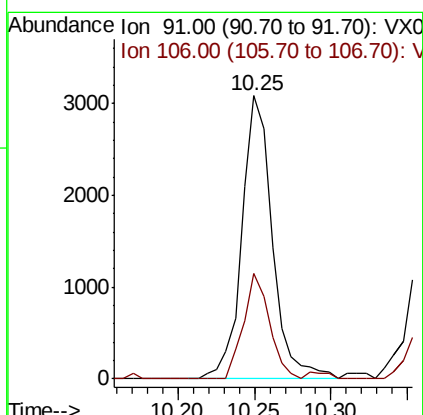

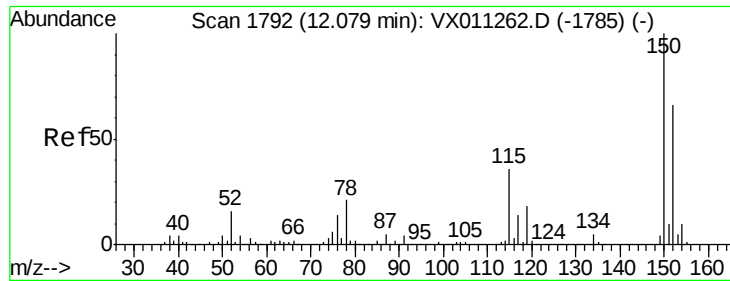


#72




1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Instrument :
MSVOA_X
ClientSampleId :
Z3-TB-2019-5

Tgt Ion:152 Resp: 128657
Ion Ratio Lower Upper
152 100
115 56.0 40.0 119.9
150 157.0 0.0 350.4

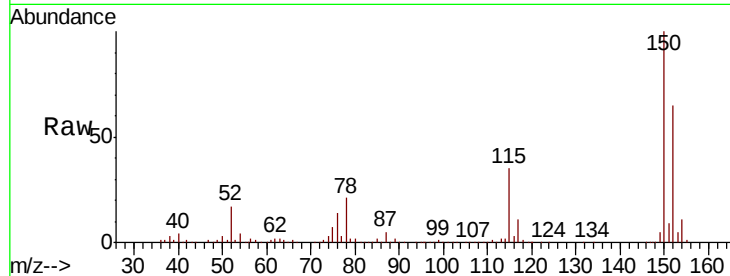


Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

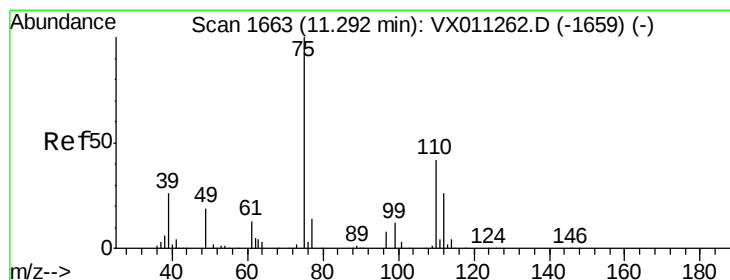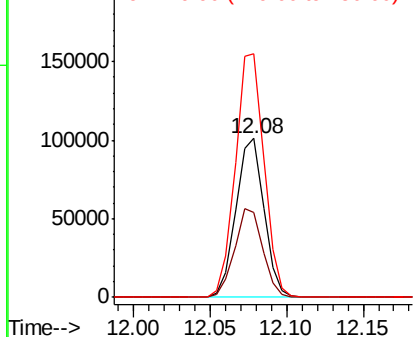



#76


1,2,3-Trichloropropane
Concen: 26.184 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.16 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Tgt Ion: 75 Resp: 61348
Ion Ratio Lower Upper
75 100
77 1.4 21.1 63.4#



Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 77.00 (76.70 to 77.70): VX0

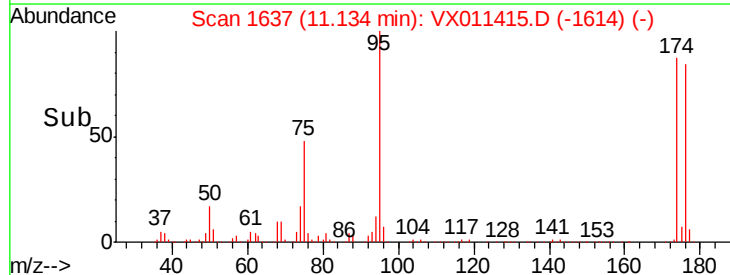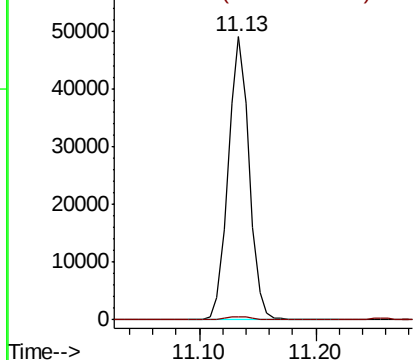



#81

trans-1,4-Dichloro-2-butene

Concen: 68.114 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :

Z3-TB-2019-5


Tgt Ion: 75 Resp: 61348

Ion Ratio Lower Upper

75 100

53 0.1 78.2 117.4#




89 0.0 37.9 56.9#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 53.00 (52.70 to 53.70): VX0

Ion 88.90 (88.60 to 89.60): VX0

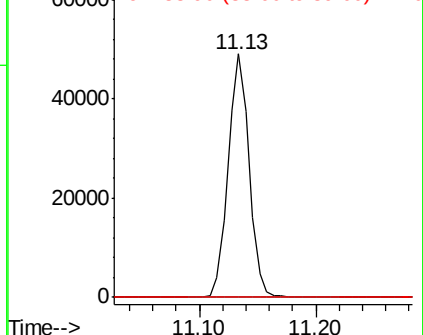

#84

1,2,4-Trimethylbenzene

Concen: 0.434 ug/l

RT: 11.80 min Scan# 1747

Delta R.T. -0.00 min

Lab File: VX011415.D


Acq: 09 Aug 2019 17:15

Tgt Ion:105 Resp: 3182

Ion Ratio Lower Upper



105 100


120 45.9 23.0 69.0



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

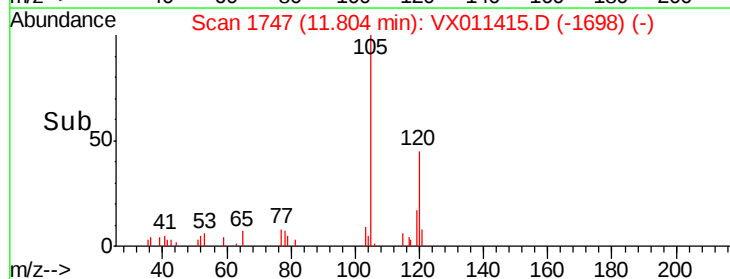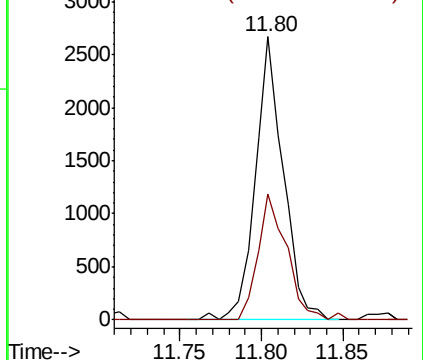







#93
 1,2,4-Trichlorobenzene
 Concen: 0.293 ug/l
 RT: 13.65 min Scan# 2049
 Delta R.T. -0.00 min
 Lab File: VX011415.D
 Acq: 09 Aug 2019 17:15

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-TB-2019-5

Tgt Ion:180 Resp: 842
 Ion Ratio Lower Upper
 180 100
 182 118.2 47.8 143.4
 145 32.5 14.8 44.3

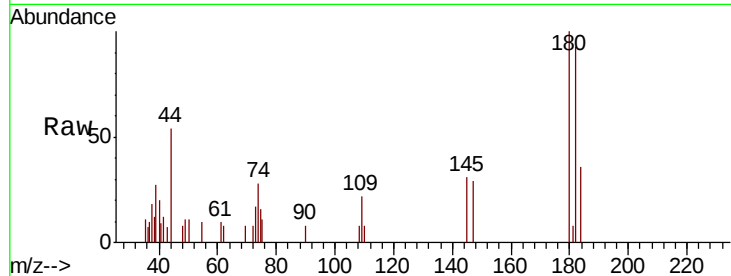


Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.80 (144.50 to 145.50): V


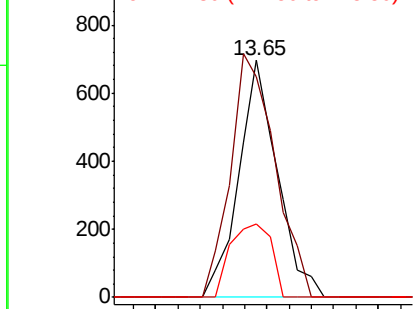



#94
 Hexachlorobutadiene
 Concen: 0.203 ug/l
 RT: 13.77 min Scan# 2070
 Delta R.T. -0.01 min
 Lab File: VX011415.D
 Acq: 09 Aug 2019 17:15

Tgt Ion:225 Resp: 296
 Ion Ratio Lower Upper
 225 100
 223 73.6 31.0 93.0
 227 88.9 32.2 96.6



Abundance Ion 224.70 (224.40 to 225.40): V
 Ion 222.70 (222.40 to 223.40): V
 Ion 226.70 (226.40 to 227.40): V




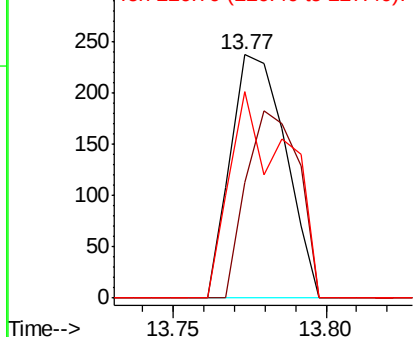




#95
Naphthalene
Concen: 0.515 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Instrument :
MSVOA_X
ClientSampleId :
Z3-TB-2019-5

Tgt Ion:128 Resp: 4324
Ion Ratio Lower Upper
128 100
127 18.7 10.4 15.6#
129 12.1 8.9 13.3

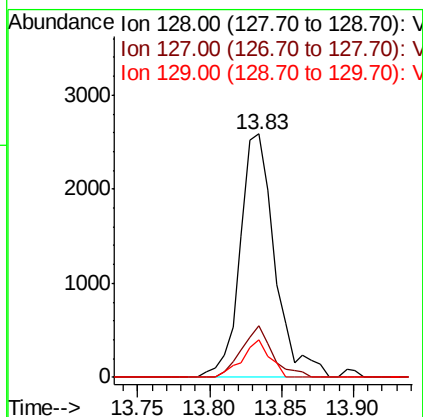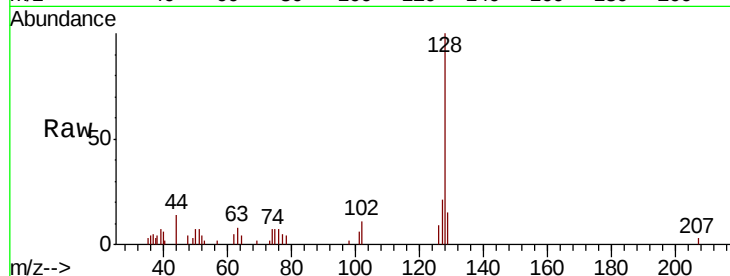

#96
1,2,3-Trichlorobenzene
Concen: 0.266 ug/l
RT: 14.02 min Scan# 2110
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Tgt Ion:180 Resp: 778
Ion Ratio Lower Upper
180 100
182 98.5 47.4 142.3
145 41.3 15.2 45.6

