

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX080919\
 Data File : VX011415.D
 Acq On : 09 Aug 2019 17:15
 Operator : JC/SP
 Sample : K4278-15
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-TB-2019-5

Quant Time: Aug 11 00:54:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 02 01:55:00 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.65	168	216403	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.85	114	315983	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	274250	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	128657	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	112599	51.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.34%	
35) Dibromofluoromethane	5.49	113	94982	46.04	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.08%	
50) Toluene-d8	8.71	98	361239	46.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.78%	
62) 4-Bromofluorobenzene	11.13	95	123140	44.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.58%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX080919\
Data File : VX011415.D
Acq On : 09 Aug 2019 17:15
Operator : JC/SP
Sample : K4278-15
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-TB-2019-5

Quant Time: Aug 11 00:54:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Quant Title : SW846 8260
QLast Update : Fri Aug 02 01:55:00 2019
Response via : Initial Calibration

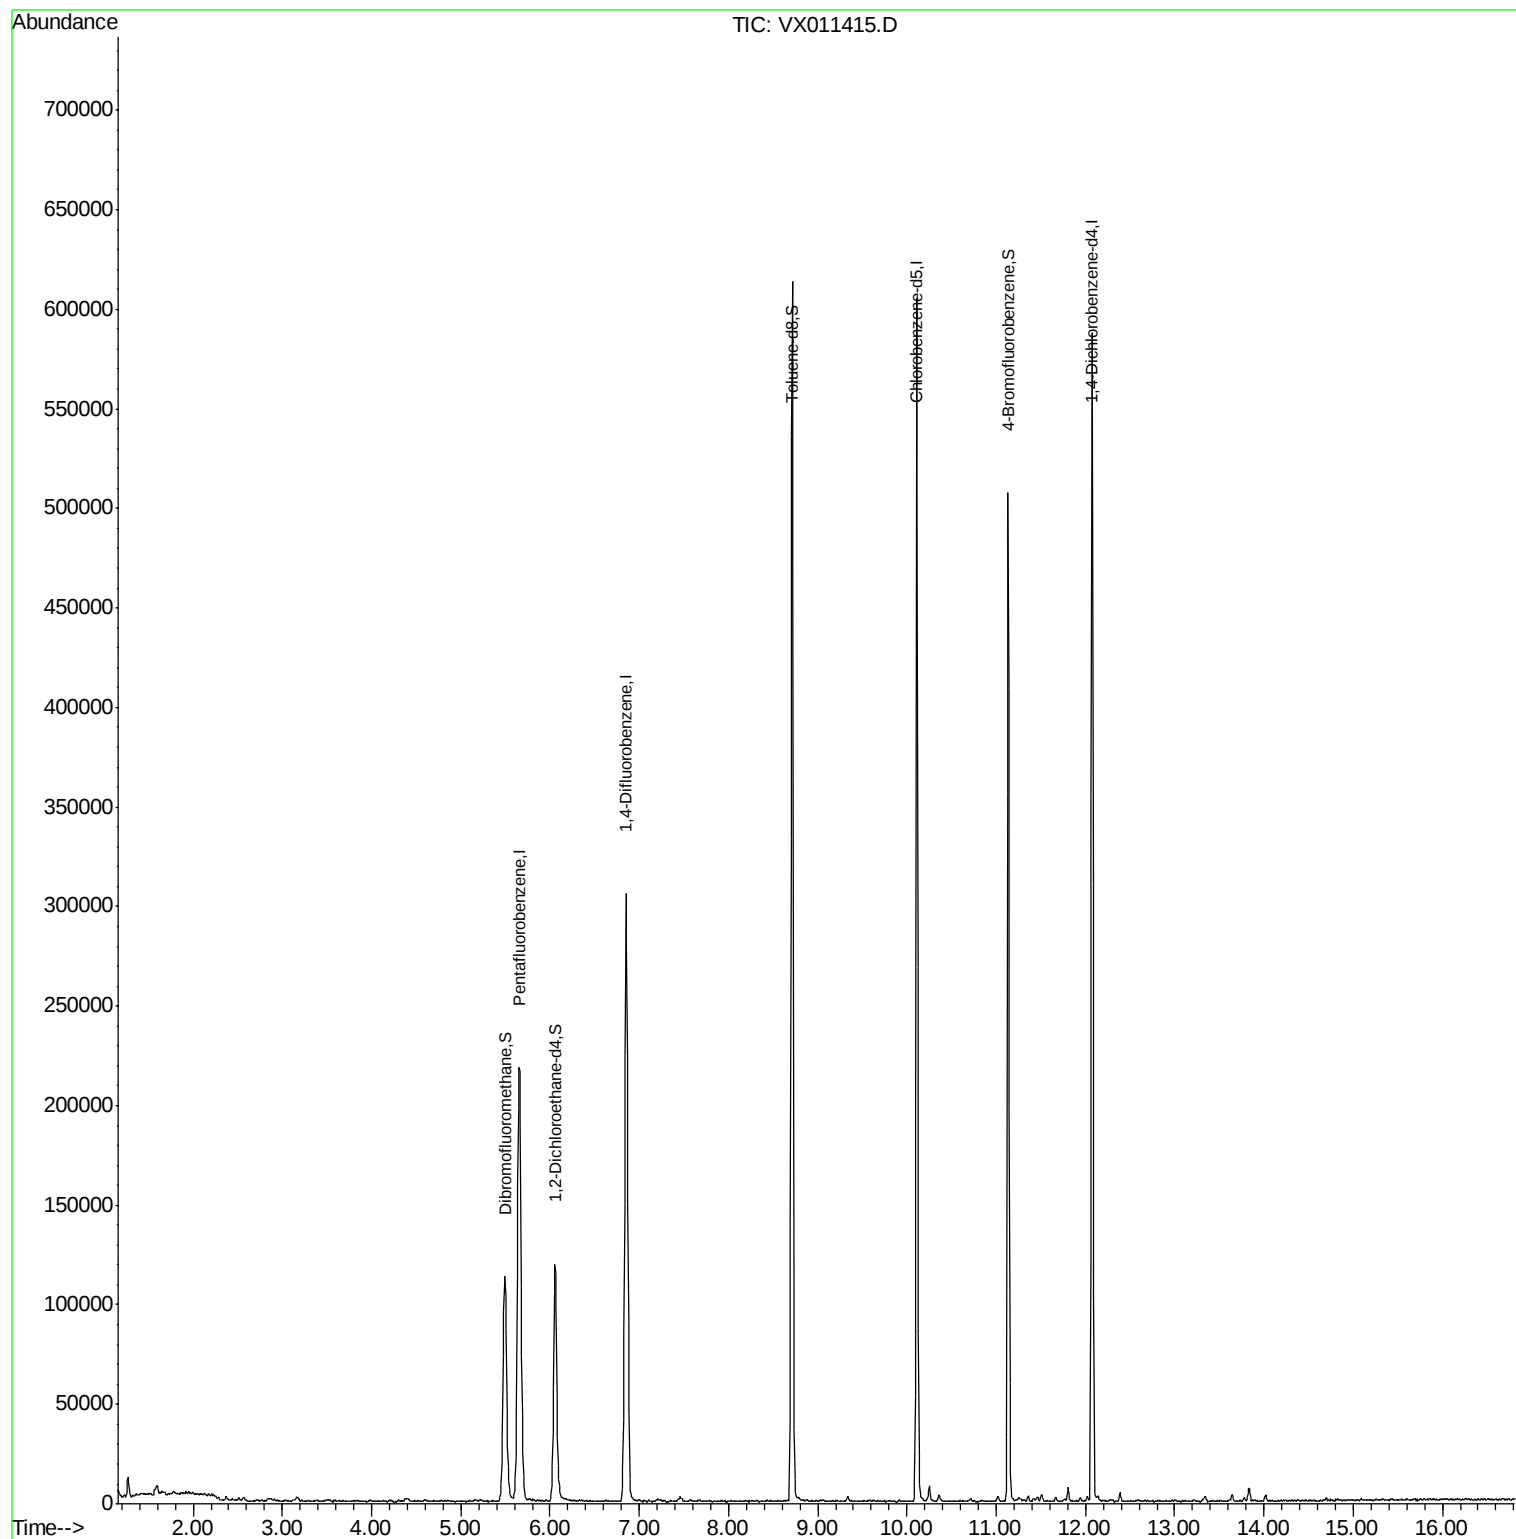



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.65 min Scan# 738

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :


Z3-TB-2019-5

Tot Ion:168 Resp: 216403

Ion Ratio Lower Upper




168 100

99 52.9 38.5 57.7

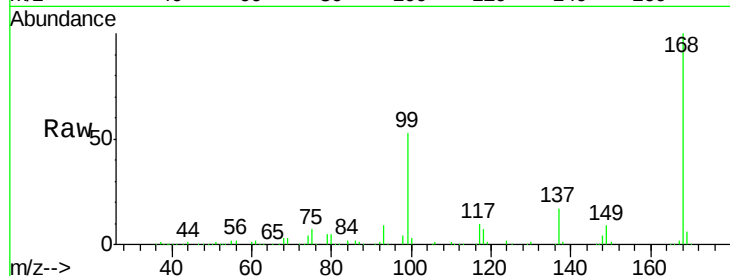

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

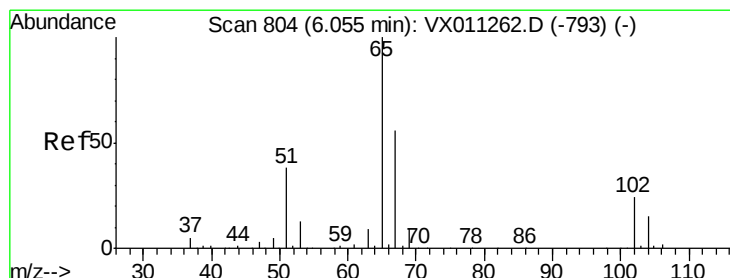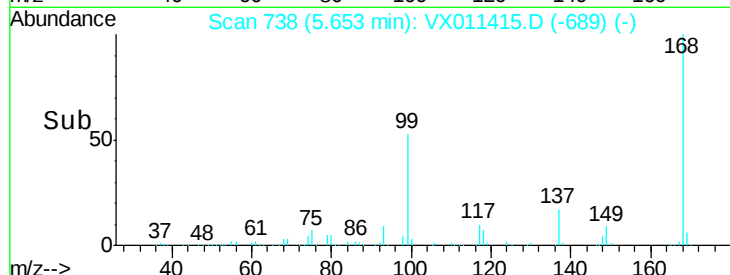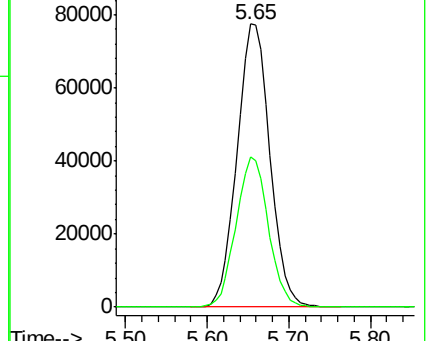

#33

1,2-Dichloroethane-d4

Concen: 51.668 ug/l

RT: 6.06 min Scan# 804

Delta R.T. -0.00 min

Lab File: VX011415.D


Acq: 09 Aug 2019 17:15

Tgt Ion: 65 Resp: 112599

Ion Ratio Lower Upper



65 100


67 51.6 0.0 110.6

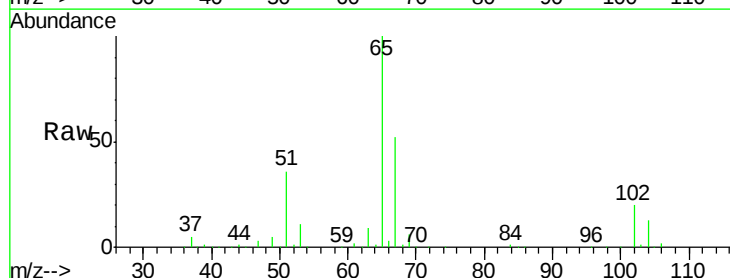

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

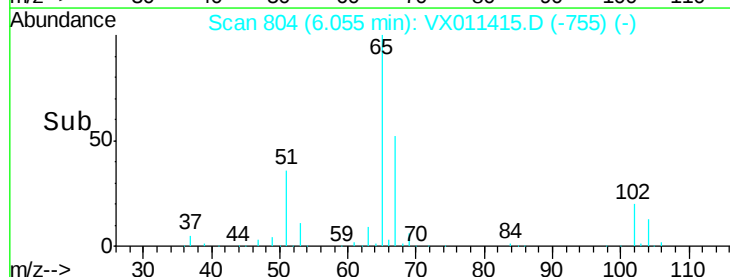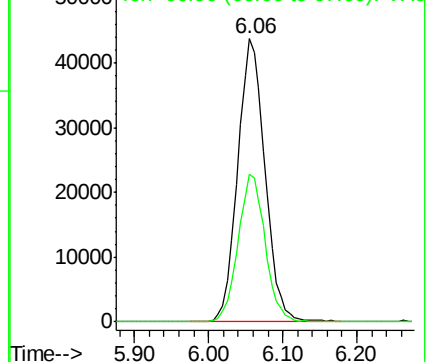

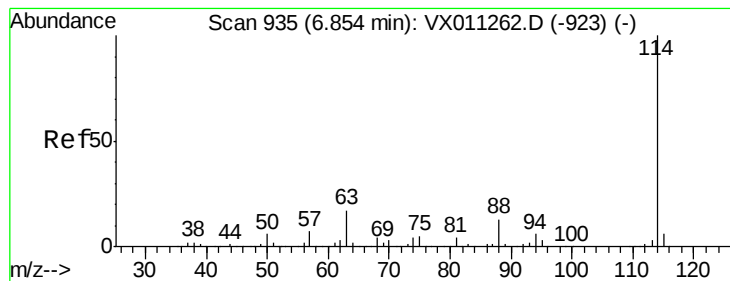

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.85 min Scan# 935

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampleId :

Z3-TB-2019-5


Tot Ion:114 Resp: 315983

Ion Ratio Lower Upper

114 100

63 18.3 0.0 34.0




88 14.3 0.0 26.4

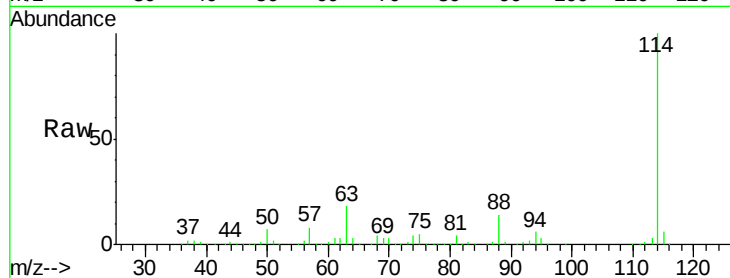

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

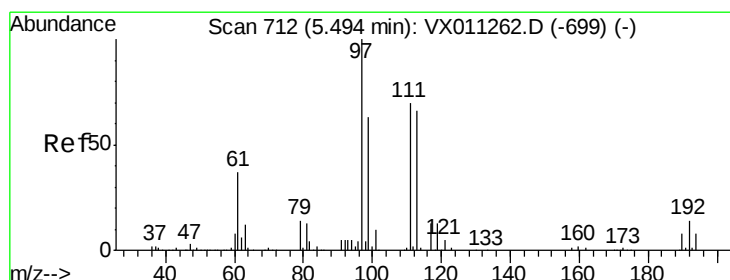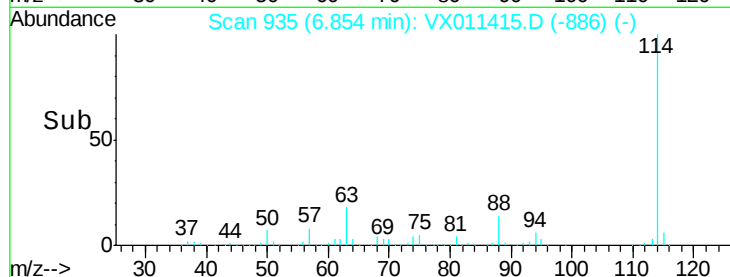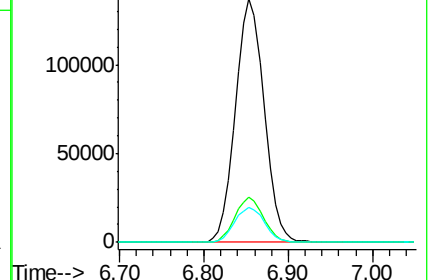

#35

Dibromofluoromethane

Concen: 46.041 ug/l

RT: 5.49 min Scan# 712

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15


Tgt Ion:113 Resp: 94982

Ion Ratio Lower Upper

113 100

111 101.6 81.9 122.9



192 21.7 17.8 26.8

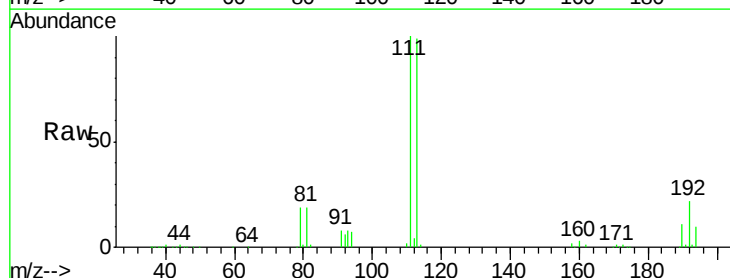


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

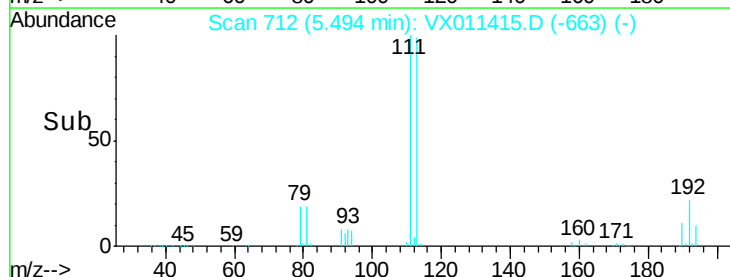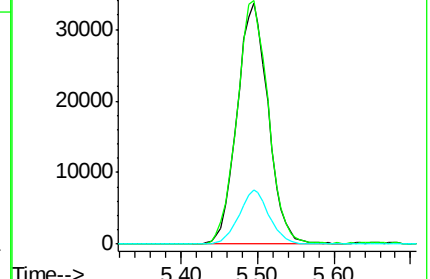

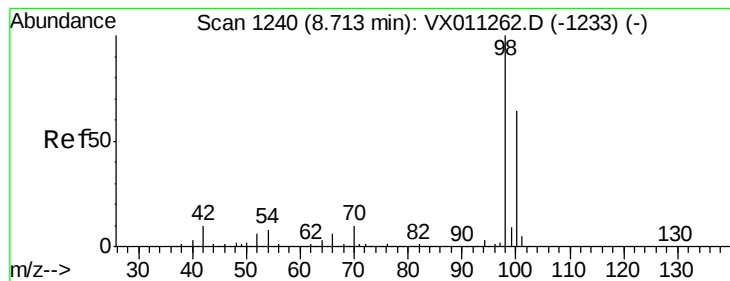

#50

Toluene-d8

Concen: 46.389 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15

Instrument :

MSVOA_X

ClientSampled :


Z3-TB-2019-5

Tot Ion: 98 Resp: 361239

Ion Ratio Lower Upper

98 100

100 64.4 51.7 77.5

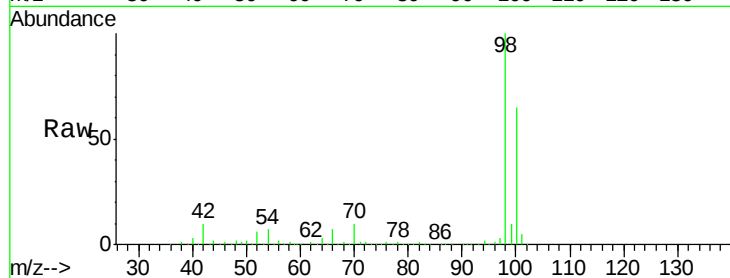

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

250000

200000

150000

100000

50000



0

8.60

8.70

8.80

Time-->

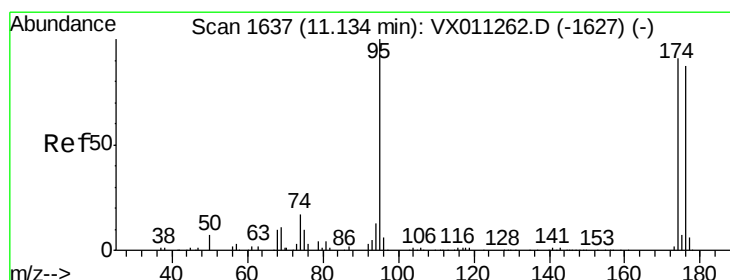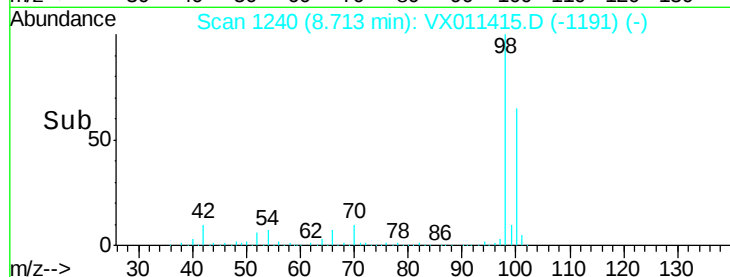

#62

4-Bromofluorobenzene

Concen: 44.291 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX011415.D

Acq: 09 Aug 2019 17:15


Tgt Ion: 95 Resp: 123140

Ion Ratio Lower Upper

95 100

174 91.6 0.0 191.2

176 87.9 0.0 184.8

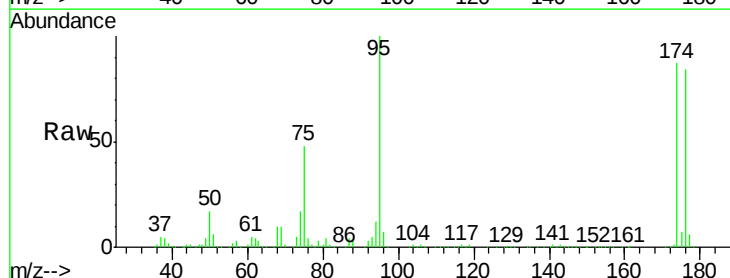

Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

100000


50000


0

11.10

11.20

Time-->




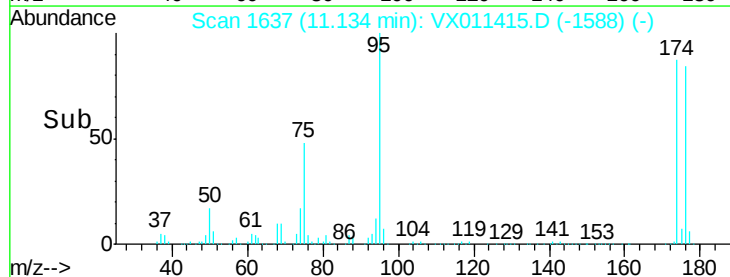


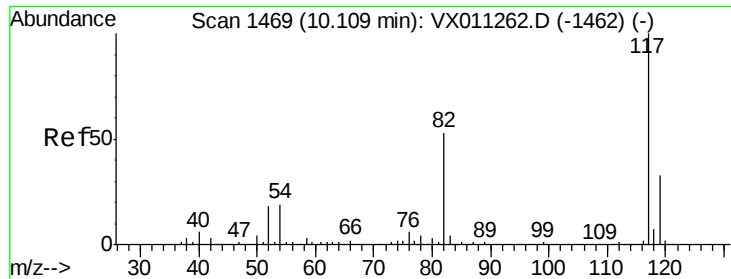

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Instrument :
MSVOA_X
ClientSampled :
Z3-TB-2019-5

Tot Ion:117 Resp: 274250
Ion Ratio Lower Upper
117 100
82 52.6 42.2 63.2
119 32.1 26.6 39.8

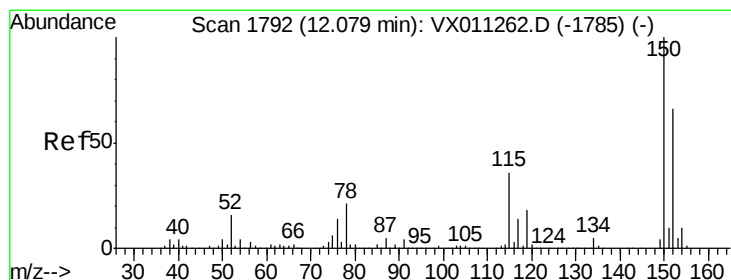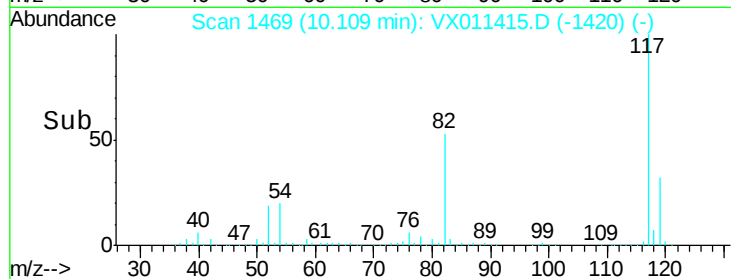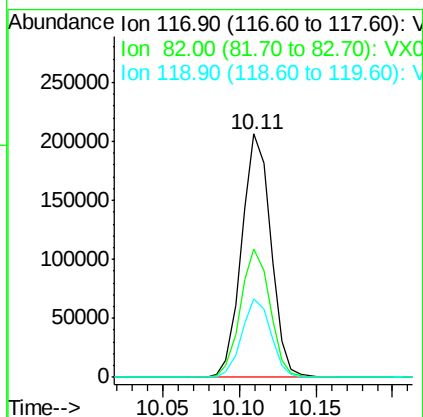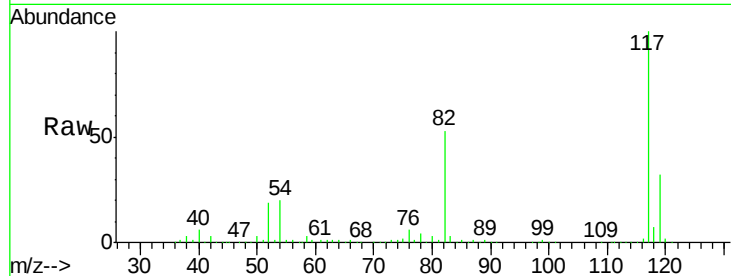

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX011415.D
Acq: 09 Aug 2019 17:15

Tgt Ion:152 Resp: 128657
Ion Ratio Lower Upper
152 100
115 56.0 40.0 119.9
150 157.0 0.0 350.4

