
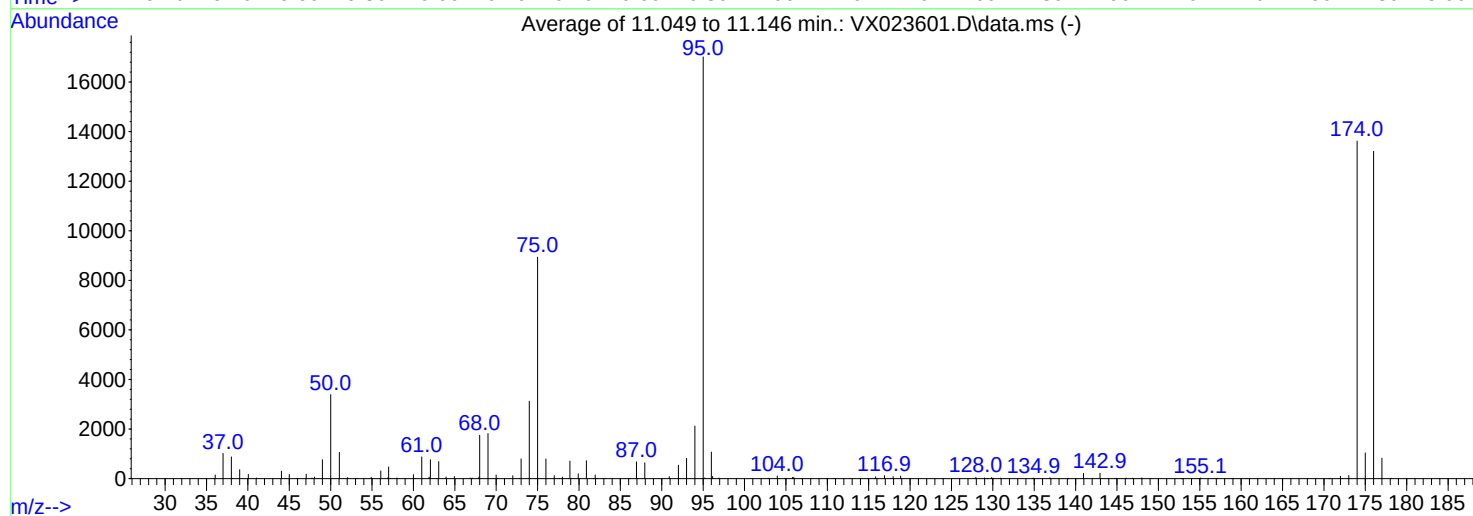


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080921\
 Data File : VX023601.D
 Acq On : 09 Aug 2021 09:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X080321W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Aug 03 12:05:42 2021

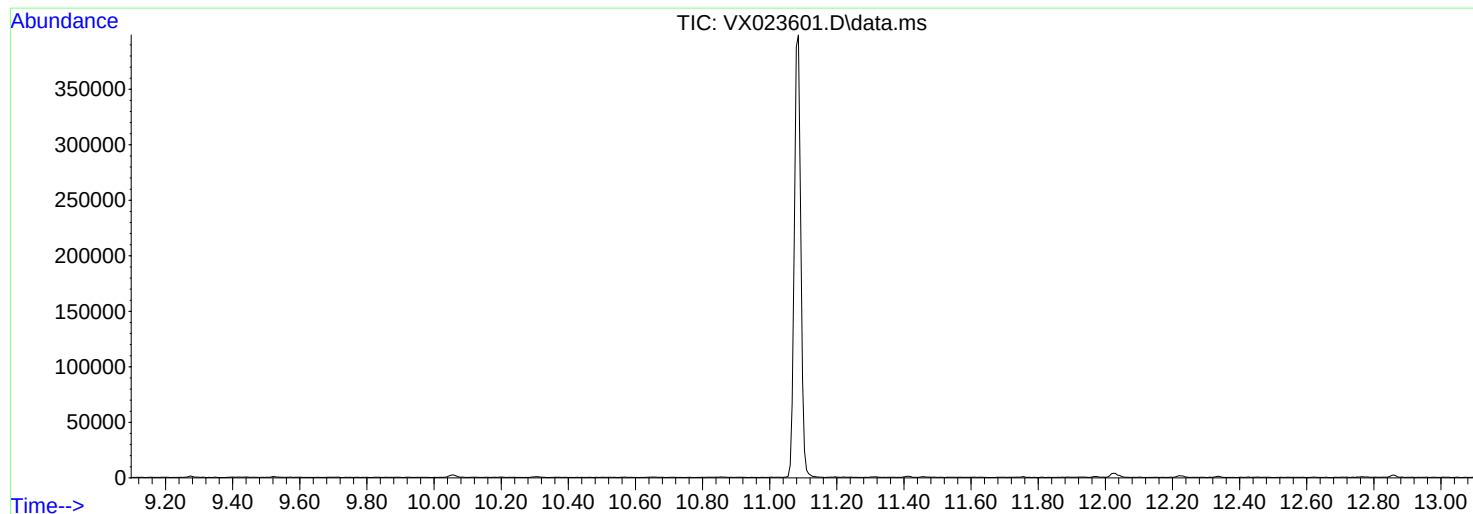

AutoFind: Averaged scan 1634 to 1650; Bkg corrected with scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	3391	PASS
75	95	30	60	52.5	8931	PASS
95	95	100	100	100.0	17014	PASS
96	95	5	9	6.3	1072	PASS
173	174	0.00	2	0.9	127	PASS
174	95	50	100	80.0	13617	PASS
175	174	5	9	7.6	1037	PASS
176	174	95	101	97.0	13207	PASS
177	176	5	9	6.3	826	PASS