

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080921\
 Data File : VX023610.D
 Acq On : 09 Aug 2021 13:40
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 LabSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260

Signal : TIC: VX023610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	71	79	82	rBV5	7132	12858	1.27%	0.196%
2	5.397	695	707	718	rBV2	111901	320077	31.63%	4.891%
3	5.562	722	734	750	rVB	190888	542060	53.57%	8.284%
4	5.964	789	800	815	rBV	125500	335462	33.15%	5.127%
5	6.769	920	932	948	rBV	304770	727611	71.91%	11.119%
6	8.653	1234	1241	1251	rBV	658128	1011863	100.00%	15.463%
7	10.055	1466	1471	1479	rBV	649603	884173	87.38%	13.512%
8	11.085	1635	1640	1651	rVB	550124	684869	67.68%	10.466%
9	12.024	1789	1794	1800	rBV	655045	807951	79.85%	12.347%
10	14.615	2216	2219	2226	rVV4	23992	40248	3.98%	0.615%
11	14.676	2226	2229	2232	rVV5	11347	14053	1.39%	0.215%
12	14.755	2240	2242	2245	rBV4	13876	15106	1.49%	0.231%
13	14.798	2246	2249	2251	rVV4	9111	10297	1.02%	0.157%
14	14.847	2254	2257	2261	rVV6	17069	25010	2.47%	0.382%
15	15.042	2286	2289	2293	rBV6	12175	25868	2.56%	0.395%
16	15.182	2309	2312	2314	rBV3	30565	38329	3.79%	0.586%
17	15.219	2315	2318	2321	rVB4	40320	49248	4.87%	0.753%
18	15.420	2348	2351	2354	rBV5	29765	41032	4.06%	0.627%
19	16.097	2457	2462	2469	rBV	550853	957451	94.62%	14.632%


Sum of corrected areas: 6543566

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080921\
Data File : VX023610.D
Acq On : 09 Aug 2021 13:40
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

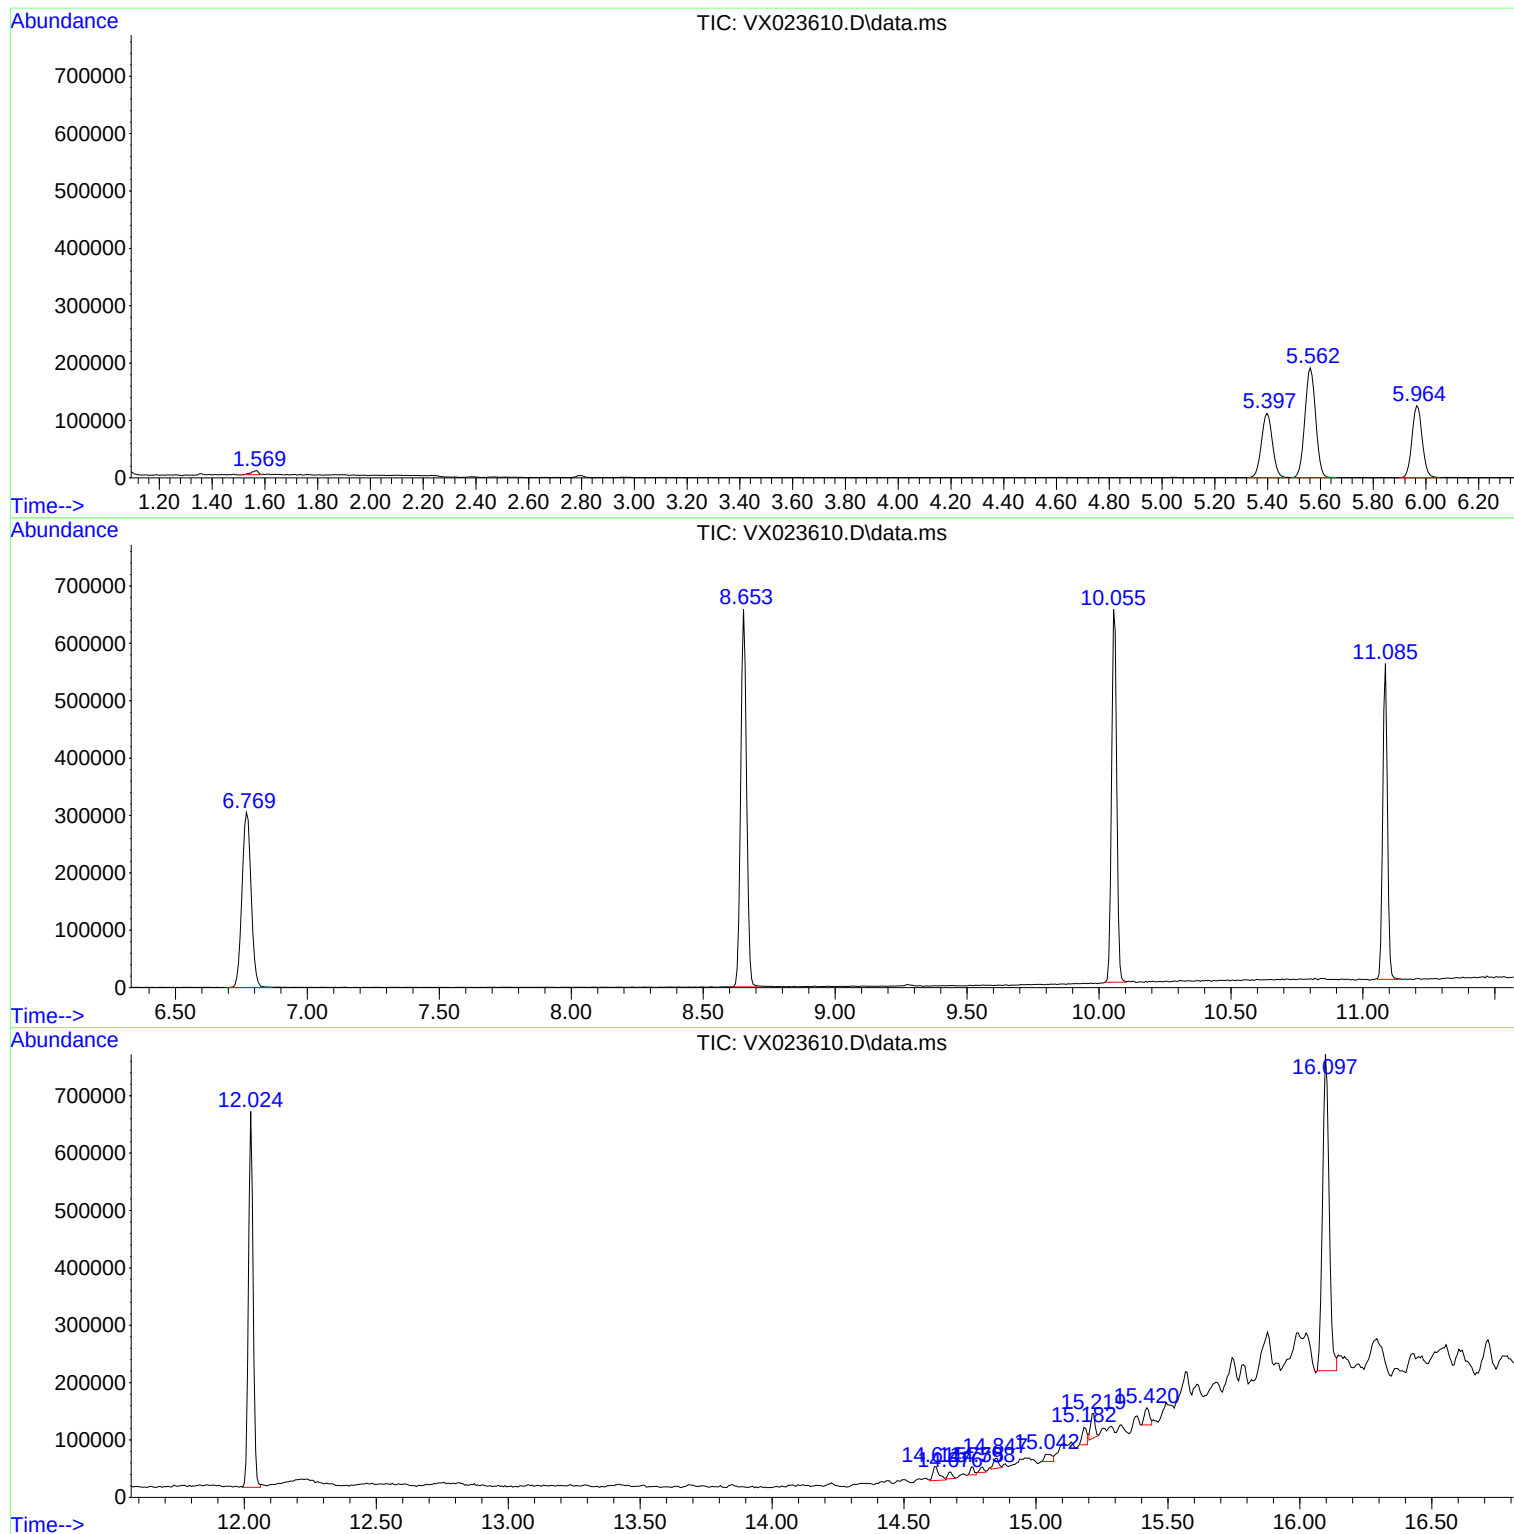

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080921\
Data File : VX023610.D
Acq On : 09 Aug 2021 13:40
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
IBLK










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butylated Hydroxytoluene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.097	59.25 ug/l	957451	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butylated Hydroxytoluene	220	C15H24O	000128-37-0	99
2			Ethyl 4-oxo-2-phenylpentanoate	220	C13H16O3	1000427-11-2	91
3			Phenol, 2,4,6-tris(1-methylethyl)-	220	C15H24O	002934-07-8	87
4			2,4,6-Tris(1,1-dimethylethyl)-4-...	276	C19H32O	019687-22-0	83
5			Phenol, 4,6-di(1,1-dimethylethyl)...	220	C15H24O	000616-55-7	81

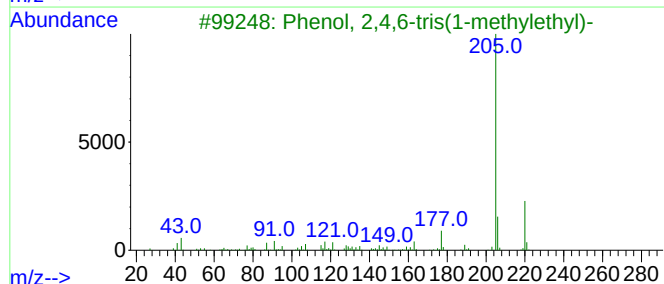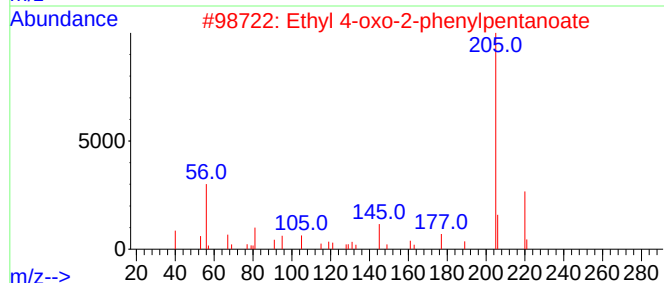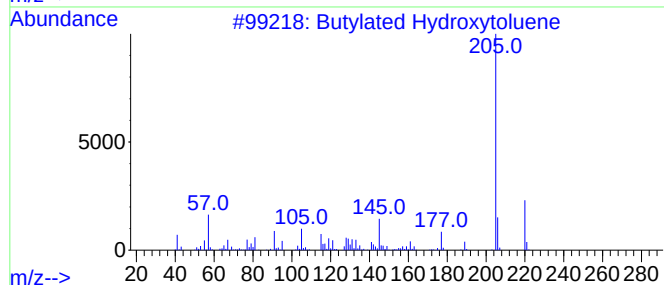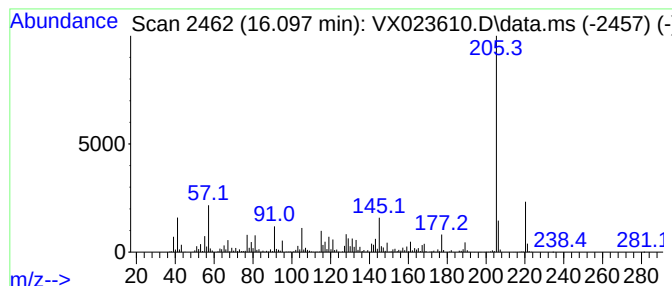

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080921\
Data File : VX023610.D
Acq On : 09 Aug 2021 13:40
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
LabSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butylated Hydro...	16.097	59.3	ug/l	957451	4	12.024	807951	50.0