
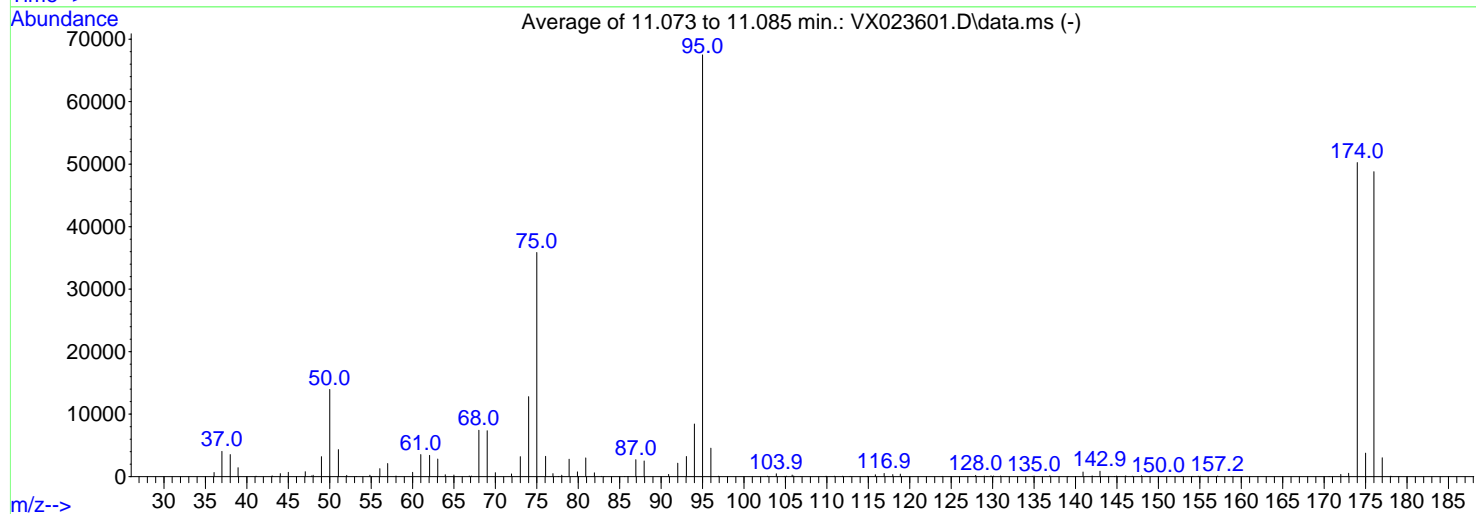


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX080921\  
 Data File : VX023601.D  
 Acq On : 09 Aug 2021 09:02  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072221W.M  
 Title : SW846 8260  
 Last Update : Fri Jul 23 06:05:38 2021

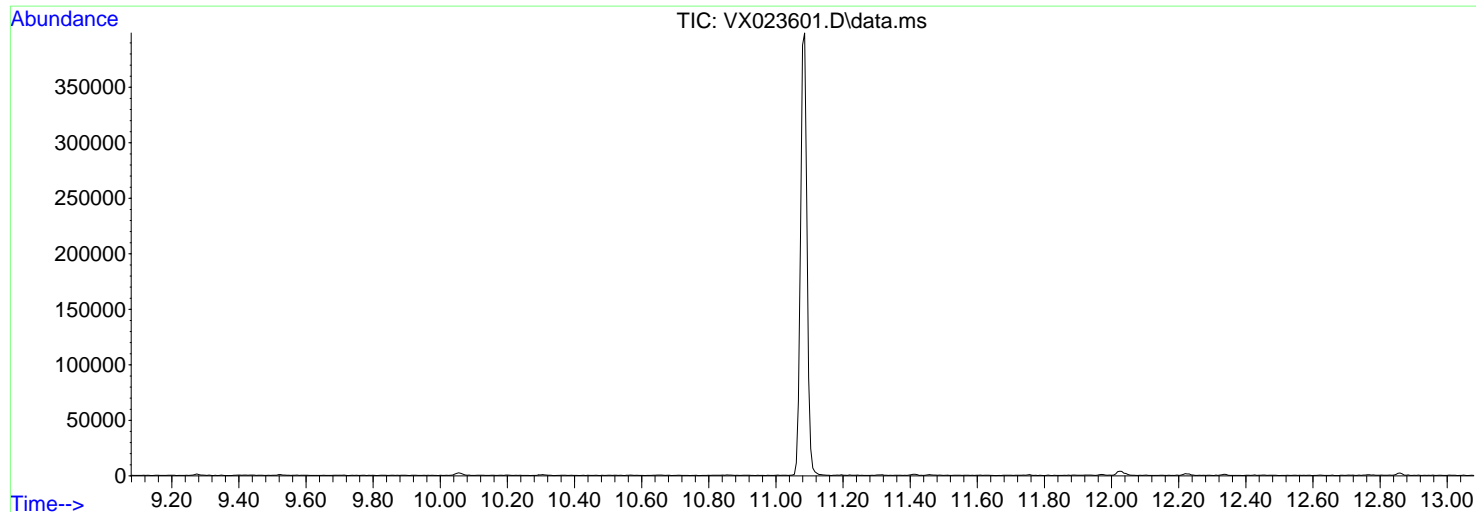

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	13945	PASS
75	95	30	60	53.2	35875	PASS
95	95	100	100	100.0	67488	PASS
96	95	5	9	6.7	4553	PASS
173	174	0.00	2	1.1	529	PASS
174	95	50	100	74.5	50261	PASS
175	174	5	9	7.5	3760	PASS
176	174	95	101	97.1	48784	PASS
177	176	5	9	6.2	3033	PASS