

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030525.D
 Acq On : 09 Aug 2022 14:03
 Operator : JC/MD
 Sample : VX0809WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK676

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M

Title : VOC Analysis

Signal : TIC: VX030525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	53	rVB	161076	176130	13.52%	1.838%
2	1.666	91	95	105	rVB	130584	163837	12.57%	1.710%
3	2.306	194	200	211	rVB	280091	428799	32.91%	4.475%
4	2.745	270	272	275	rVV2	472	488	0.04%	0.005%
5	2.788	275	279	287	rVB5	4462	8218	0.63%	0.086%
6	2.886	293	295	296	rBV2	384	314	0.02%	0.003%
7	2.946	300	305	312	rVB4	2548	5947	0.46%	0.062%
8	3.081	326	327	328	rBV	465	308	0.02%	0.003%
9	3.239	352	353	356	rBV2	325	334	0.03%	0.003%
10	3.300	361	363	367	rBV2	413	564	0.04%	0.006%
11	3.343	369	370	374	rVV2	411	404	0.03%	0.004%
12	3.550	401	404	406	rBV2	383	488	0.04%	0.005%
13	3.733	432	434	436	rBV2	302	338	0.03%	0.004%
14	4.019	479	481	484	rVB3	347	352	0.03%	0.004%
15	4.093	492	493	496	rBV	400	353	0.03%	0.004%
16	4.178	505	507	510	rBV	360	309	0.02%	0.003%
17	4.221	510	514	515	rVV2	361	395	0.03%	0.004%
18	4.397	540	543	546	rBV2	351	528	0.04%	0.006%
19	4.471	546	555	568	rBV	111564	331008	25.40%	3.454%
20	4.836	613	615	618	rBV2	431	449	0.03%	0.005%
21	5.062	641	652	670	rVB	170834	527448	40.48%	5.505%
22	5.300	689	691	693	rBV	487	407	0.03%	0.004%
23	5.361	699	701	702	rBV	530	545	0.04%	0.006%
24	5.385	702	705	706	rBV2	1039	1112	0.09%	0.012%
25	5.434	712	713	714	rVB	745	272	0.02%	0.003%
26	5.489	718	722	724	rBV2	342	461	0.04%	0.005%
27	5.550	727	732	734	rBV3	2293	3222	0.25%	0.034%
28	5.641	744	747	748	rBV2	430	368	0.03%	0.004%
29	5.751	763	765	767	rBV2	404	463	0.04%	0.005%
30	5.806	772	774	778	rBV2	281	383	0.03%	0.004%
31	5.842	778	780	782	rBV	405	268	0.02%	0.003%
32	5.976	789	802	816	rBV2	442252	1302934	100.00%	13.598%
33	6.239	843	845	848	rBV3	367	502	0.04%	0.005%
34	6.342	860	862	863	rBV	359	299	0.02%	0.003%
35	6.379	866	868	869	rBV	470	393	0.03%	0.004%
36	6.440	877	878	883	rBV3	577	885	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030525.D
 Acq On : 09 Aug 2022 14:03
 Operator : JC/MD
 Sample : VX0809WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK676

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.482	883	885	888	rVV2	631	627	0.05%	0.007%
38	6.537	892	894	896	rVV2	502	500	0.04%	0.005%
39	6.696	917	920	921	rBV	306	297	0.02%	0.003%
40	6.769	921	932	947	rBV	294717	701854	53.87%	7.325%
41	7.062	977	980	981	rBV2	445	411	0.03%	0.004%
42	7.110	982	988	997	rVV4	12151	29159	2.24%	0.304%
43	7.318	1012	1022	1032	rBV	264907	593040	45.52%	6.189%
44	7.488	1049	1050	1051	rVB	828	303	0.02%	0.003%
45	7.586	1063	1066	1067	rBV2	396	381	0.03%	0.004%
46	7.622	1071	1072	1076	rVB2	561	642	0.05%	0.007%
47	7.708	1081	1086	1087	rBV2	418	413	0.03%	0.004%
48	8.061	1139	1144	1146	rBV2	449	618	0.05%	0.006%
49	8.080	1146	1147	1151	rVB2	377	368	0.03%	0.004%
50	8.275	1177	1179	1181	rVB	470	312	0.02%	0.003%
51	8.330	1181	1188	1199	rBV	194043	308203	23.65%	3.216%
52	8.506	1215	1217	1218	rVB2	759	470	0.04%	0.005%
53	8.580	1228	1229	1230	rBV	653	369	0.03%	0.004%
54	8.653	1234	1241	1249	rBV	662210	1016906	78.05%	10.613%
55	8.799	1263	1265	1266	rBV	363	278	0.02%	0.003%
56	8.884	1277	1279	1280	rBV	400	355	0.03%	0.004%
57	8.952	1285	1290	1299	rVV	133080	201046	15.43%	2.098%
58	9.214	1331	1333	1336	rVB	491	498	0.04%	0.005%
59	9.238	1336	1337	1338	rBV	471	287	0.02%	0.003%
60	9.275	1340	1343	1350	rVB4	1610	2419	0.19%	0.025%
61	9.336	1351	1353	1356	rBV2	527	476	0.04%	0.005%
62	9.390	1356	1362	1374	rBV	514527	726779	55.78%	7.585%
63	9.592	1393	1395	1397	rVB	568	379	0.03%	0.004%
64	9.610	1397	1398	1399	rBV	592	270	0.02%	0.003%
65	9.707	1408	1414	1422	rVB3	3337	5749	0.44%	0.060%
66	9.854	1437	1438	1440	rBV2	488	329	0.03%	0.003%
67	9.957	1453	1455	1457	rBV	522	425	0.03%	0.004%
68	10.055	1465	1471	1482	rVV	606683	813287	62.42%	8.488%
69	10.232	1498	1500	1501	rVB	614	336	0.03%	0.004%
70	10.463	1536	1538	1542	rVB2	498	699	0.05%	0.007%
71	10.506	1542	1545	1546	rBV	582	438	0.03%	0.005%
72	10.652	1563	1569	1574	rBV3	875	2558	0.20%	0.027%
73	10.713	1576	1579	1583	rVB2	469	662	0.05%	0.007%
74	10.756	1583	1586	1589	rBV2	547	735	0.06%	0.008%
75	11.073	1635	1638	1639	rBV	750	839	0.06%	0.009%
76	11.091	1639	1641	1643	rVB	736	553	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030525.D
 Acq On : 09 Aug 2022 14:03
 Operator : JC/MD
 Sample : VX0809WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK676

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.195	1652	1658	1668	rBV	467545	589276	45.23%	6.150%
78	11.329	1678	1680	1683	rBV2	369	459	0.04%	0.005%
79	11.628	1727	1729	1731	rBV2	536	356	0.03%	0.004%
80	11.707	1740	1742	1749	rBV3	772	1192	0.09%	0.012%
81	11.756	1749	1750	1753	rVB	630	436	0.03%	0.005%
82	12.024	1789	1794	1804	rBV	621984	745595	57.22%	7.781%
83	12.225	1822	1827	1837	rBV3	7460	12446	0.96%	0.130%
84	12.323	1837	1843	1852	rBV	672237	843370	64.73%	8.802%
85	12.518	1873	1875	1877	rBV2	470	375	0.03%	0.004%
86	12.689	1901	1903	1905	rVB	443	307	0.02%	0.003%
87	12.859	1927	1931	1935	rBV3	2804	3209	0.25%	0.033%
88	13.115	1971	1973	1977	rVB2	609	600	0.05%	0.006%
89	13.243	1992	1994	1995	rBV	492	391	0.03%	0.004%
90	13.695	2064	2068	2075	rBV4	2551	3879	0.30%	0.040%
91	13.932	2106	2107	2109	rBV2	577	366	0.03%	0.004%
92	13.957	2109	2111	2115	rVB4	451	393	0.03%	0.004%
93	14.079	2130	2131	2133	rBV	615	478	0.04%	0.005%
94	14.134	2137	2140	2145	rVB3	666	1187	0.09%	0.012%
95	14.572	2210	2212	2213	rBV	610	383	0.03%	0.004%
96	14.719	2234	2236	2240	rVB2	800	683	0.05%	0.007%
97	14.975	2276	2278	2279	rVB	1061	513	0.04%	0.005%
98	14.999	2279	2282	2283	rBV2	553	479	0.04%	0.005%
99	15.969	2438	2441	2442	rBV	774	917	0.07%	0.010%
100	16.664	2553	2555	2558	rBV2	904	905	0.07%	0.009%


Sum of corrected areas: 9581990

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030525.D
Acq On : 09 Aug 2022 14:03
Operator : JC/MD
Sample : VX0809WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

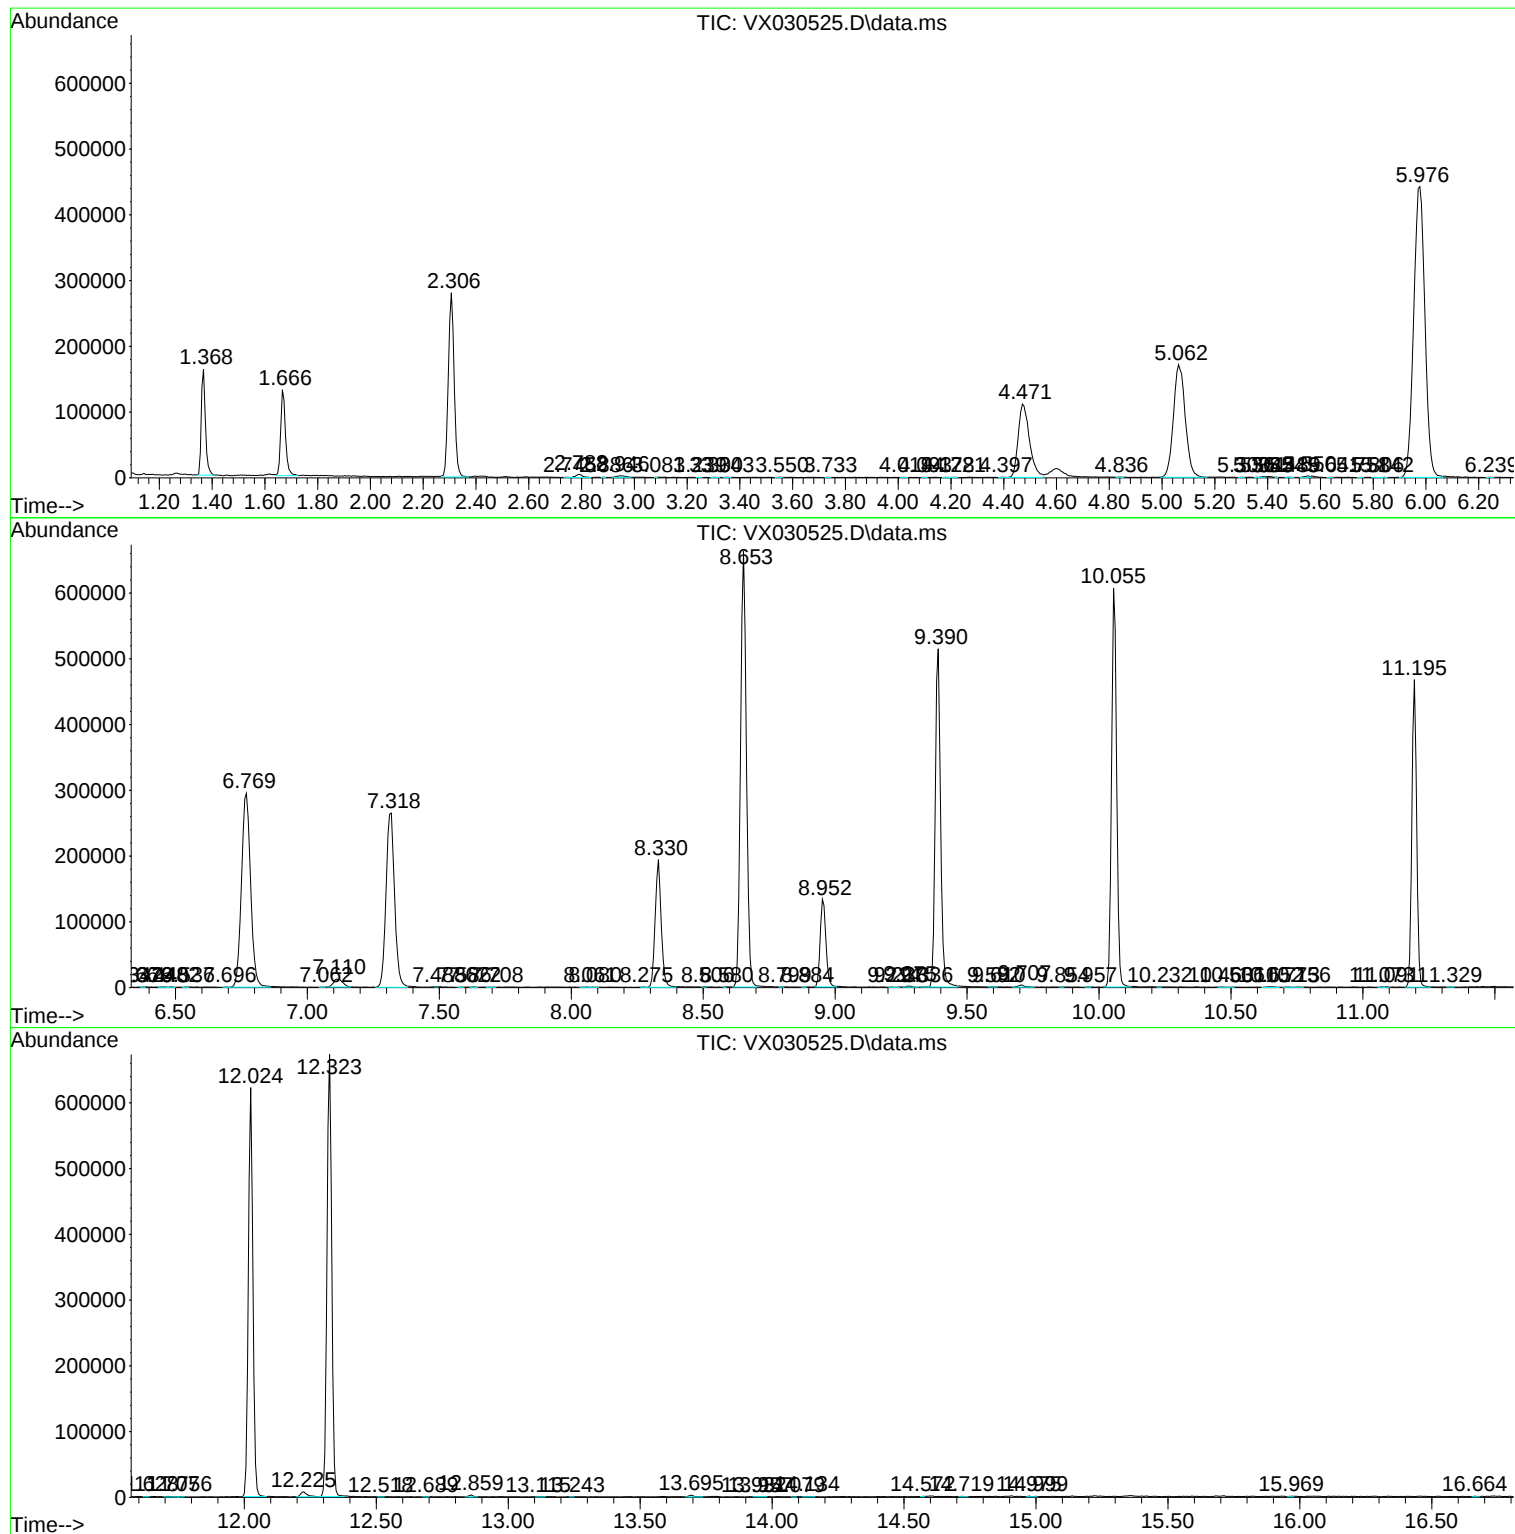

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030525.D
Acq On : 09 Aug 2022 14:03
Operator : JC/MD
Sample : VX0809WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030525.D
Acq On : 09 Aug 2022 14:03
Operator : JC/MD
Sample : VX0809WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK676

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc