

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030526.D
 Acq On : 09 Aug 2022 14:31
 Operator : JC/MD
 Sample : N4066-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

Signal : TIC: VX030526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	42	46	57	rVB	158871	174282	13.35%	1.756%
2	1.666	91	95	104	rVB	127845	156886	12.02%	1.581%
3	2.306	194	200	211	rVB	284239	444791	34.08%	4.482%
4	2.514	230	234	235	rBV2	582	835	0.06%	0.008%
5	2.556	238	241	242	rBV	568	395	0.03%	0.004%
6	2.788	275	279	288	rVB2	4805	8687	0.67%	0.088%
7	2.940	298	304	305	rBV2	2280	3148	0.24%	0.032%
8	3.008	313	315	317	rBV2	359	312	0.02%	0.003%
9	3.050	320	322	325	rBV	420	511	0.04%	0.005%
10	3.093	327	329	334	rVB2	498	414	0.03%	0.004%
11	3.136	334	336	338	rBV2	338	252	0.02%	0.003%
12	3.154	338	339	341	rVB	356	229	0.02%	0.002%
13	3.379	373	376	380	rVV2	475	690	0.05%	0.007%
14	3.446	384	387	388	rBV	465	338	0.03%	0.003%
15	3.544	398	403	406	rBV2	447	878	0.07%	0.009%
16	3.617	414	415	418	rVB3	472	353	0.03%	0.004%
17	3.648	418	420	423	rBV2	262	294	0.02%	0.003%
18	3.751	433	437	439	rBV2	561	719	0.06%	0.007%
19	3.885	458	459	460	rVV	531	238	0.02%	0.002%
20	4.007	477	479	482	rVV2	407	380	0.03%	0.004%
21	4.178	505	507	508	rBV	346	244	0.02%	0.002%
22	4.269	520	522	524	rVB	397	227	0.02%	0.002%
23	4.306	524	528	529	rBV	649	488	0.04%	0.005%
24	4.373	537	539	541	rBV2	404	374	0.03%	0.004%
25	4.471	545	555	569	rBV	109015	332327	25.46%	3.349%
26	4.958	631	635	637	rBV2	363	360	0.03%	0.004%
27	5.068	640	653	669	rVV2	176468	528943	40.53%	5.330%
28	5.263	684	685	687	rVB	720	380	0.03%	0.004%
29	5.294	688	690	694	rVB2	417	442	0.03%	0.004%
30	5.513	723	726	727	rBV2	564	638	0.05%	0.006%
31	5.702	755	757	762	rBV2	480	852	0.07%	0.009%
32	5.787	768	771	772	rBV2	789	789	0.06%	0.008%
33	5.842	777	780	782	rBV	621	625	0.05%	0.006%
34	5.970	789	801	822	rBV2	448827	1305092	100.00%	13.152%
35	6.208	838	840	844	rBV3	458	568	0.04%	0.006%
36	6.330	857	860	863	rBV2	387	421	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030526.D
 Acq On : 09 Aug 2022 14:31
 Operator : JC/MD
 Sample : N4066-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

37	6.361	863	865	866	rBV2	501	273	0.02%	0.003%
38	6.452	878	880	882	rBV2	484	621	0.05%	0.006%
39	6.537	891	894	898	rBV3	536	826	0.06%	0.008%
40	6.653	911	913	915	rBV	361	343	0.03%	0.003%
41	6.763	920	931	947	rBV	333385	785894	60.22%	7.920%
42	7.056	976	979	982	rBV2	478	617	0.05%	0.006%
43	7.117	982	989	996	rVV3	12140	28533	2.19%	0.288%
44	7.312	1010	1021	1034	rBV	274119	607538	46.55%	6.122%
45	7.659	1076	1078	1080	rBV2	390	358	0.03%	0.004%
46	7.805	1100	1102	1105	rBV2	339	429	0.03%	0.004%
47	7.854	1108	1110	1114	rVV2	515	682	0.05%	0.007%
48	7.891	1114	1116	1119	rVB2	367	275	0.02%	0.003%
49	8.013	1135	1136	1140	rVB2	490	343	0.03%	0.003%
50	8.043	1140	1141	1144	rBV	405	346	0.03%	0.003%
51	8.171	1161	1162	1164	rBV	330	238	0.02%	0.002%
52	8.330	1181	1188	1200	rBV	189300	306573	23.49%	3.089%
53	8.586	1227	1230	1231	rBV	676	681	0.05%	0.007%
54	8.653	1234	1241	1257	rBV	678718	1035423	79.34%	10.434%
55	8.848	1271	1273	1274	rBV	452	212	0.02%	0.002%
56	8.952	1285	1290	1301	rBV	143559	207798	15.92%	2.094%
57	9.116	1314	1317	1319	rBV2	737	758	0.06%	0.008%
58	9.269	1338	1342	1346	rBV4	897	1418	0.11%	0.014%
59	9.391	1356	1362	1374	rBV	510800	727339	55.73%	7.330%
60	9.708	1409	1414	1419	rVB3	3936	6267	0.48%	0.063%
61	9.805	1428	1430	1432	rVB2	436	347	0.03%	0.003%
62	9.842	1432	1436	1437	rBV2	477	468	0.04%	0.005%
63	9.921	1447	1449	1450	rBV	420	239	0.02%	0.002%
64	10.055	1466	1471	1483	rBV	660034	865669	66.33%	8.724%
65	10.201	1491	1495	1498	rVB2	769	1159	0.09%	0.012%
66	10.311	1511	1513	1515	rVB2	753	467	0.04%	0.005%
67	10.427	1528	1532	1534	rBV2	412	525	0.04%	0.005%
68	10.561	1552	1554	1557	rBV2	473	396	0.03%	0.004%
69	10.732	1581	1582	1584	rBV2	250	253	0.02%	0.003%
70	10.835	1597	1599	1602	rBV2	359	392	0.03%	0.004%
71	10.902	1606	1610	1612	rVB3	379	554	0.04%	0.006%
72	10.933	1613	1615	1616	rBV	307	229	0.02%	0.002%
73	11.195	1652	1658	1667	rBV	474458	587561	45.02%	5.921%
74	11.317	1677	1678	1679	rBV	586	260	0.02%	0.003%
75	11.415	1692	1694	1696	rBV2	605	657	0.05%	0.007%
76	11.671	1735	1736	1739	rBV	448	529	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
 Data File : VX030526.D
 Acq On : 09 Aug 2022 14:31
 Operator : JC/MD
 Sample : N4066-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
 Title : VOC Analysis

77	11.829	1759	1762	1763	rVB2	409	330	0.03%	0.003%
78	11.847	1763	1765	1766	rBV	519	284	0.02%	0.003%
79	11.969	1783	1785	1788	rBV2	522	656	0.05%	0.007%
80	12.024	1789	1794	1803	rVV	702124	844800	64.73%	8.513%
81	12.225	1820	1827	1832	rBV4	6838	11789	0.90%	0.119%
82	12.323	1837	1843	1853	rVV	726922	910894	69.80%	9.179%
83	12.506	1871	1873	1874	rBV	459	378	0.03%	0.004%
84	12.548	1878	1880	1884	rVV3	420	356	0.03%	0.004%
85	12.597	1887	1888	1889	rVB	542	206	0.02%	0.002%
86	12.664	1897	1899	1900	rBV	452	267	0.02%	0.003%
87	12.768	1914	1916	1919	rBV2	446	424	0.03%	0.004%
88	12.859	1928	1931	1936	rVB3	2416	2523	0.19%	0.025%
89	13.152	1977	1979	1982	rVB3	719	649	0.05%	0.007%
90	13.396	2018	2019	2021	rBV	416	358	0.03%	0.004%
91	13.573	2046	2048	2049	rBV2	417	392	0.03%	0.004%
92	13.695	2064	2068	2071	rBV3	1955	2617	0.20%	0.026%
93	13.945	2105	2109	2112	rBV2	424	741	0.06%	0.007%
94	14.127	2137	2139	2140	rBV2	789	578	0.04%	0.006%
95	14.268	2160	2162	2163	rBV2	544	359	0.03%	0.004%
96	14.487	2196	2198	2203	rBV4	684	964	0.07%	0.010%
97	14.542	2205	2207	2208	rBV2	618	390	0.03%	0.004%
98	14.627	2218	2221	2223	rBV2	589	632	0.05%	0.006%
99	14.957	2272	2275	2278	rBV4	1048	1329	0.10%	0.013%
100	15.219	2316	2318	2319	rBV2	778	483	0.04%	0.005%


Sum of corrected areas: 9923291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030526.D
Acq On : 09 Aug 2022 14:31
Operator : JC/MD
Sample : N4066-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

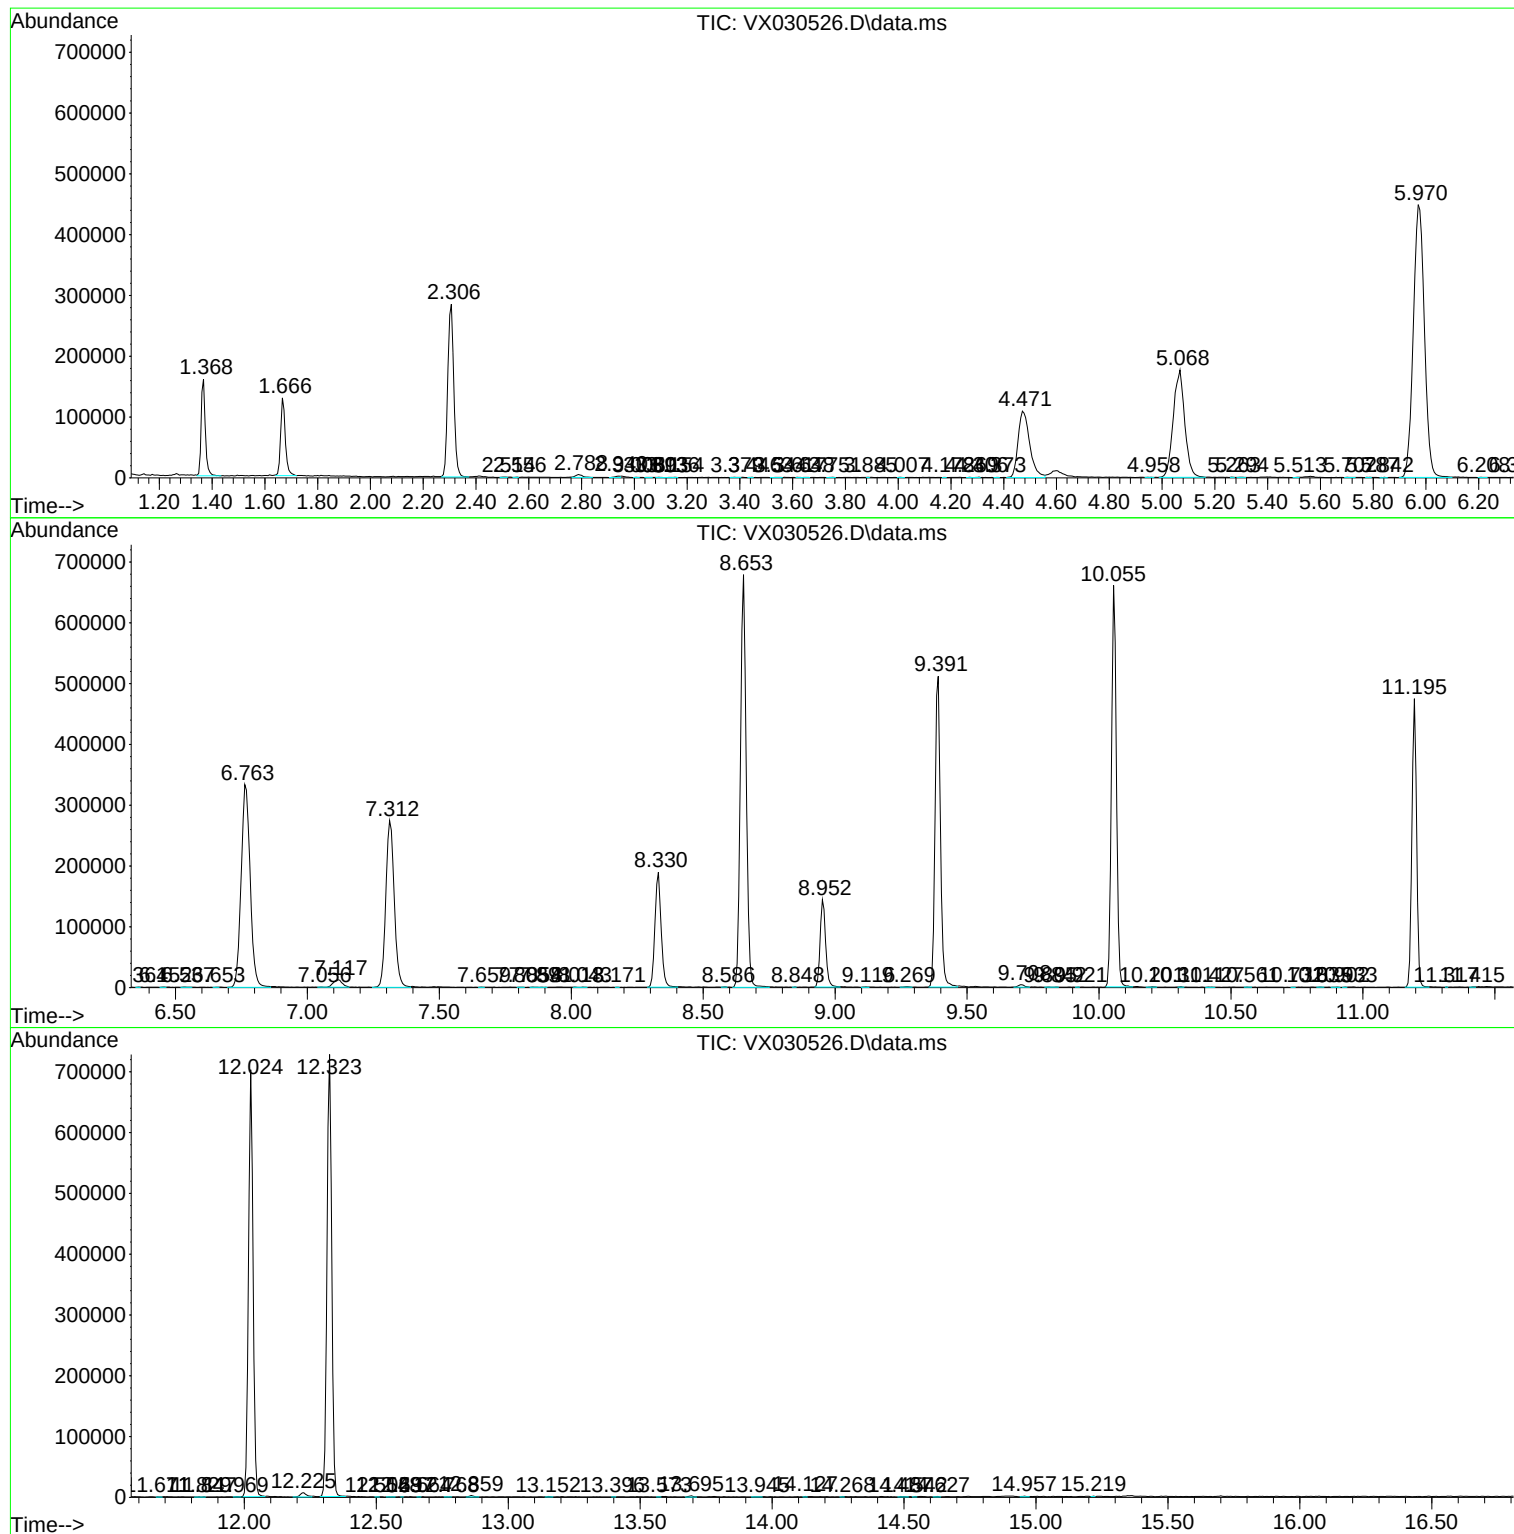

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030526.D
Acq On : 09 Aug 2022 14:31
Operator : JC/MD
Sample : N4066-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080922\
Data File : VX030526.D
Acq On : 09 Aug 2022 14:31
Operator : JC/MD
Sample : N4066-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML080422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc